
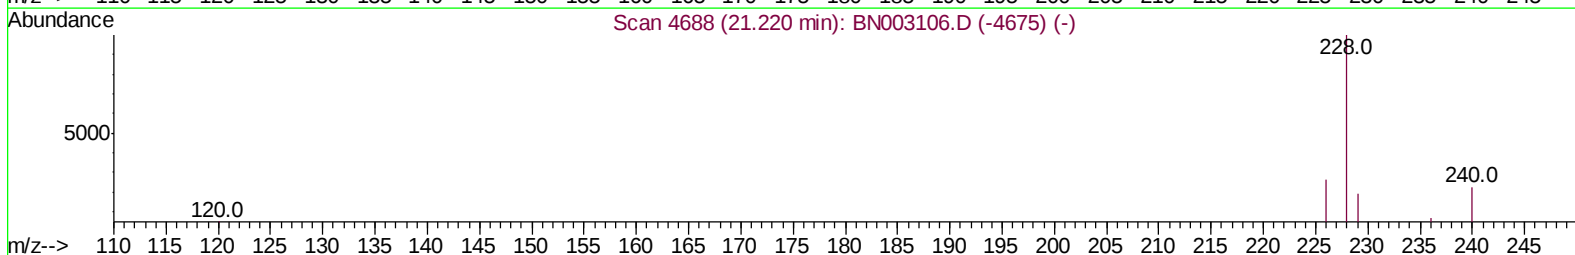
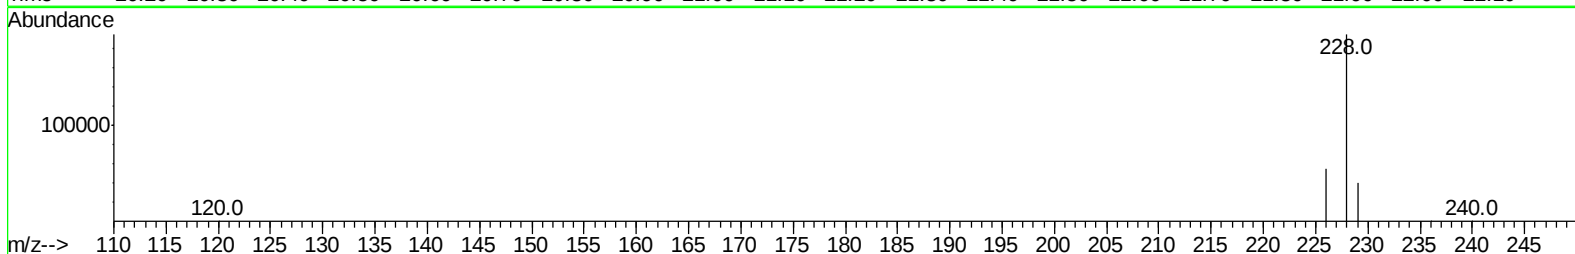


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003118.D
Acq On : 12 Oct 2018 00:08
Operator : MJ/SJ
Sample : J5230-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 12 07:14:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

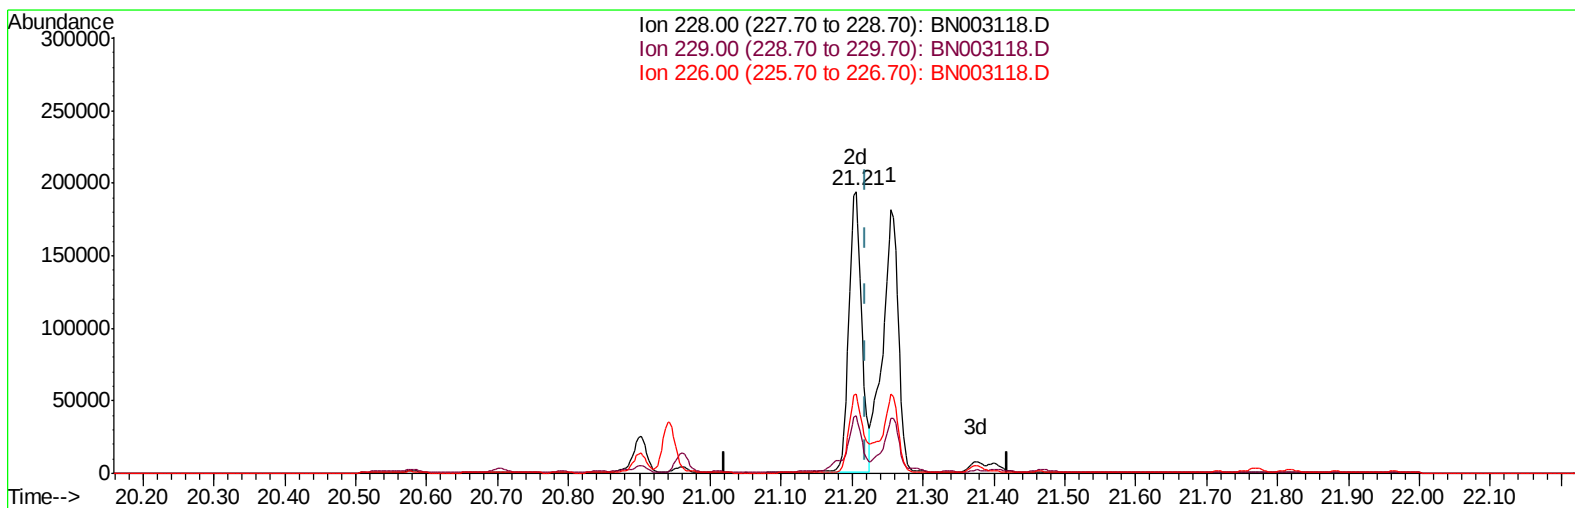

TIC: BN003118.D

(18) Benzo(a)anthracene

21.206min (-0.015) 11.16ng/ul m

response 242737

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	20.60
226.00	27.90	28.15
0.00	0.00	0.00