
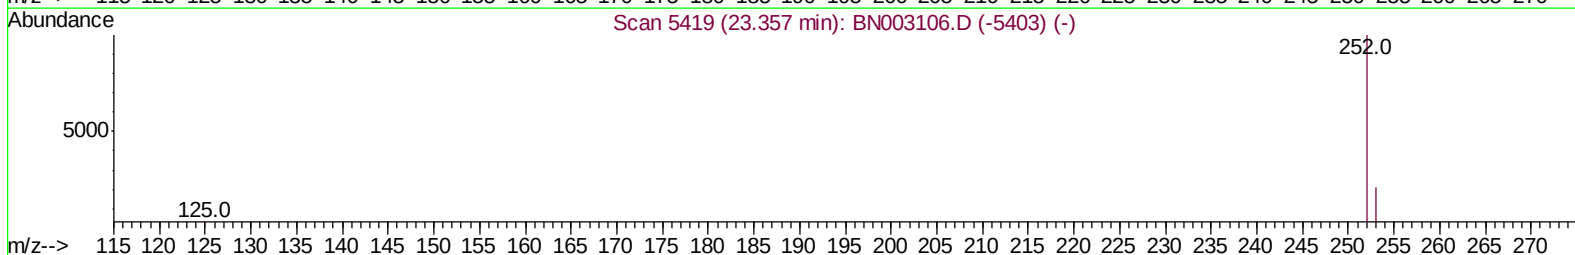
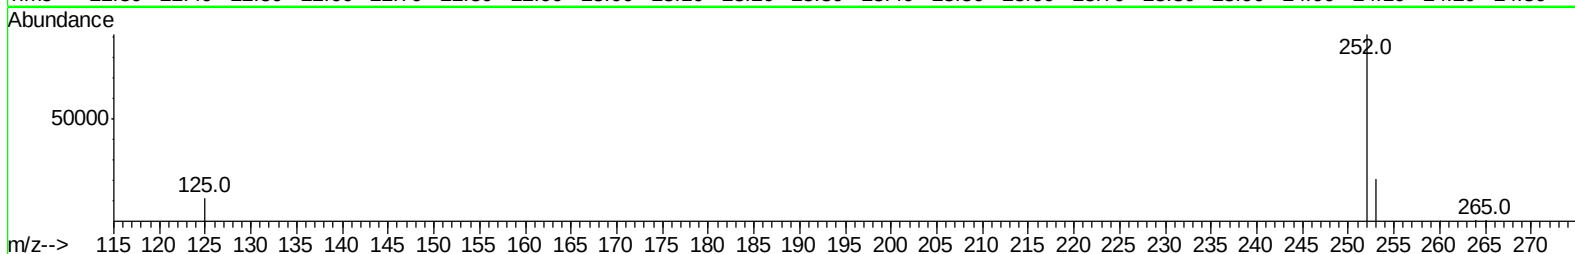


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003118.D
Acq On : 12 Oct 2018 00:08
Operator : MJ/SJ
Sample : J5230-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 12 07:15:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

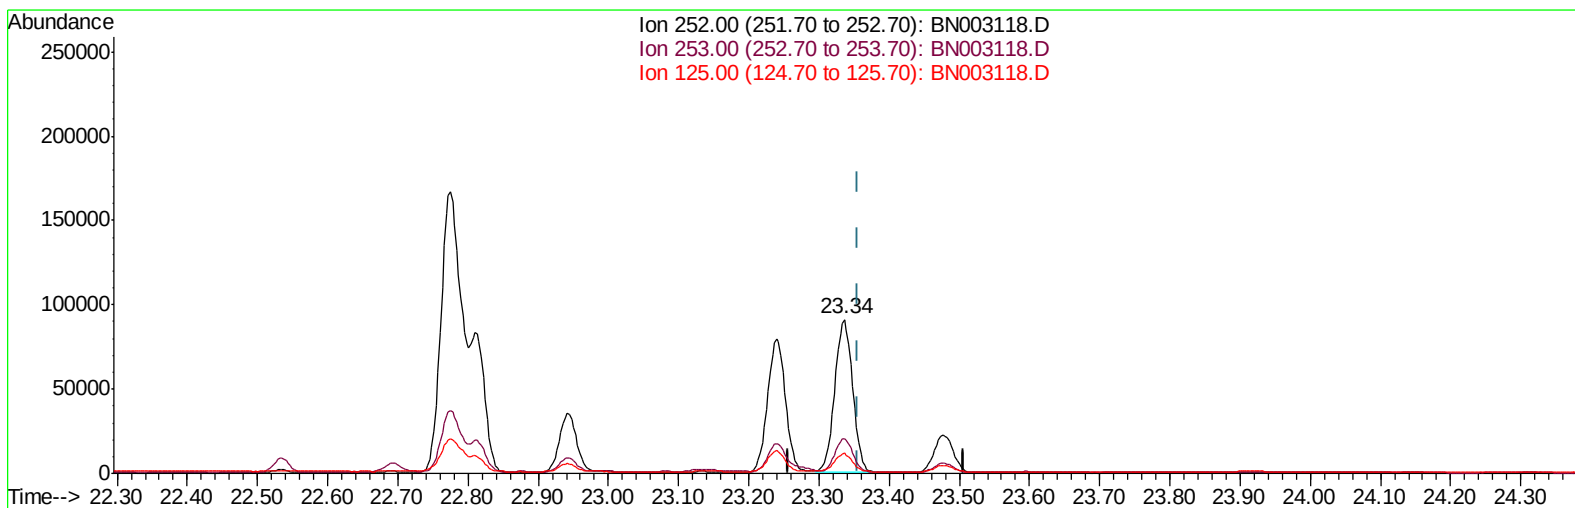

TIC: BN003118.D

(23) Benzo(a)pyrene (C)

23.336min (-0.021) 8.88ng/ul m

response 160229

Ion	Exp%	Act%
252.00	100	100
253.00	28.90	22.72#
125.00	21.10	12.95#
0.00	0.00	0.00