
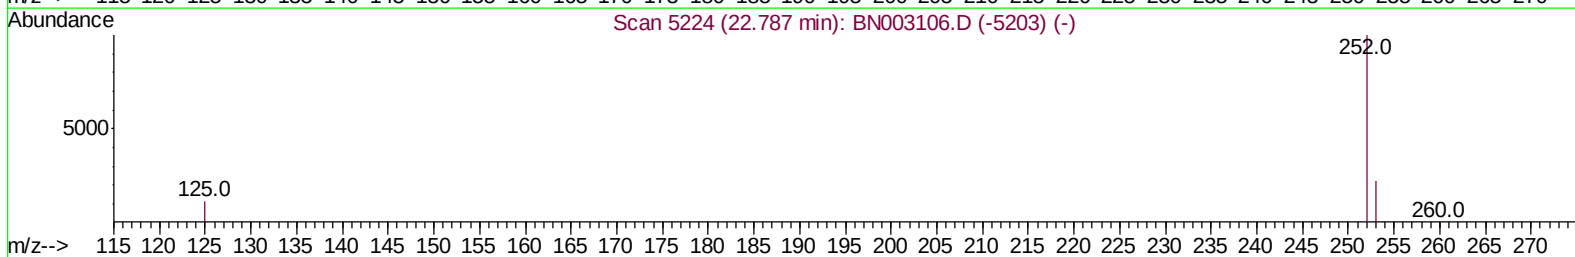
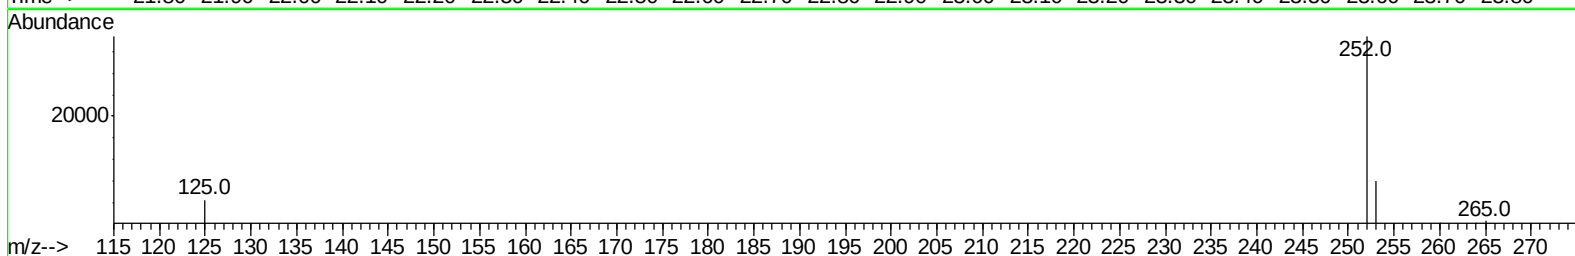


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003119.D
Acq On : 12 Oct 2018 00:43
Operator : MJ/SJ
Sample : J5230-11DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 12 05:38:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

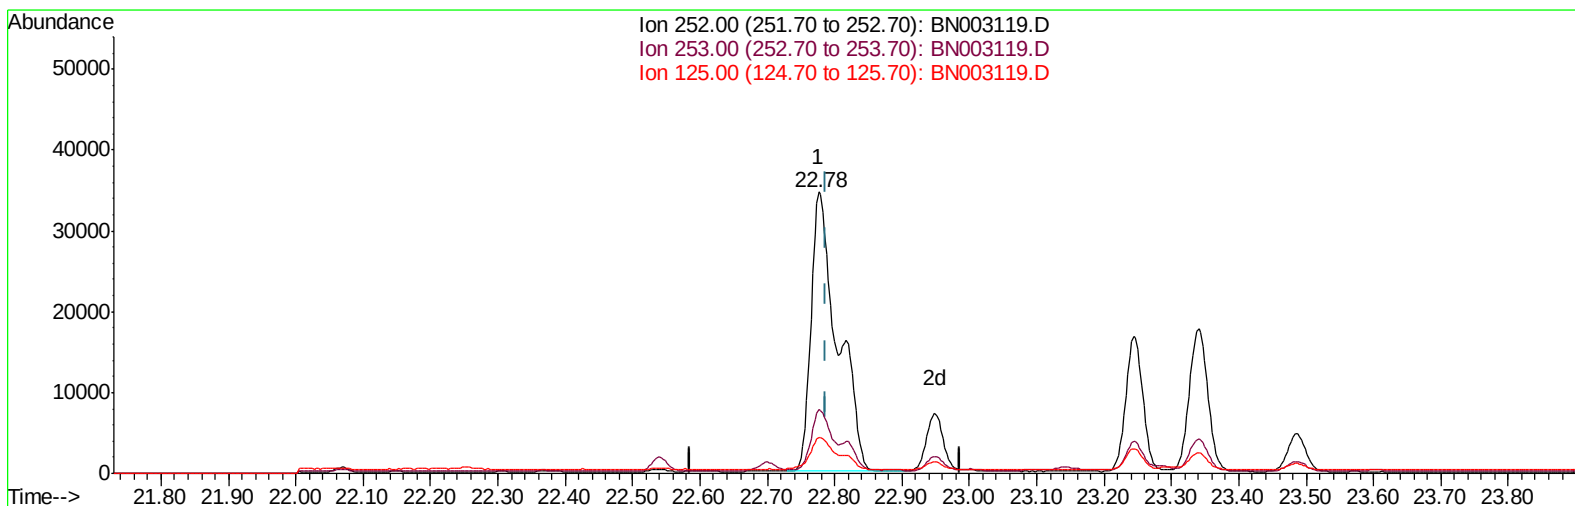

TIC: BN003119.D

(21) Benzo(b)fluoranthene
22.776min (-0.010) 4.95ng/ul
response 94762

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.91
125.00	17.10	12.63
0.00	0.00	0.00