
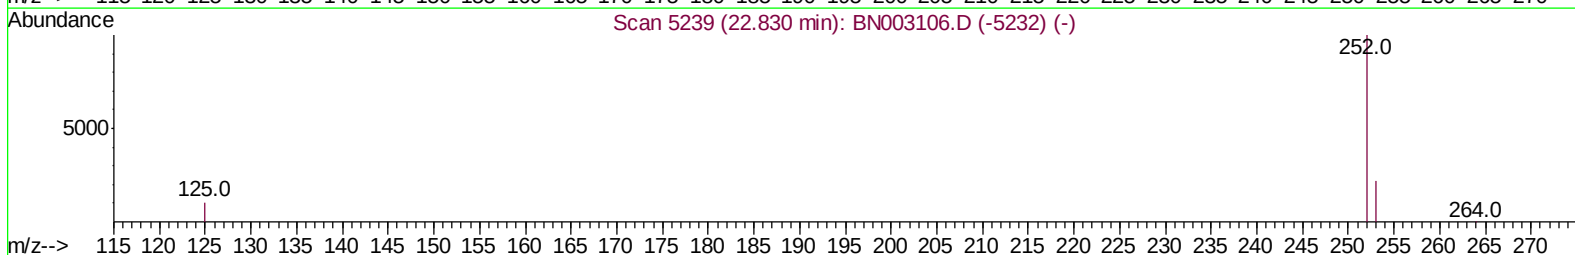
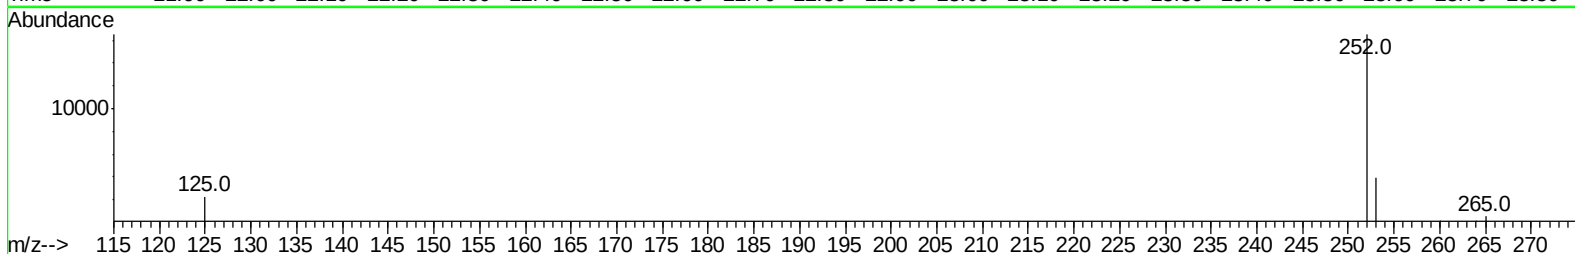


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003119.D
Acq On : 12 Oct 2018 00:43
Operator : MJ/SJ
Sample : J5230-11DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 12 05:38:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

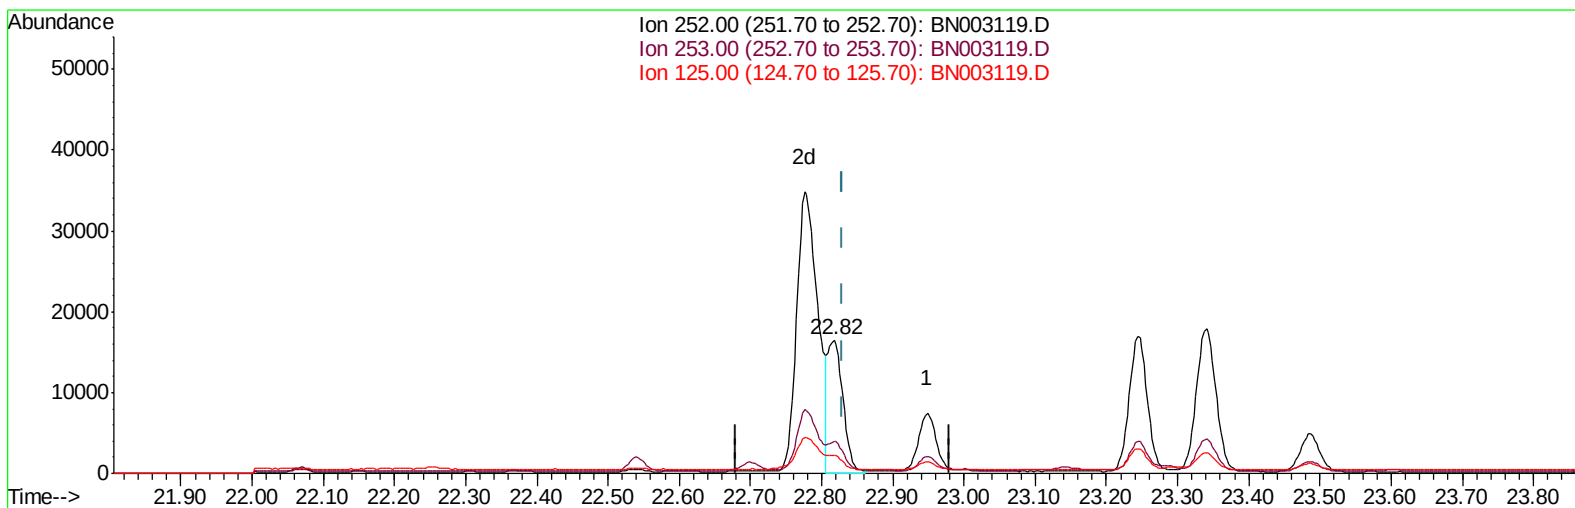

TIC: BN003119.D

(22) Benzo(k)fluoranthene

22.817min (-0.013) 1.23ng/ul m

response 24392

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.06
125.00	17.60	13.81#
0.00	0.00	0.00