
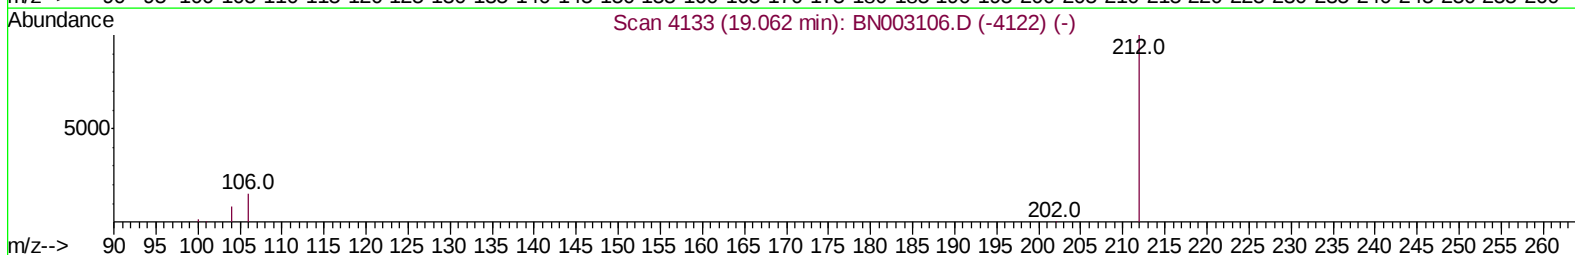
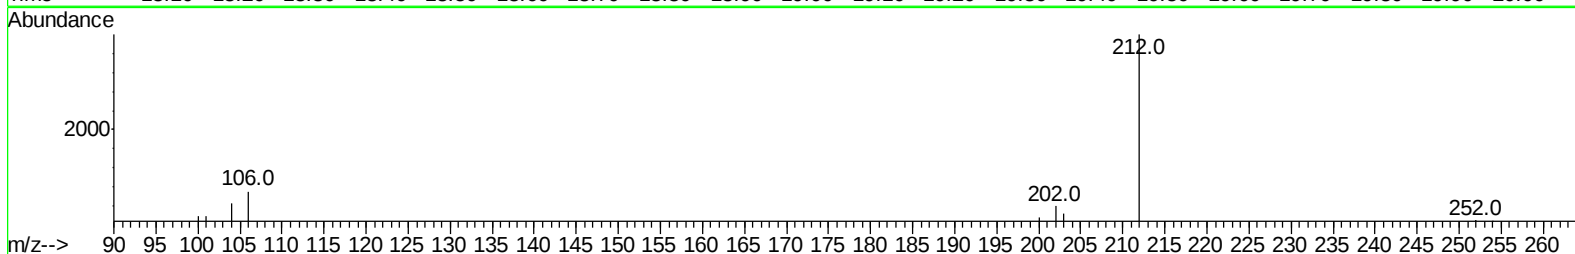


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003120.D
Acq On : 12 Oct 2018 01:18
Operator : MJ/SJ
Sample : J5230-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 12 07:21:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

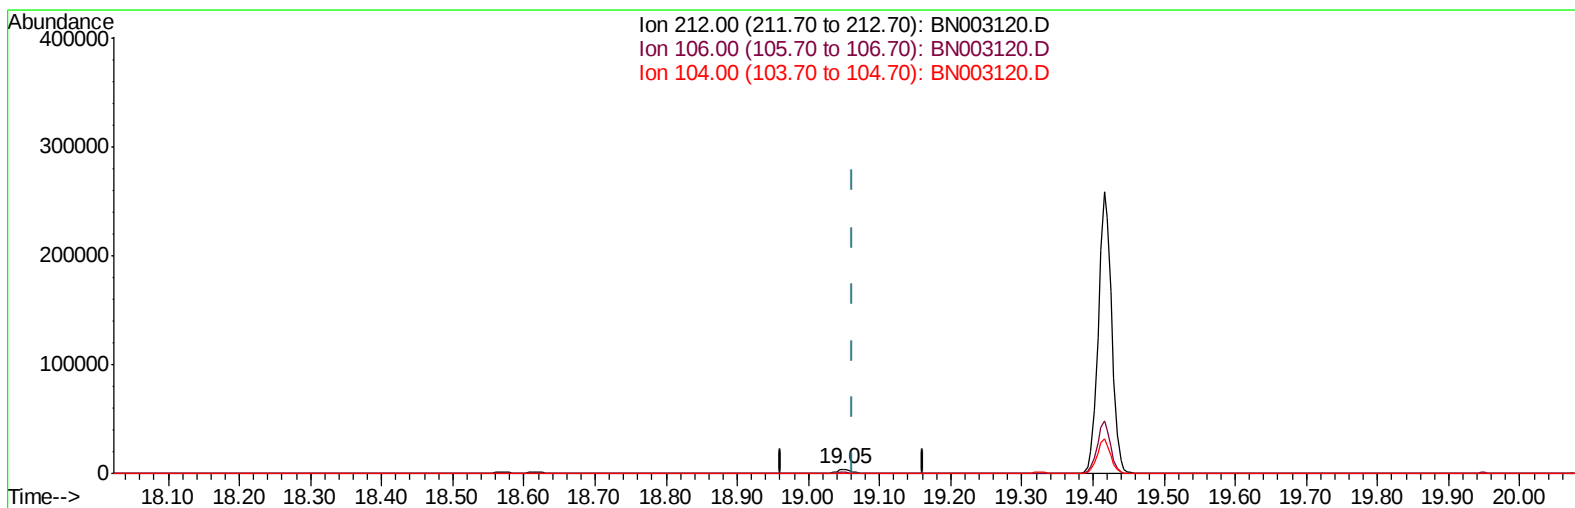

TIC: BN003120.D

(14) Fluoranthene-d10 (Surr)

19.049min (-0.014) 0.23ng/ul m

response 5518

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	1.09#
0.00	0.00	0.00