
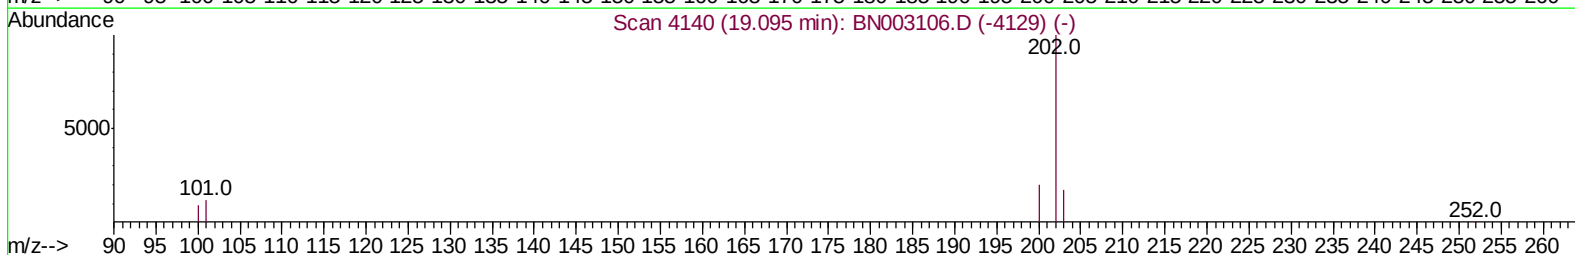
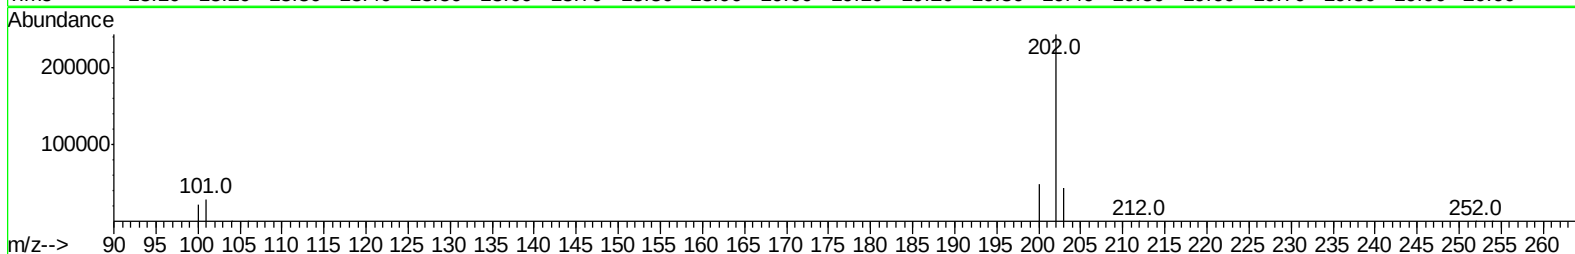


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003120.D
Acq On : 12 Oct 2018 01:18
Operator : MJ/SJ
Sample : J5230-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 12 07:21:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

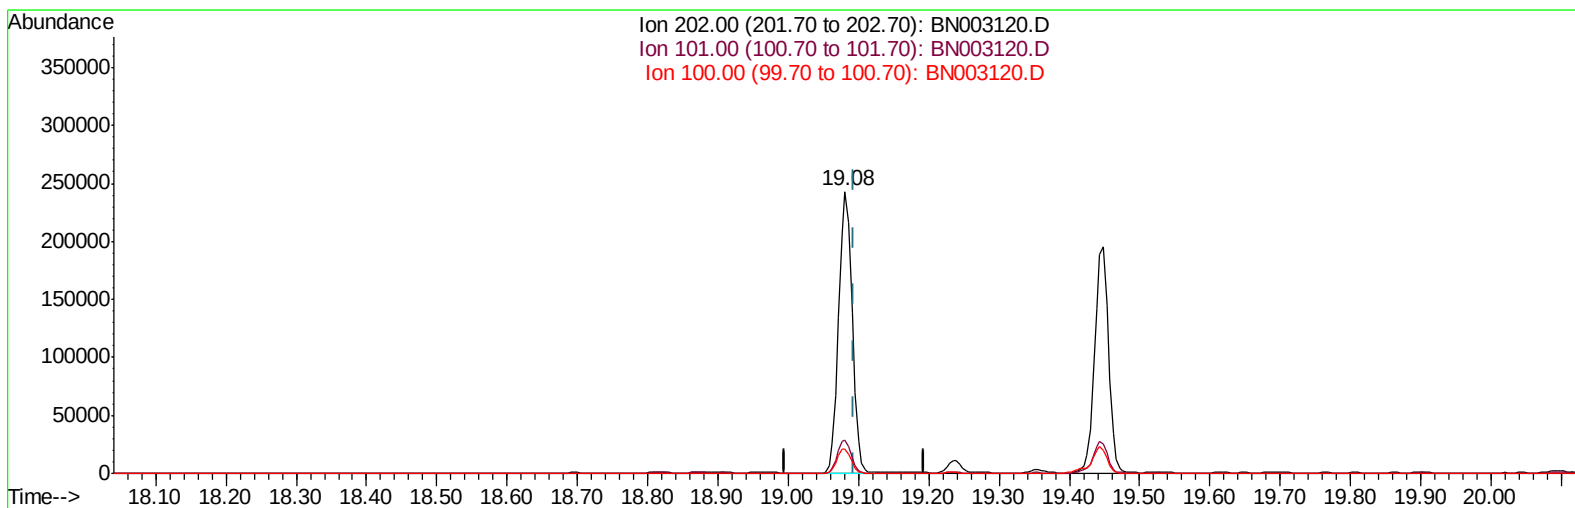

TIC: BN003120.D

(15) Fluoranthene (C)

19.081min (-0.014) 11.73ng/ul m

response 321553

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	11.96
100.00	9.10	8.86
0.00	0.00	0.00