
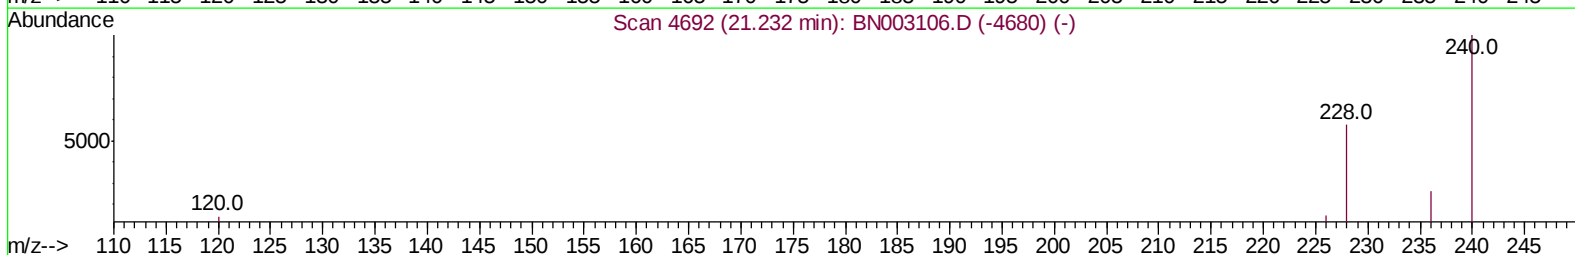
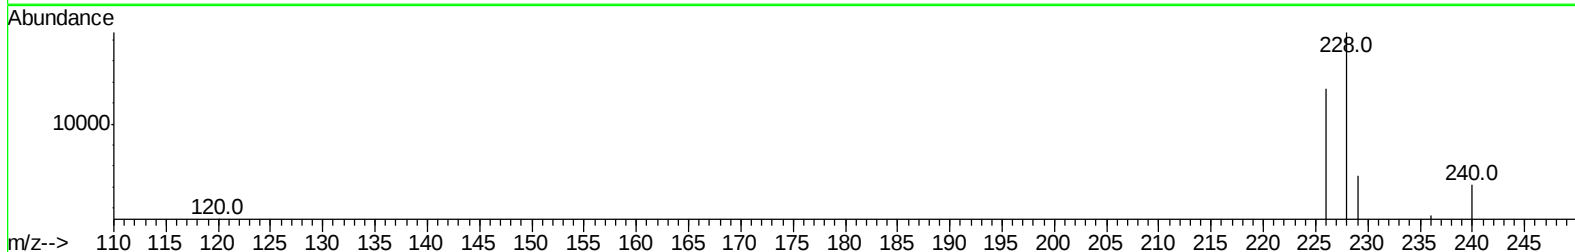


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003120.D
Acq On : 12 Oct 2018 01:18
Operator : MJ/SJ
Sample : J5230-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 12 07:21:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

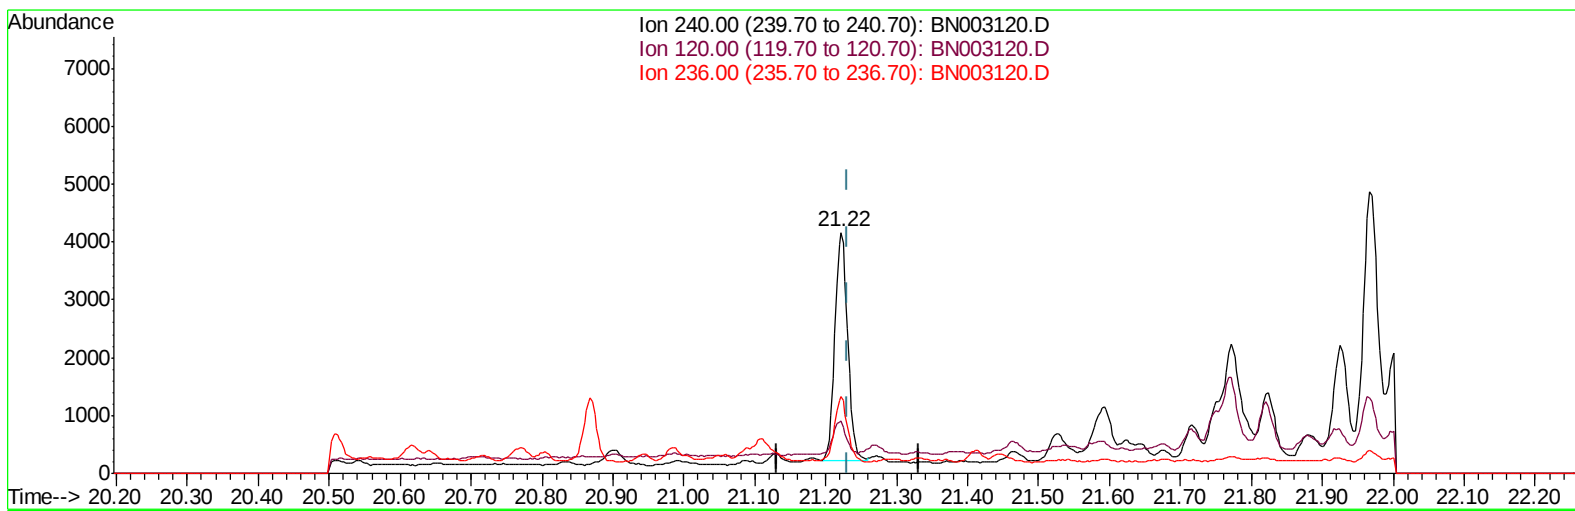

TIC: BN003120.D

(16) Chrysene-d12 (I)

21.222min (-0.010) 0.40ng/ul m

response 4954

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	21.87#
236.00	28.10	31.84
0.00	0.00	0.00