
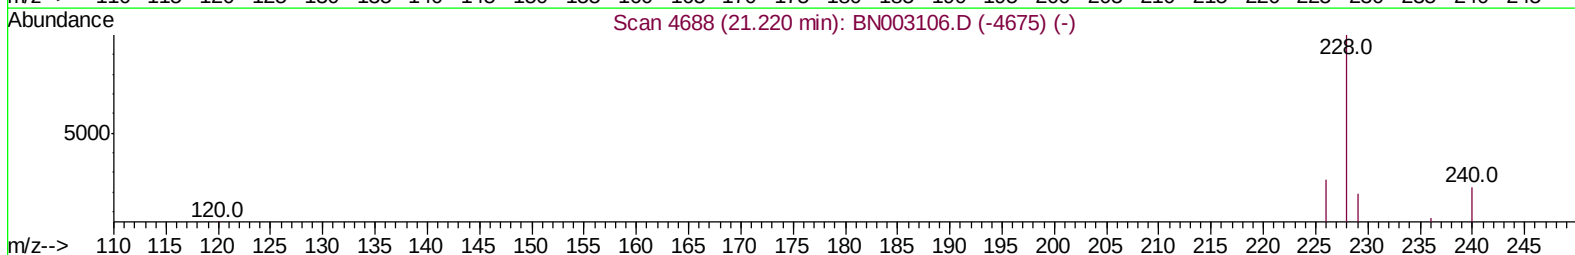
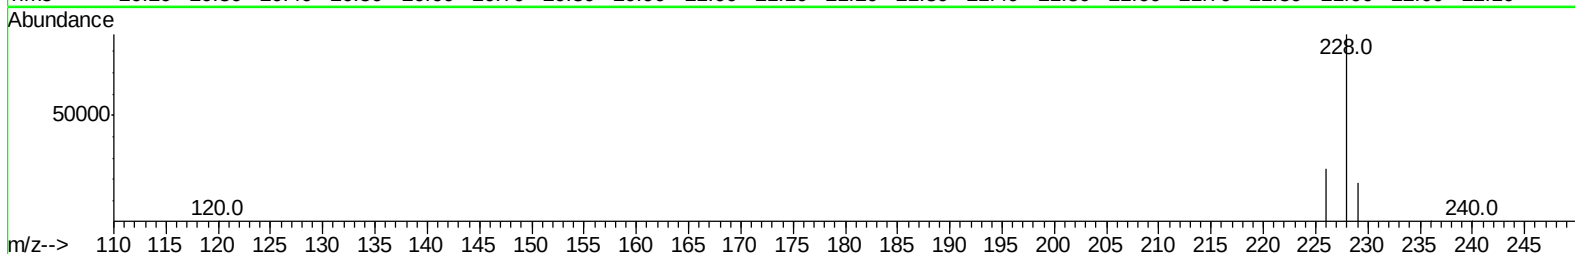


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003120.D
Acq On : 12 Oct 2018 01:18
Operator : MJ/SJ
Sample : J5230-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 12 07:23:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

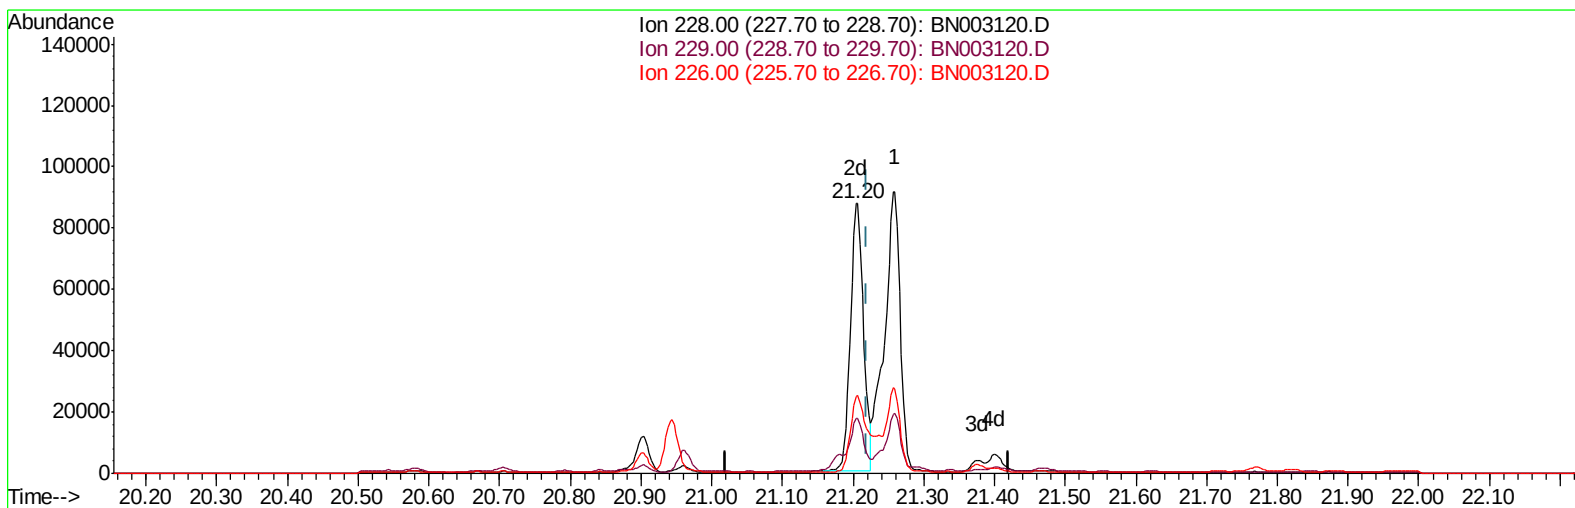

TIC: BN003120.D

(18) Benzo(a)anthracene

21.204min (-0.016) 7.04ng/ul m

response 112239

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	20.57
226.00	27.90	28.46
0.00	0.00	0.00