
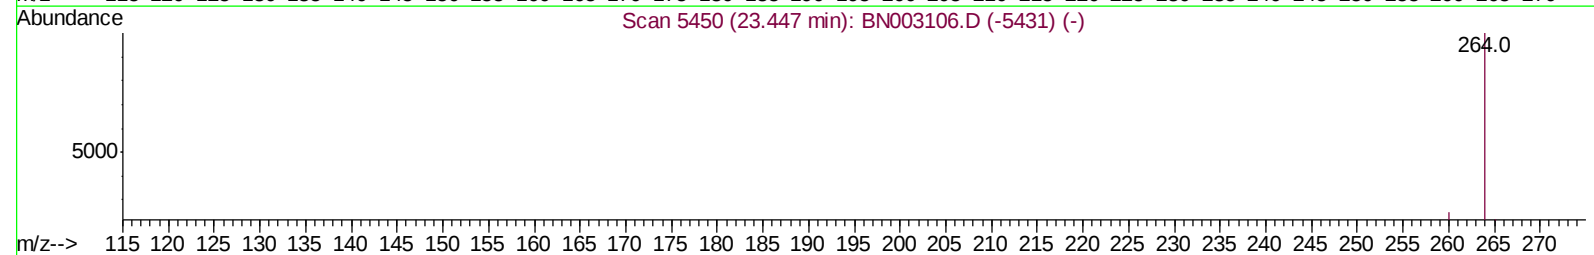
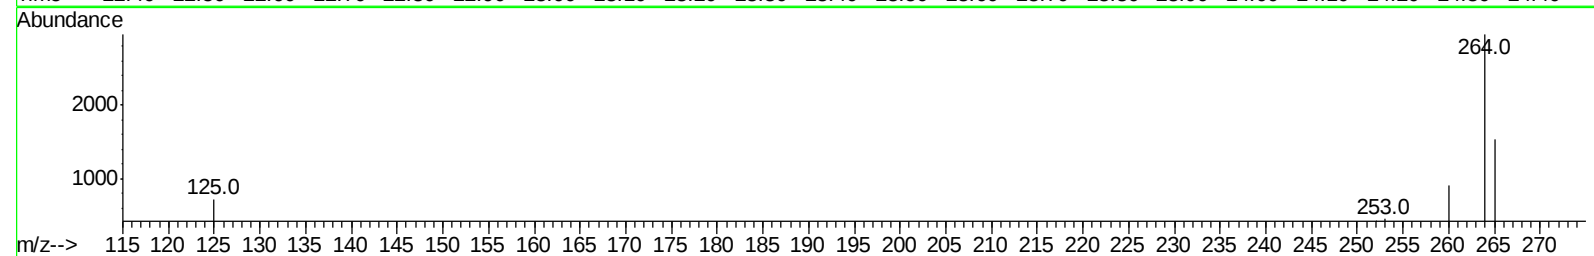


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003120.D
Acq On : 12 Oct 2018 01:18
Operator : MJ/SJ
Sample : J5230-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 12 07:23:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

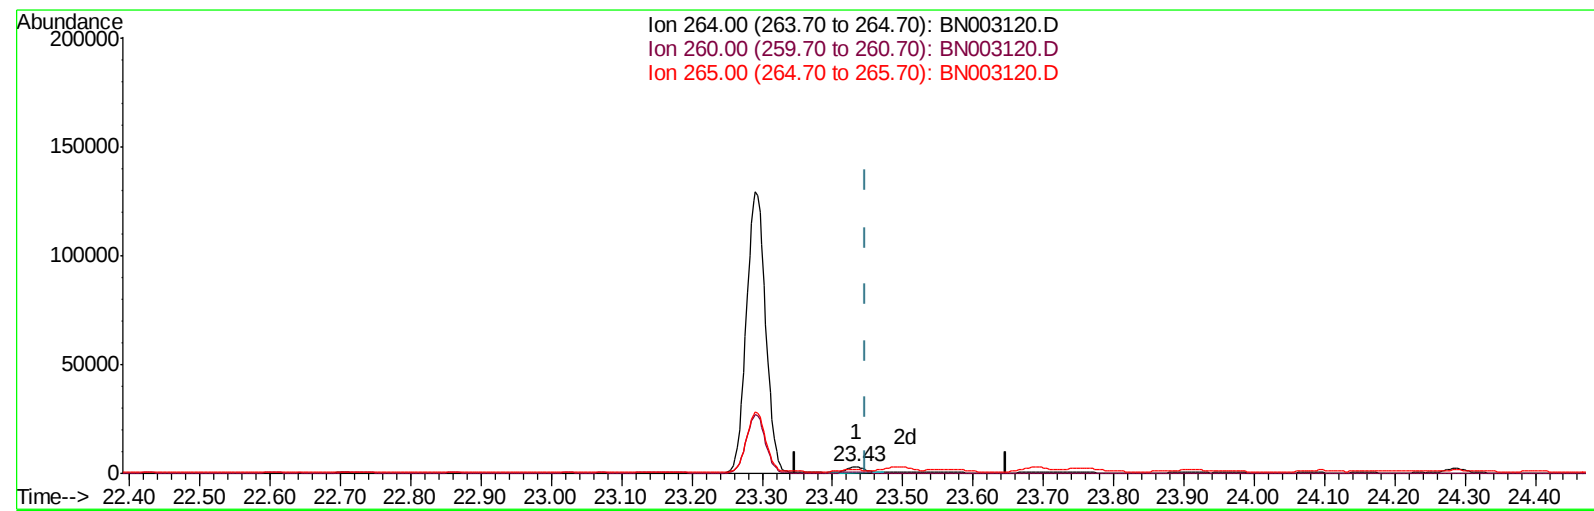

TIC: BN003120.D

(20) Perylene-d12 (I)

23.434min (-0.013) 0.40ng/ul m

response 4920

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	30.35
265.00	45.40	51.50
0.00	0.00	0.00