
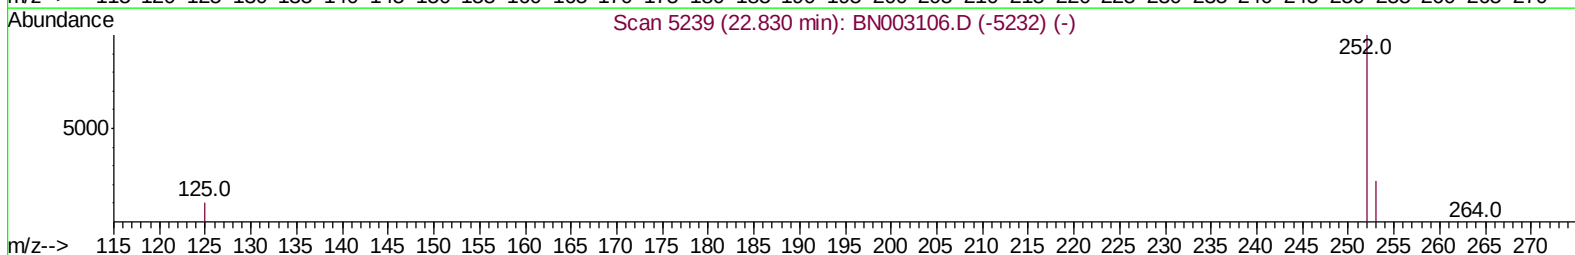
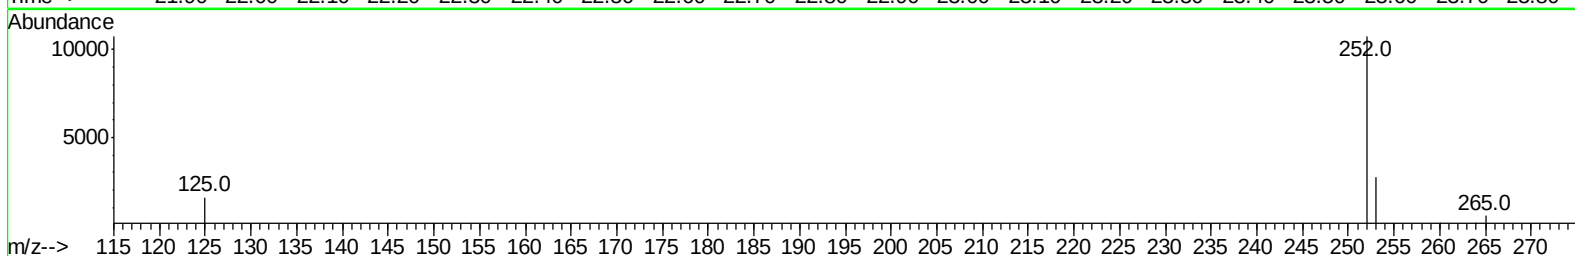


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 12 05:38:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

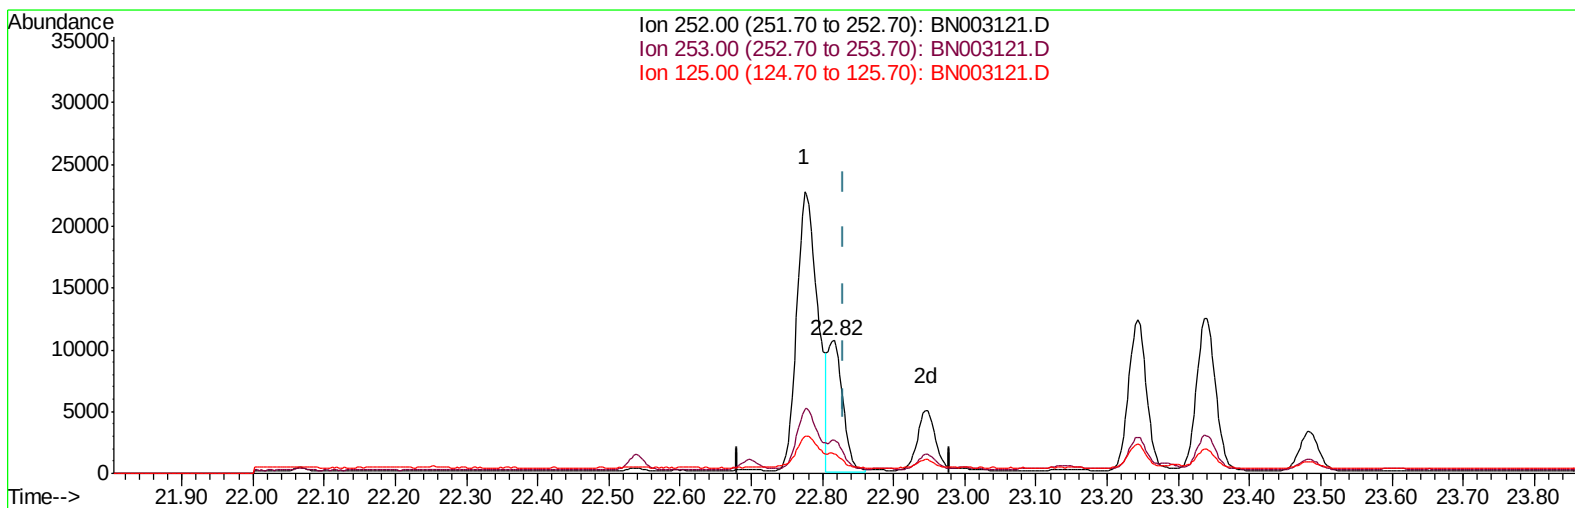

TIC: BN003121.D

(22) Benzo(k)fluoranthene

22.816min (-0.014) 0.75ng/ul m

response 15877

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.21
125.00	17.60	14.91
0.00	0.00	0.00