
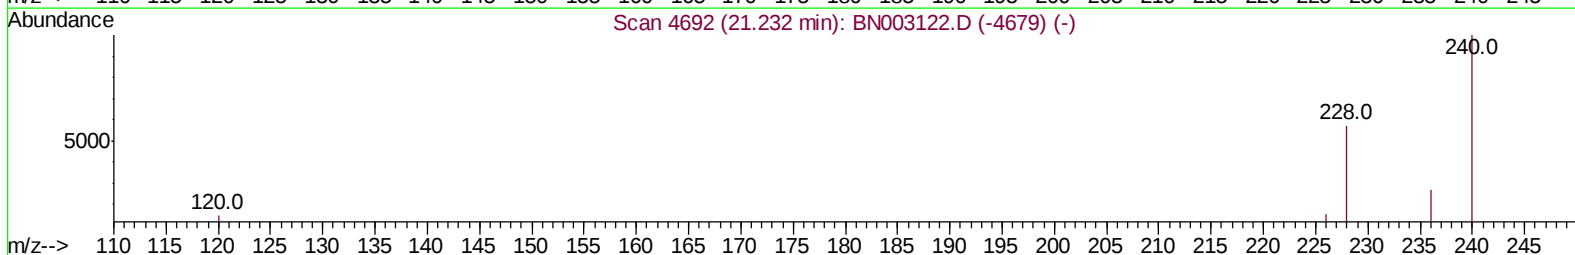
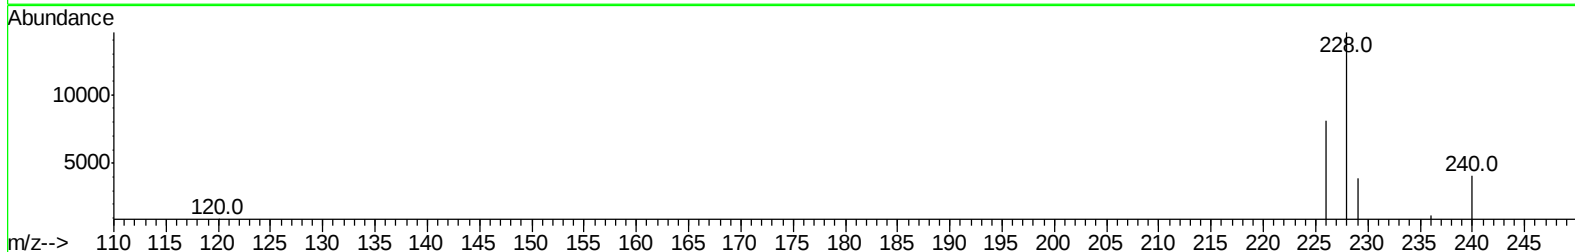


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003123.D
Acq On : 12 Oct 2018 03:04
Operator : MJ/SJ
Sample : J5230-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Oct 12 07:33:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

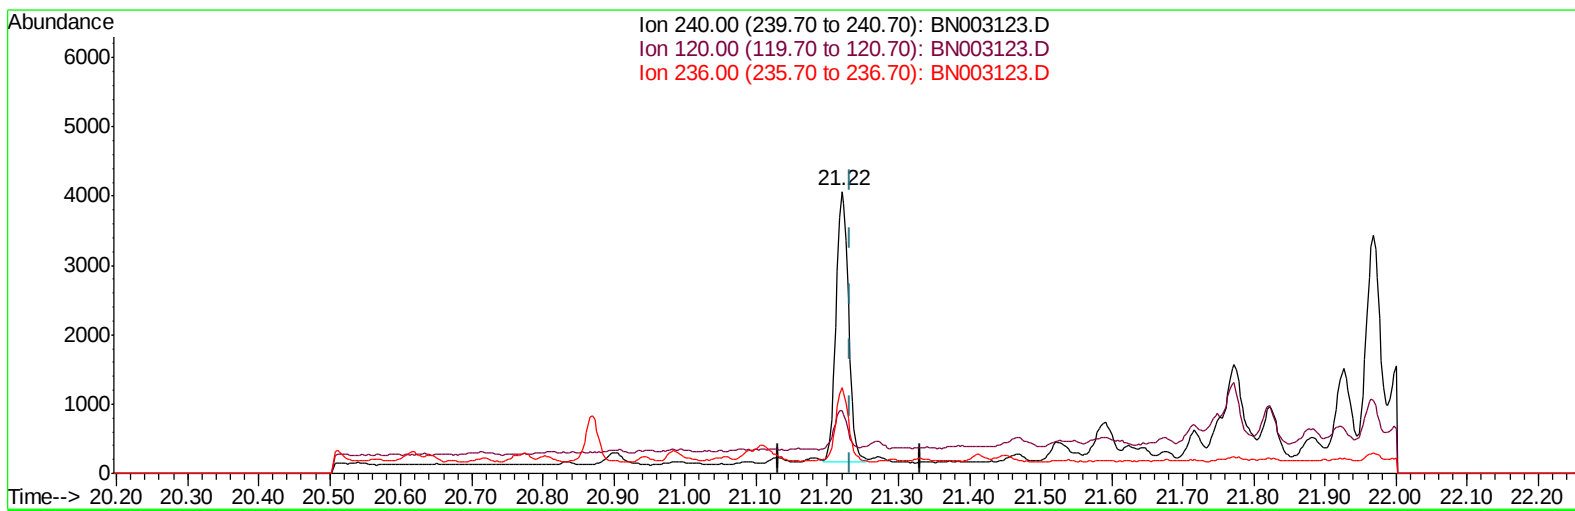

TIC: BN003123.D

(16) Chrysene-d12 (I)

21.220min (-0.012) 0.40ng/ul m

response 4741

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	22.44#
236.00	28.10	30.49
0.00	0.00	0.00