
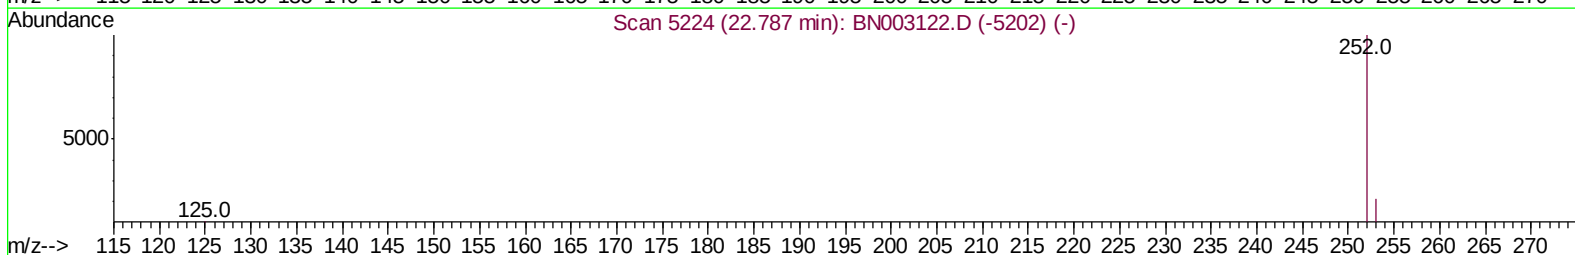
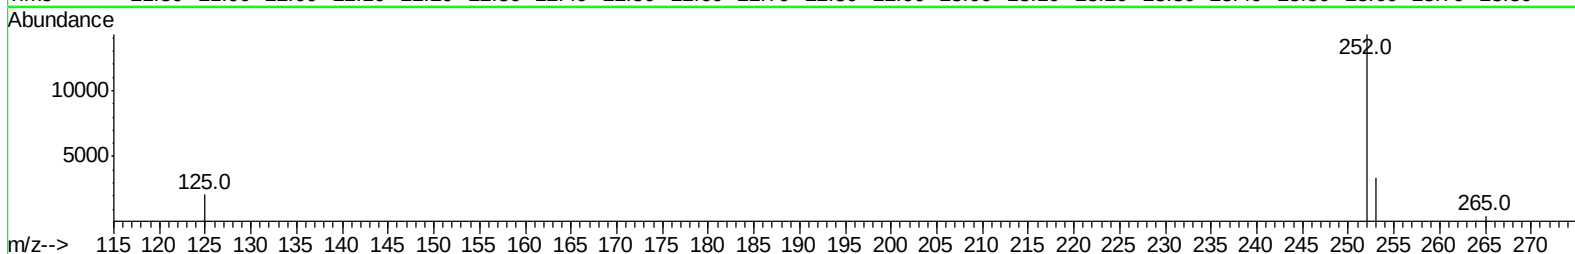


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\  
Data File : BN003124.D  
Acq On : 12 Oct 2018 03:39  
Operator : MJ/SJ  
Sample : J5230-14DL 5X  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Oct 12 07:31:57 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 12 07:27:48 2018  
Response via : Initial Calibration

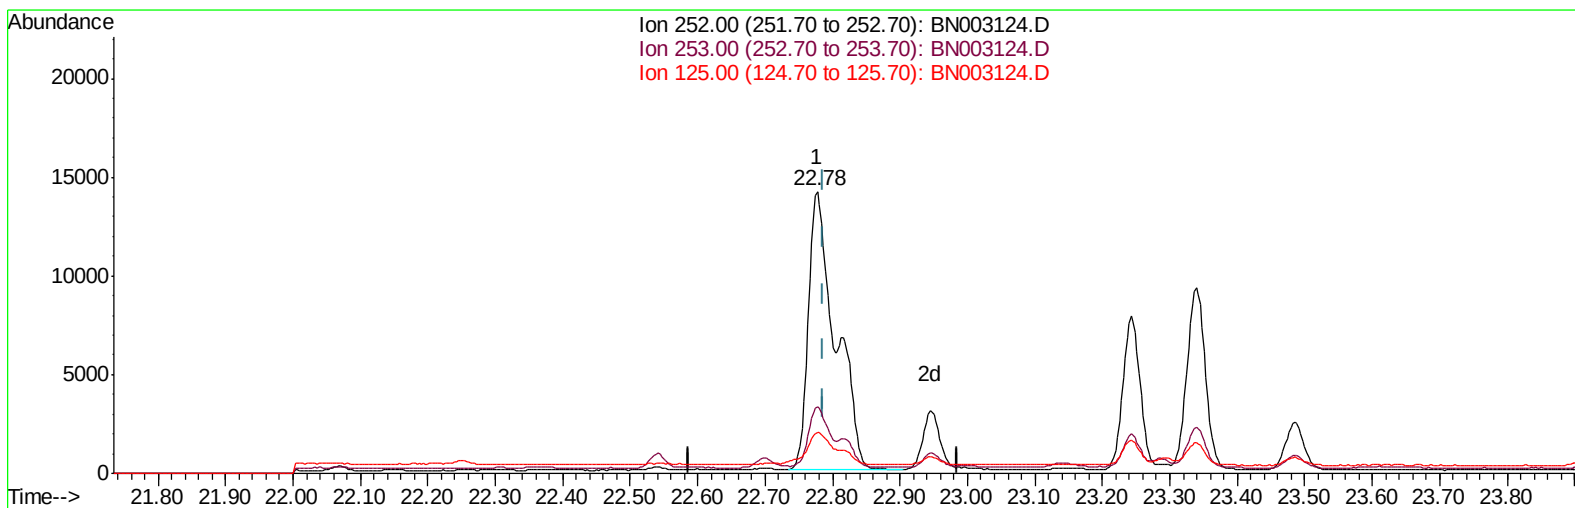

TIC: BN003124.D

(21) Benzo(b)fluoranthene  
22.778min (-0.009) 2.08ng/ul  
response 39271

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 26.60 | 23.75 |
| 125.00 | 17.10 | 14.66 |
| 0.00   | 0.00  | 0.00  |