
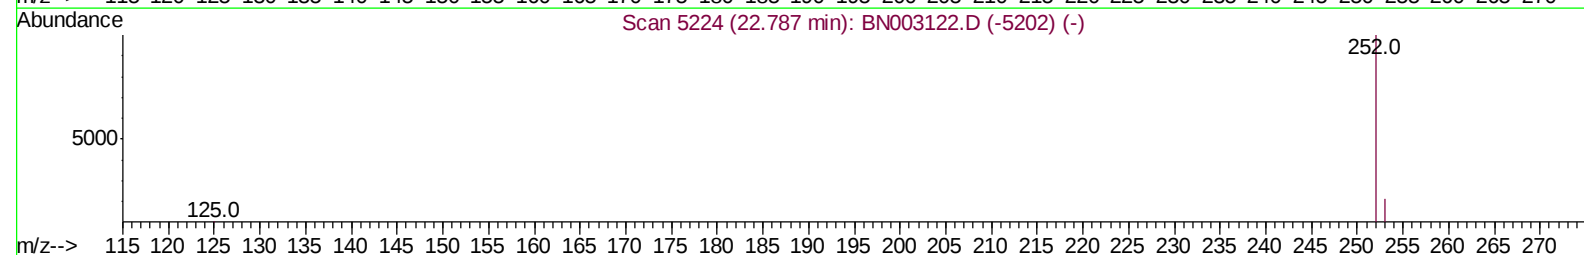
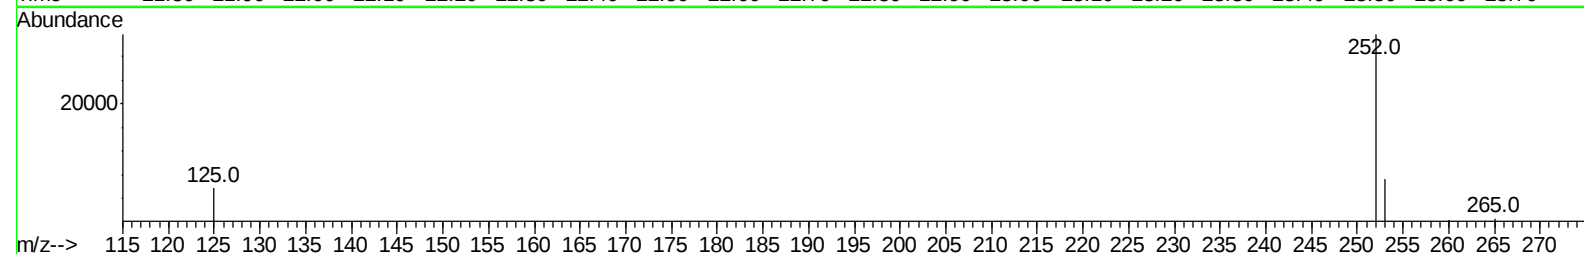


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003125.D
Acq On : 12 Oct 2018 04:14
Operator : MJ/SJ
Sample : J5295-02DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Oct 12 07:32:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

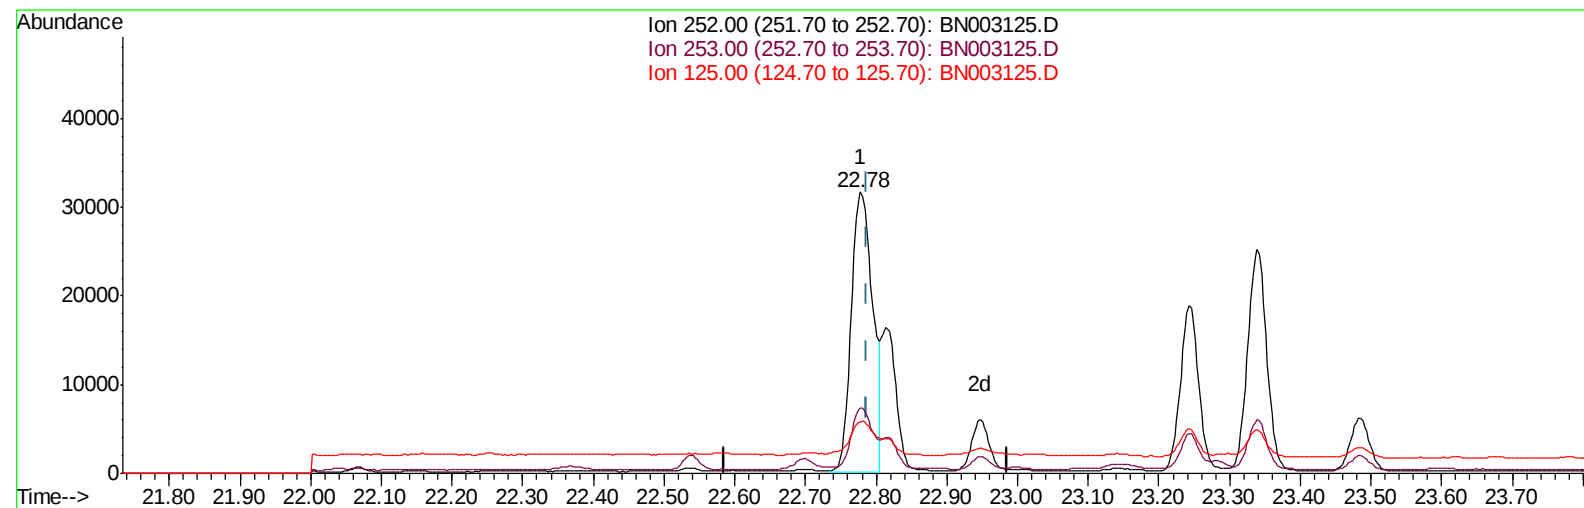

TIC: BN003125.D

(21) Benzo(b)fluoranthene

22.778min (-0.009) 3.41ng/ul m

response 66220

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.20
125.00	17.10	18.30
0.00	0.00	0.00