
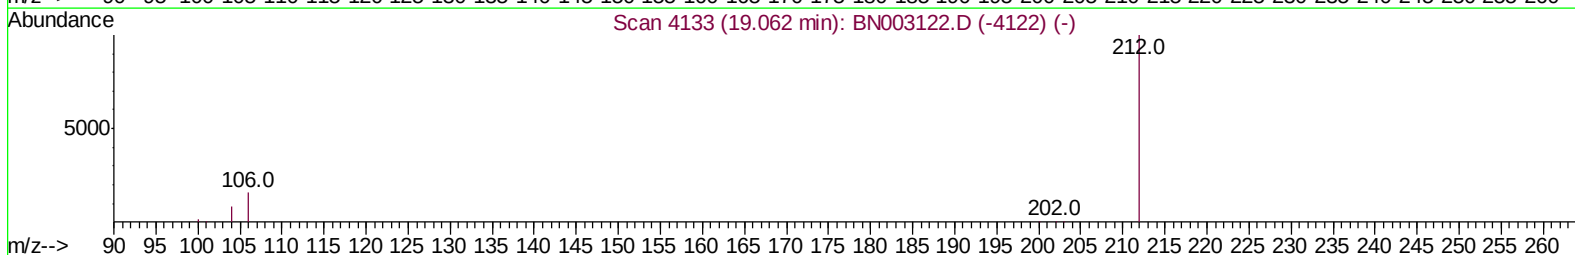
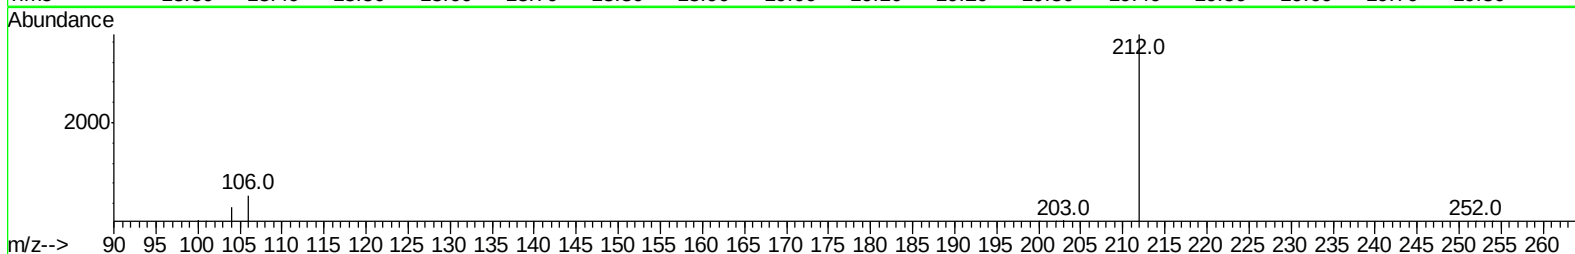


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003127.D
Acq On : 12 Oct 2018 05:25
Operator : MJ/SJ
Sample : PB113595BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 12 07:45:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

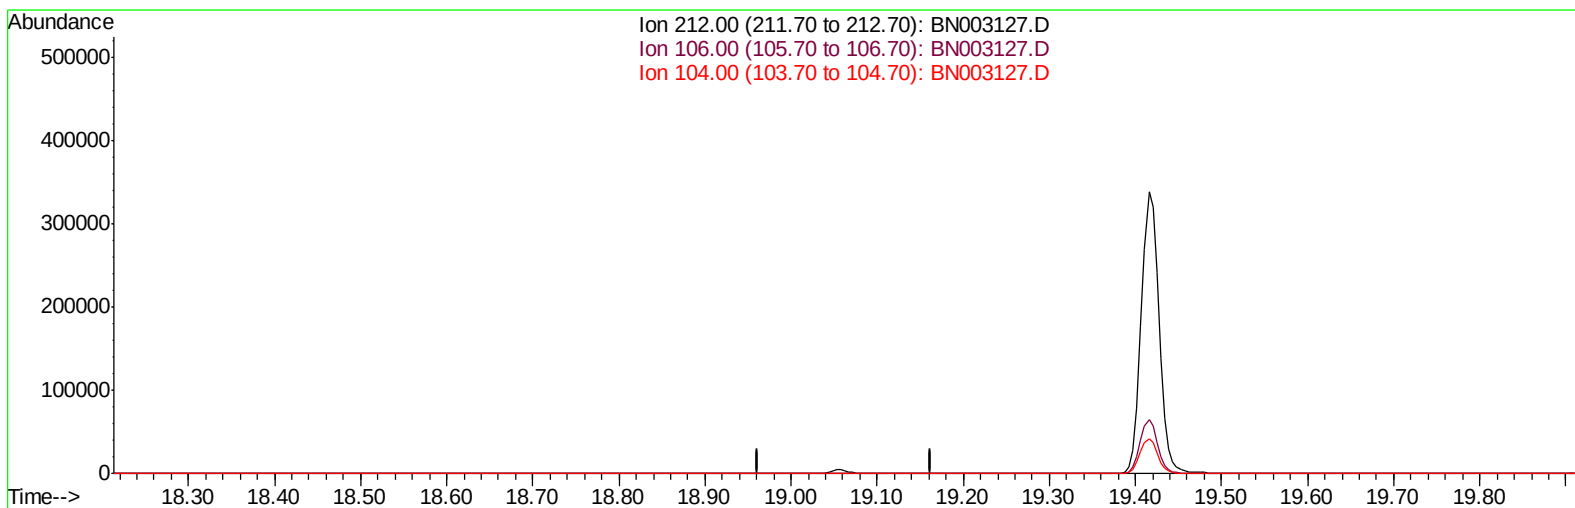

TIC: BN003127.D

(14) Fluoranthene-d10 (SURR)

19.062min (-19.062) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00