
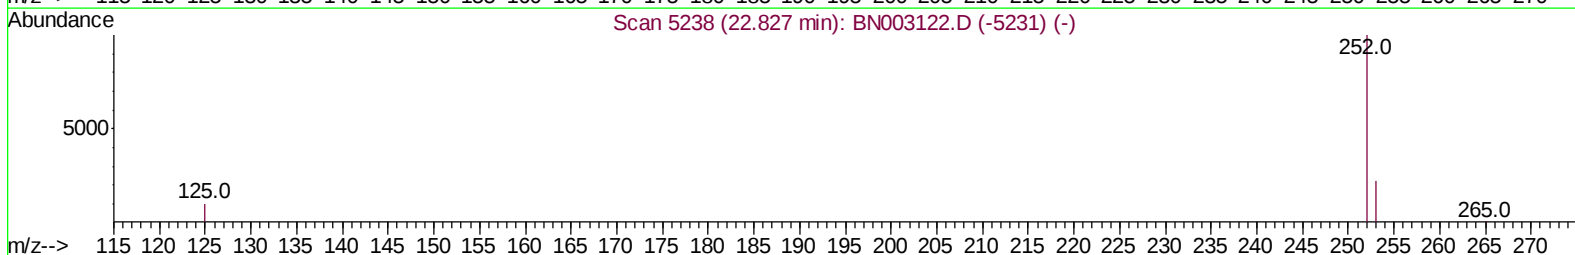
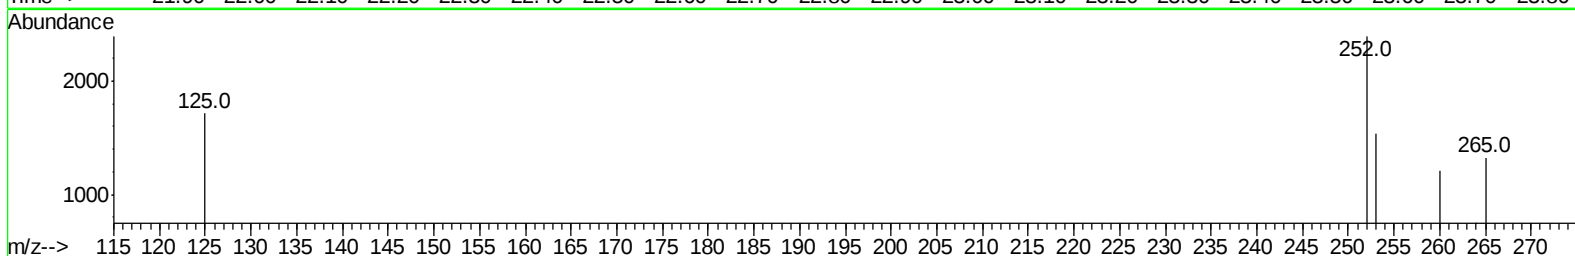


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003128.D
Acq On : 12 Oct 2018 06:00
Operator : MJ/SJ
Sample : J5234-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 12 07:55:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

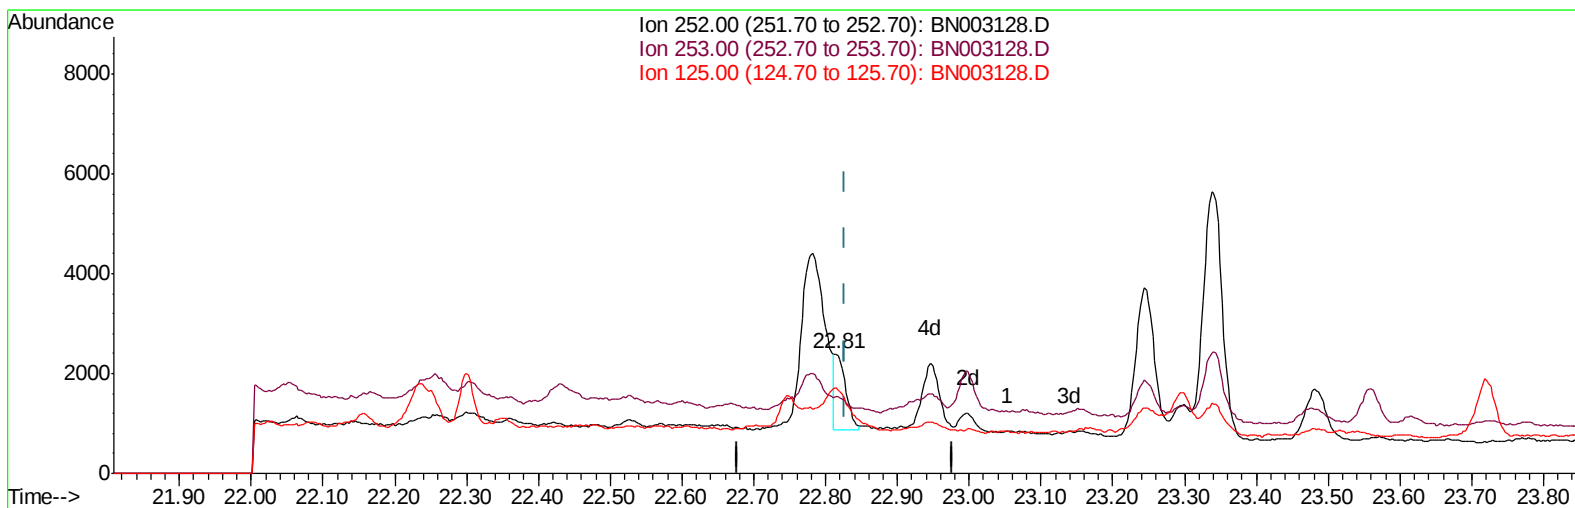

TIC: BN003128.D

(22) Benzo(k)fluoranthene

22.814min (-0.013) 0.09ng/ul m

response 1585

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	64.02#
125.00	17.60	71.67#
0.00	0.00	0.00