
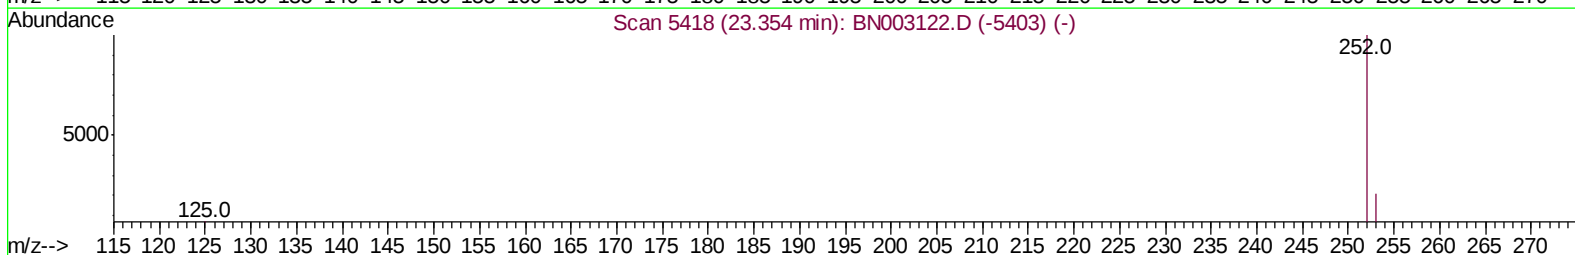
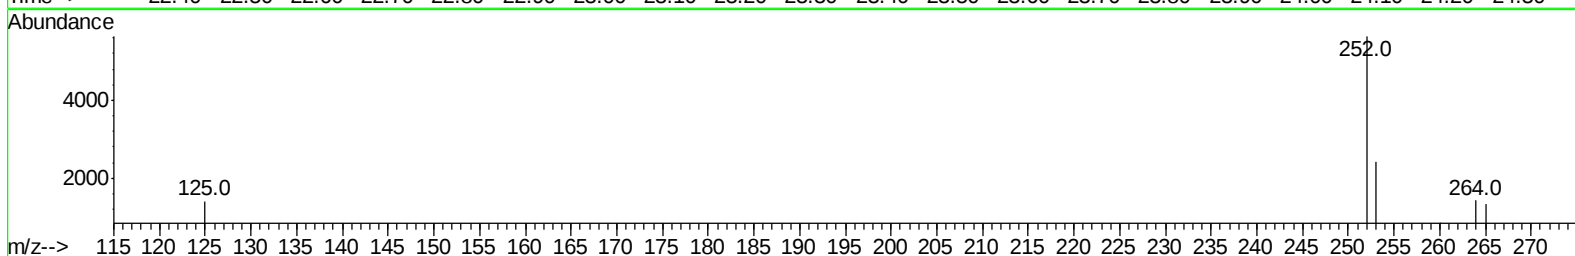


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003128.D
Acq On : 12 Oct 2018 06:00
Operator : MJ/SJ
Sample : J5234-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 12 07:55:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

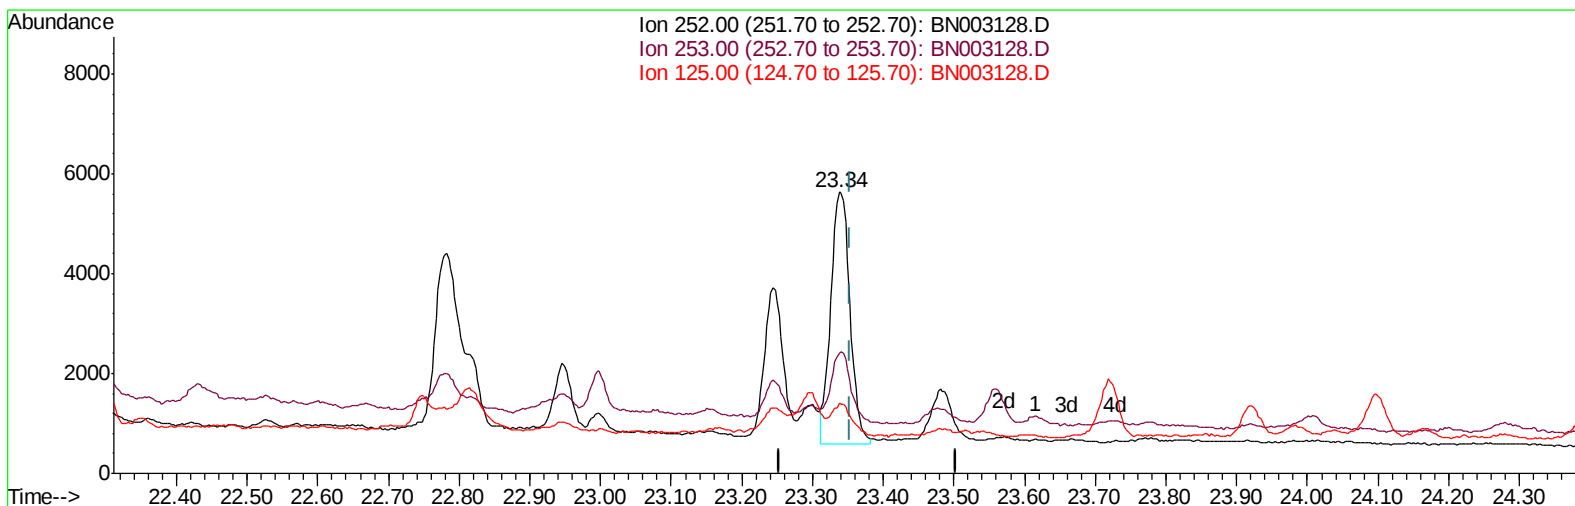

TIC: BN003128.D

(23) Benzo(a)pyrene (C)

23.338min (-0.016) 0.60ng/ul m

response 9458

Ion	Exp%	Act%
252.00	100	100
253.00	28.90	42.82#
125.00	21.10	24.80
0.00	0.00	0.00