
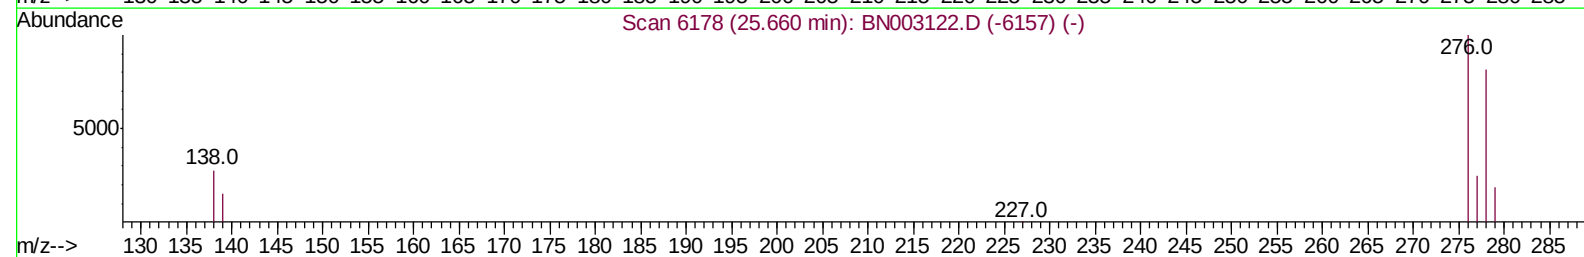
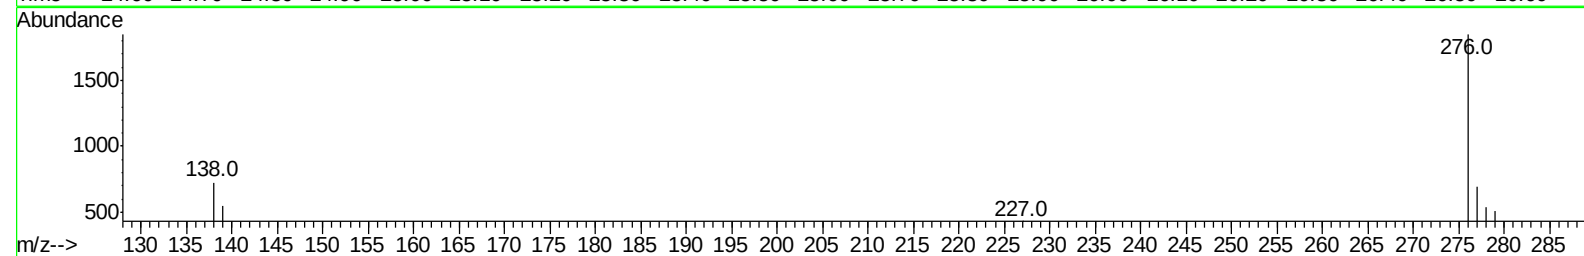


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003128.D
Acq On : 12 Oct 2018 06:00
Operator : MJ/SJ
Sample : J5234-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 12 07:55:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

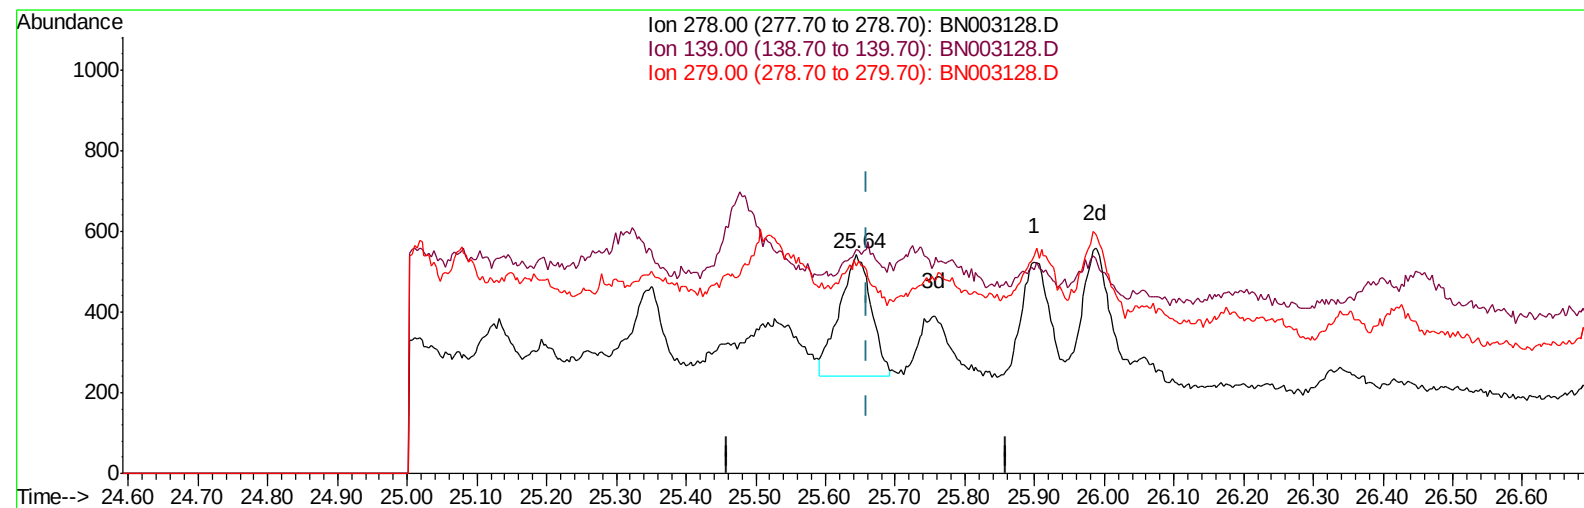

TIC: BN003128.D

(25) Dibenzo(a,h)anthracene

25.645min (-0.015) 0.07ng/ul m

response 951

Ion	Exp%	Act%
278.00	100	100
139.00	25.30	102.03#
279.00	29.80	94.66#
0.00	0.00	0.00