
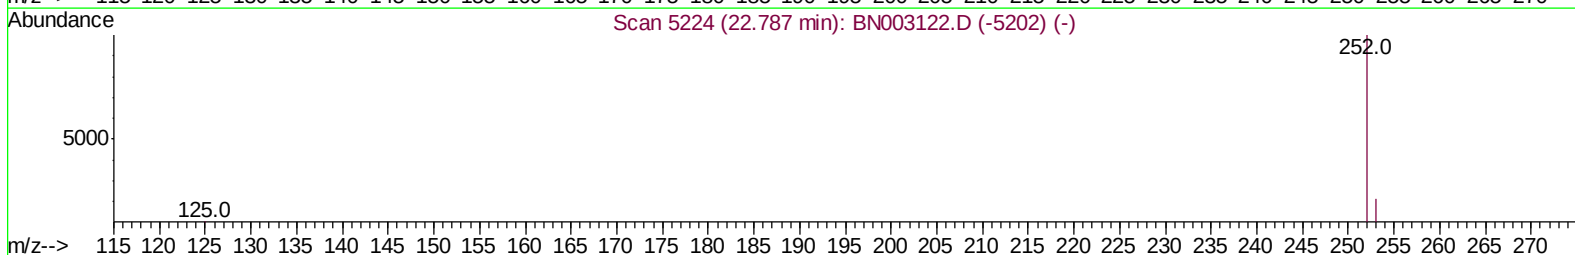
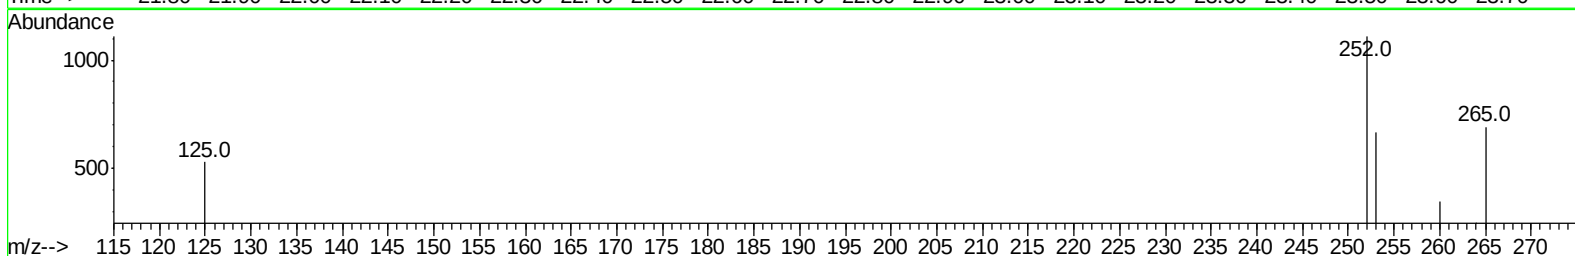


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003129.D
Acq On : 12 Oct 2018 06:35
Operator : MJ/SJ
Sample : J5234-16DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 12 07:32:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 07:27:48 2018
Response via : Initial Calibration

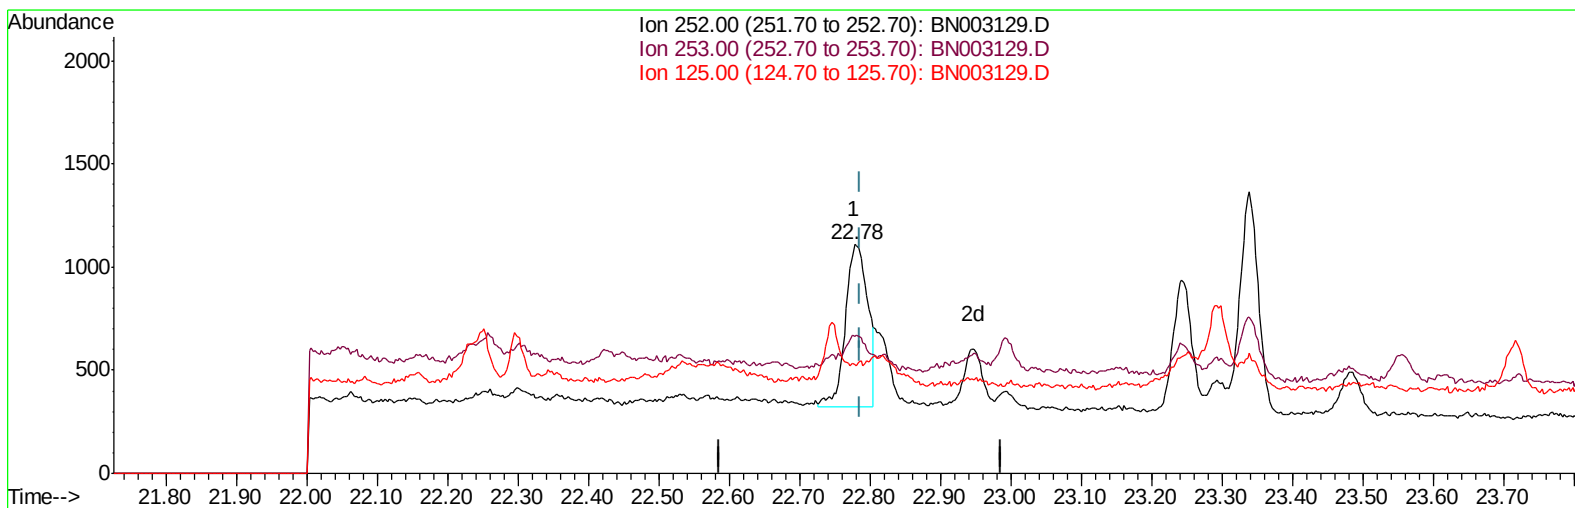

TIC: BN003129.D

(21) Benzo(b)fluoranthene

22.778min (-0.009) 0.09ng/ul m

response 1738

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	60.00#
125.00	17.10	47.39#
0.00	0.00	0.00