


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:52:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

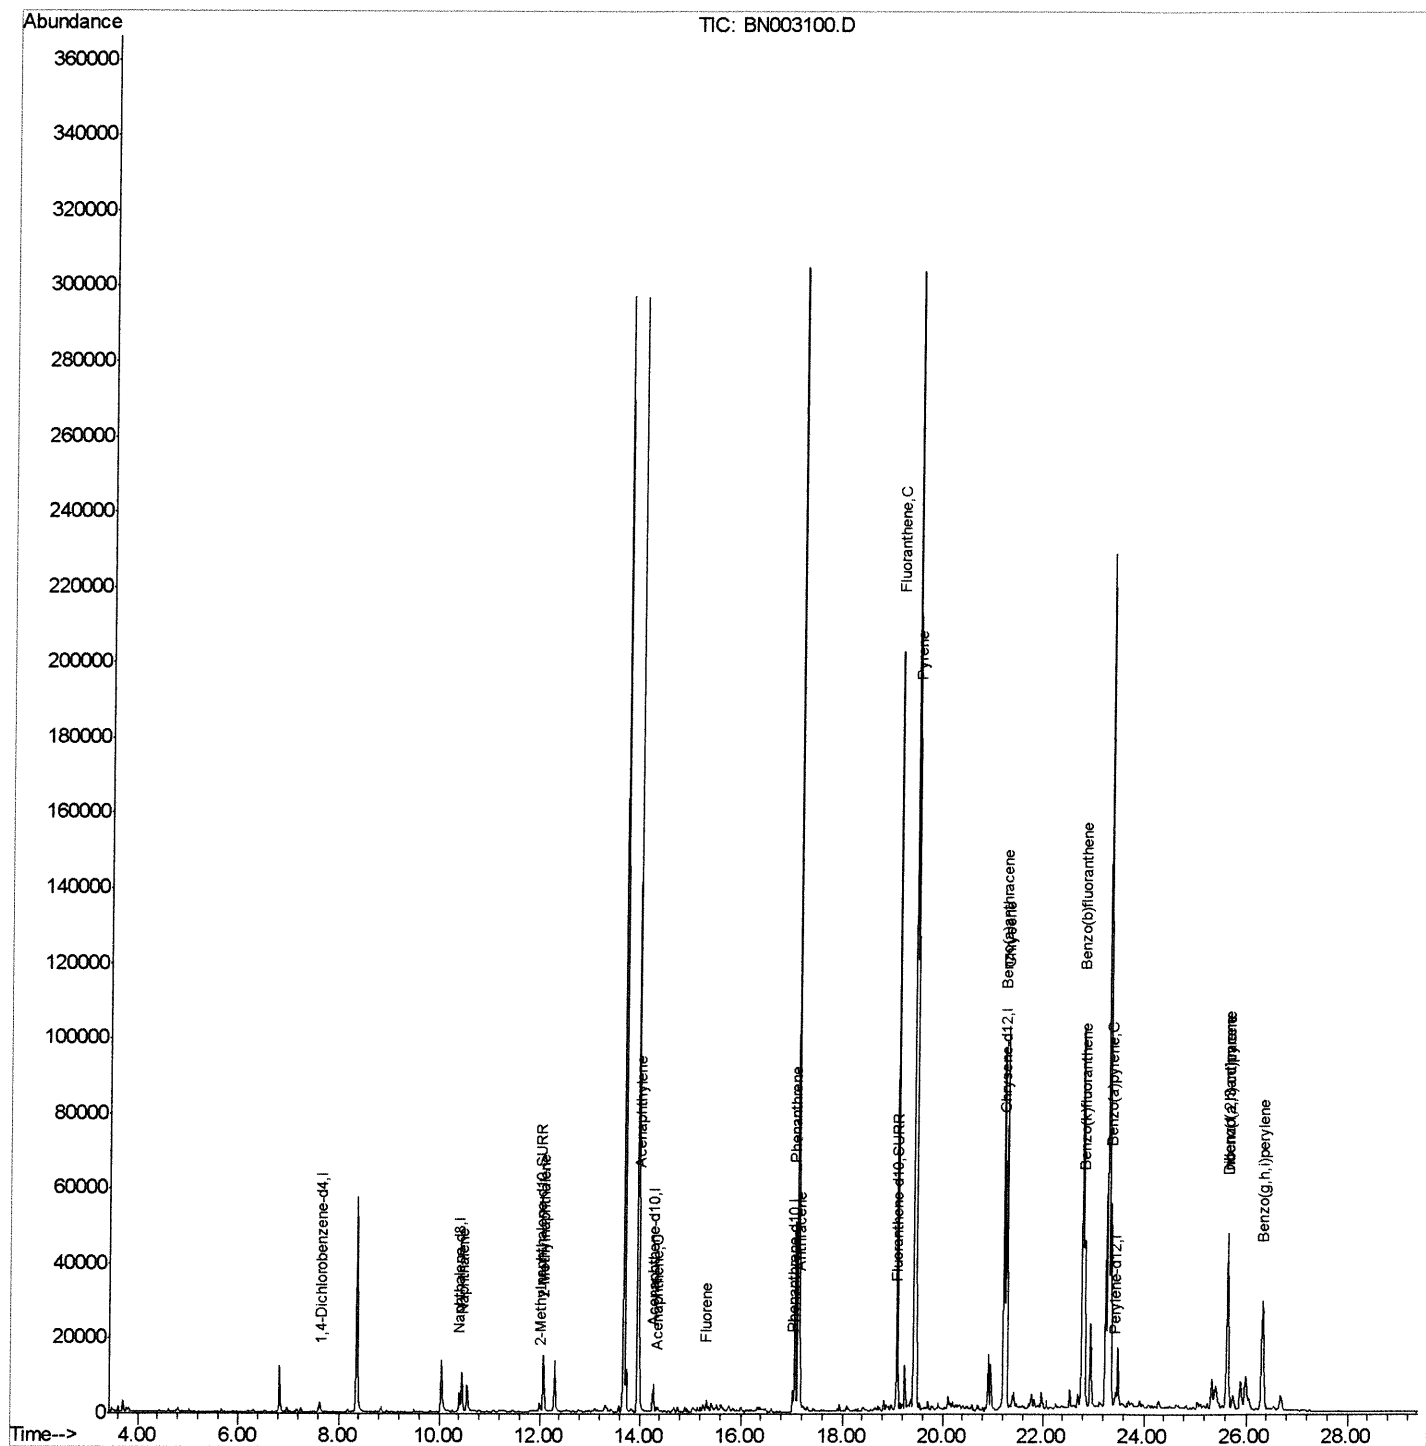

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:46:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

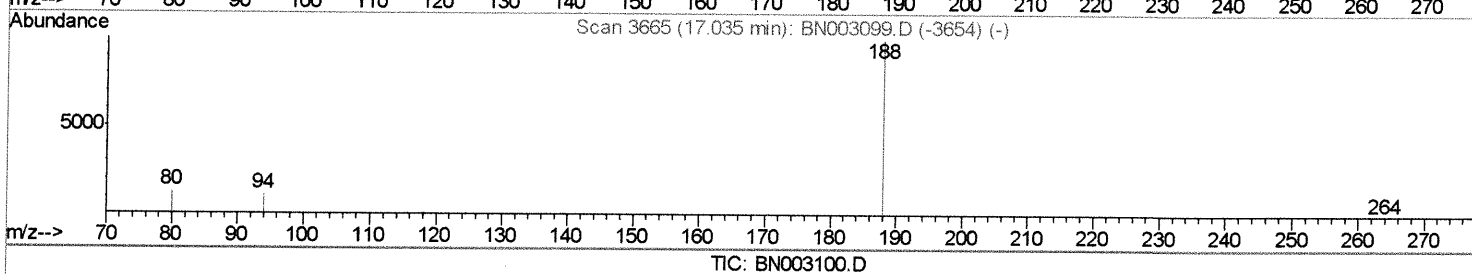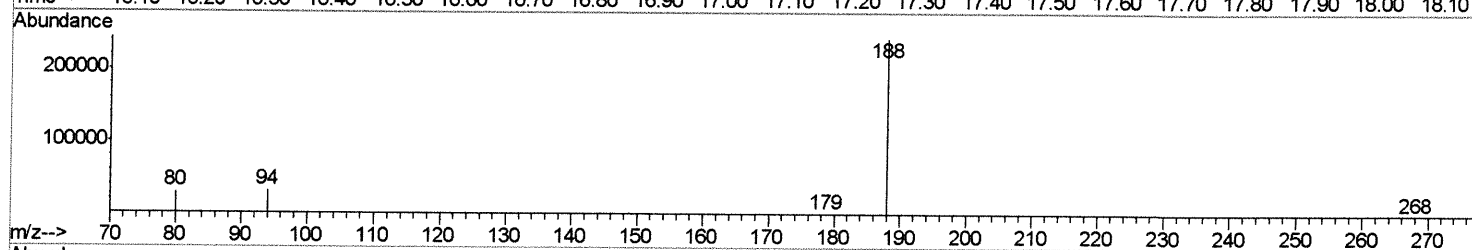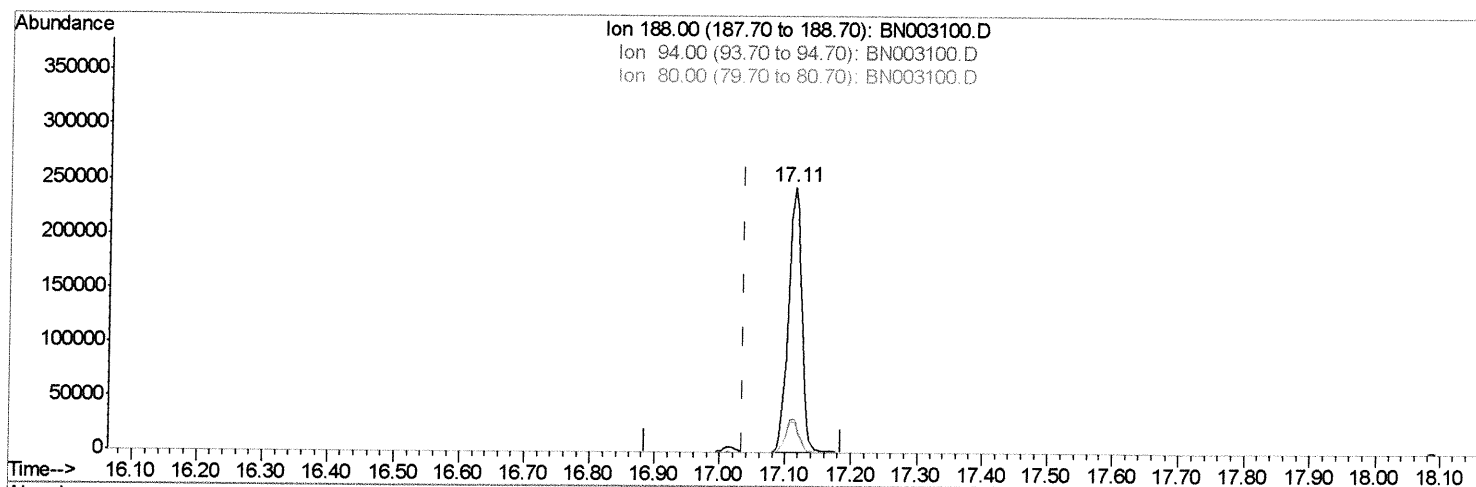

(10) Phenanthrene-d10 (I)

17.111min (+0.076) 0.40ng/ul

response 345645

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.89
80.00	12.70	11.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:46:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

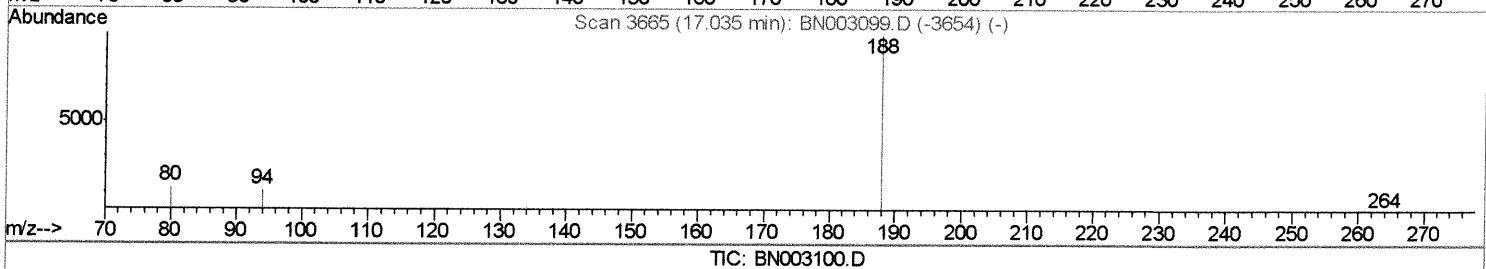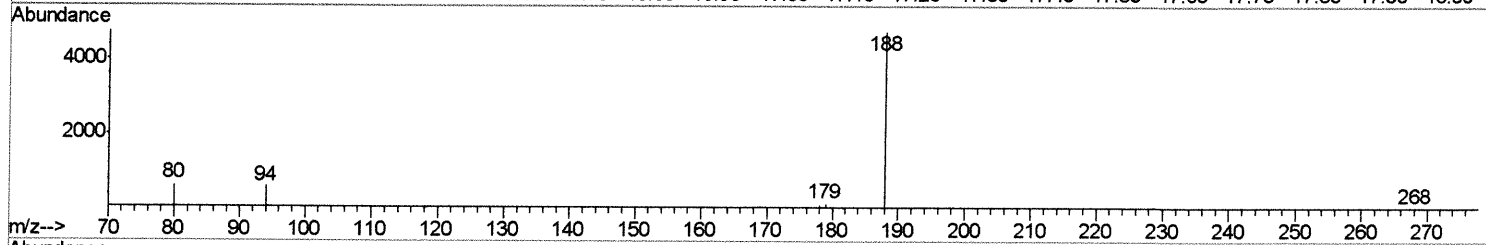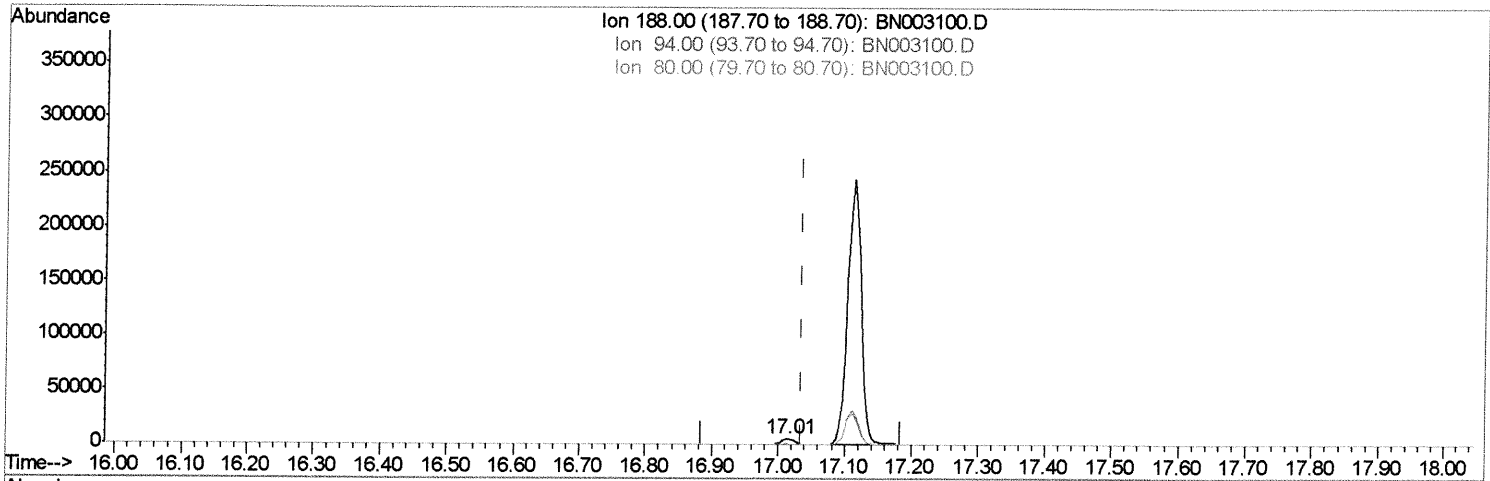

(10) Phenanthrene-d10 (I)

17.014min (-0.021) 0.40ng/ul m > SJ 10/12/18

response 6672

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.45
80.00	12.70	13.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

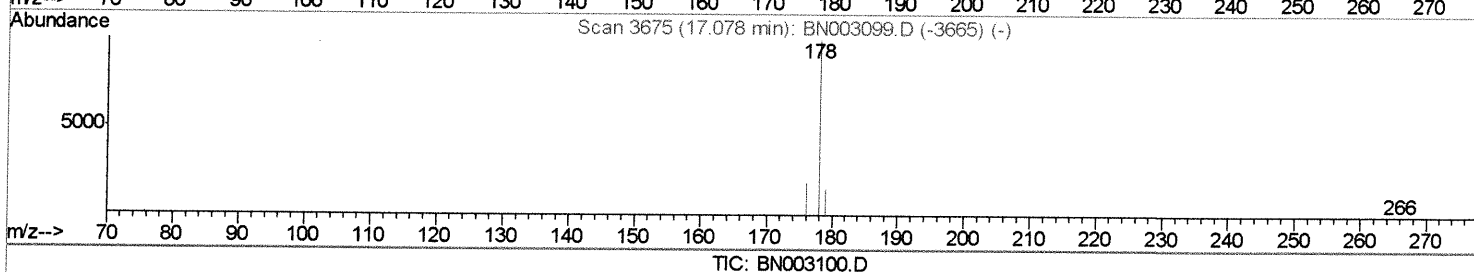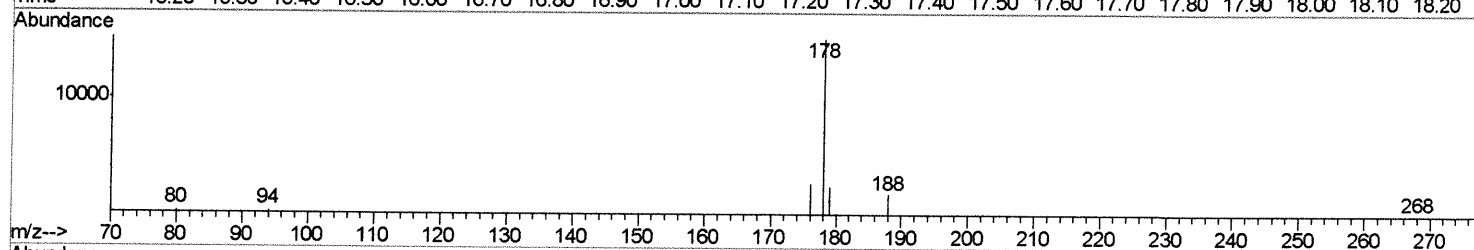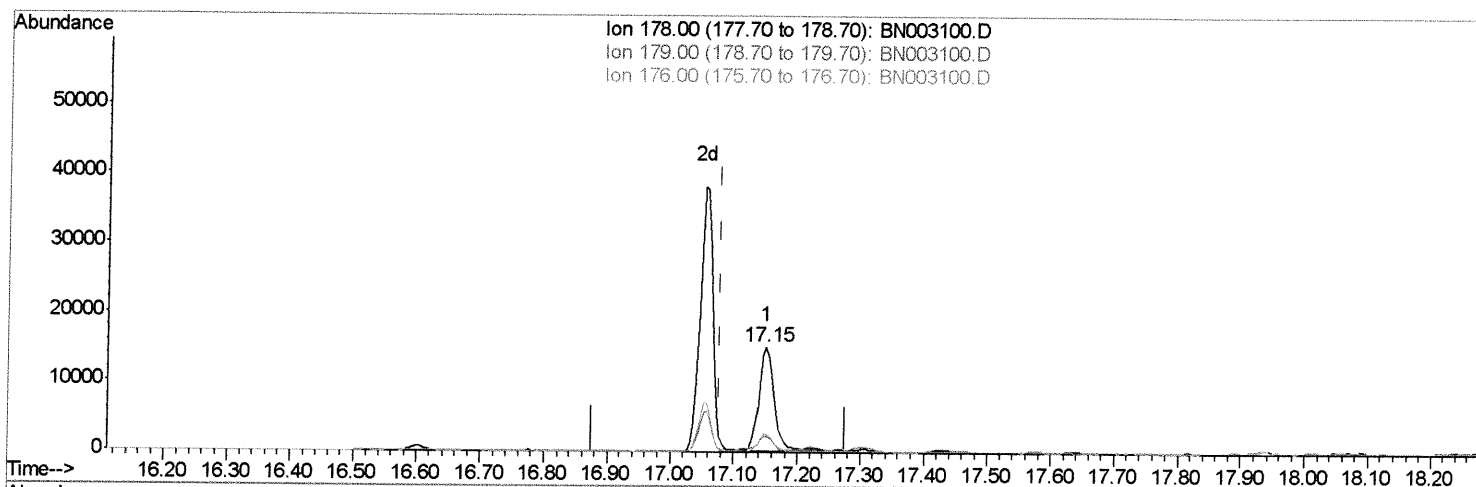

TIC: BN003100.D

(12) Phenanthrene

17.149min (+0.072) 1.36ng/ul

response 25312

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	16.08
176.00	19.30	18.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

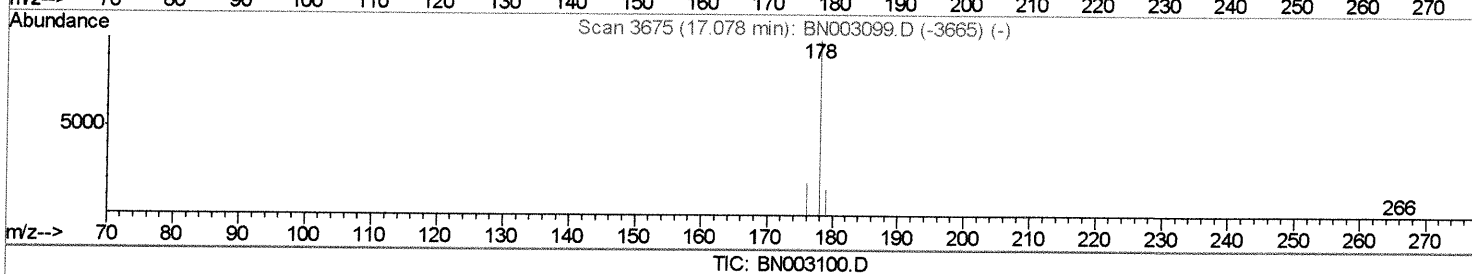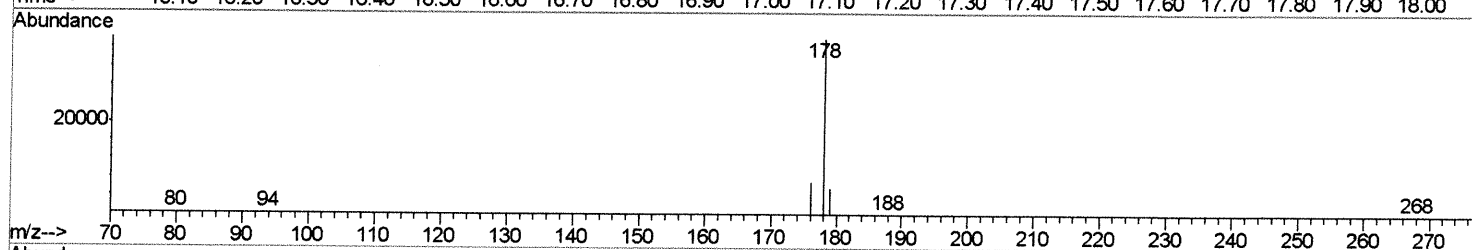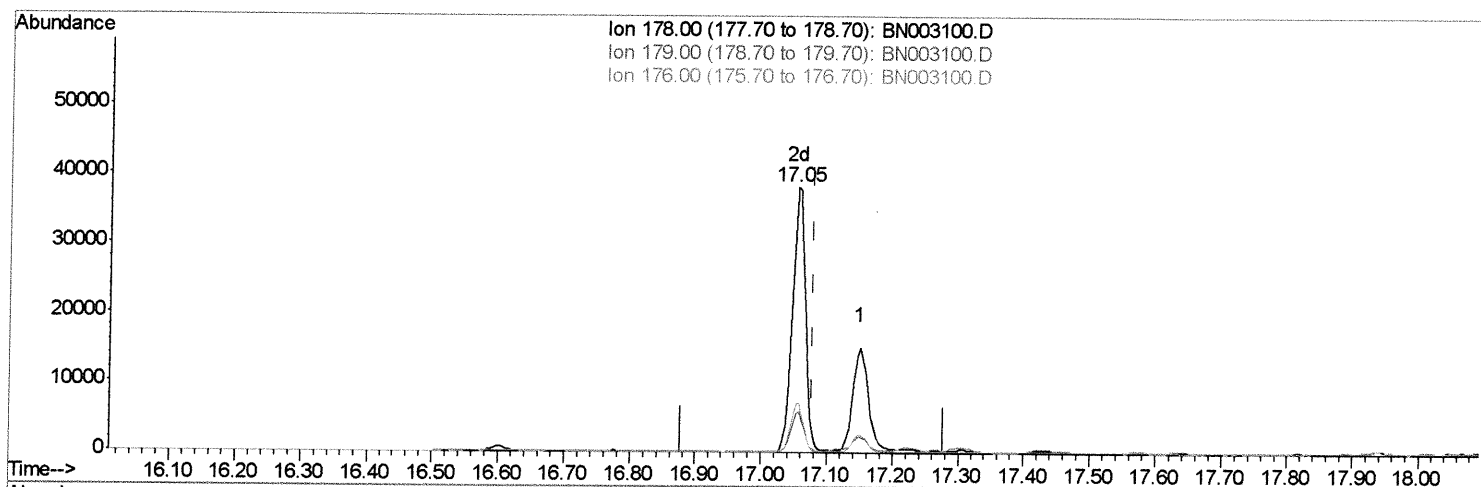

(12) Phenanthrene

17.052min (-0.025) 2.87ng/ul m> SJ 10/12/18

response 53428

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	15.19
176.00	19.30	18.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

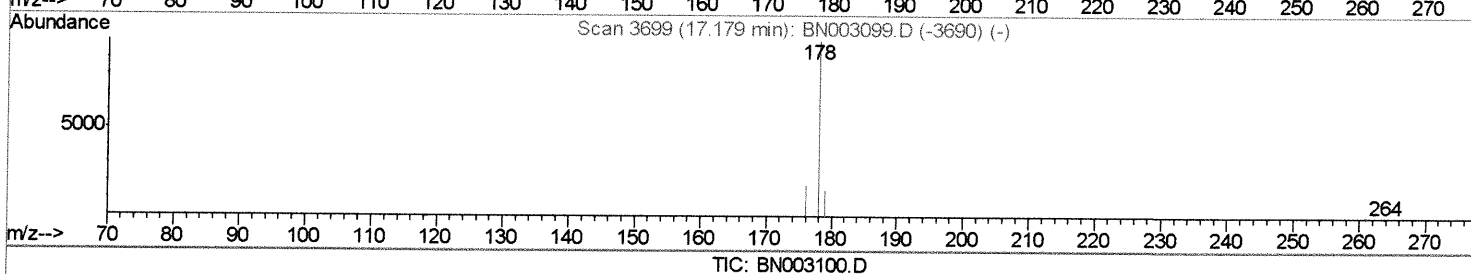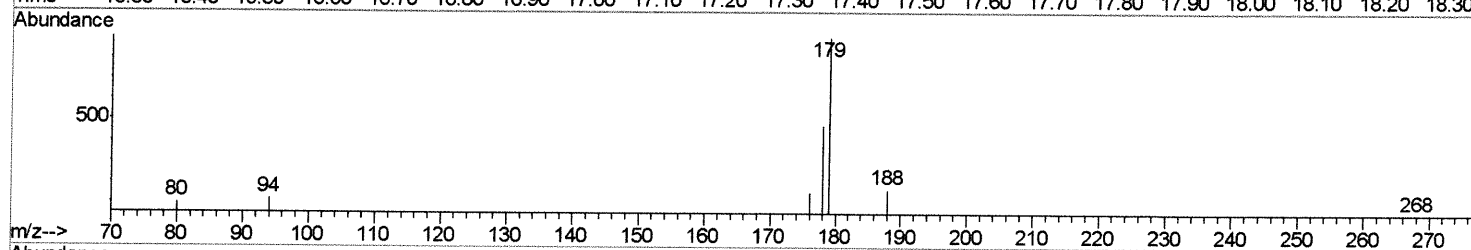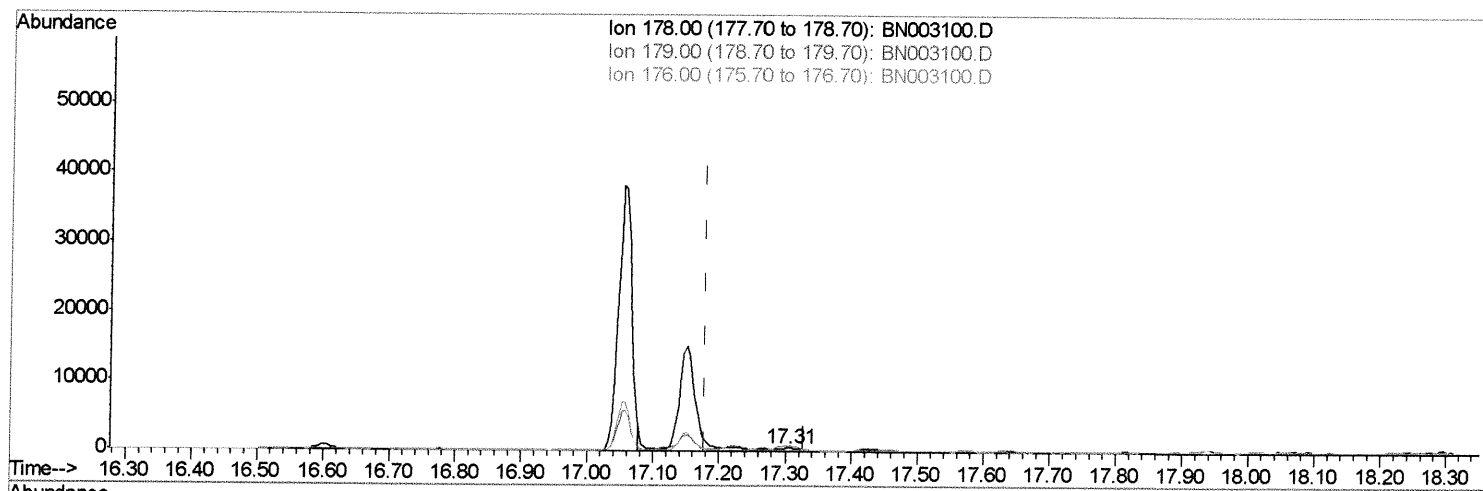

(13) Anthracene

17.305min (+0.127) 0.04ng/ul

response 629

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	190.68#
176.00	19.10	30.51#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

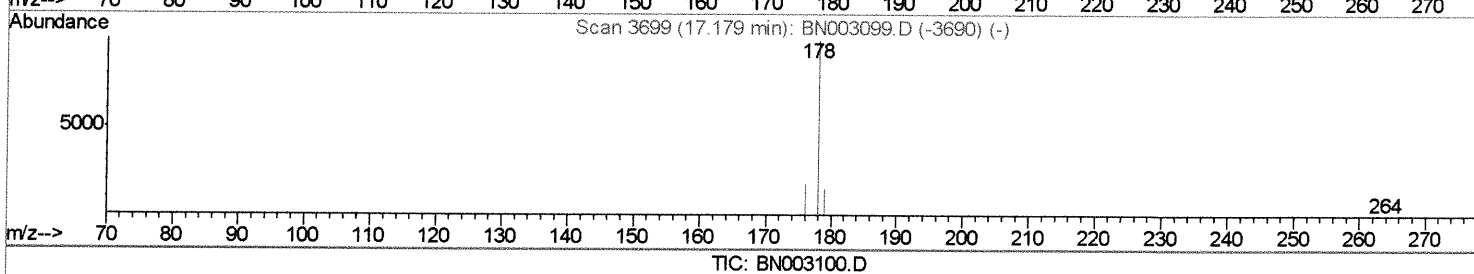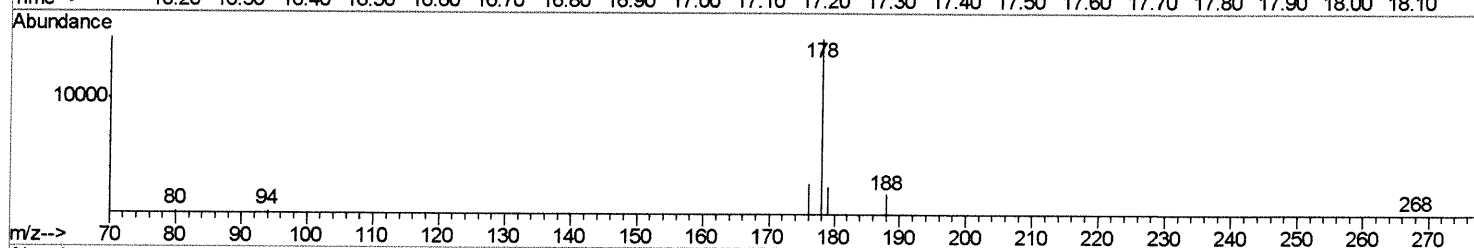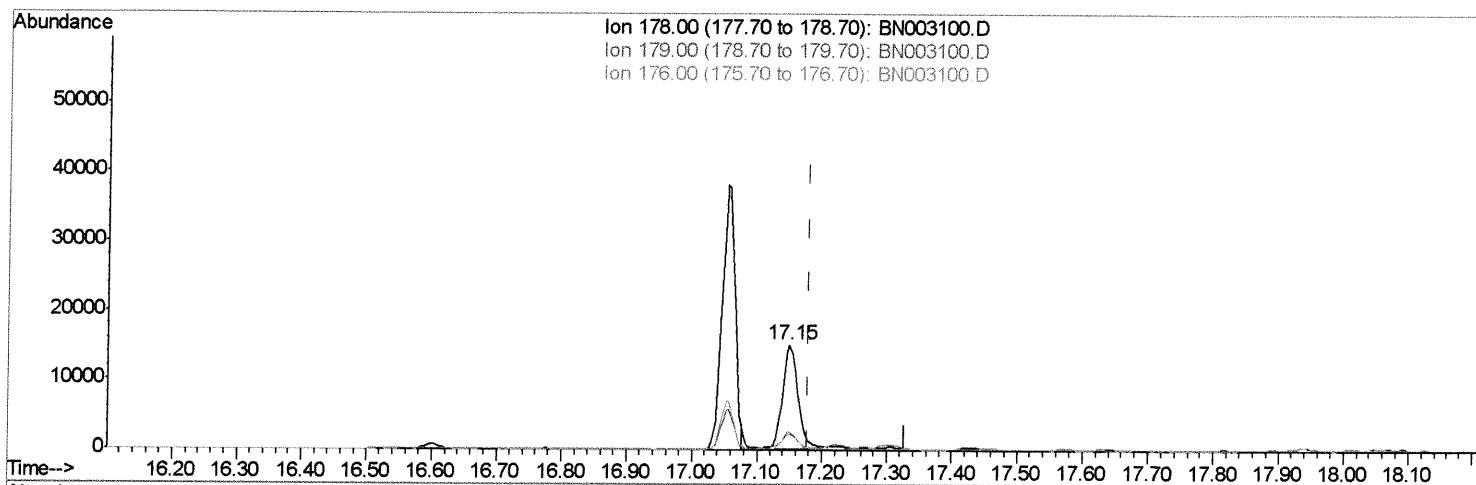

(13) Anthracene

17.149min (-0.030) 1.46ng/ul m > SJ 10/12/18

response 25650

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	16.08
176.00	19.10	18.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

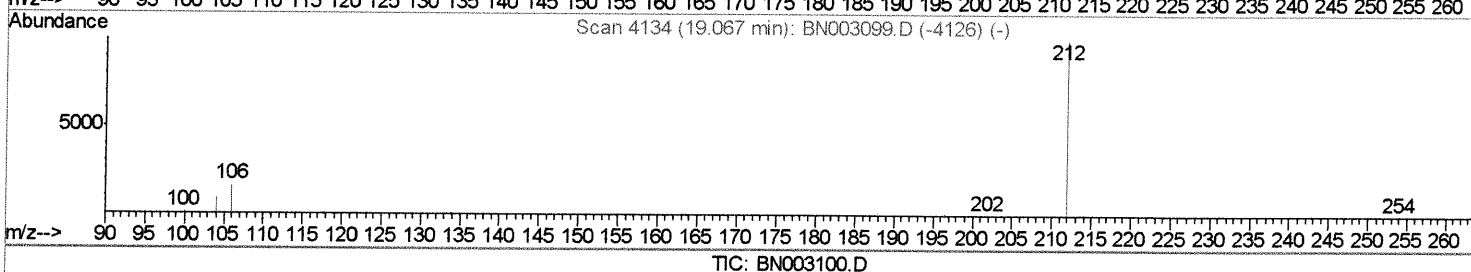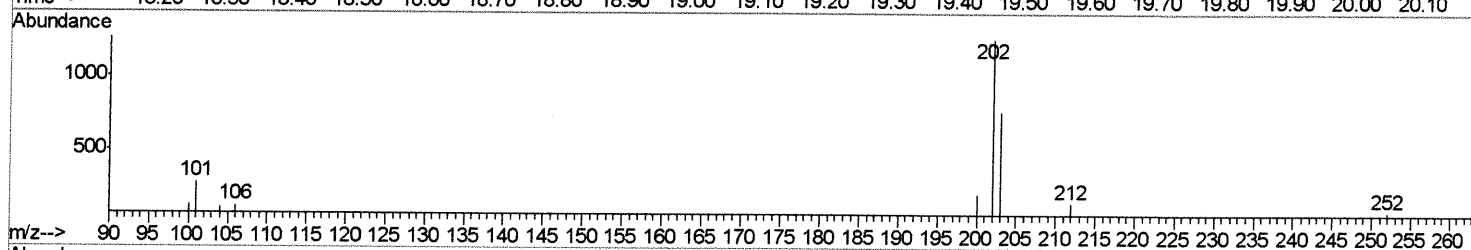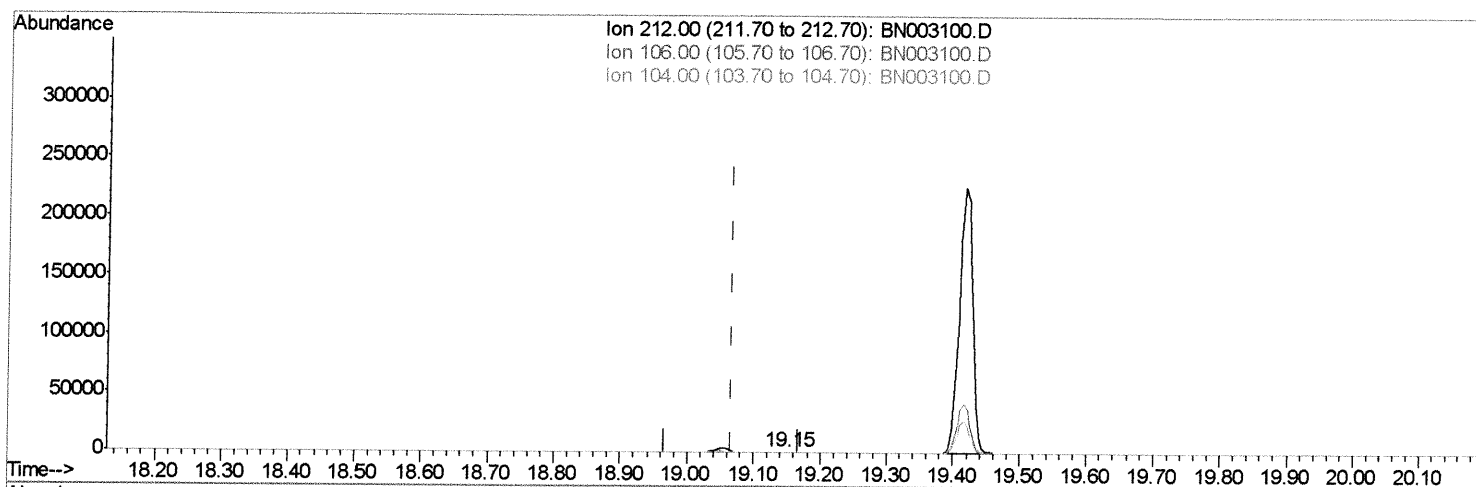

TIC: BN003100.D

(14) Fluoranthene-d10 (SURR)

19.150min (+0.084) 0.01ng/ul

response 118

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	21.19#
104.00	8.60	24.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

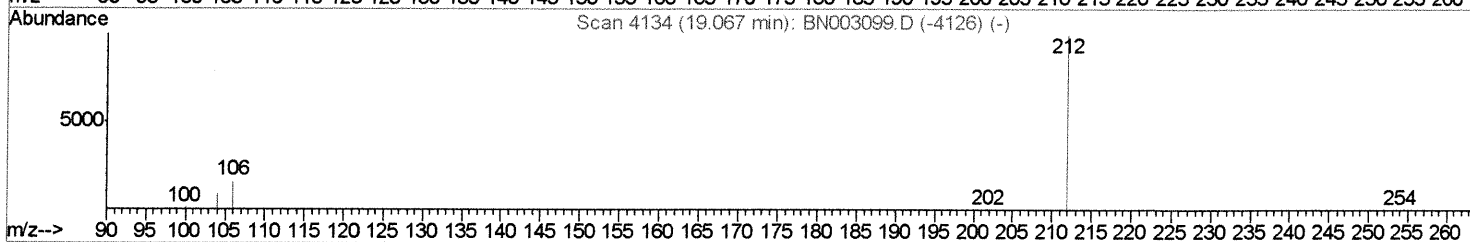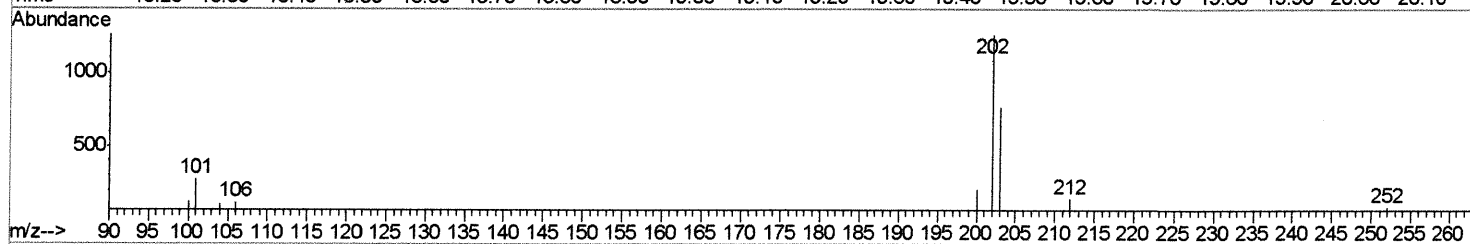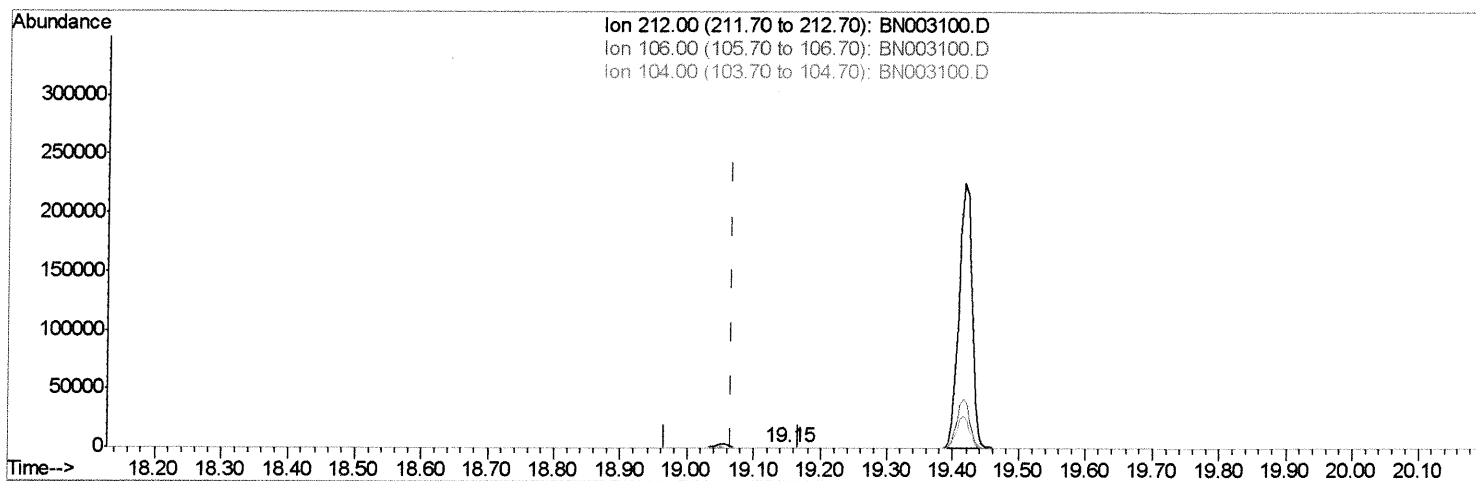

TIC: BN003100.D

(14) Fluoranthene-d10 (SURR)

19.150min (+0.084) 0.01ng/ul

response 118

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	21.19#
104.00	8.60	24.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

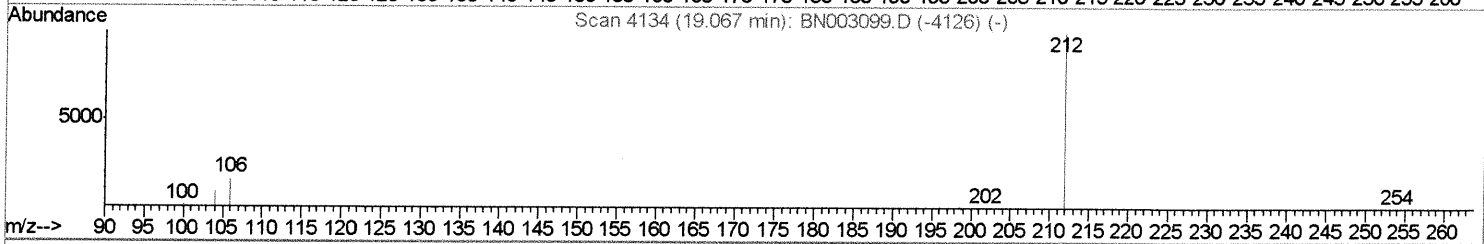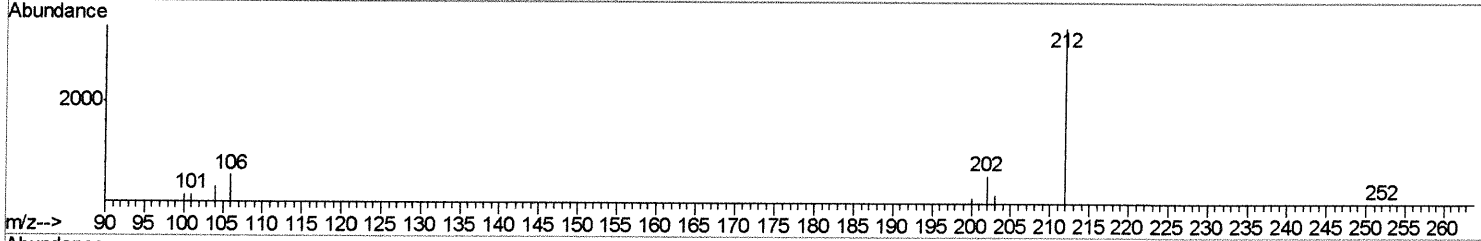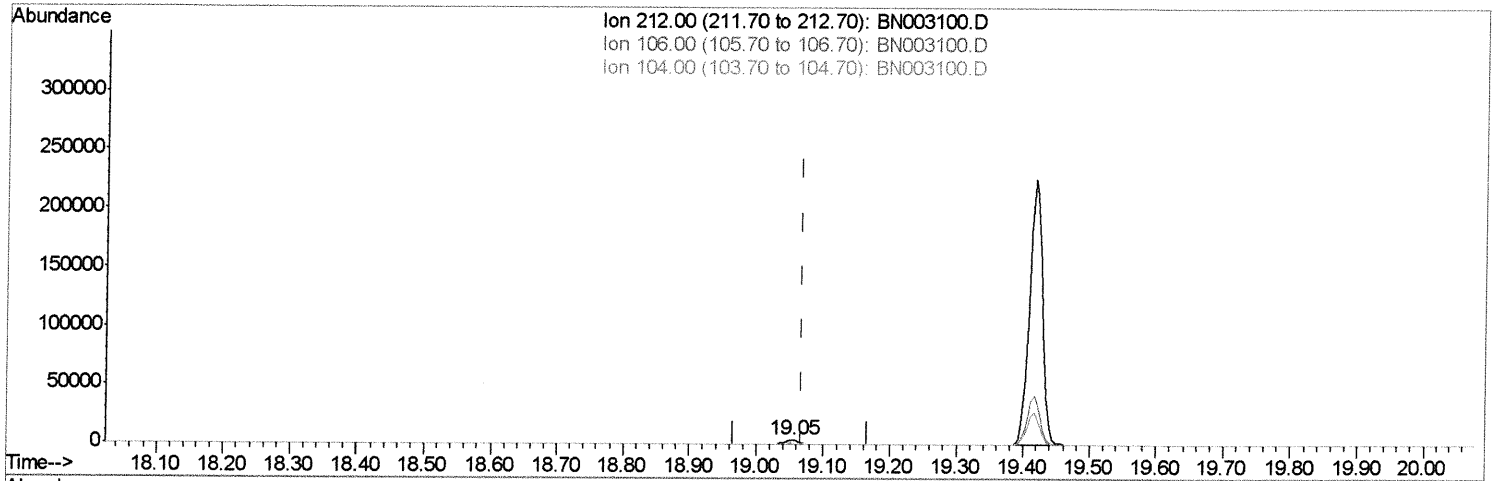

TIC: BN003100.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.014) 0.26ng/ul m

53 10/12/18

response 4868

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.51#
104.00	8.60	0.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

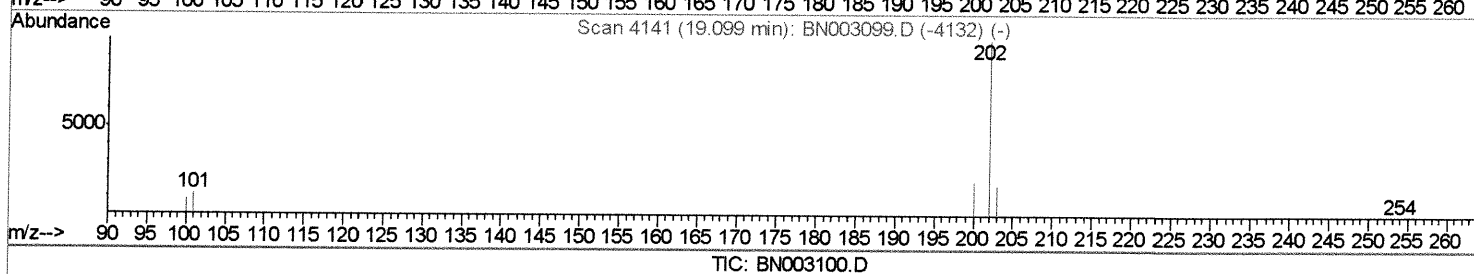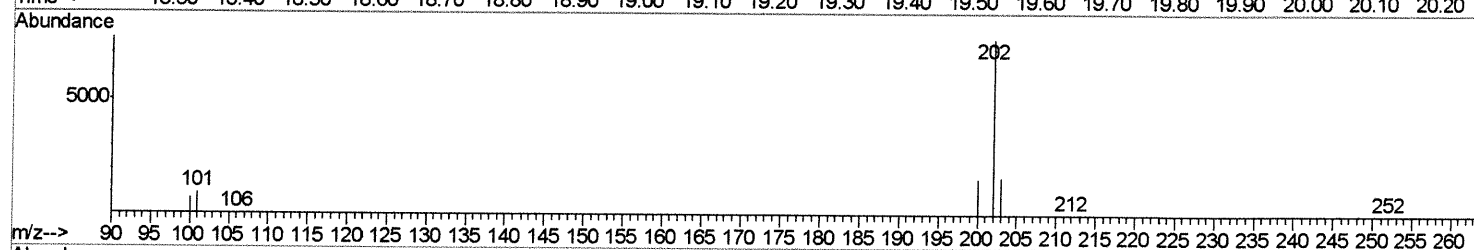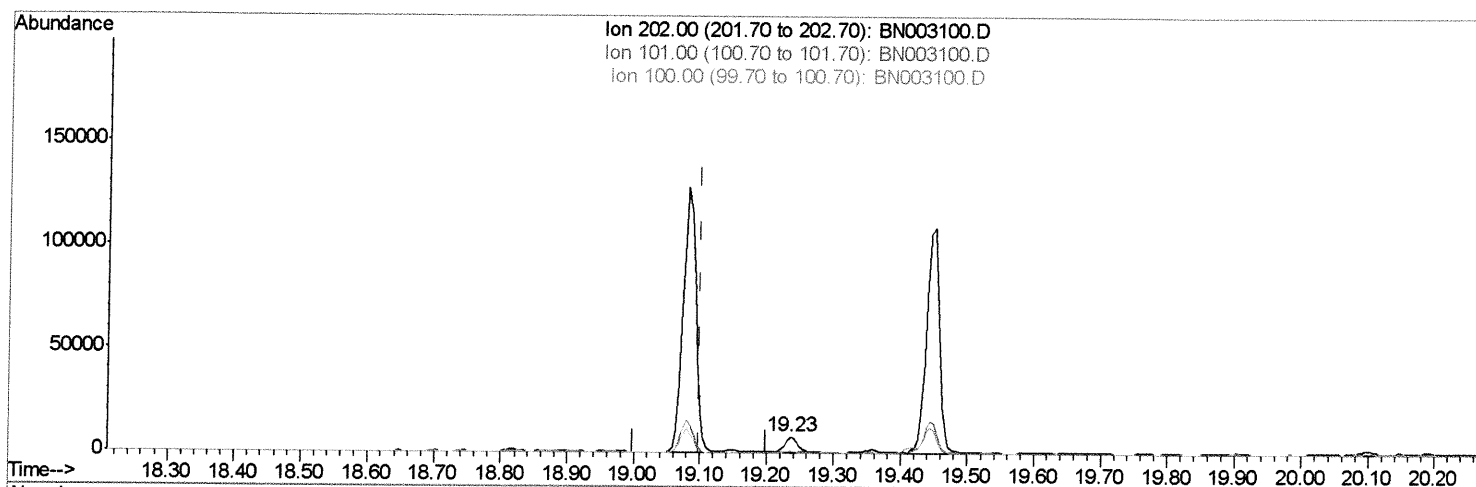

TIC: BN003100.D

(15) Fluoranthene (C)

19.234min (+0.135) 0.45ng/ul

response 9857

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.63
100.00	9.10	9.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

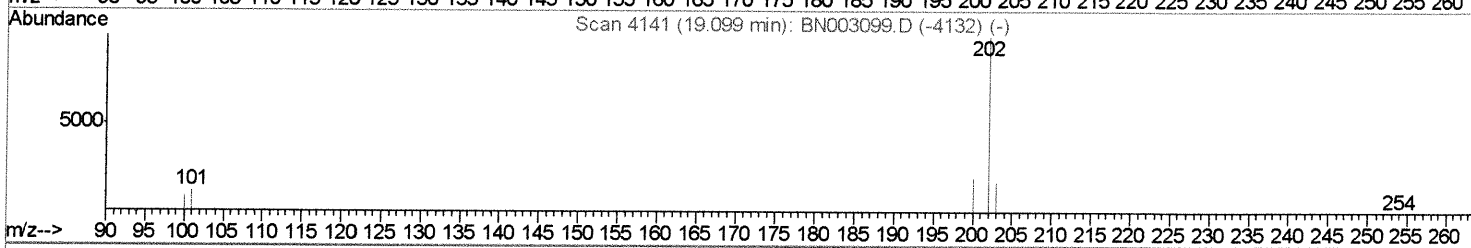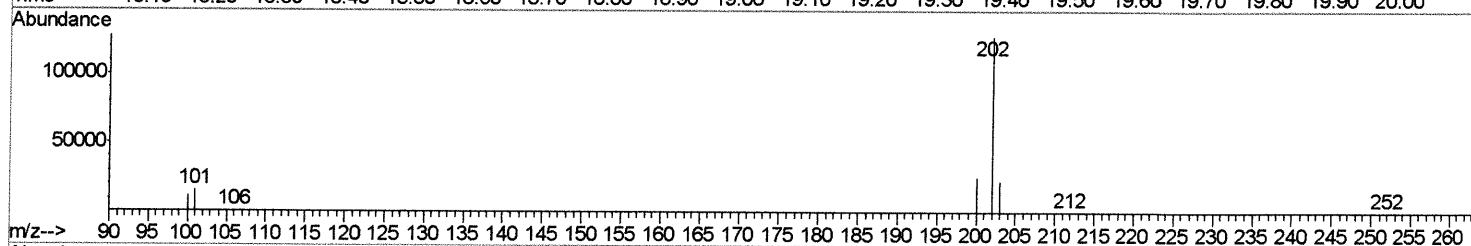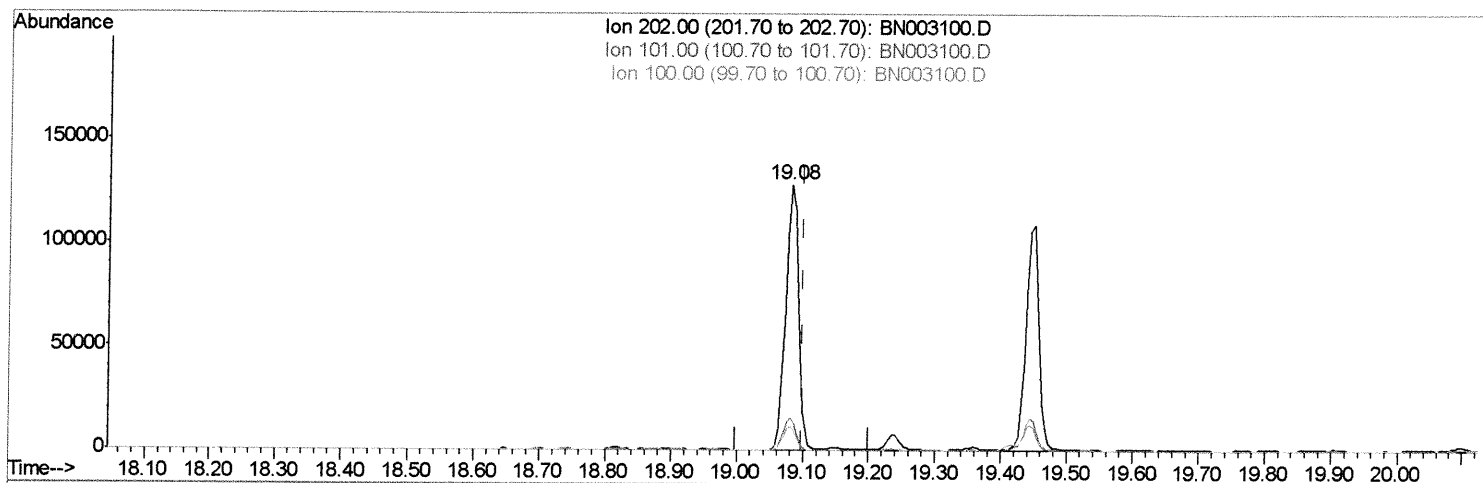

TIC: BN003100.D

(15) Fluoranthene (C)

19.081min (-0.019) 7.82ng/ul m > SJ 10/12/18

response 170600

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.15
100.00	9.10	9.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

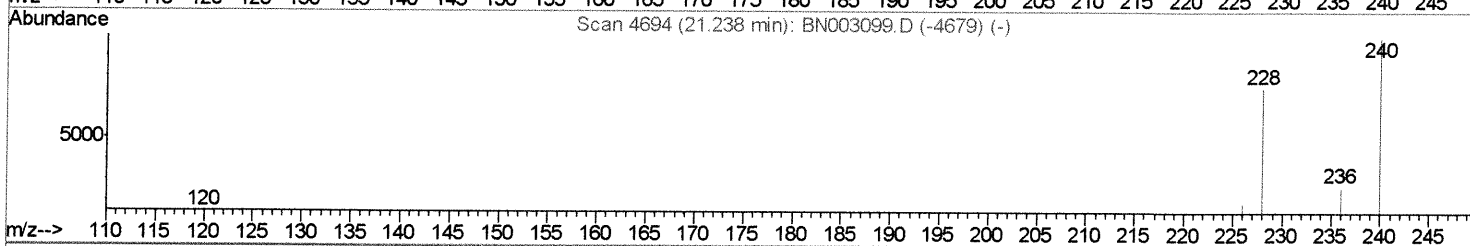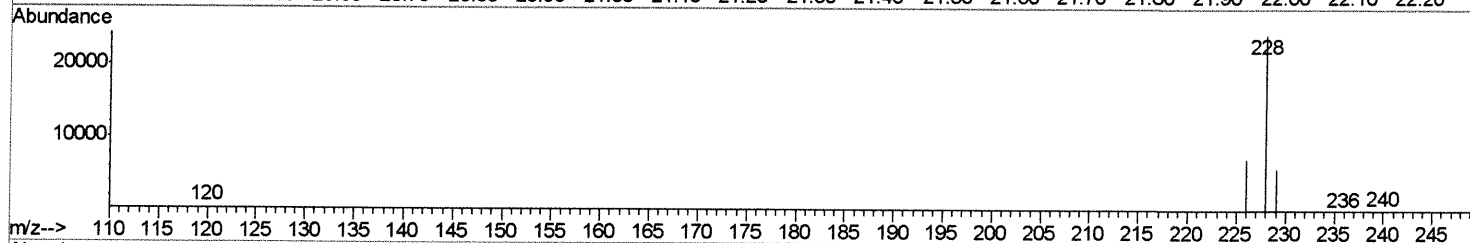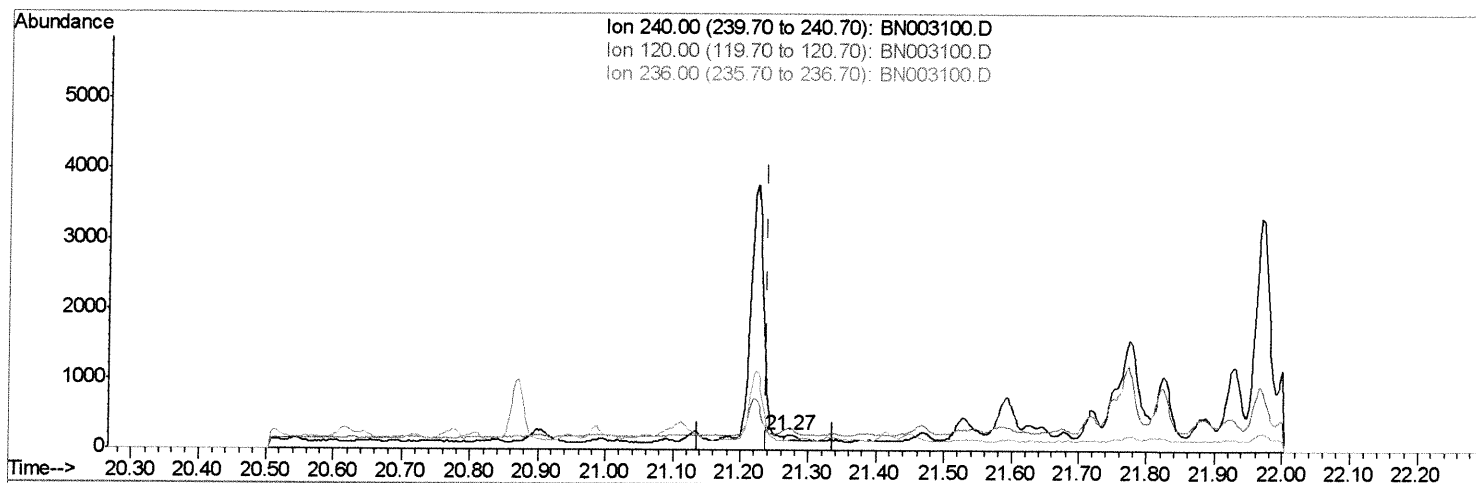

TIC: BN003100.D

(16) Chrysene-d12 (I)

21.270min (+0.032) 0.40ng/ul

response 77

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	146.95#
236.00	28.10	67.14#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:47:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

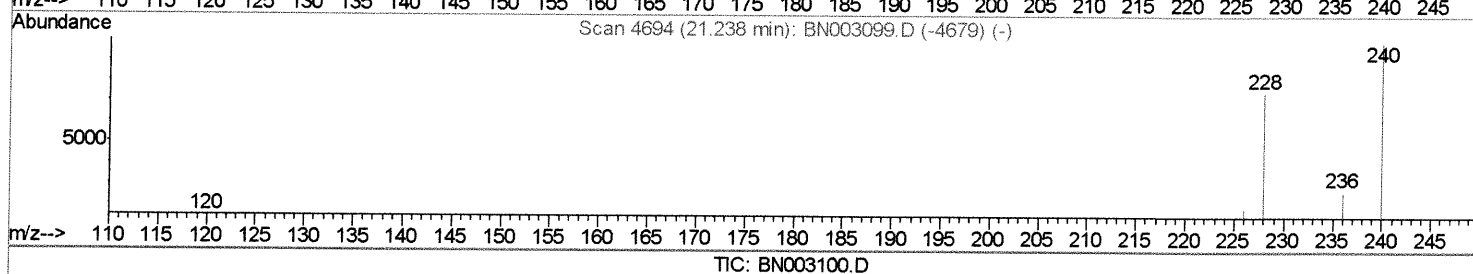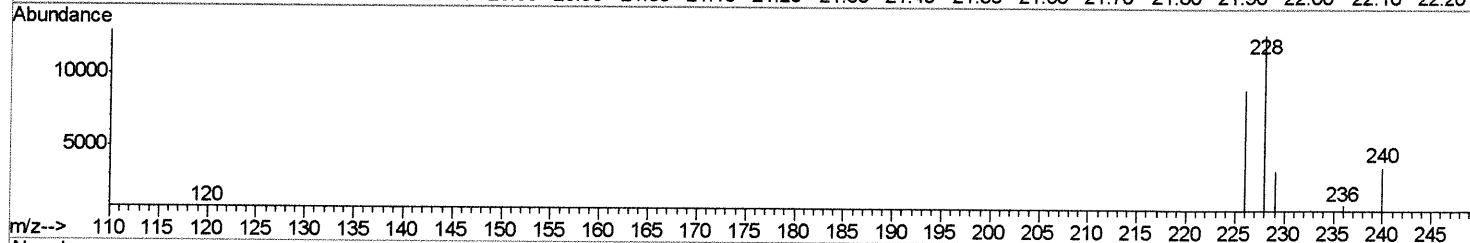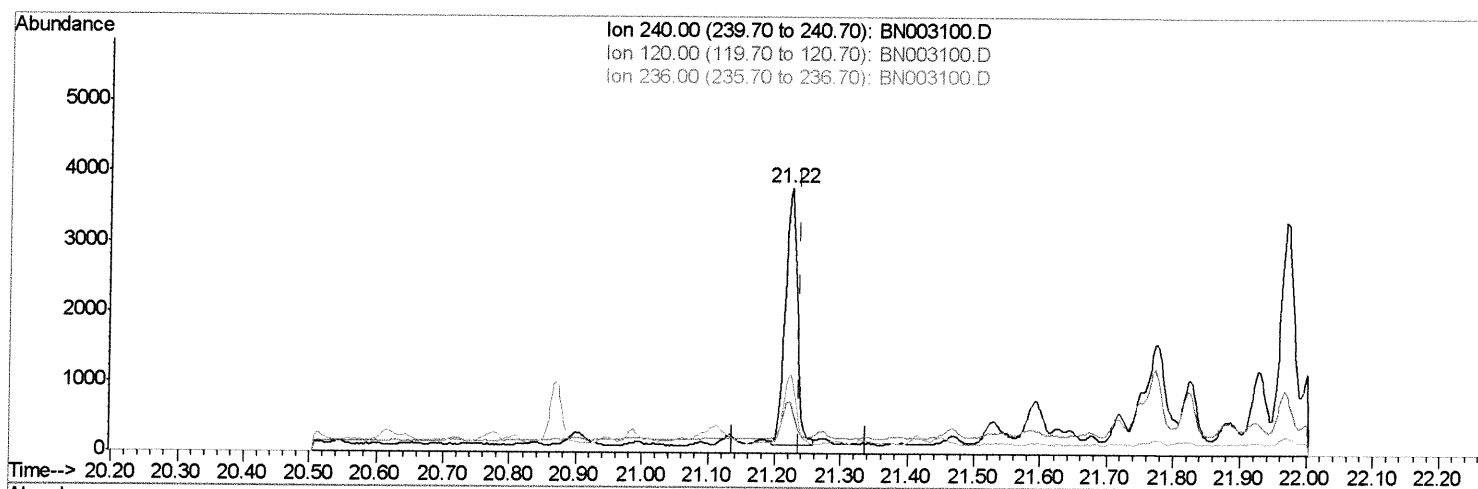

(16) Chrysene-d12 (I)

21.223min (-0.015) 0.40ng/ul m > SJ 10/12/18

response 4614

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	19.13
236.00	28.10	29.97
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

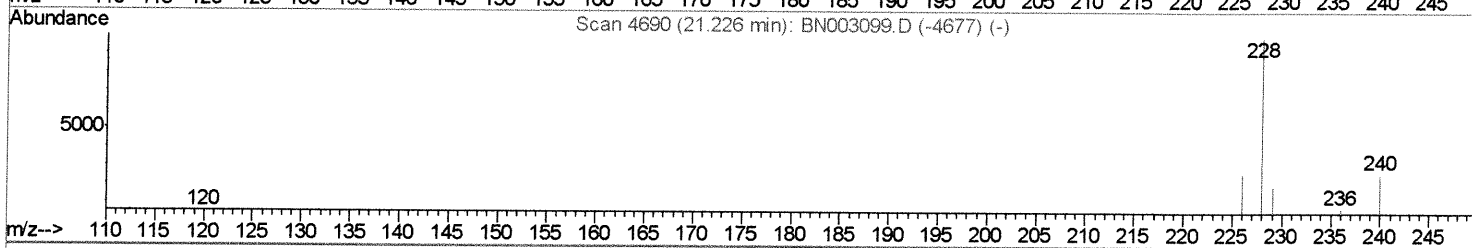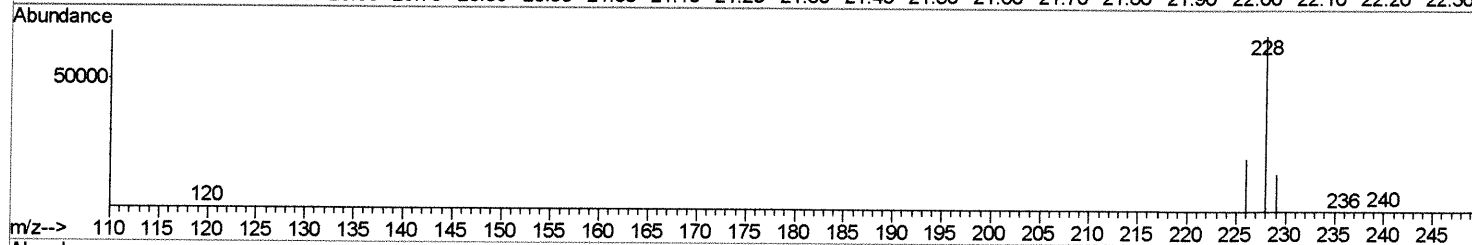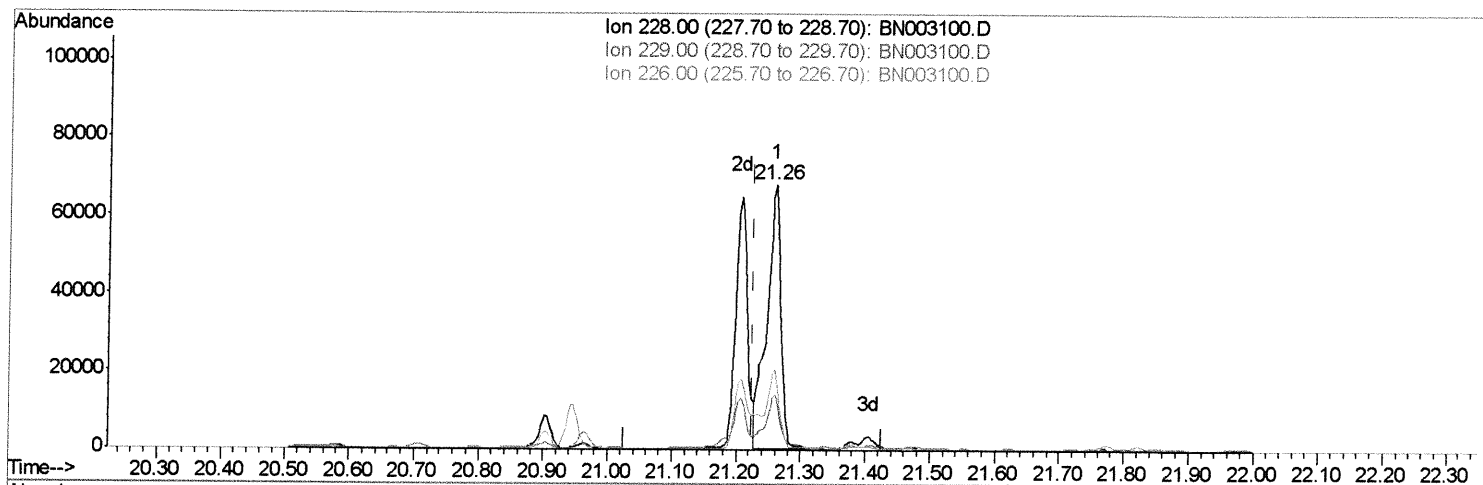

TIC: BN003100.D

(18) Benzo(a)anthracene
 21.258min (+0.032) 7.00ng/ul
 response 103870

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	21.14
226.00	27.90	30.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

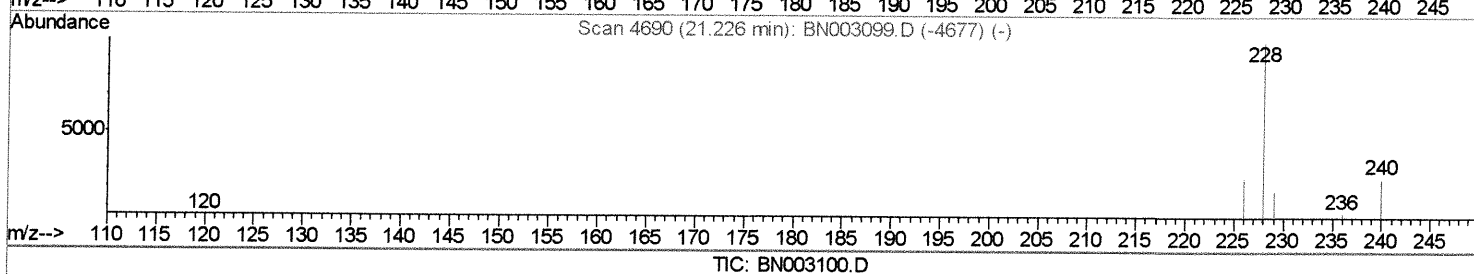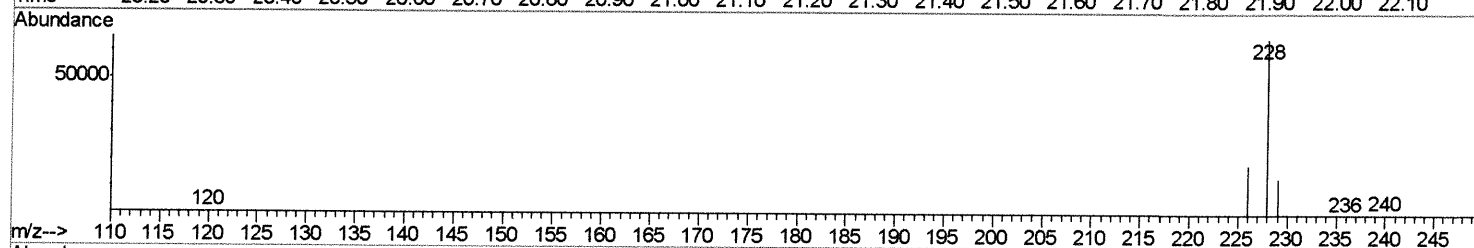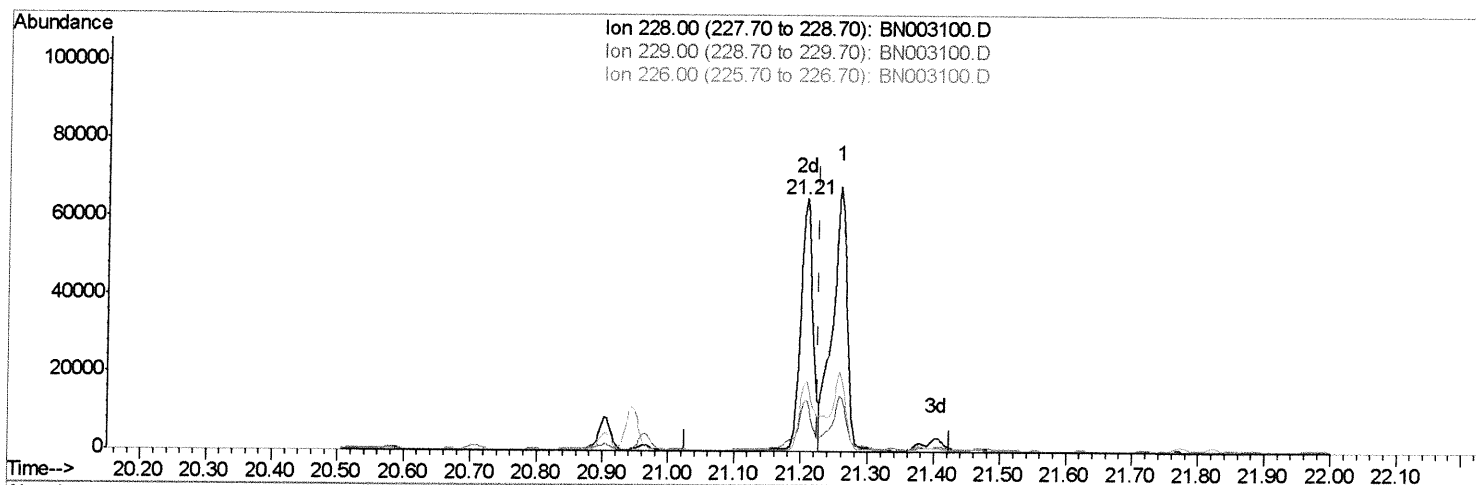

(18) Benzo(a)anthracene

21.206min (-0.021) 5.64ng/ul m > SJ 10/12/18

response 83738

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	20.72
226.00	27.90	28.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

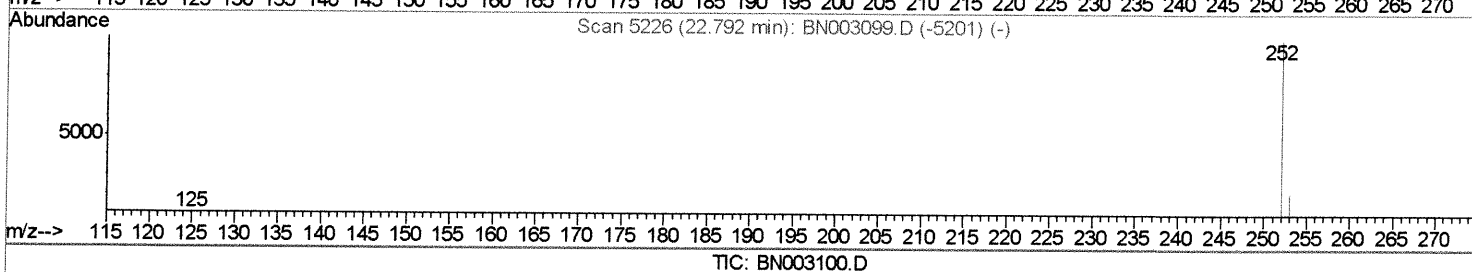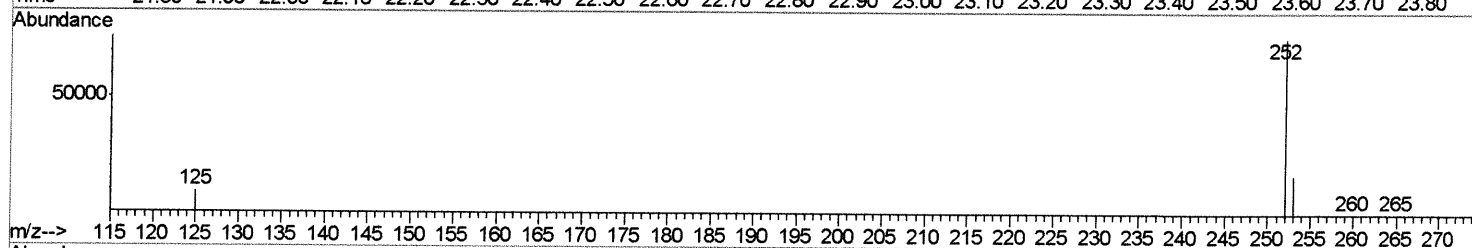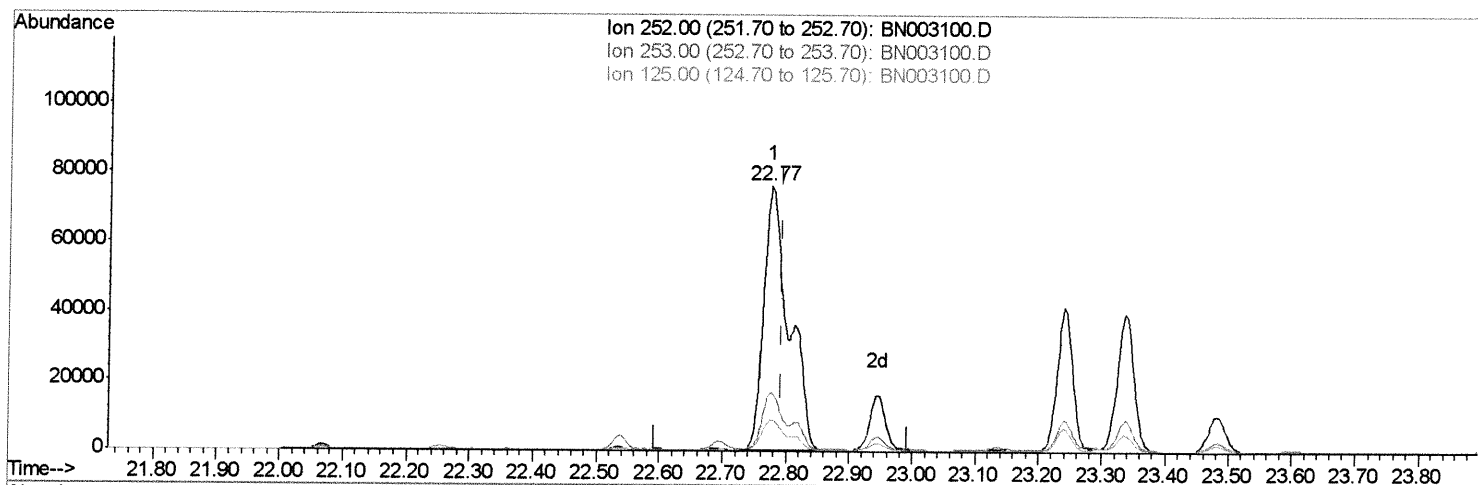

(21) Benzo(b)fluoranthene

22.775min (-0.018) 12.22ng/ul

response 210452

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.40
125.00	17.10	12.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
Data File : BN003100.D
Acq On : 11 Oct 2018 13:35
Operator : MJ/SJ
Sample : J5230-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z04

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 16:42:09 2018
Response via : Initial Calibration

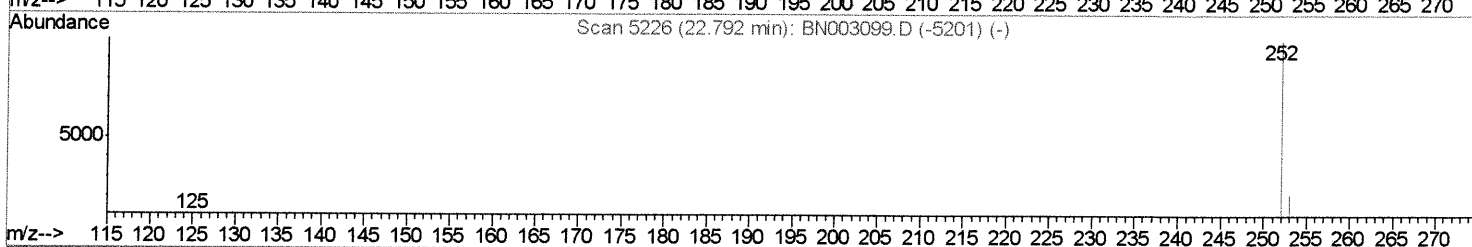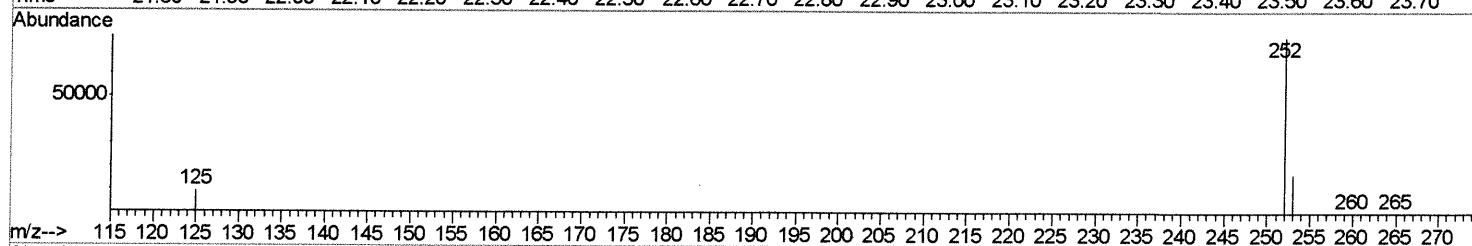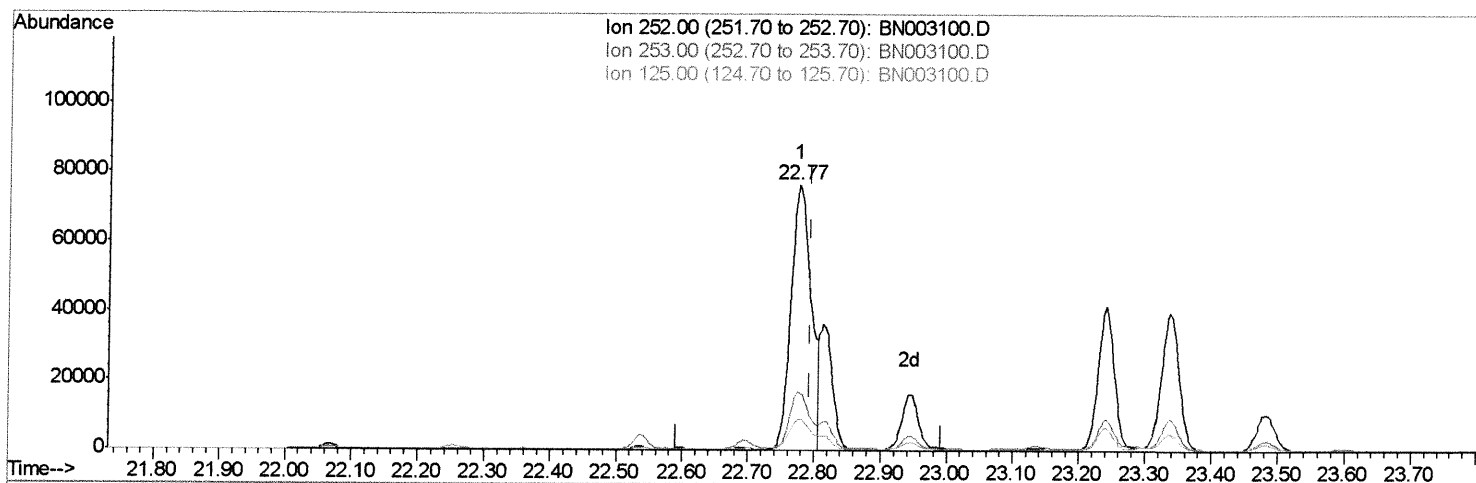

TIC: BN003100.D

(21) Benzo(b)fluoranthene

22.775min (-0.018) 9.42ng/ul m> SJ 10/12/18

response 162280

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.40
125.00	17.10	12.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

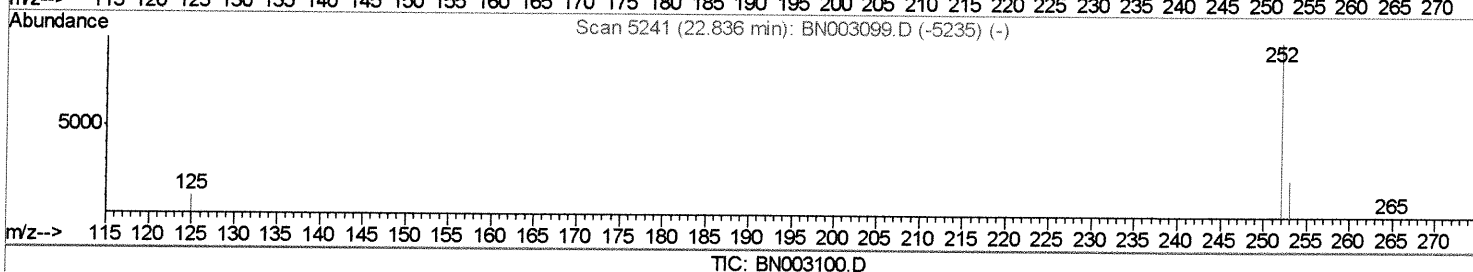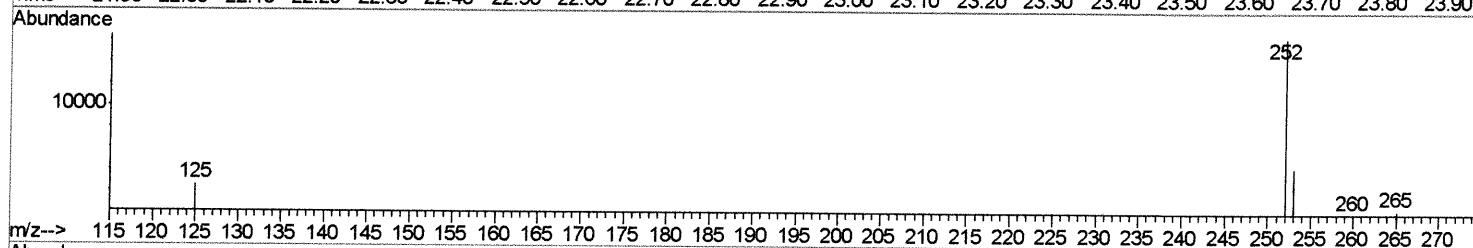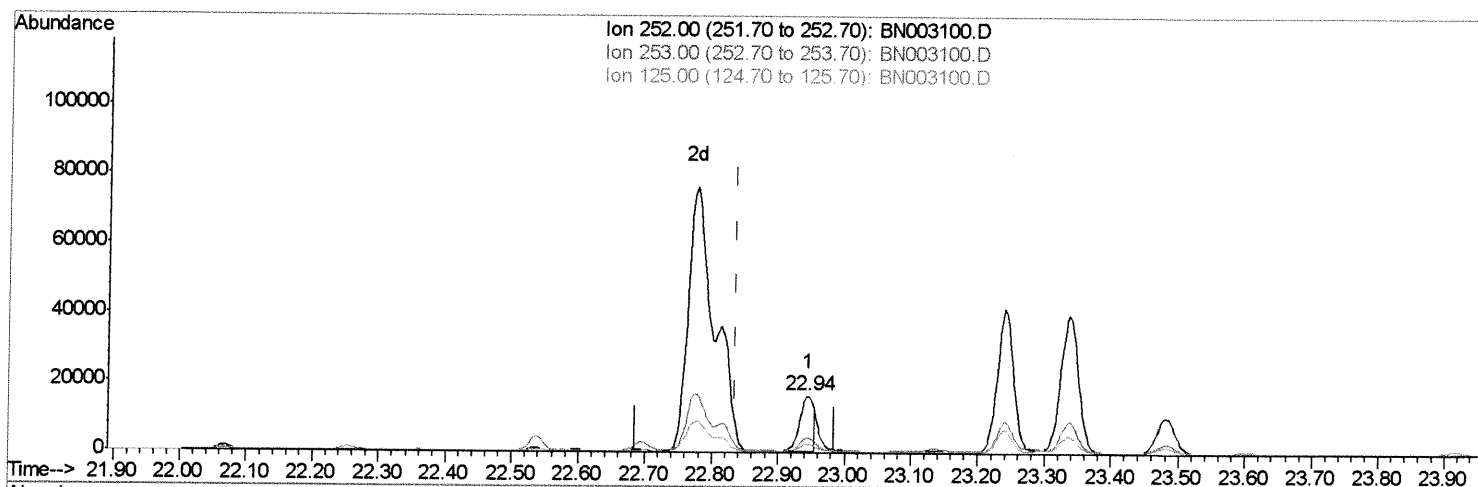

(22) Benzo(k)fluoranthene

22.944min (+0.108) 1.24ng/ul

response 22061

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.86
125.00	17.60	15.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:51:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

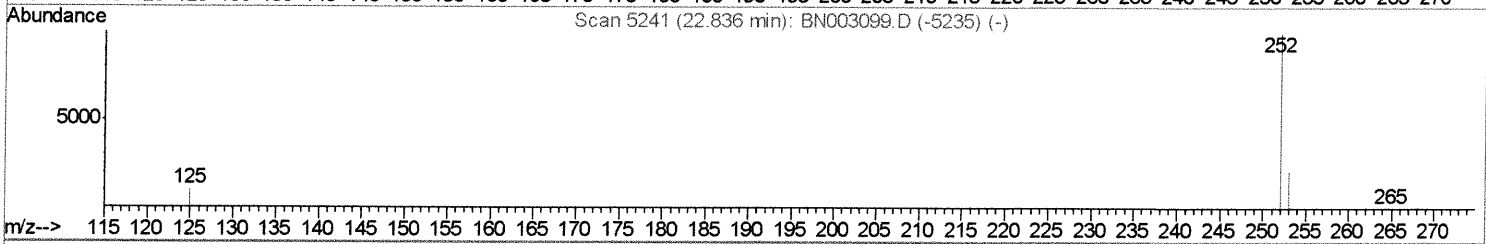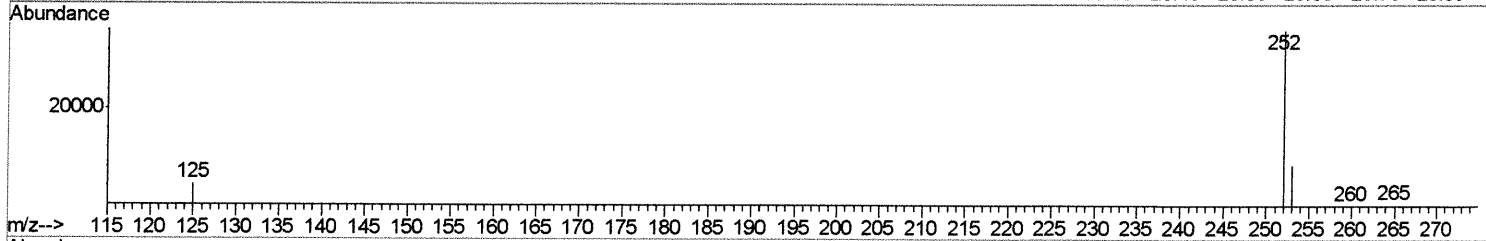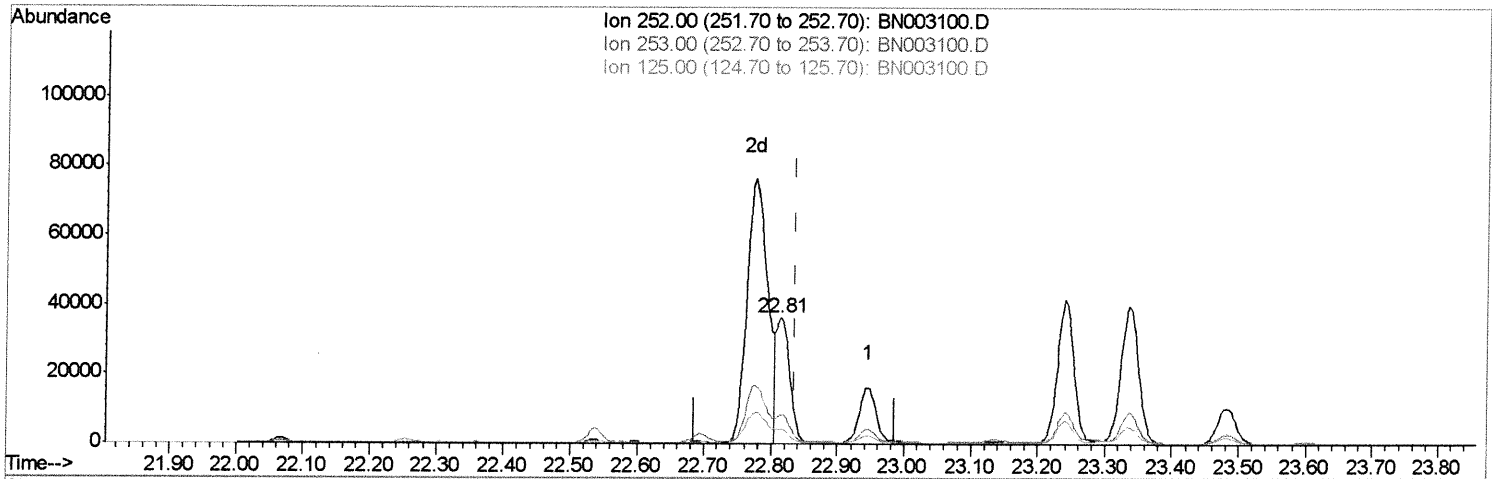

(22) Benzo(k)fluoranthene

22.813min (-0.023) 2.86ng/ul m > SJ 10/12/18

response 50961

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.28
125.00	17.60	12.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101218\
 Data File : BN003100.D
 Acq On : 11 Oct 2018 13:35
 Operator : MJ/SJ
 Sample : J5230-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z04

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:09 PM

Quant Time: Oct 11 16:52:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 16:42:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1711	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6856	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3726	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	6672m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.22	240	4614m	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	4781	0.40	ng/ul	-0.02

SJ 10/12/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.00	152	3095	0.29	ng/ul	-0.02
14) Fluoranthene-d10	19.05	212	4868m	0.26	ng/ul	-0.01

SJ 10/12/18

Target Compounds

					Qvalue	
3) Naphthalene	10.44	128	14953	0.850	ng/ul	97
5) 2-Methylnaphthalene	12.07	142	12538	1.035	ng/ul	97
7) Acenaphthylene	13.98	152	29314	1.720	ng/ul	99
8) Acenaphthene	14.32	153	920	0.071	ng/ul#	92
9) Fluorene	15.32	166	1822	0.123	ng/ul#	81
12) Phenanthrene	17.05	178	53428m	2.873	ng/ul	
13) Anthracene	17.15	178	25650m	1.460	ng/ul	
15) Fluoranthene	19.08	202	170600m	7.819	ng/ul	
17) Pyrene	19.45	202	146418	8.170	ng/ul	95
18) Benzo(a)anthracene	21.21	228	83738m	5.640	ng/ul	
19) Chrysene	21.26	228	103552	6.868	ng/ul	100
21) Benzo(b)fluoranthene	22.77	252	162280m	9.425	ng/ul	
22) Benzo(k)fluoranthene	22.81	252	50961m	2.855	ng/ul	
23) Benzo(a)pyrene	23.34	252	73707	4.777	ng/ul#	86
24) Indeno(1,2,3-cd)pyrene	25.64	276	68817	3.881	ng/ul#	94
25) Dibenzo(a,h)anthracene	25.64	278	19692	1.387	ng/ul	96
26) Benzo(g,h,i)perylene	26.31	276	57523	3.847	ng/ul	93

SJ 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed