


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:38:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

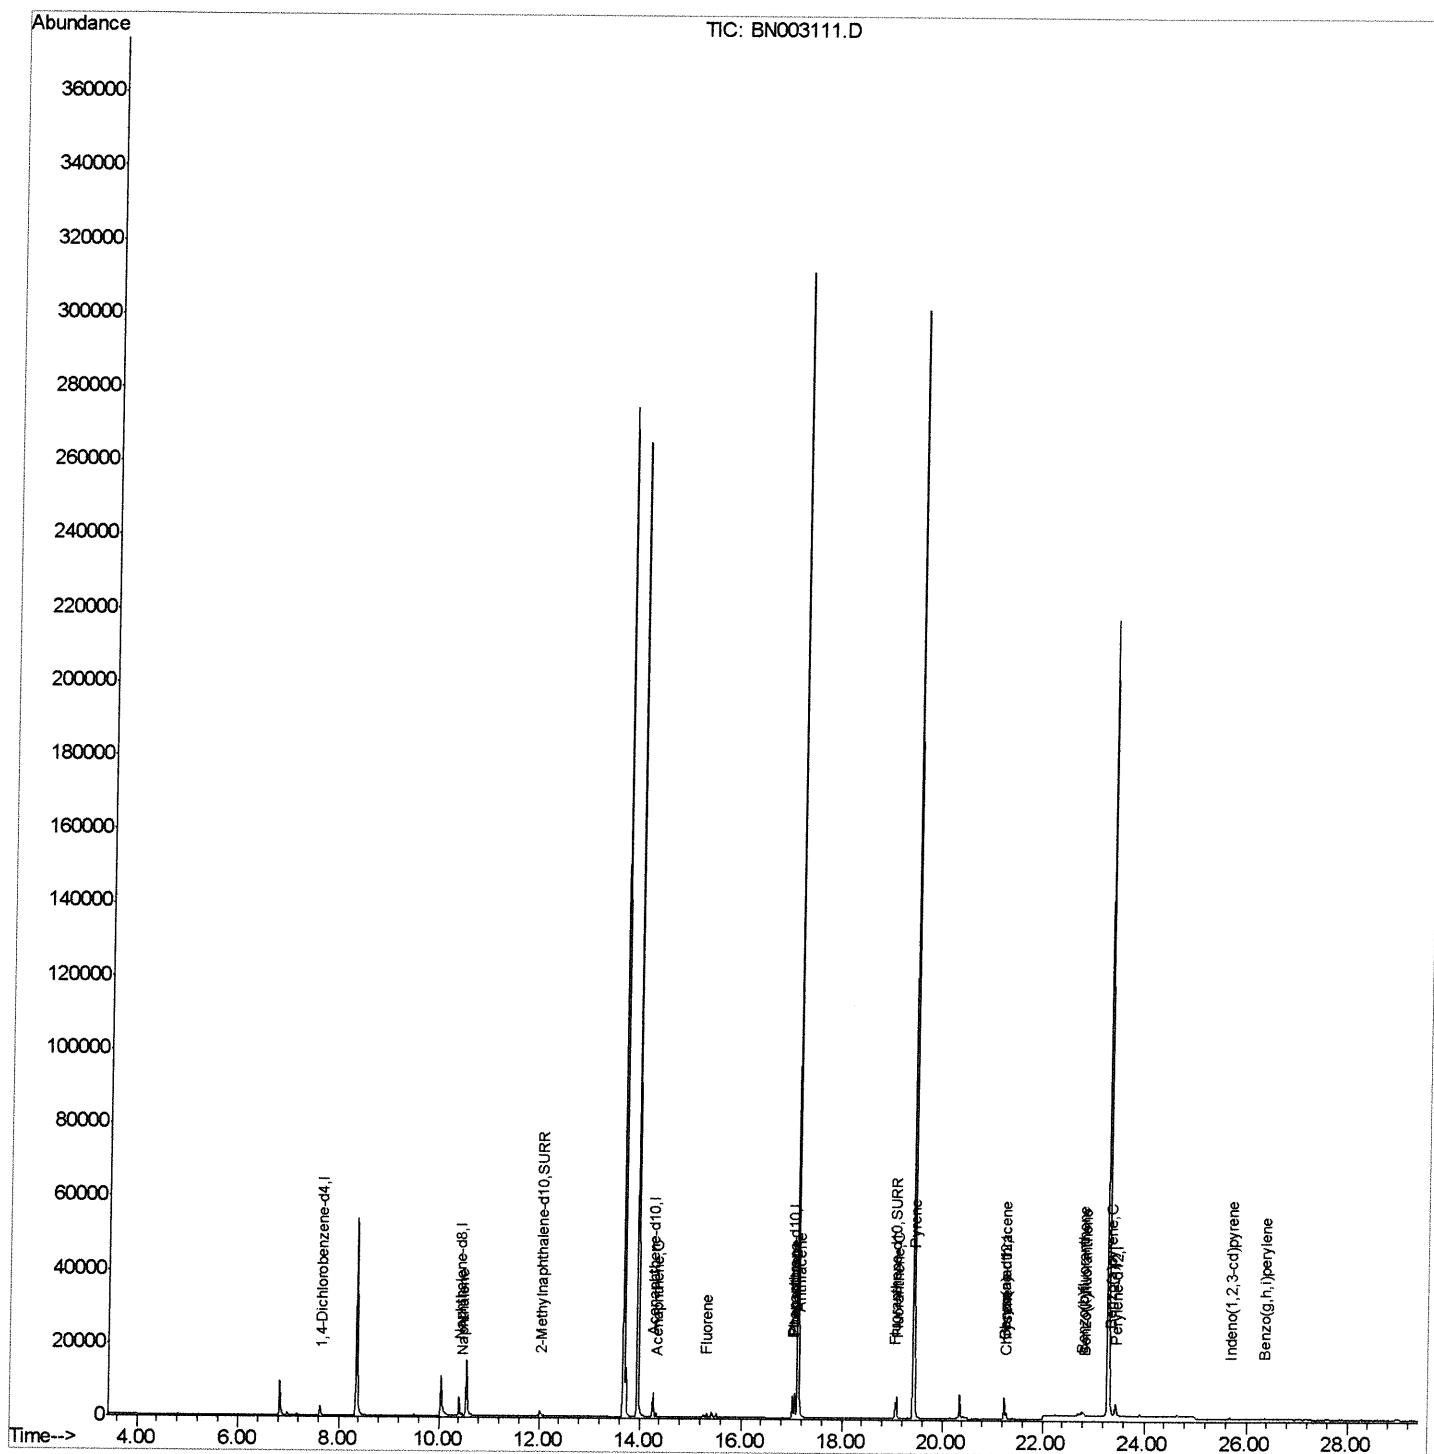

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 05:37:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

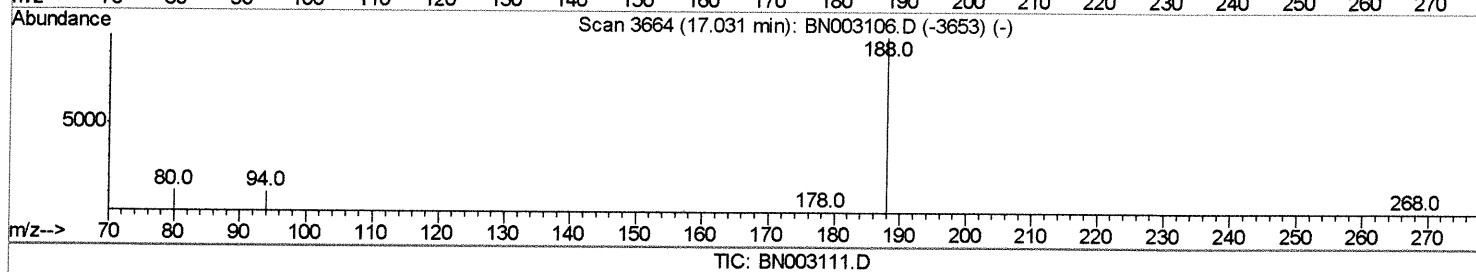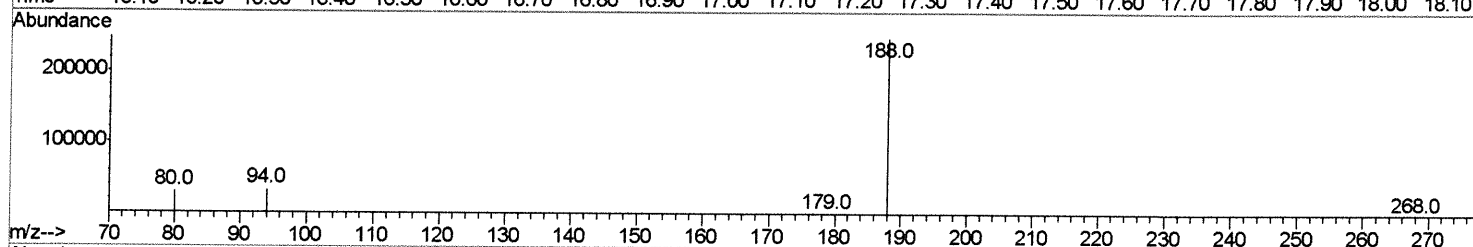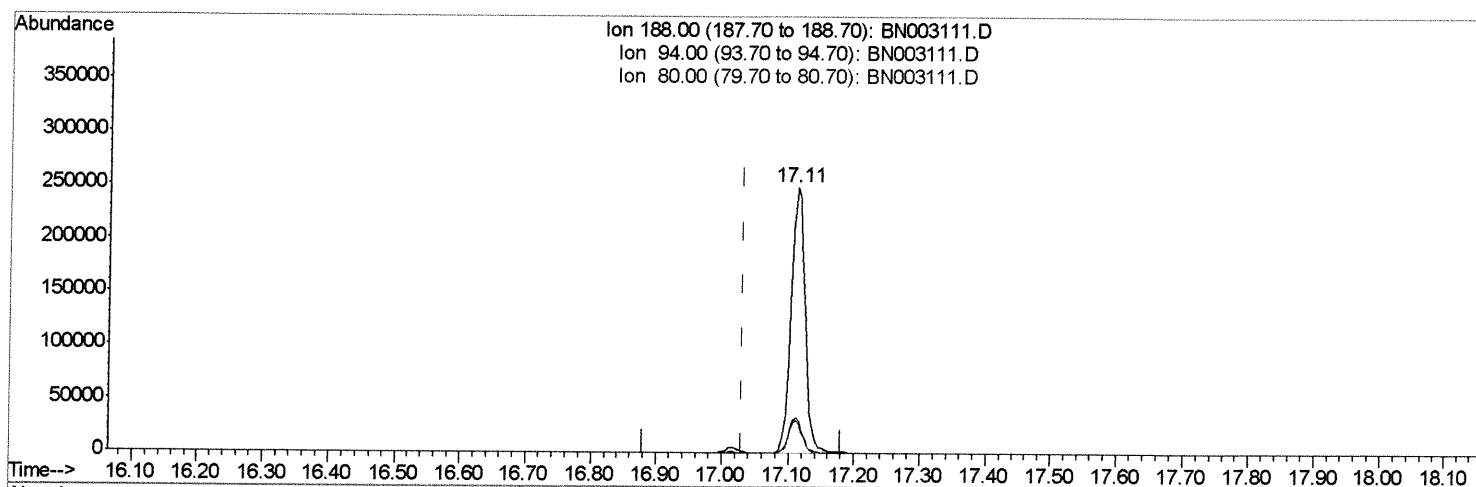

(10) Phenanthrene-d10 (I)

17.111min (+0.080) 0.40ng/ul

response 365331

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.26
80.00	12.70	12.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 05:37:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

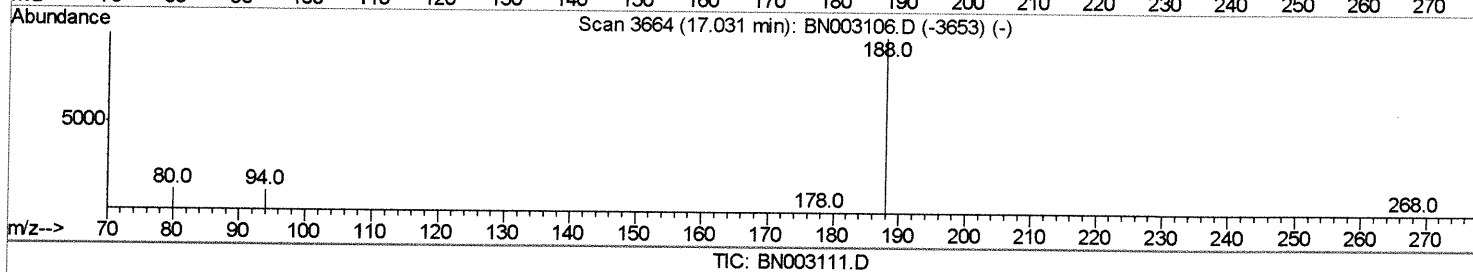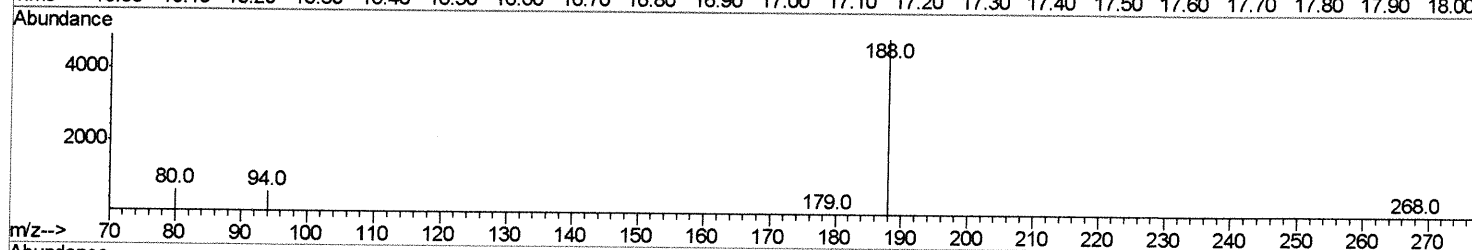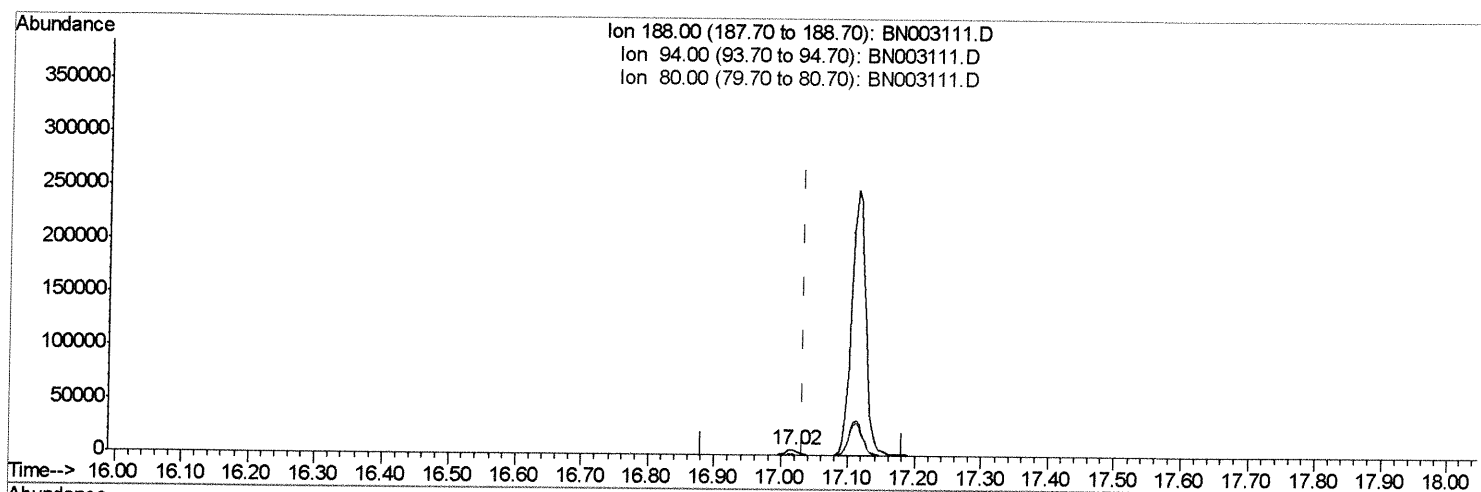

(10) Phenanthrene-d10 (I)

17.018min (-0.013) 0.40ng/ul m> SD

10/12/18

response 7121

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.05
80.00	12.70	12.77
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

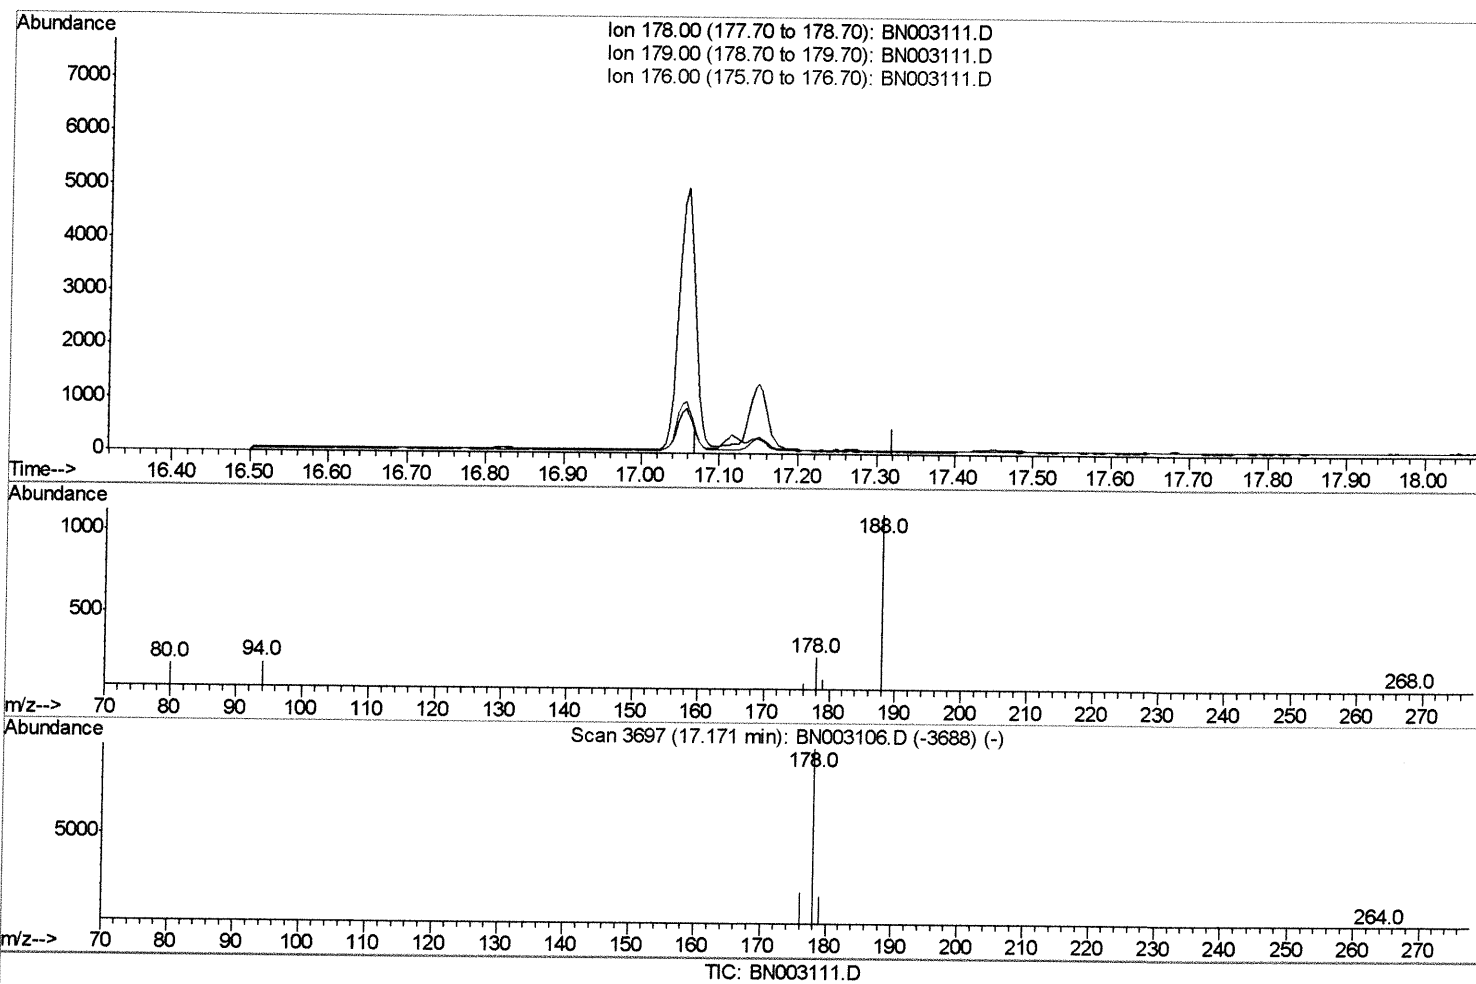

(13) Anthracene

17.171min (-17.171) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	16.30	0.00#
176.00	19.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

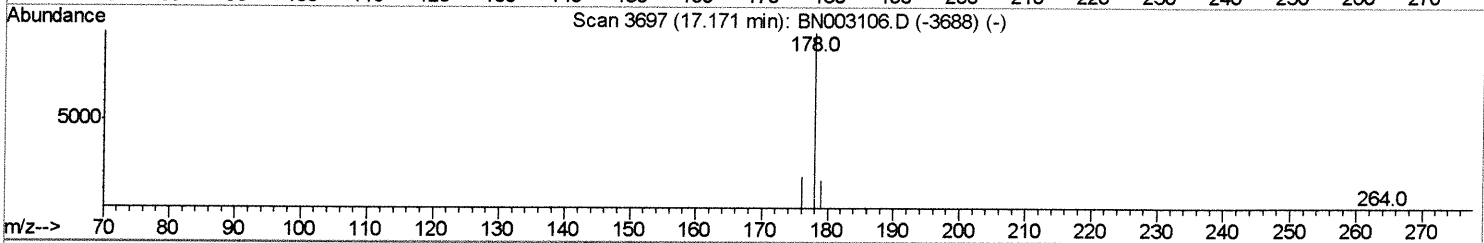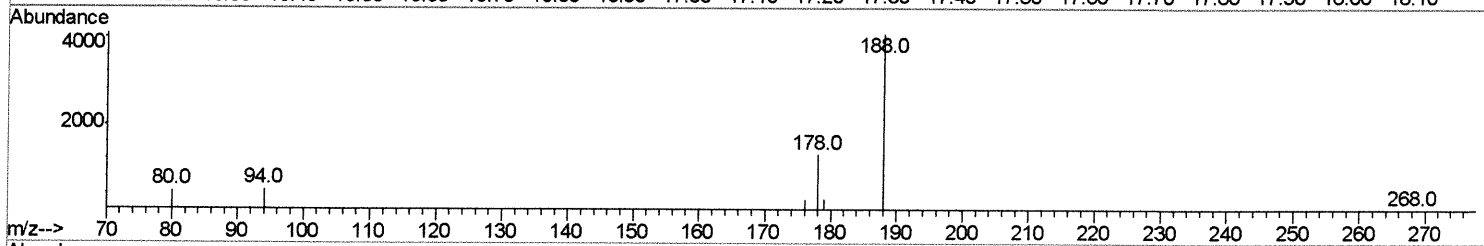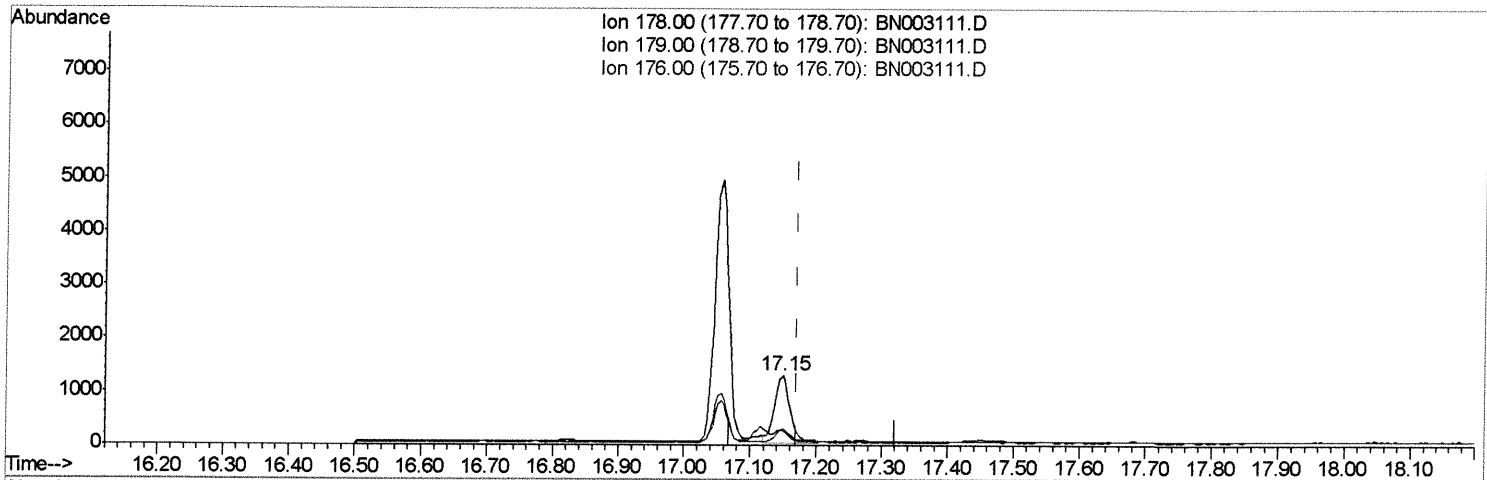

TIC: BN003111.D

(13) Anthracene

17.149min (-0.021) 0.11ng/ul m > SJ 10/12/18

response 2058

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	23.39#
176.00	19.10	21.18
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

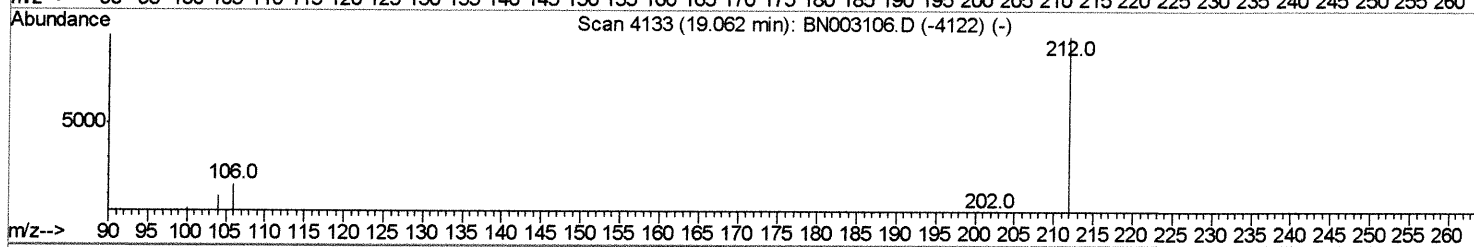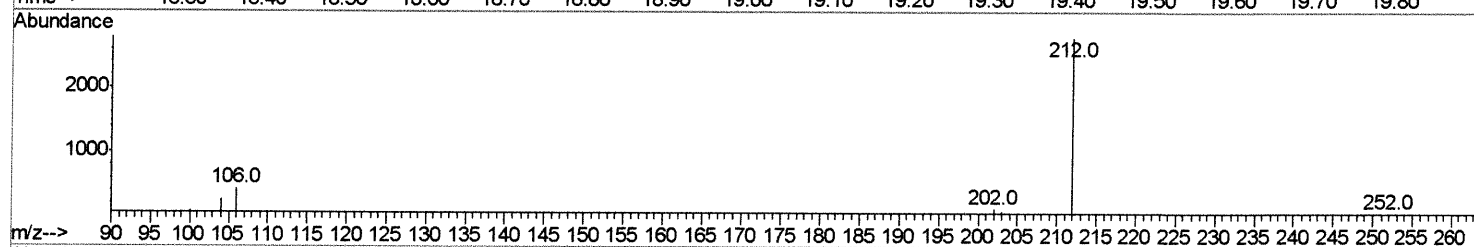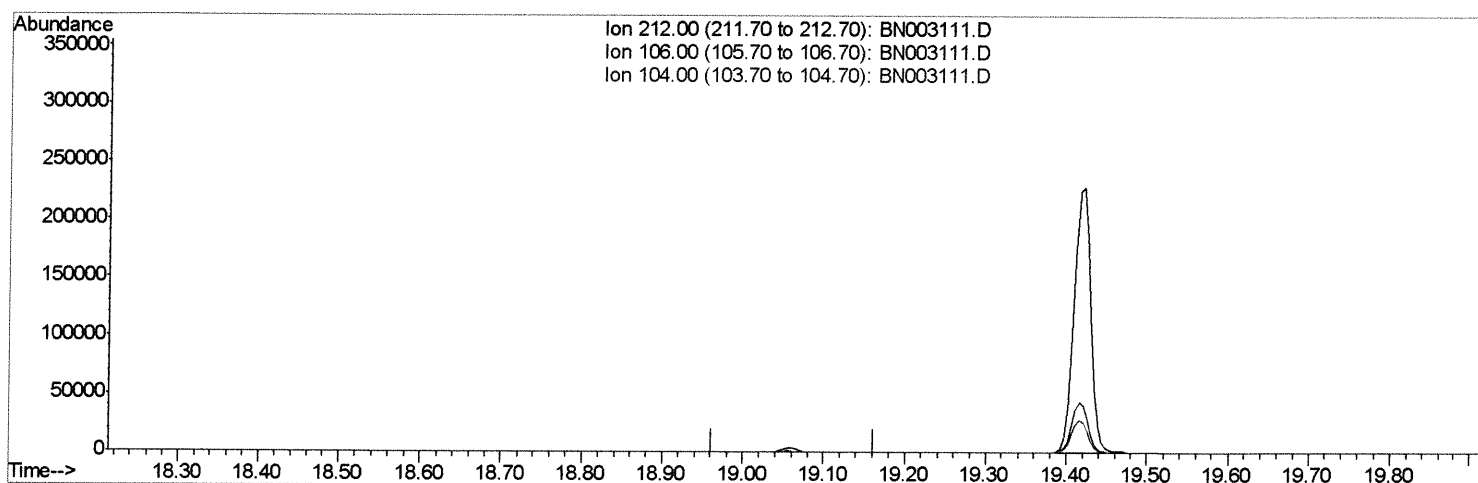

TIC: BN003111.D

(14) Fluoranthene-d10 (SURR)

19.062min (-19.062) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

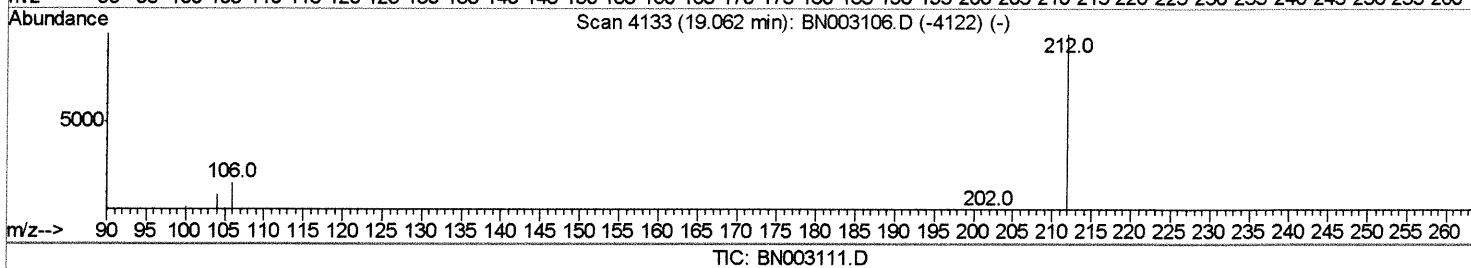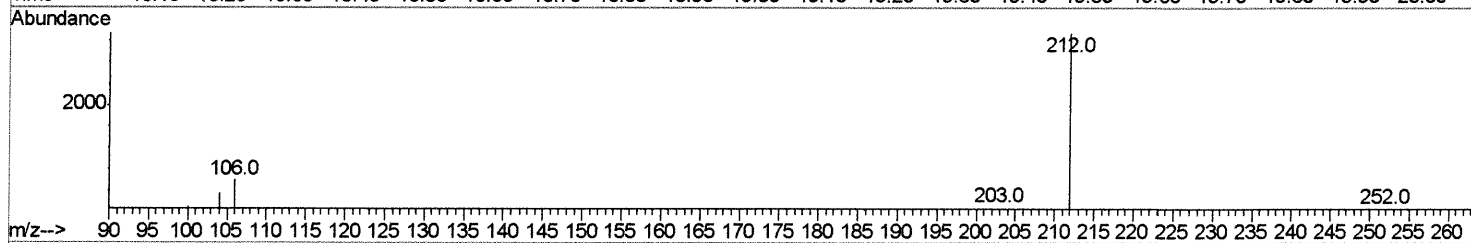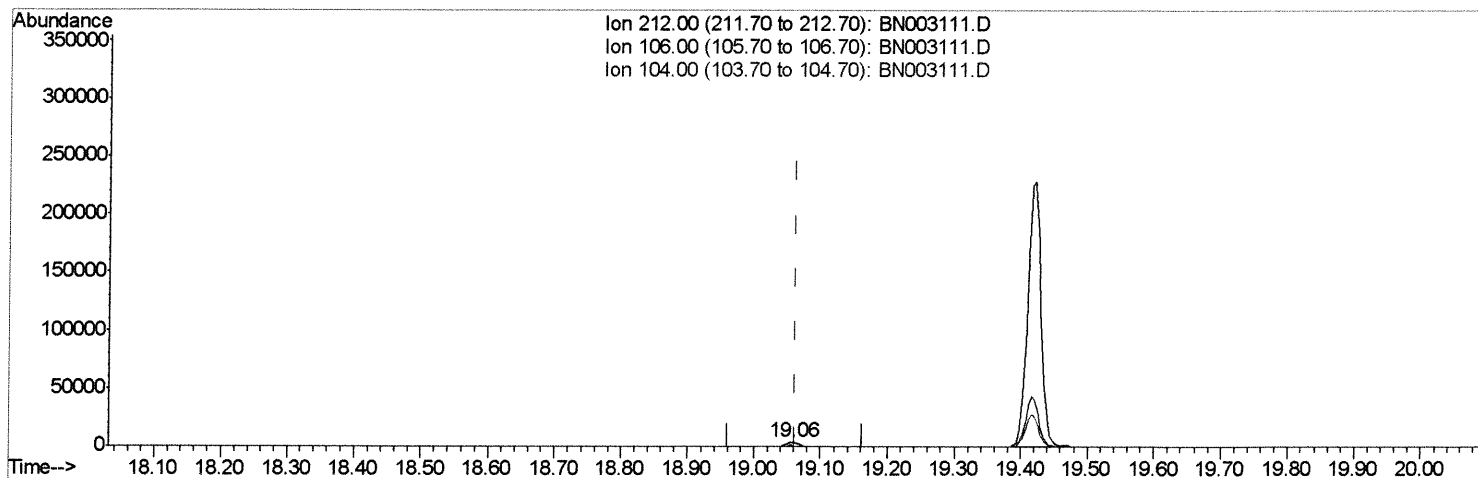

(14) Fluoranthene-d10 (SURR)

19.058min (-0.005) 0.23ng/ul m

> SJ 10/12/18

response 4719

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

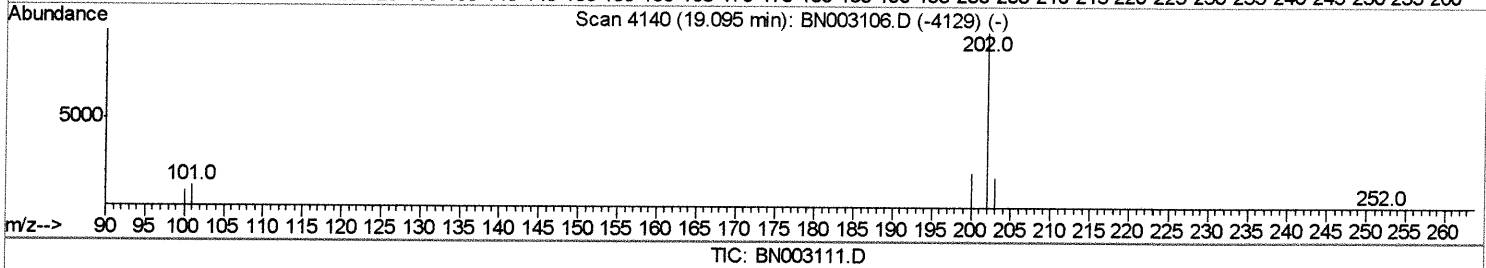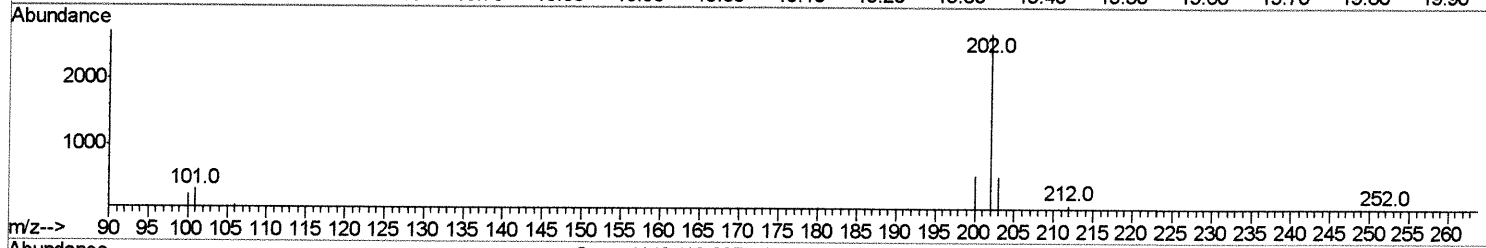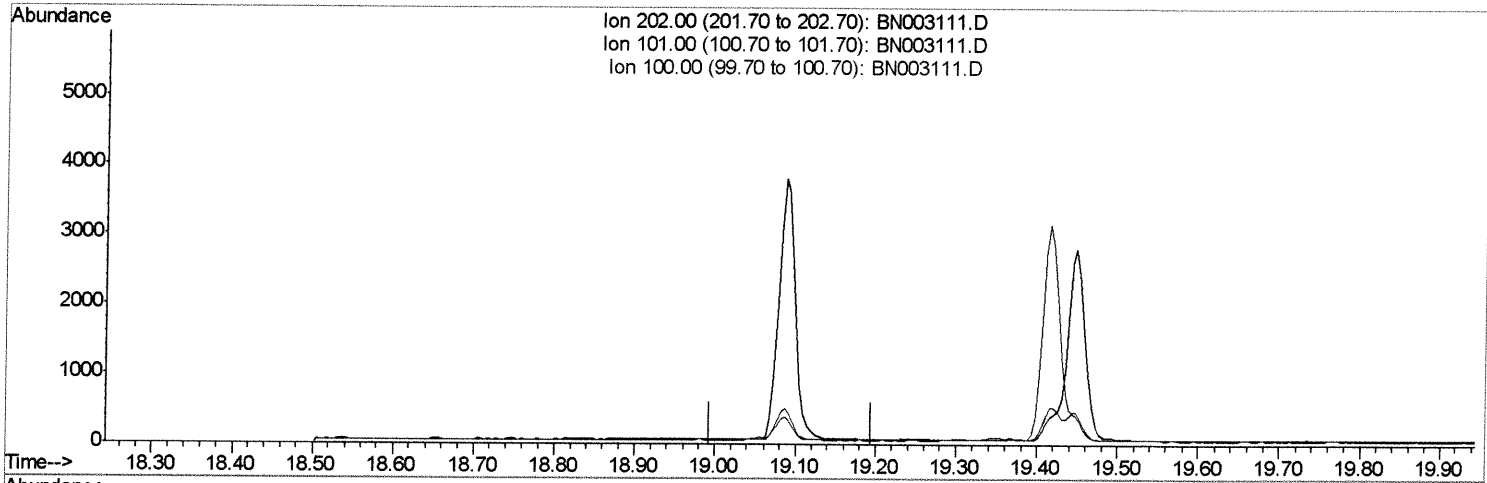

(15) Fluoranthene (C)

19.095min (-19.095) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

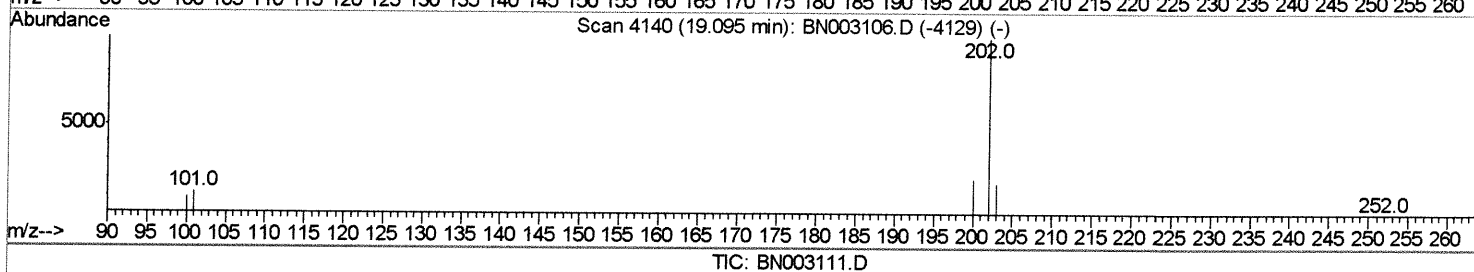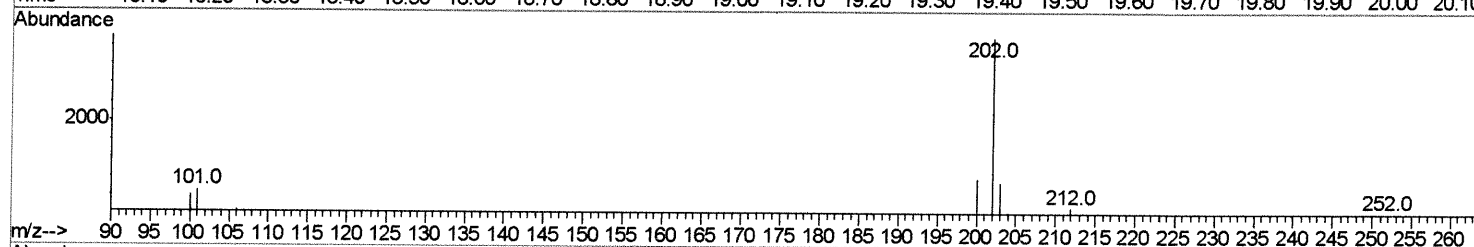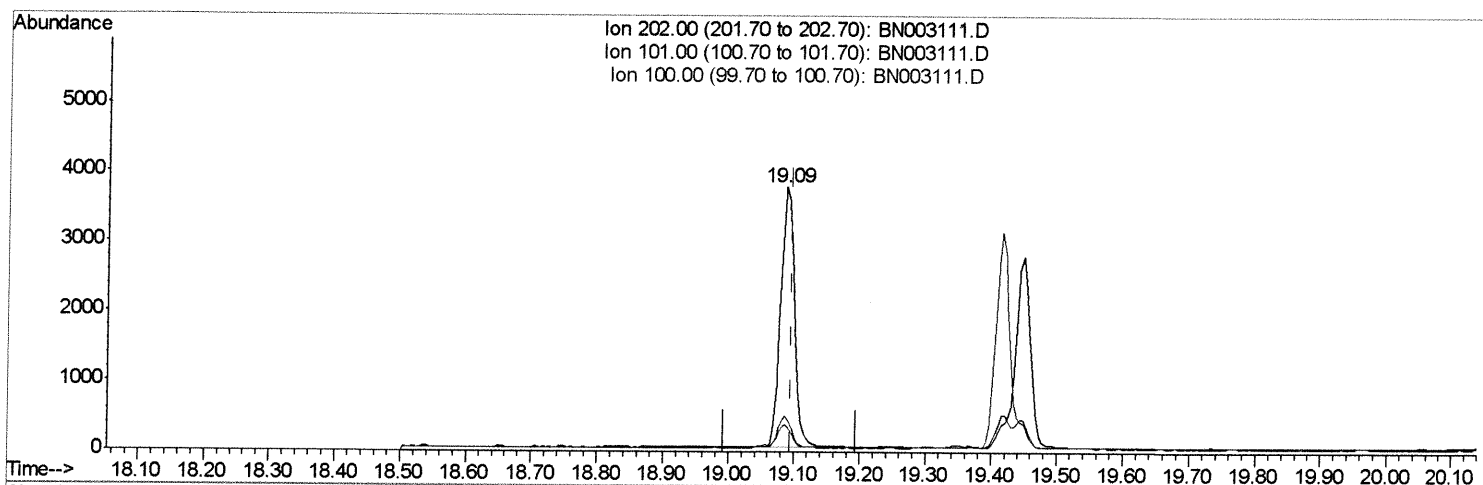

(15) Fluoranthene (C)

19.085min (-0.009) 0.23ng/ul m) SJ 10/12/18

response 5400

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.50
100.00	9.10	10.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

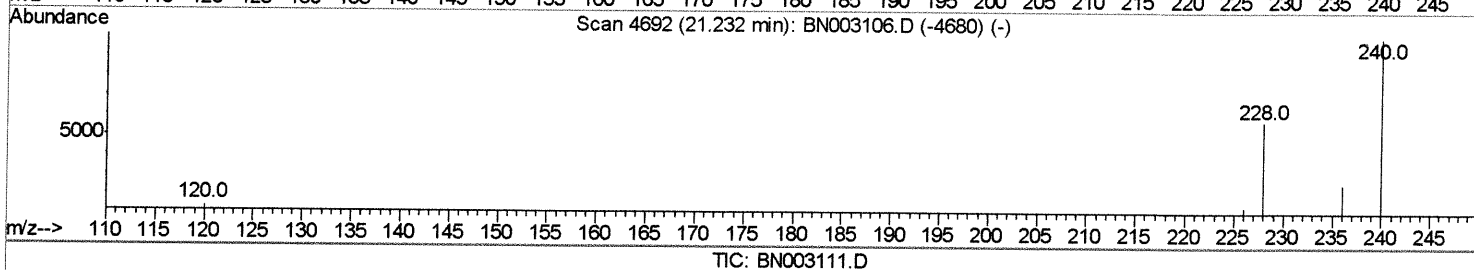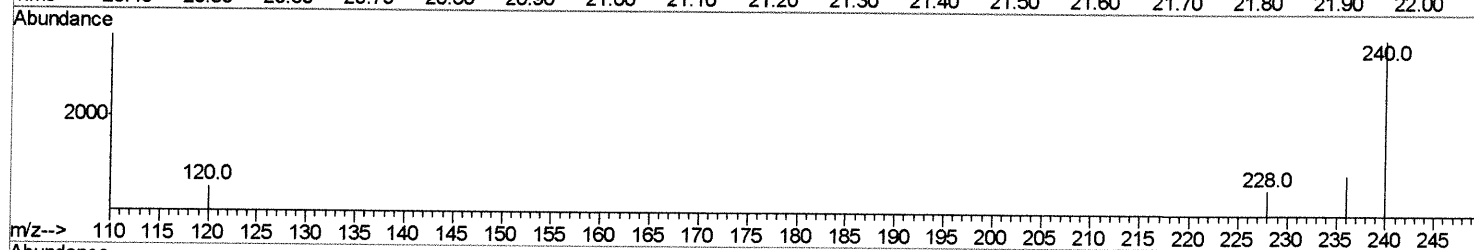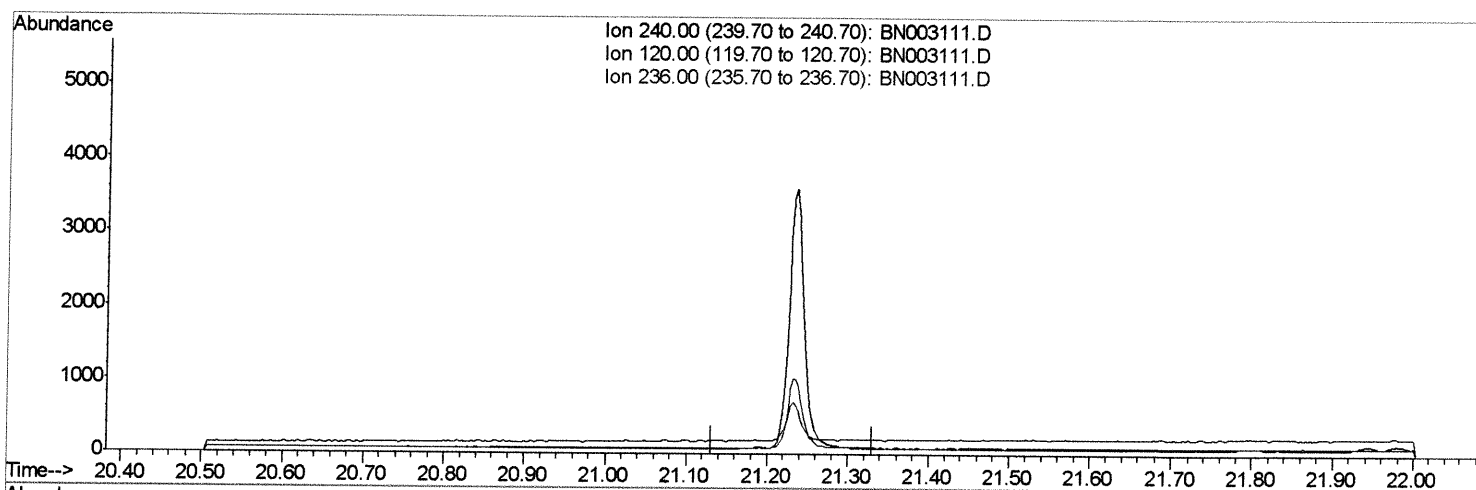

TIC: BN003111.D

(16) Chrysene-d12 (I)

21.232min (-21.232) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:02:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

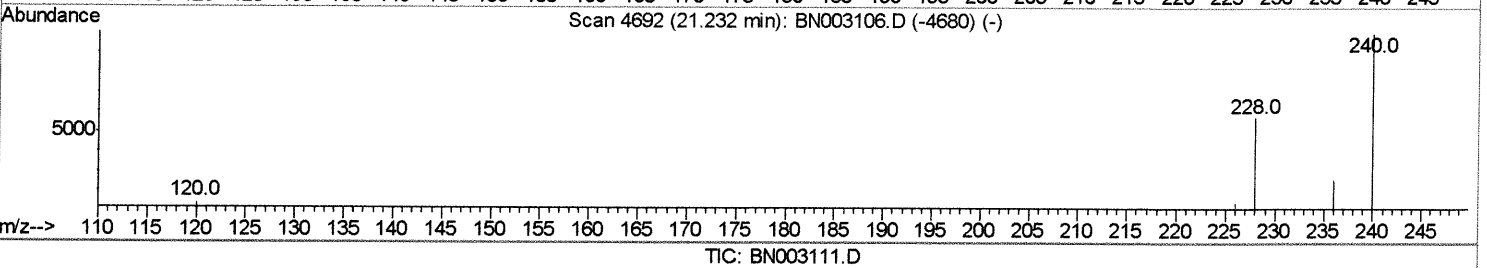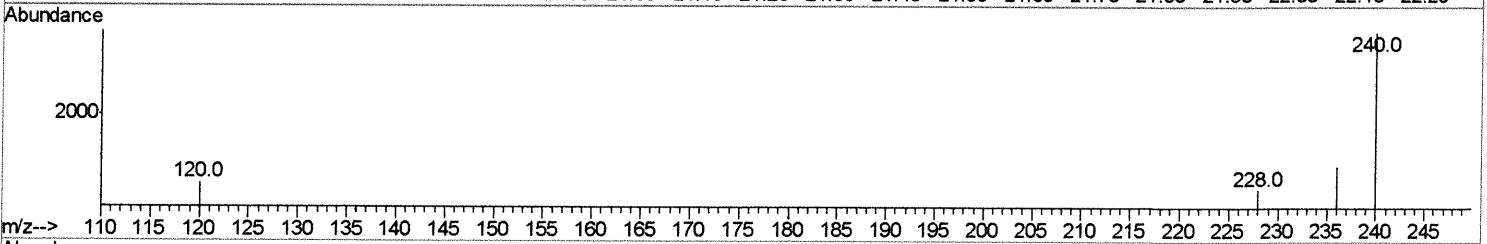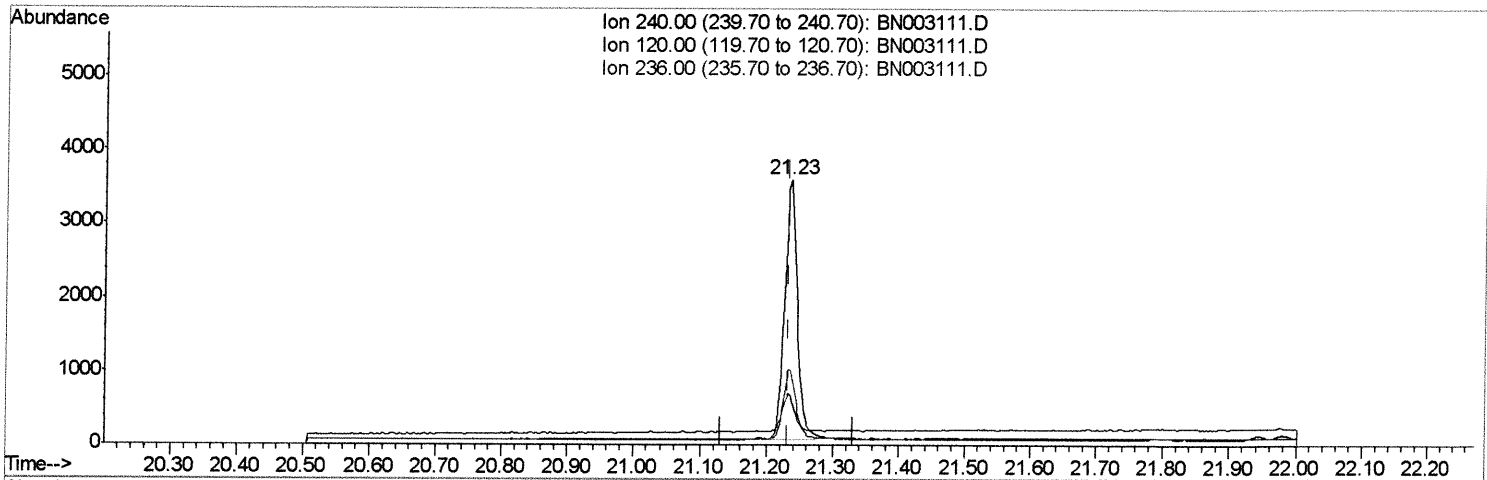

(16) Chrysene-d12 (I)

21.235min (+0.003) 0.40ng/ul m) SJ 10/12/18

response 4639

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	18.70
236.00	28.10	28.33
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:03:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

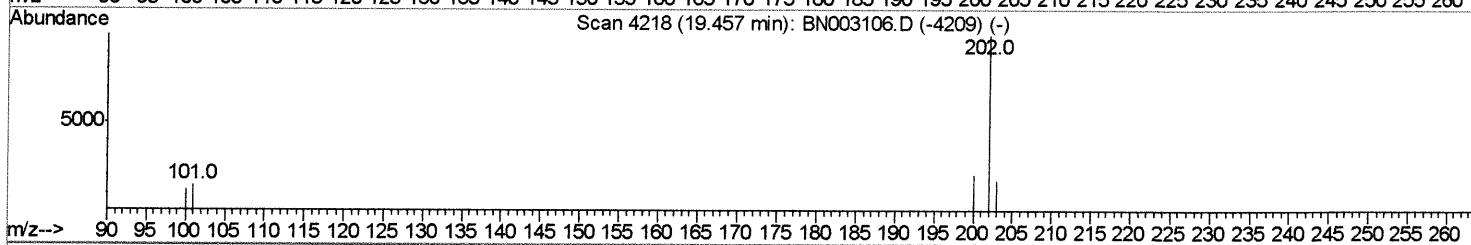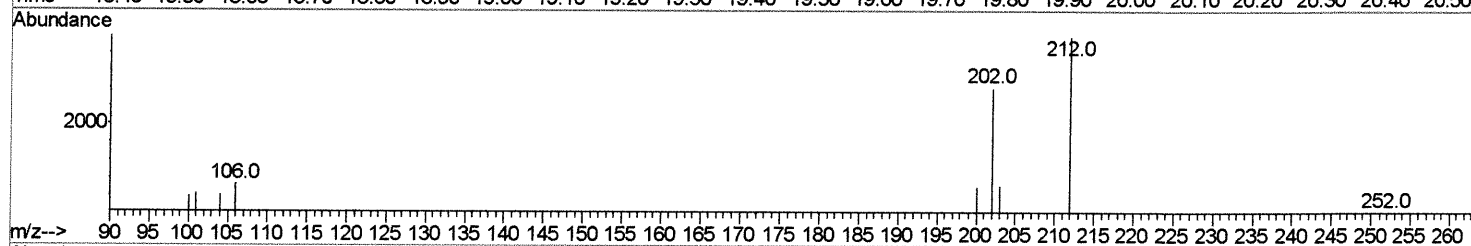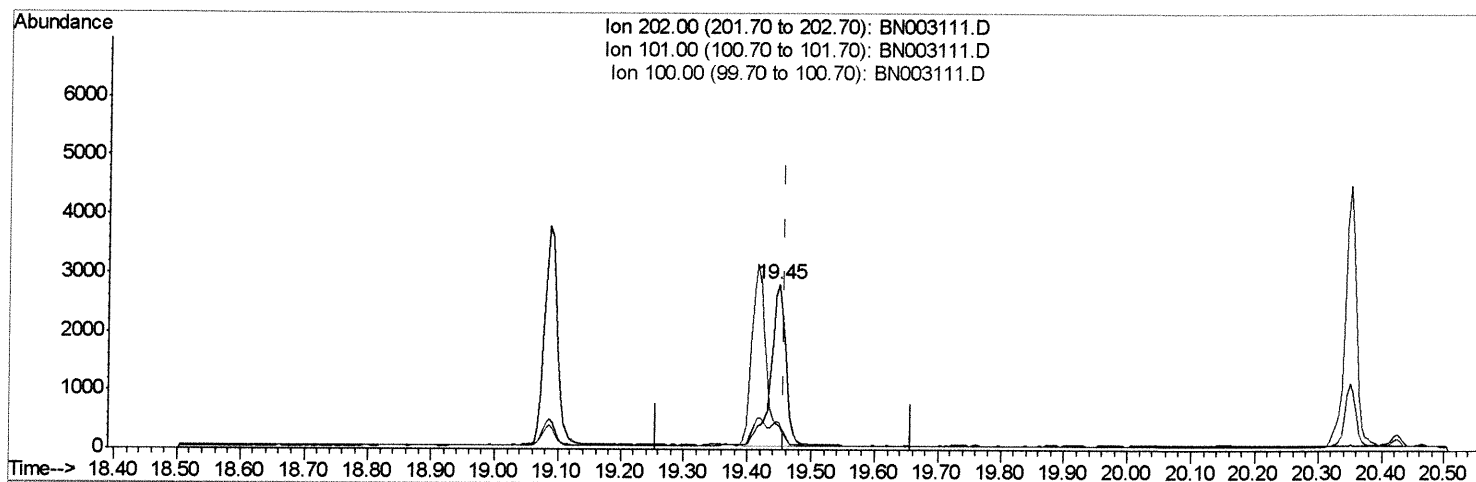

TIC: BN003111.D

(17) Pyrene

19.448min (-0.009) 0.25ng/ul

response 4512

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	16.63
100.00	12.40	14.61
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:03:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

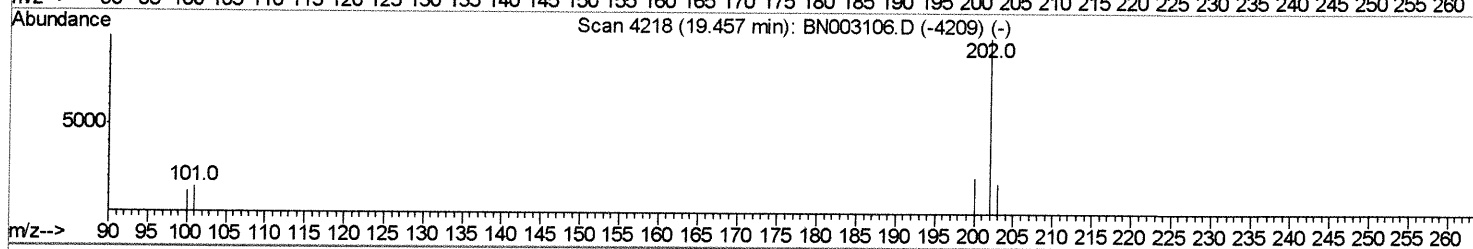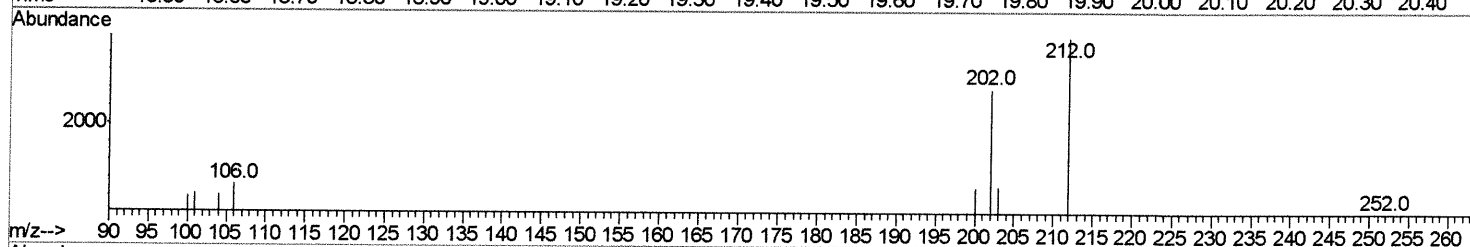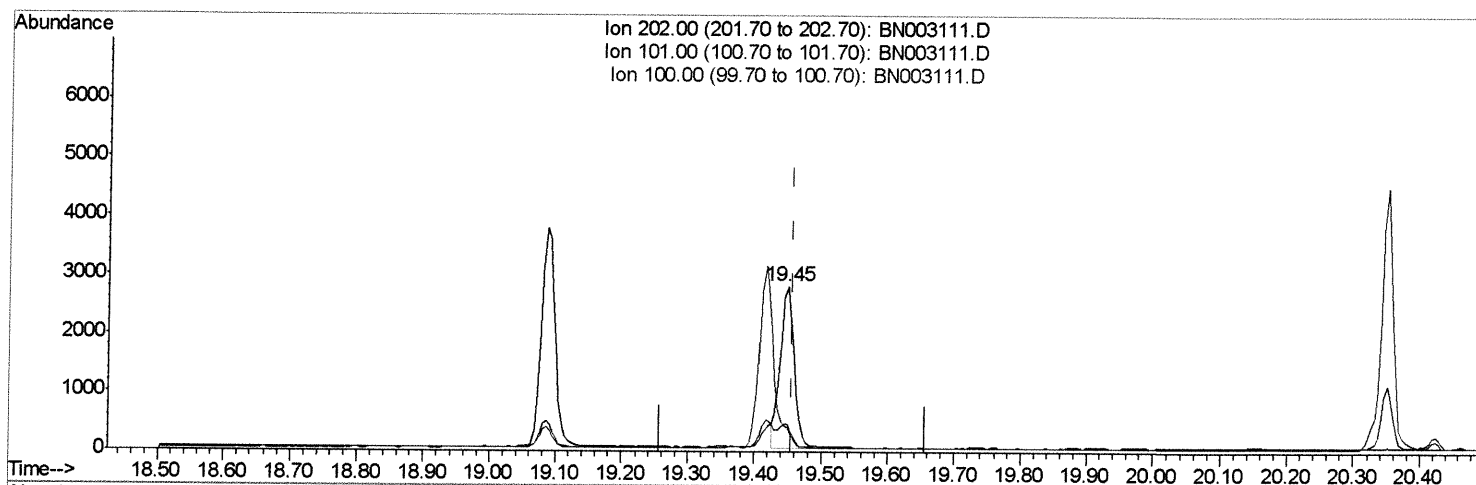

TIC: BN003111.D

(17) Pyrene

19.448min (-0.009) 0.23ng/ul m) SJ 10/12/18

response 4070

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	16.63
100.00	12.40	14.61
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:03:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

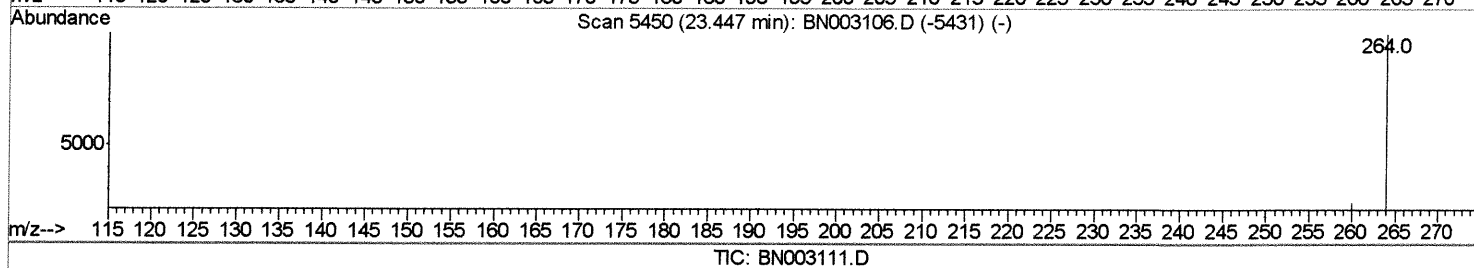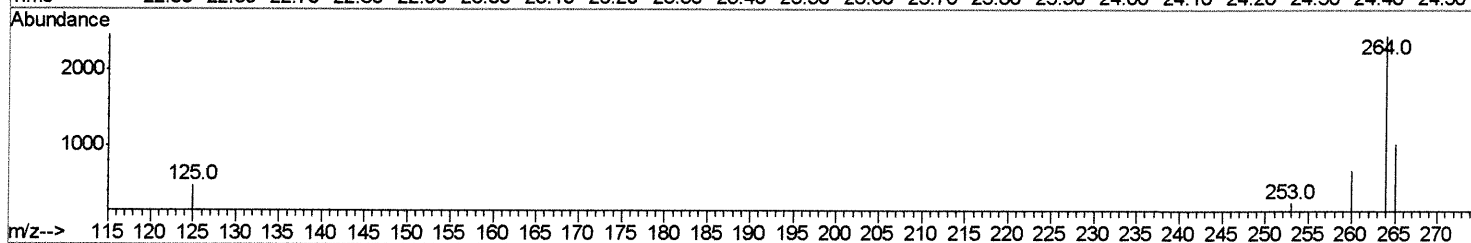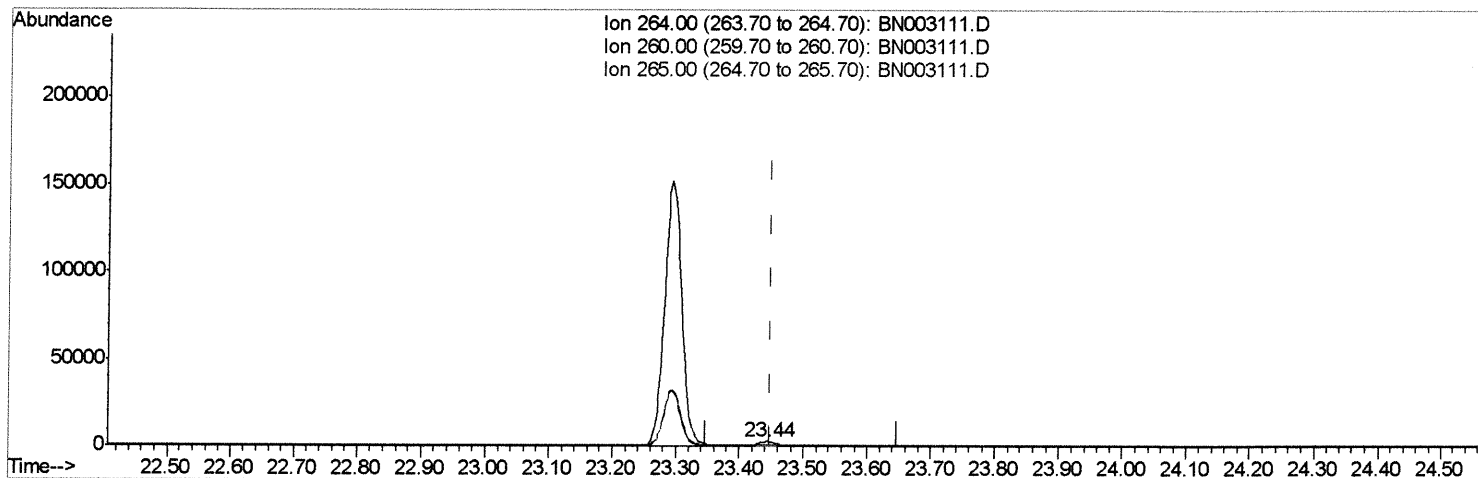

(20) Perylene-d12 (I)

23.444min (-0.003) 0.40ng/ul

response 5163

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	28.11
265.00	45.40	42.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:03:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

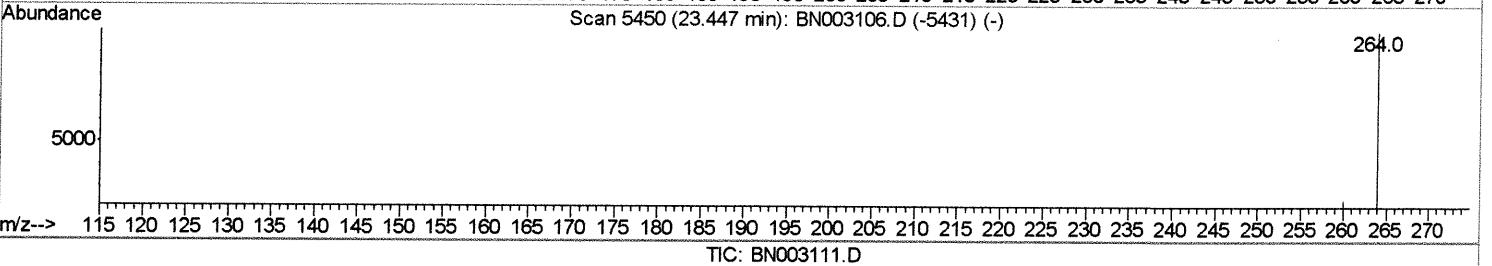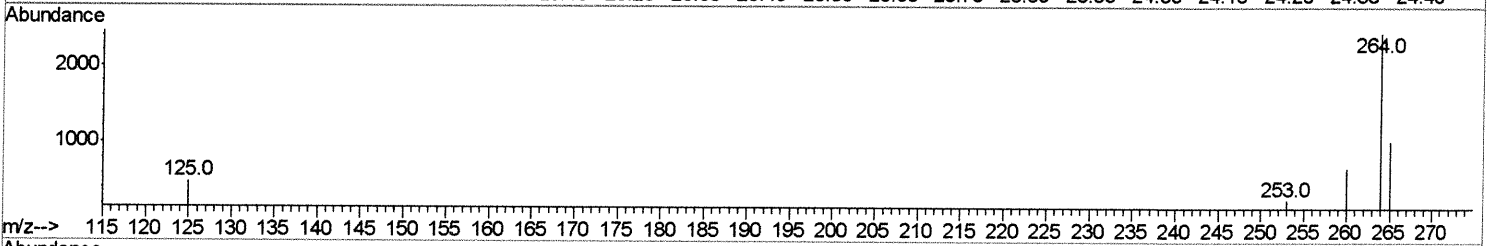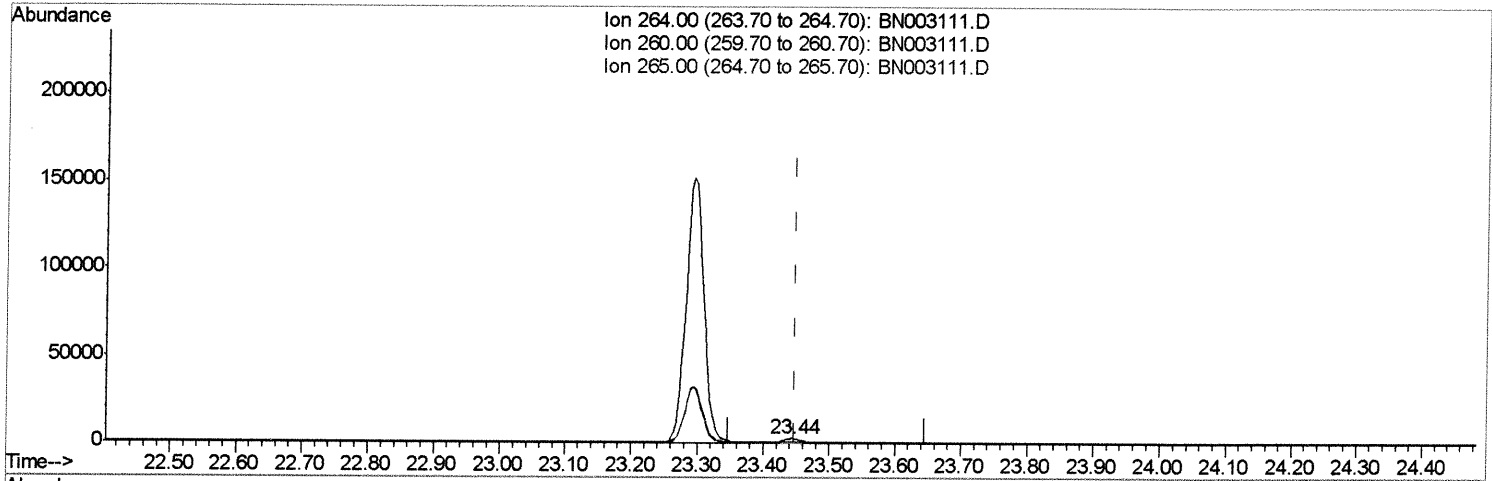

(20) Perylene-d12 (I)

23.444min (-0.003) 0.40ng/ul m > SJ 10/12/18

response 4397

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	28.11
265.00	45.40	42.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:04:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

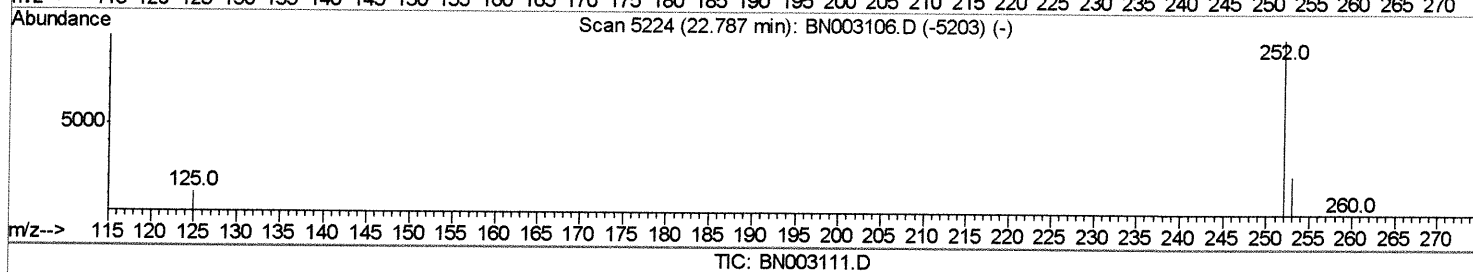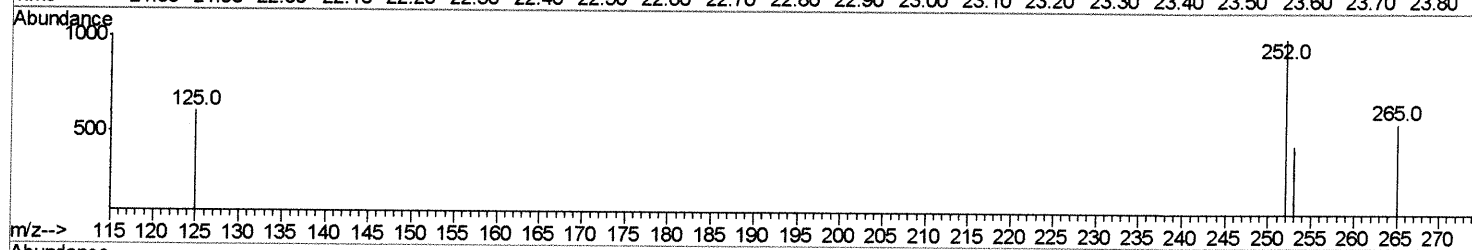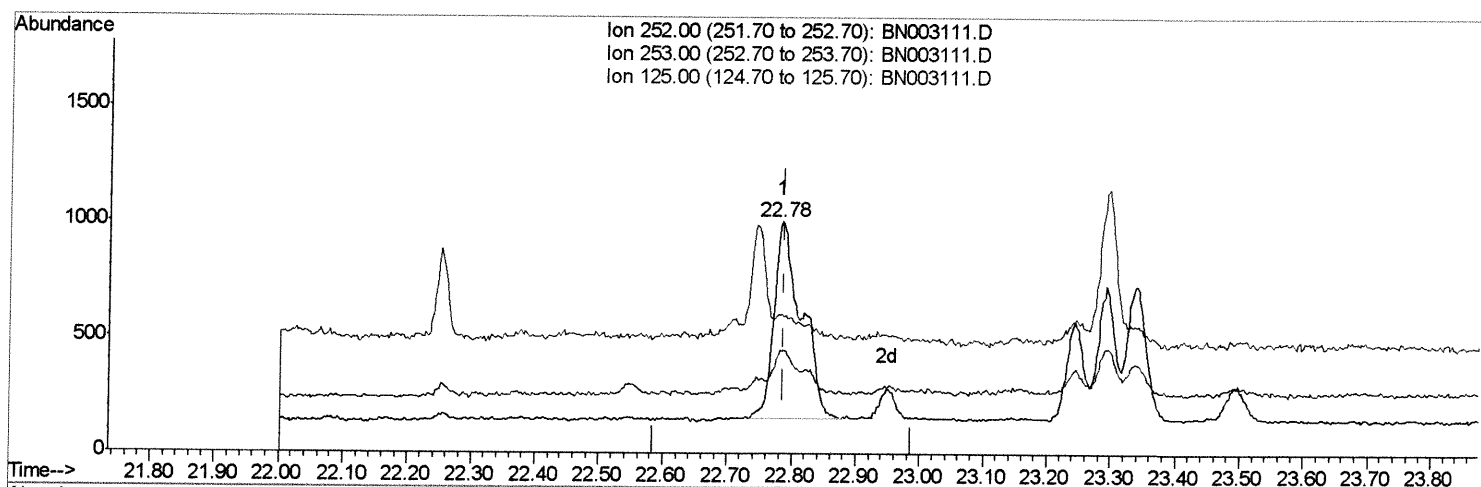

(21) Benzo(b)fluoranthene

22.784min (-0.003) 0.16ng/ul

response 2553

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	44.37
125.00	17.10	60.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:04:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

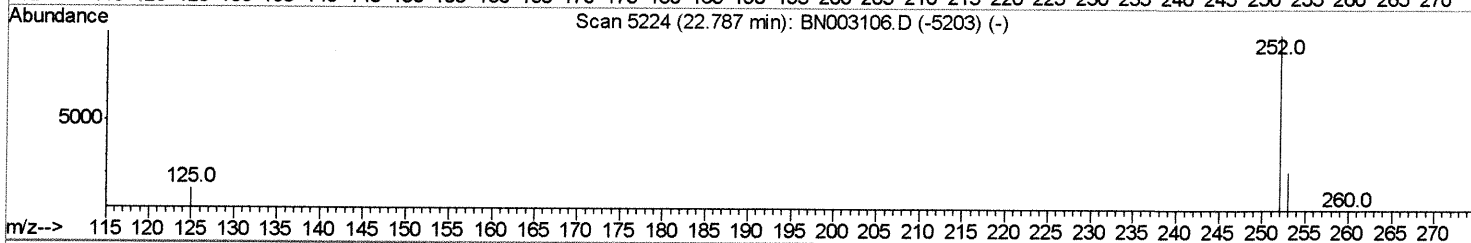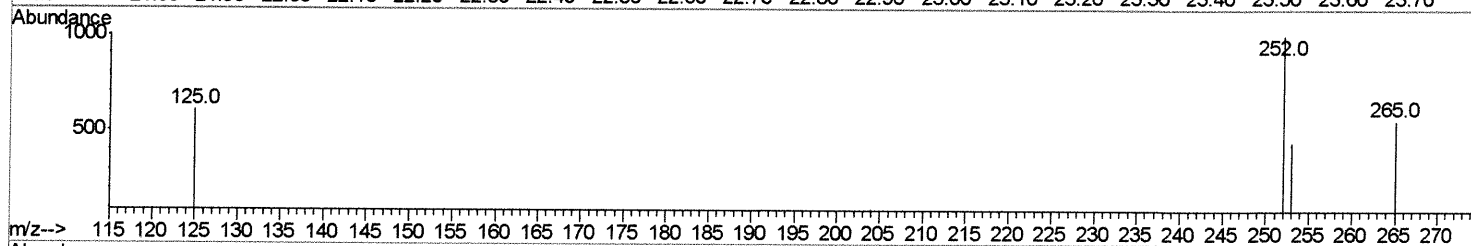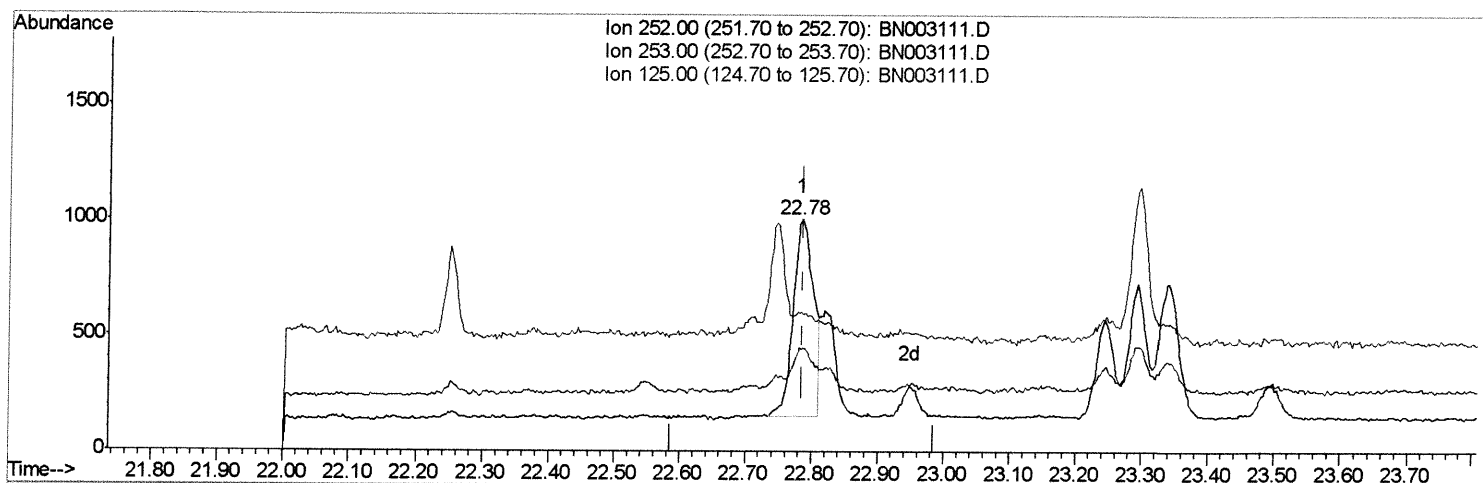

TIC: BN003111.D

(21) Benzo(b)fluoranthene

22.784min (-0.003) 0.12ng/ul m) SJ 10/12/18

response 1834

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	44.37
125.00	17.10	60.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z00

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:04:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

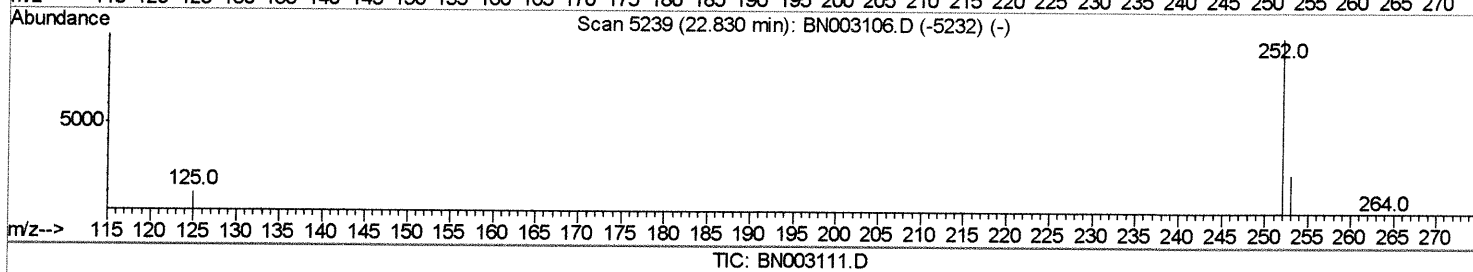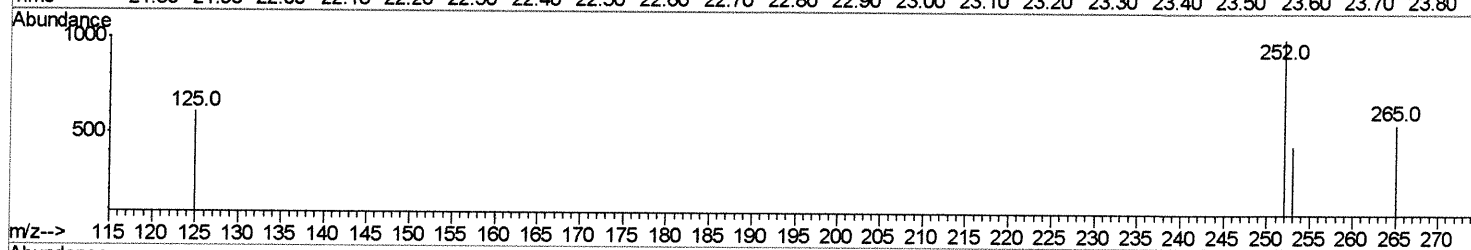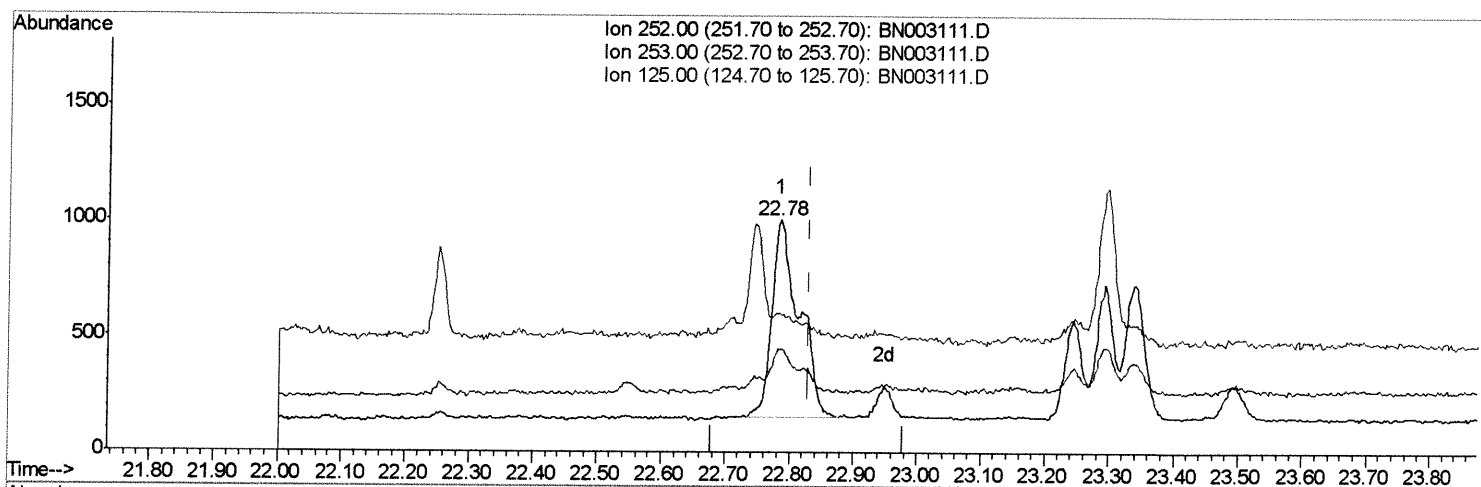

(22) Benzo(k)fluoranthene

22.784min (-0.047) 0.16ng/ul

response 2553

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	44.37#
125.00	17.60	60.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:04:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

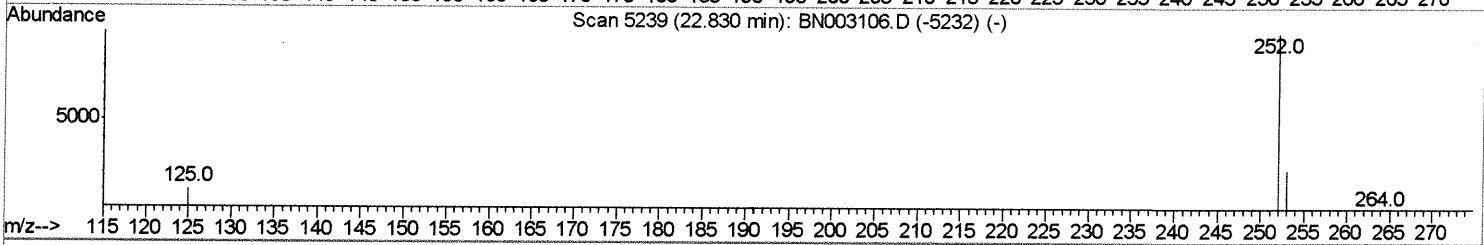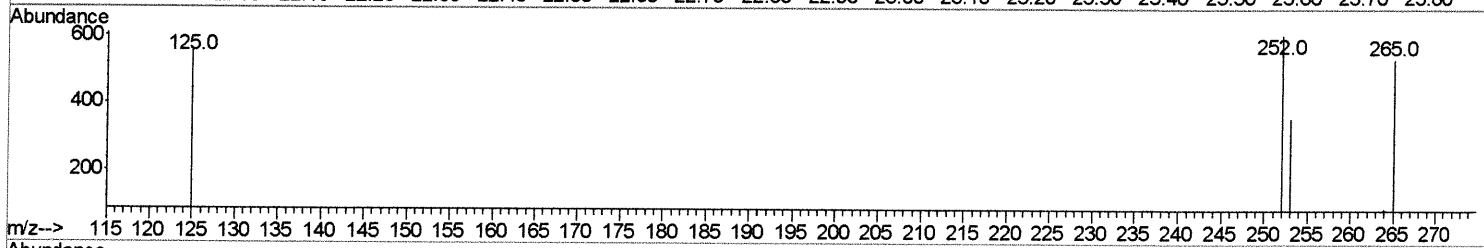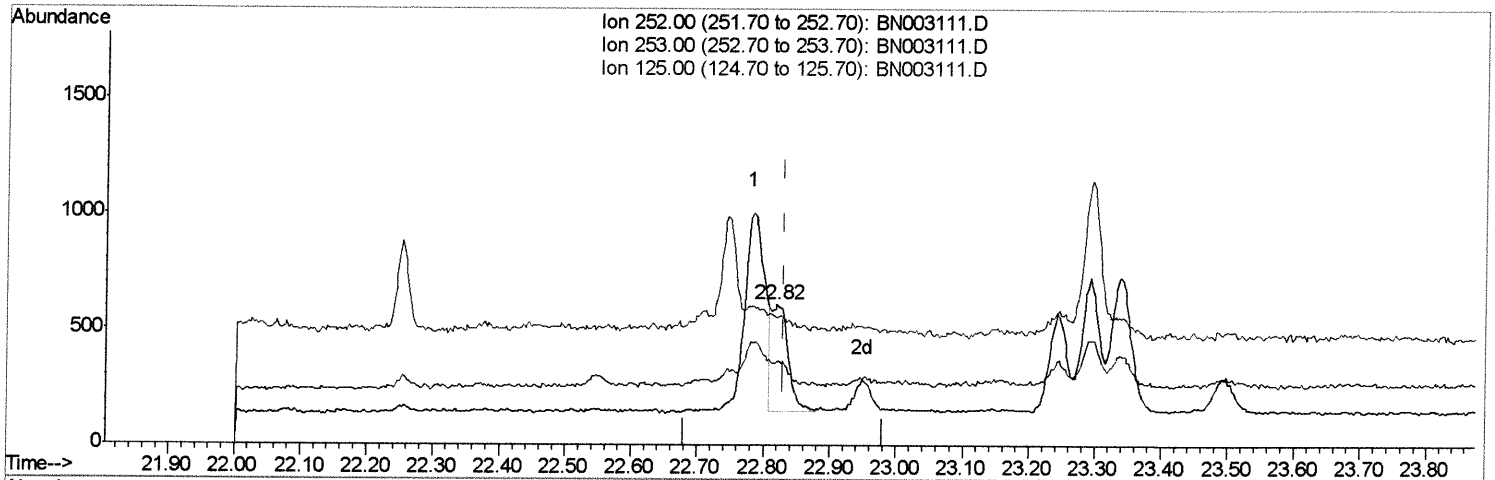

TIC: BN003111.D

(22) Benzo(k)fluoranthene

22.819min (-0.012) 0.05ng/ul m > 50 10/12/18

response 820

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	59.05#
125.00	17.60	90.95#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003111.D
 Acq On : 11 Oct 2018 20:01
 Operator : MJ/SJ
 Sample : J5368-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z00

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:20 PM

Quant Time: Oct 12 06:38:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1649	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6857	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.26	164	3681	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	7121m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.23	240	4639m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4397m	0.40	ng/ul	0.00

SJ 10/12/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.01	152	2531	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	4719m	0.23	ng/ul	0.00

SJ 10/12/18

Target Compounds

					Ovalue	
3) Naphthalene	10.44	128	803	0.046	ng/ul#	81
8) Acenaphthene	14.32	153	627	0.049	ng/ul	94
9) Fluorene	15.32	166	896	0.061	ng/ul#	96
12) Phenanthrene	17.06	178	7202	0.363	ng/ul	99
13) Anthracene	17.15	178	2058m	0.110	ng/ul	
15) Fluoranthene	19.09	202	5400m	0.232	ng/ul	
17) Pyrene	19.45	202	4070m	0.226	ng/ul	
18) Benzo(a)anthracene	21.22	228	1597	0.107	ng/ul#	89
19) Chrysene	21.27	228	1609	0.106	ng/ul#	87
21) Benzo(b)fluoranthene	22.78	252	1834m	0.116	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	820m	0.050	ng/ul	
23) Benzo(a)pyrene	23.34	252	1190	0.084	ng/ul#	24
24) Indeno(1,2,3-cd)pyrene	25.69	276	814	0.050	ng/ul#	94
26) Benzo(a,h,i)perylene	26.36	276	773	0.056	ng/ul#	36

SJ 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed