


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:47:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

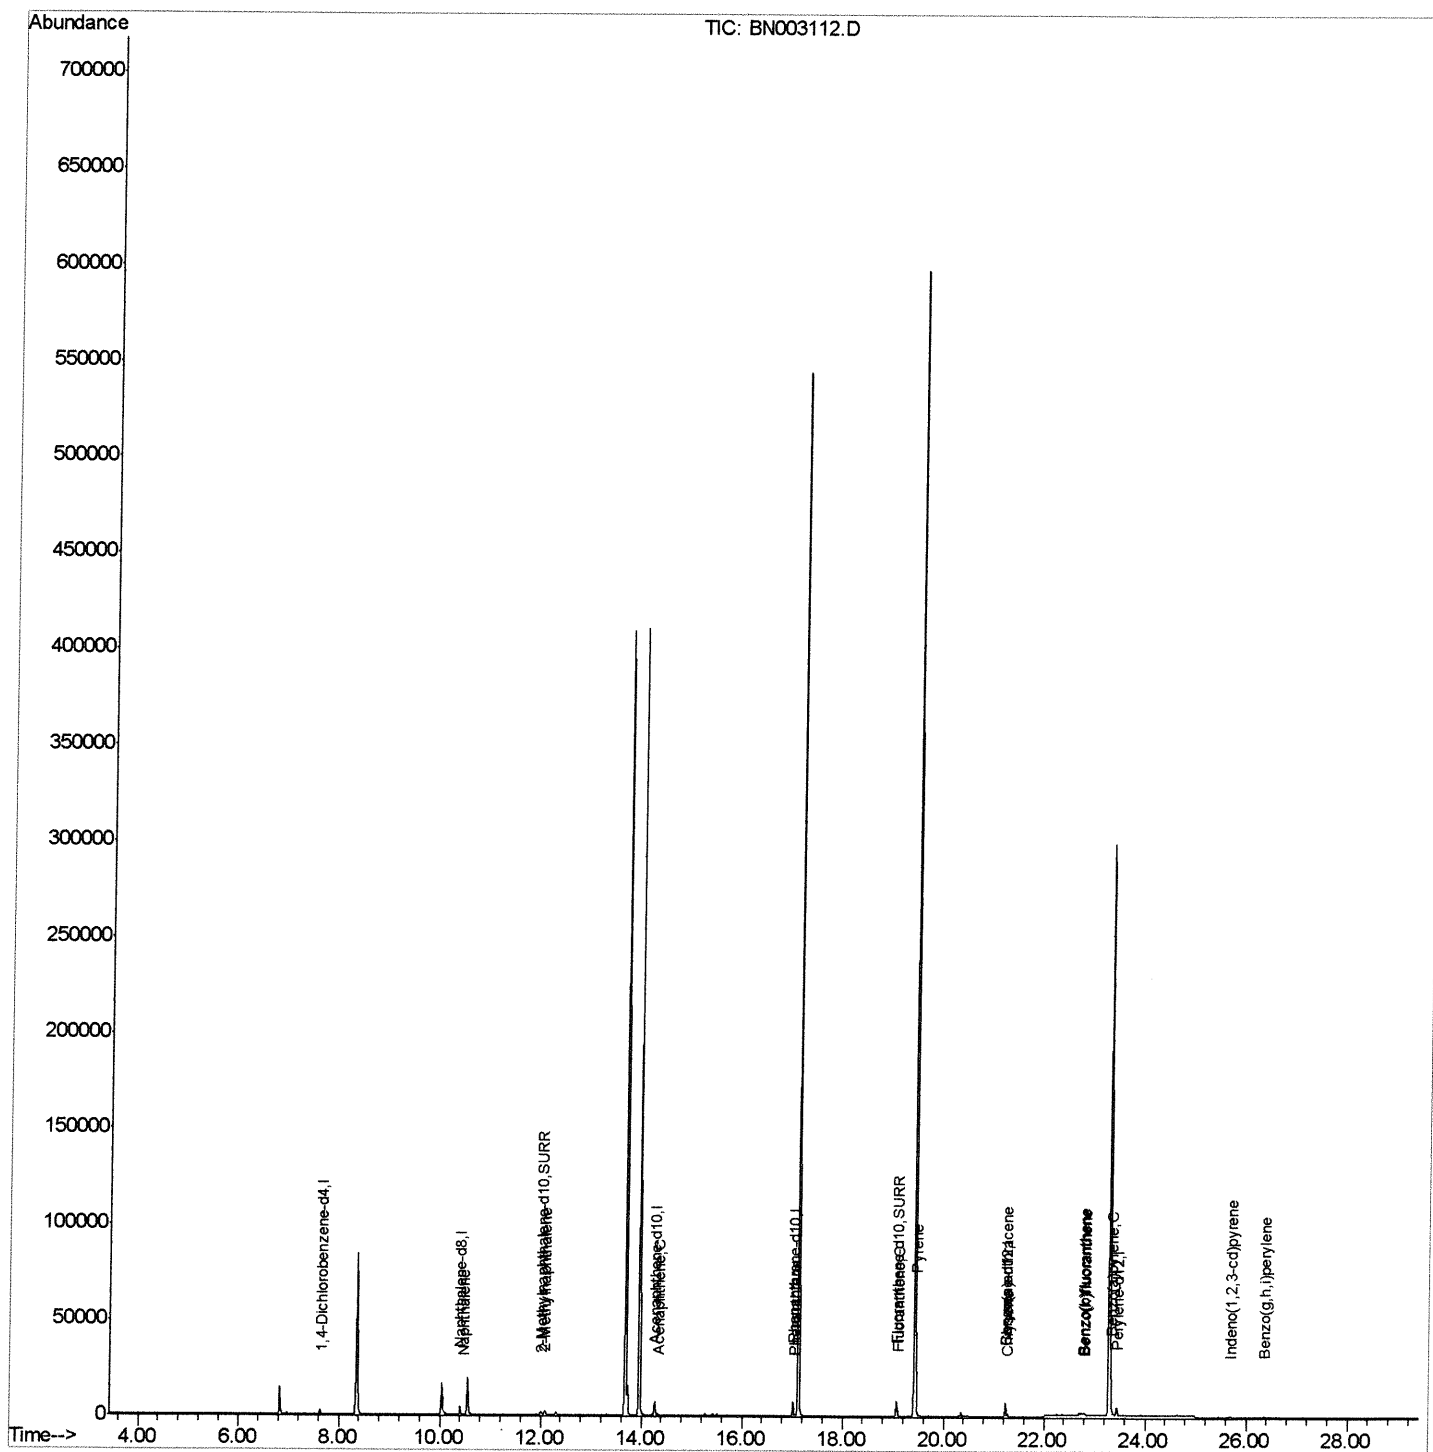

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:44:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

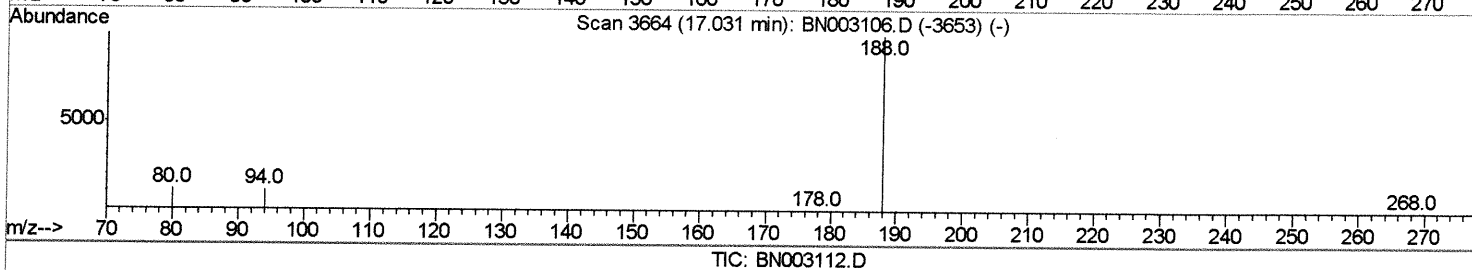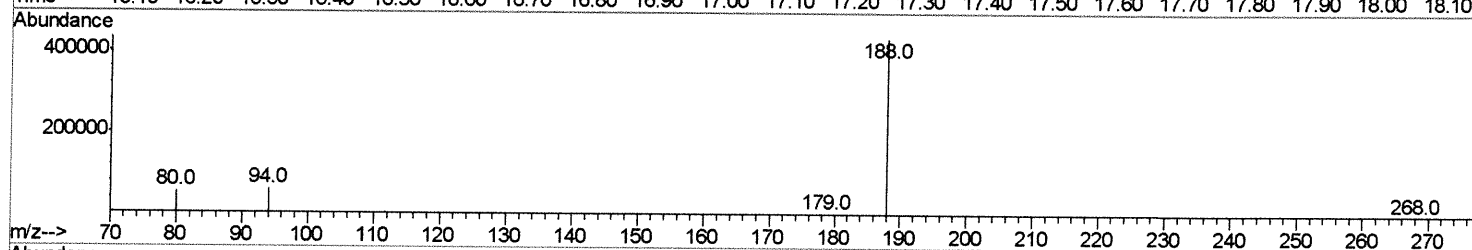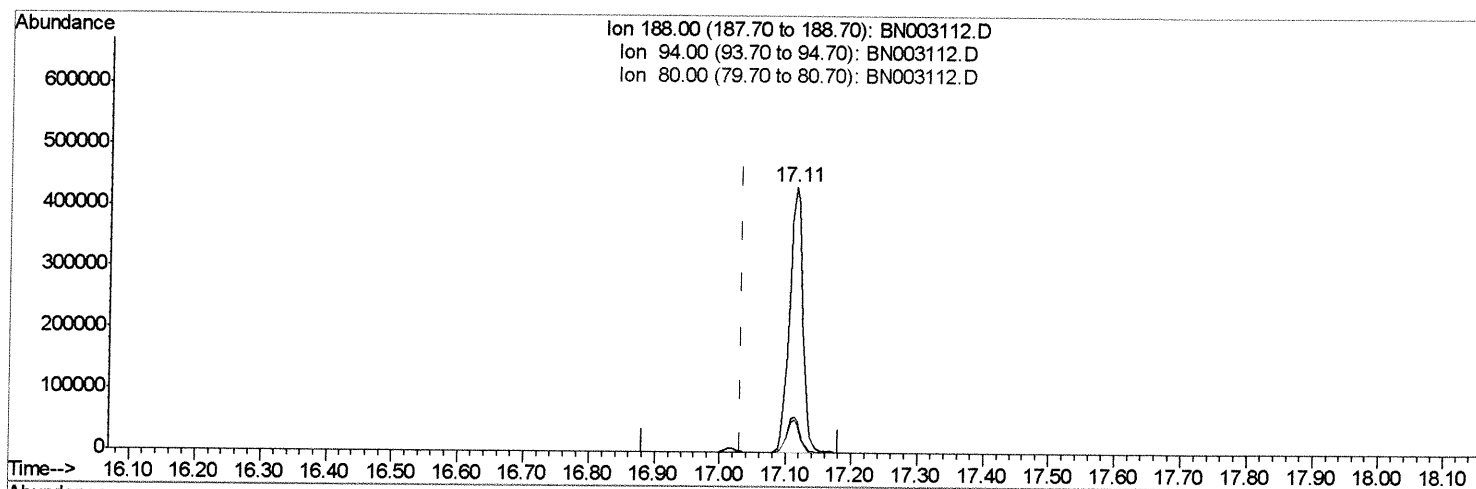

(10) Phenanthrene-d10 (I)

17.112min (+0.080) 0.40ng/ul

response 628604

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.43
80.00	12.70	12.25
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:44:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

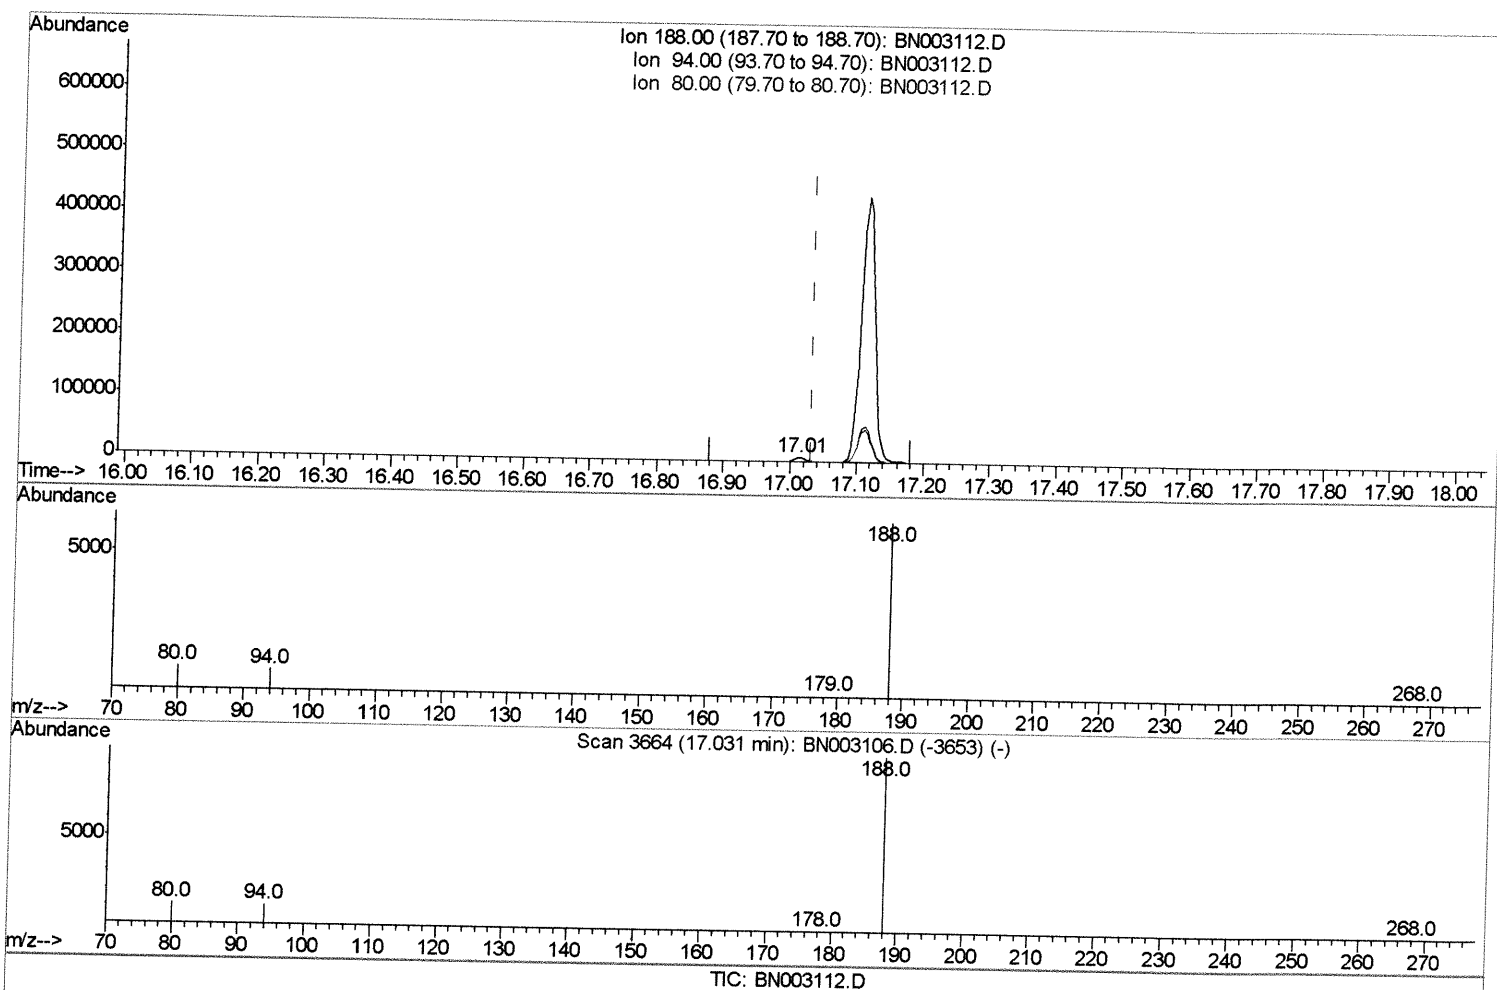

(10) Phenanthrene-d10 (I)

17.014min (-0.017) 0.40ng/ul m) SJ 10/12/18

response 8785

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.16
80.00	12.70	13.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

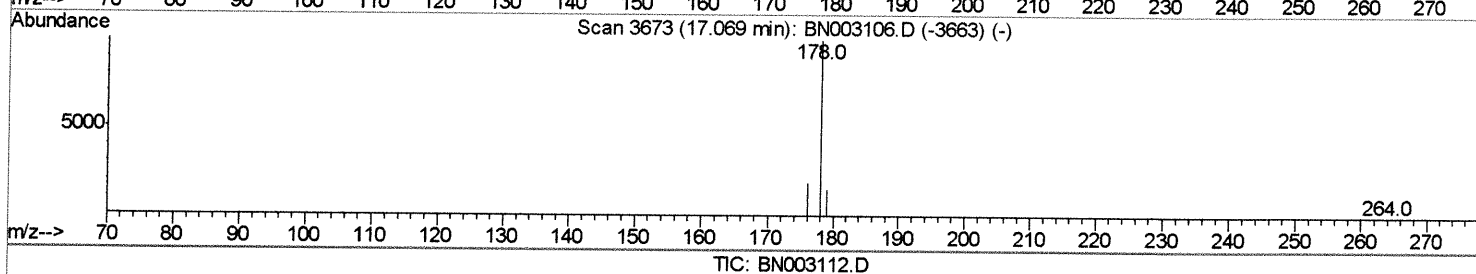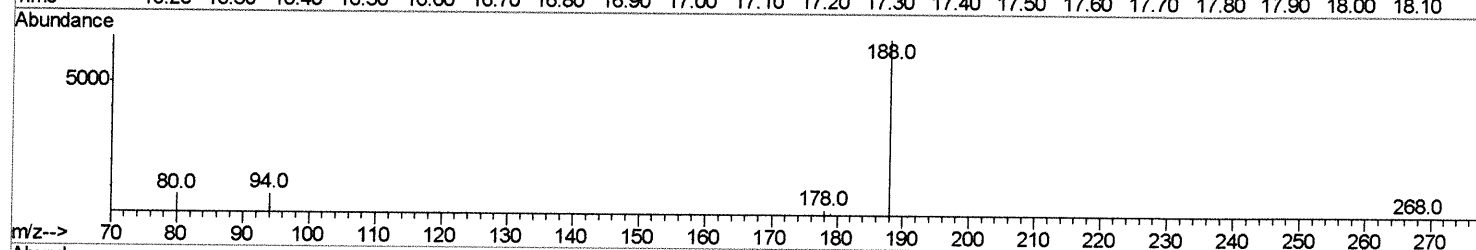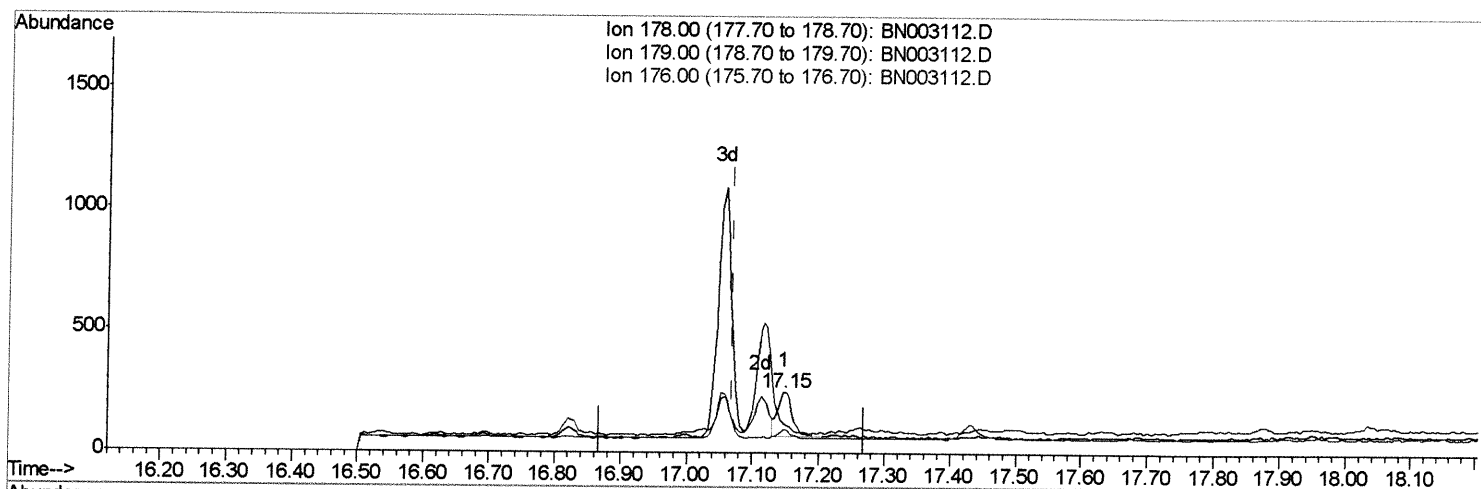

(12) Phenanthrene

17.145min (+0.076) 0.01ng/ul

response 274

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	50.41#
176.00	19.30	38.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

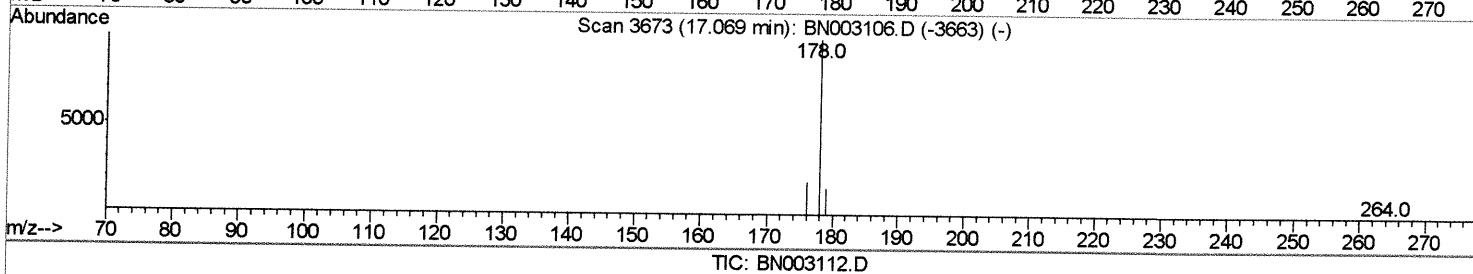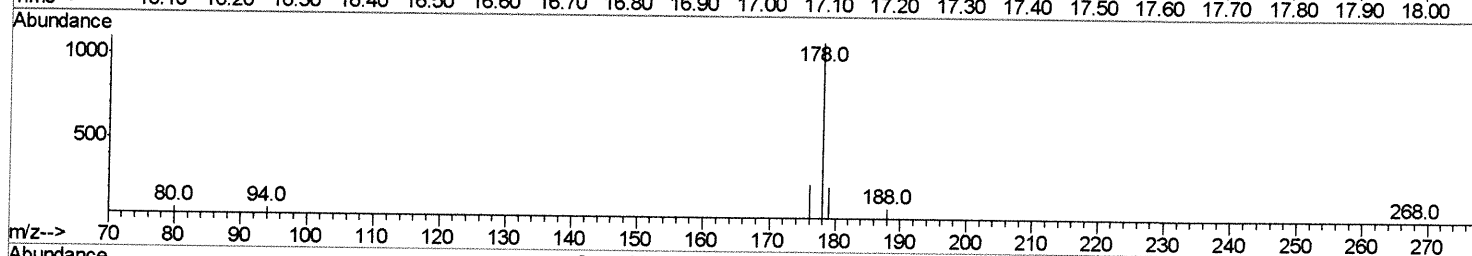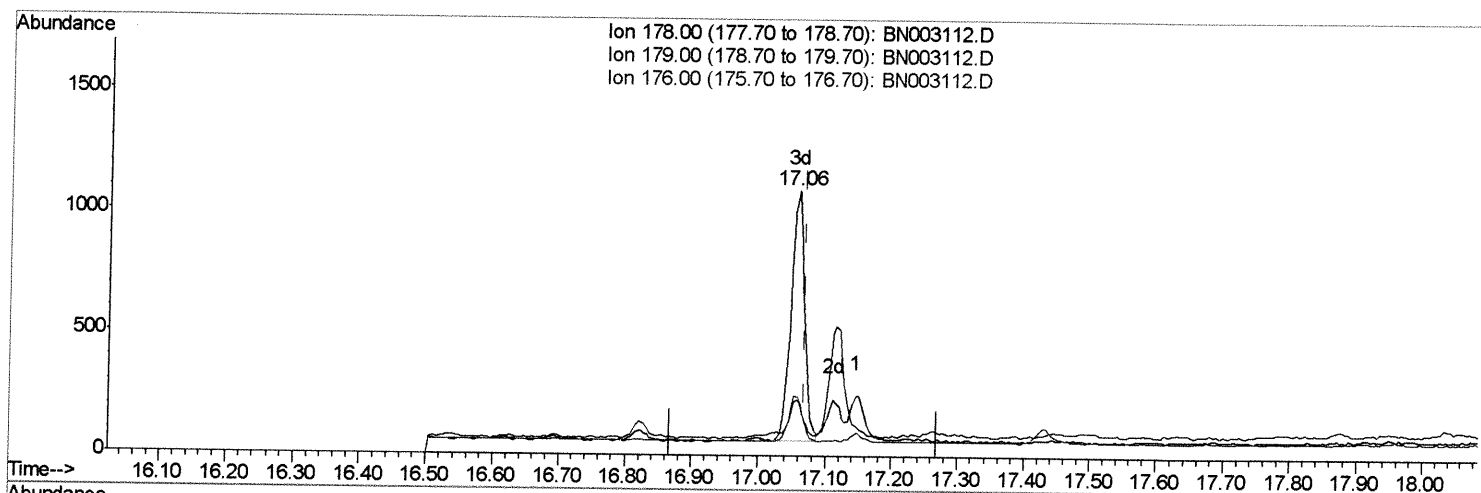

(12) Phenanthrene

17.057min (-0.013) 0.06ng/ul m > SD 10/12/18

response 1441

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	21.17#
176.00	19.30	22.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

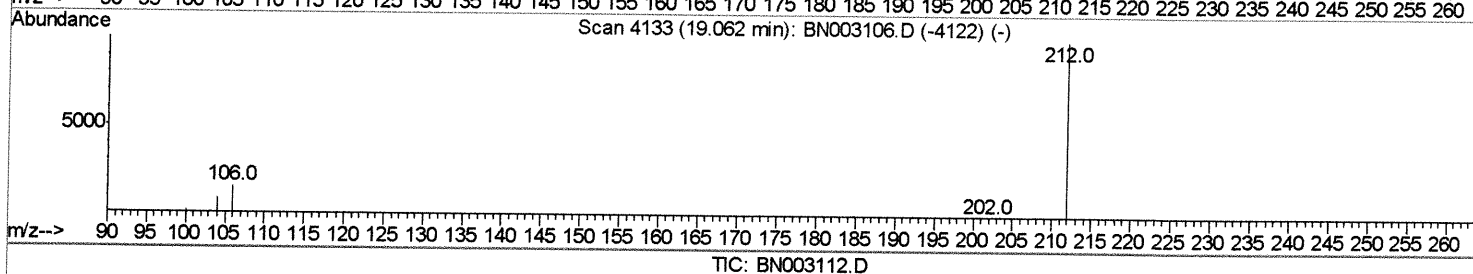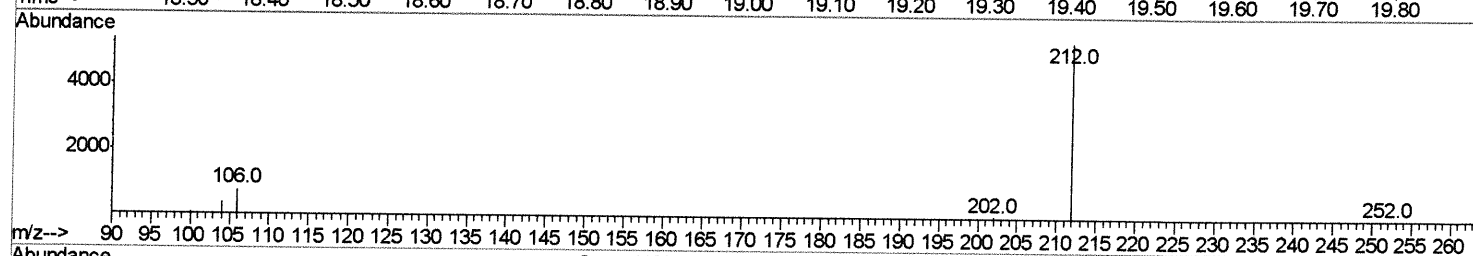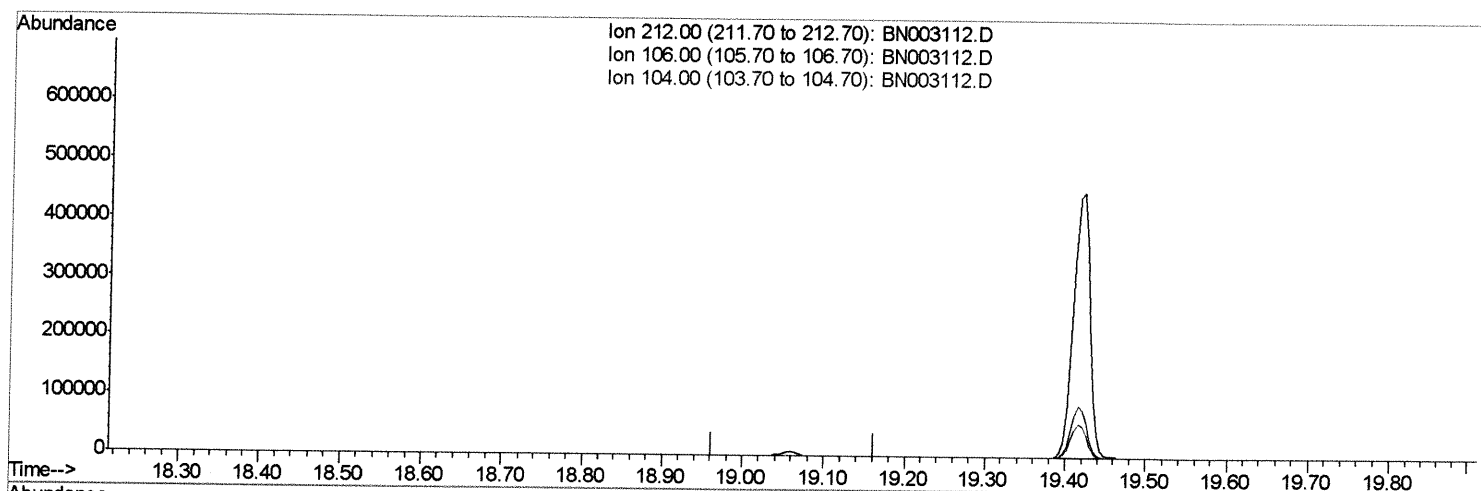

(14) Fluoranthene-d10 (SURR)

19.062min (-19.062) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

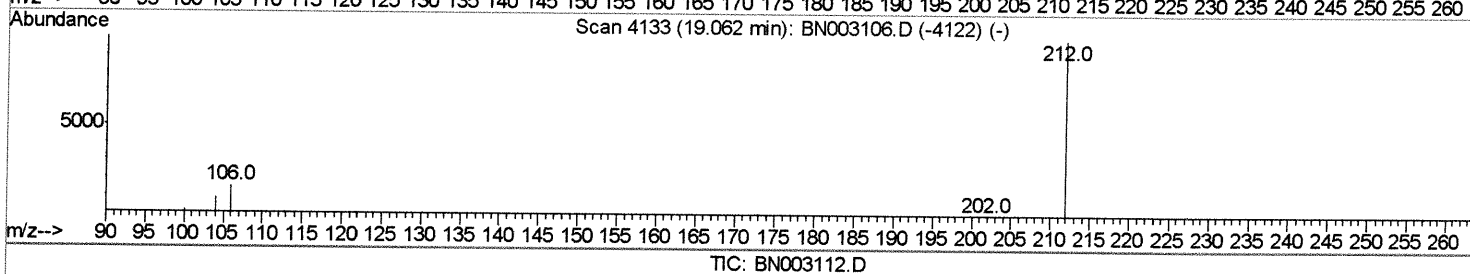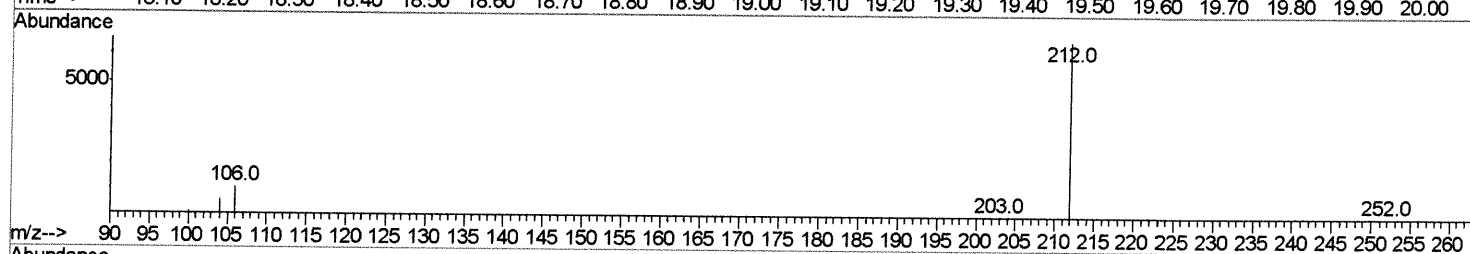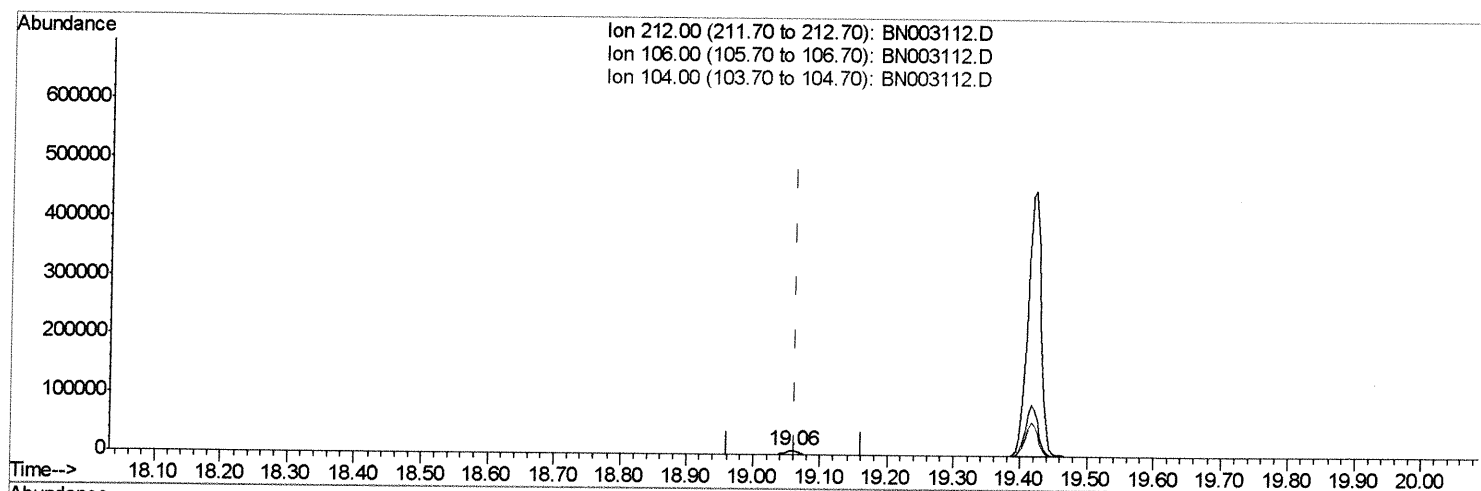

(14) Fluoranthene-d10 (SURR)

19.058min (-0.005) 0.37ng/ul m> SJ 10/12/18

response 9367

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

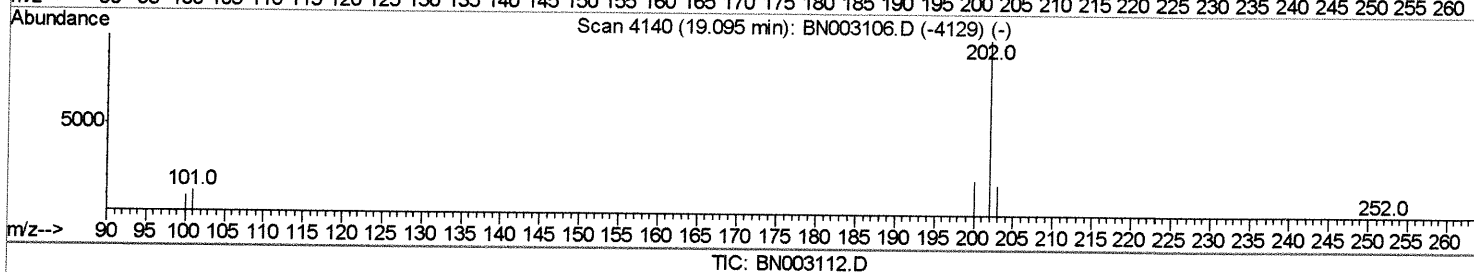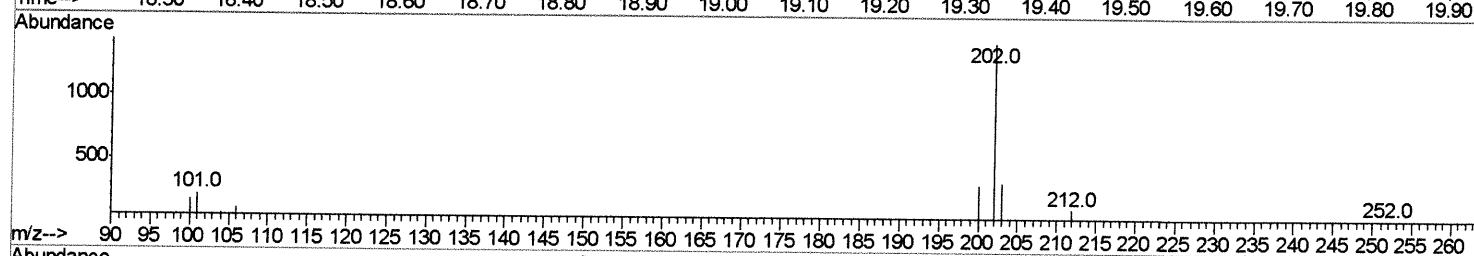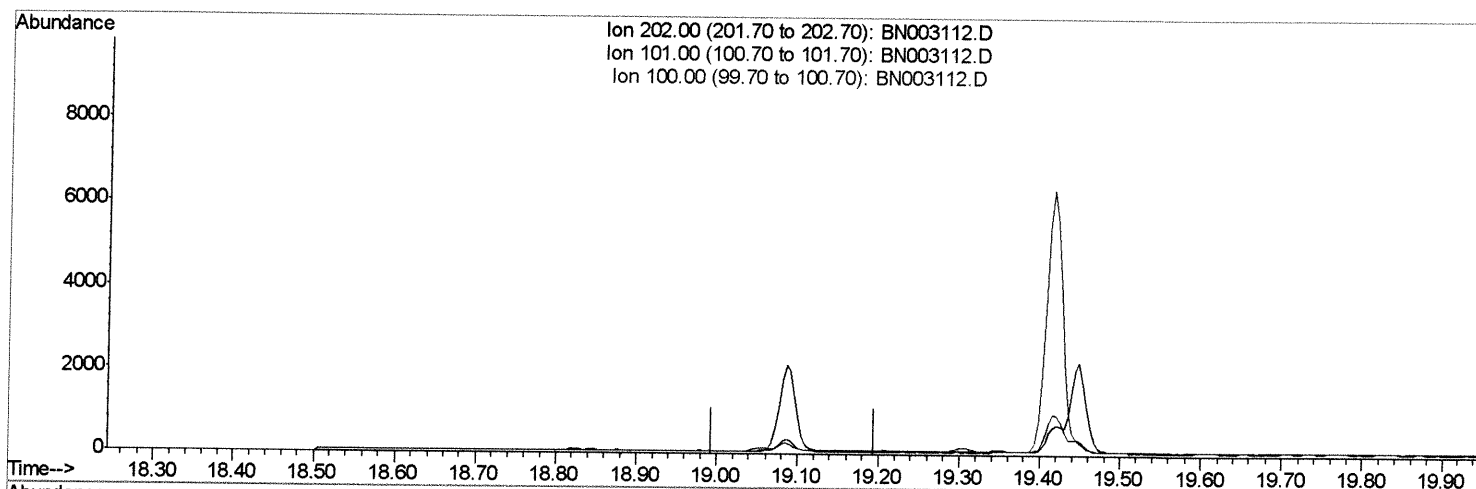

(15) Fluoranthene (C)

19.095min (-19.095) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

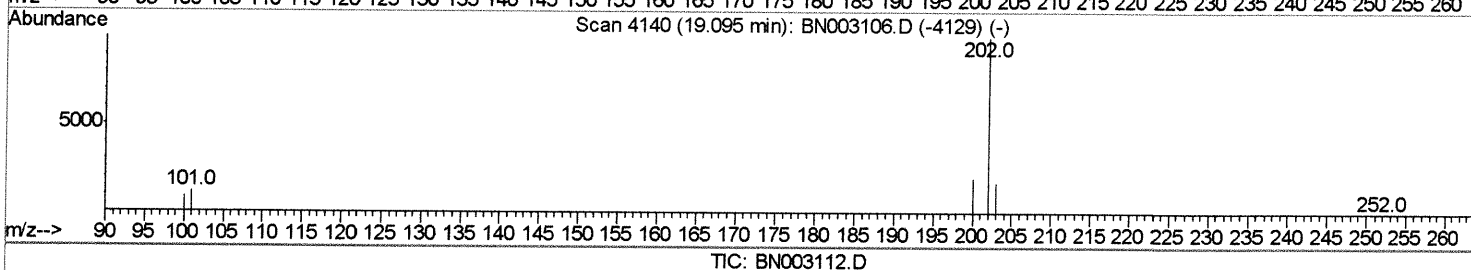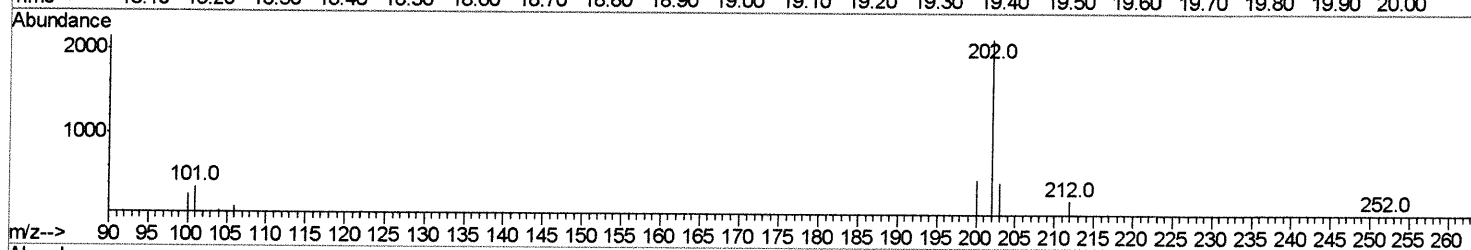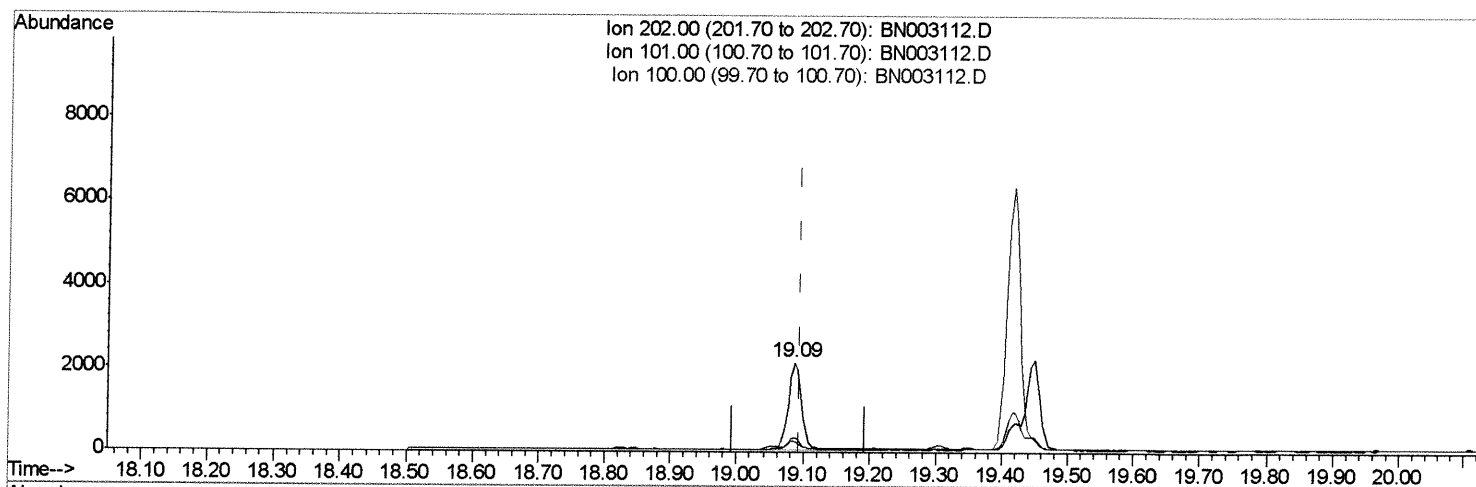

(15) Fluoranthene (C)

19.086min (-0.009) 0.10ng/ul m > SD 10/12/18

response 2944

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	16.81
100.00	9.10	12.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

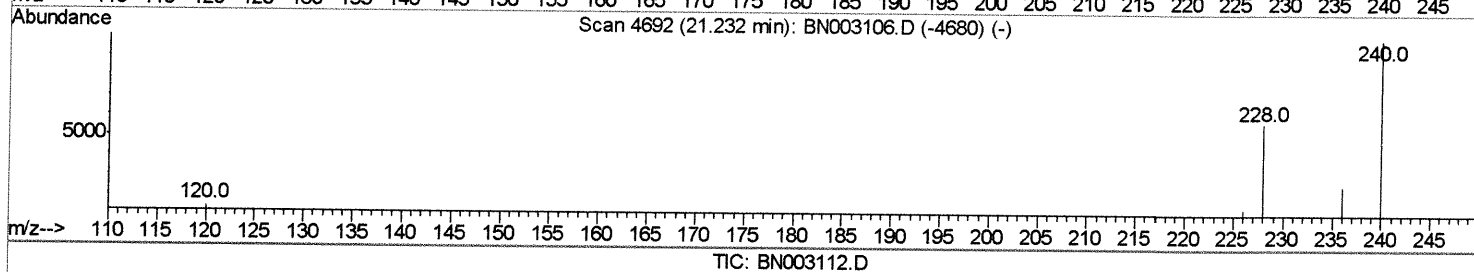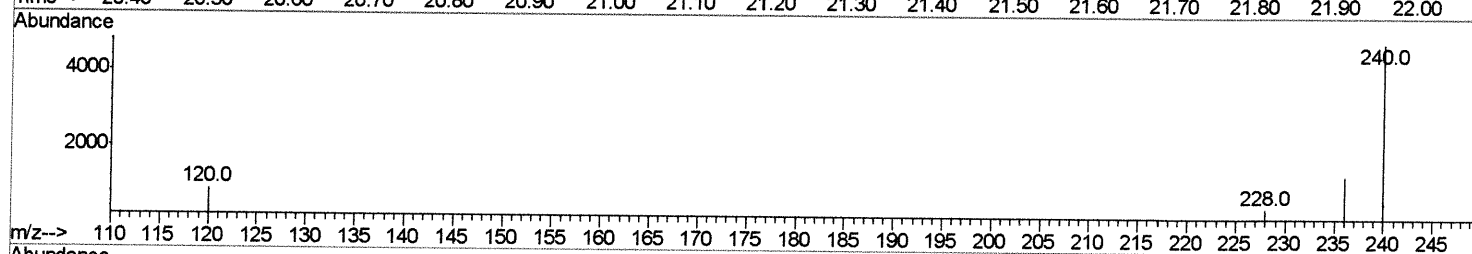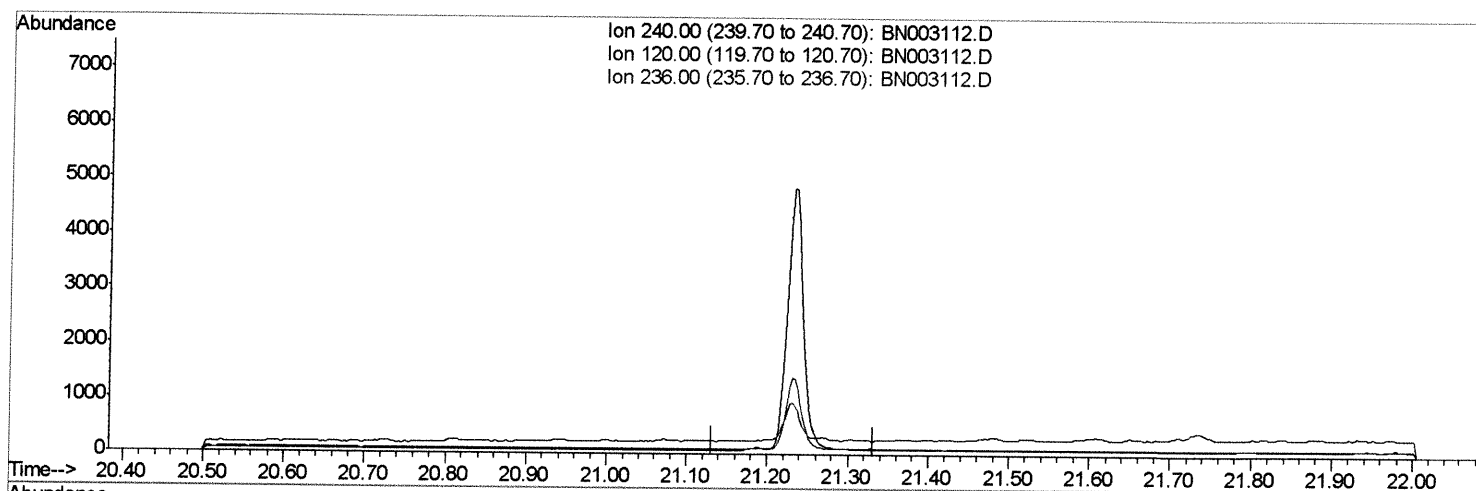

(16) Chrysene-d12 (I)

21.232min (-21.232) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

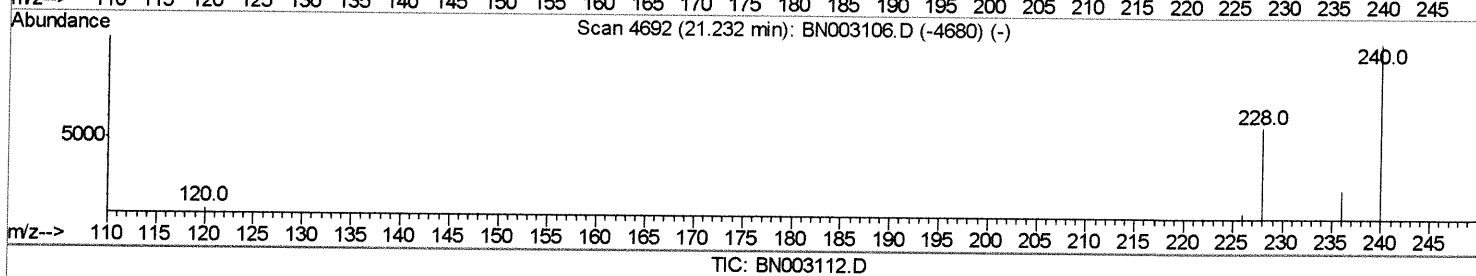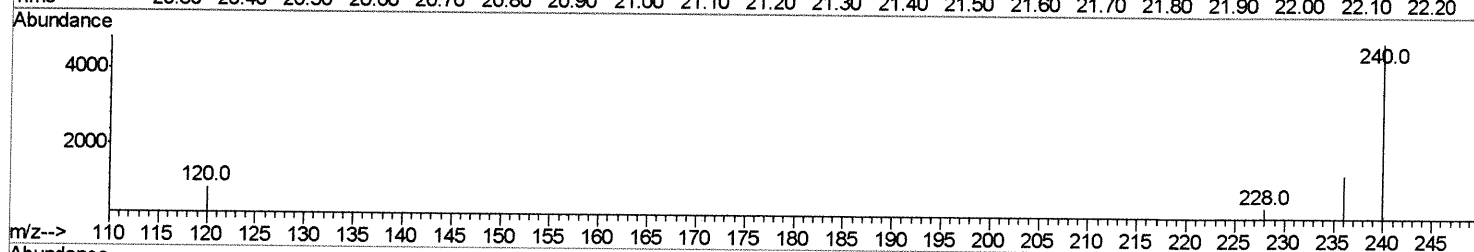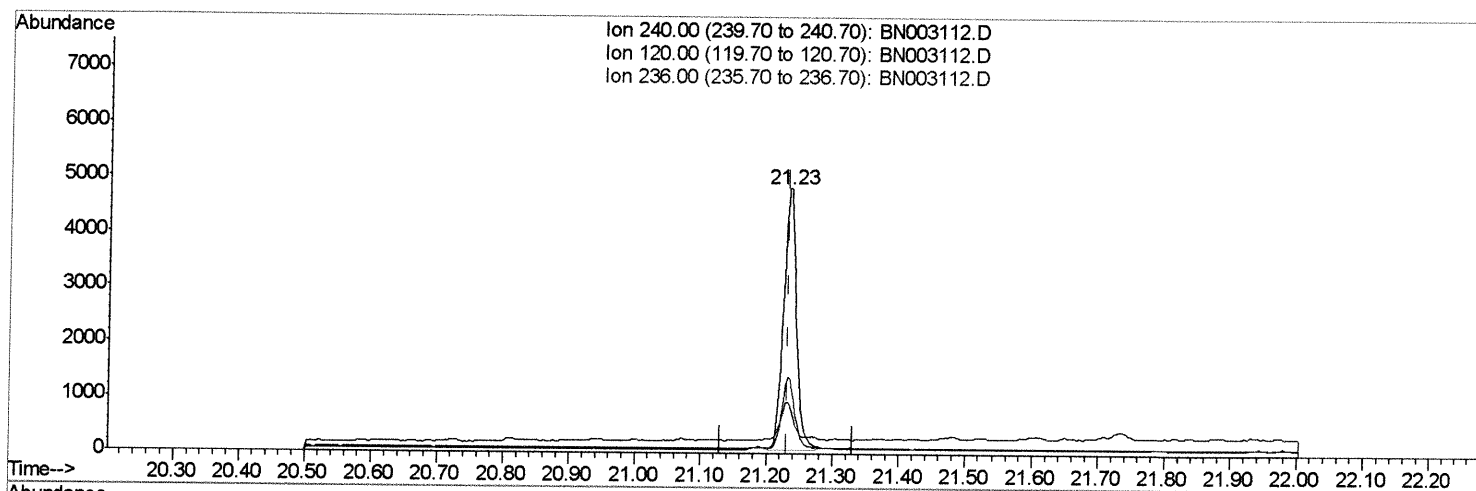

TIC: BN003112.D

(16) Chrysene-d12 (I)

21.233min (+0.001) 0.40ng/ul m > SD 10/12/18

response 6472

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	18.21
236.00	28.10	28.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

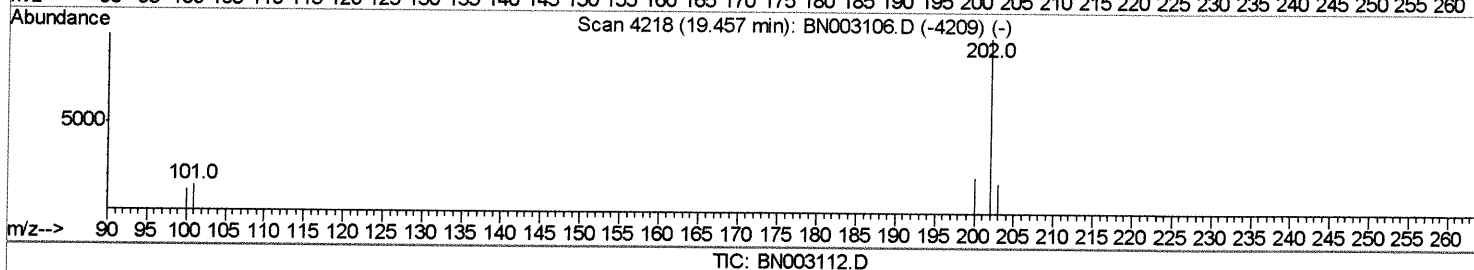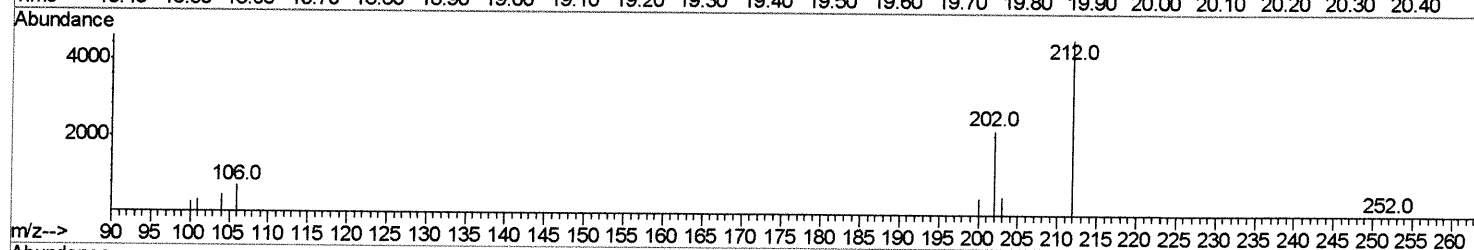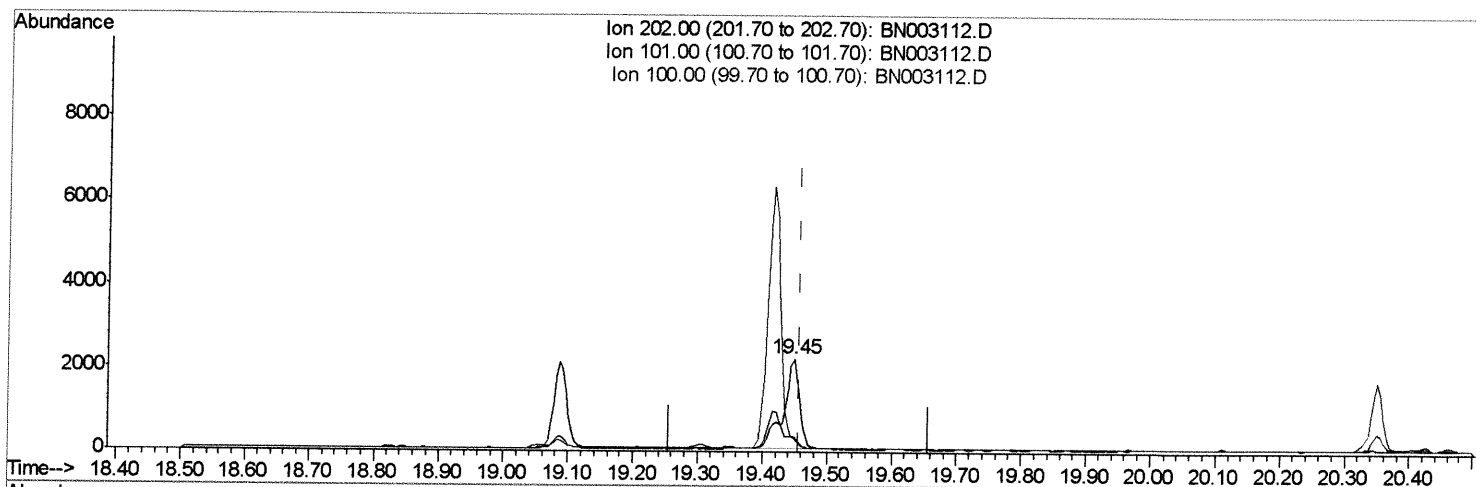

(17) Pyrene

19.448min (-0.009) 0.15ng/ul

response 3800

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	16.39
100.00	12.40	14.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

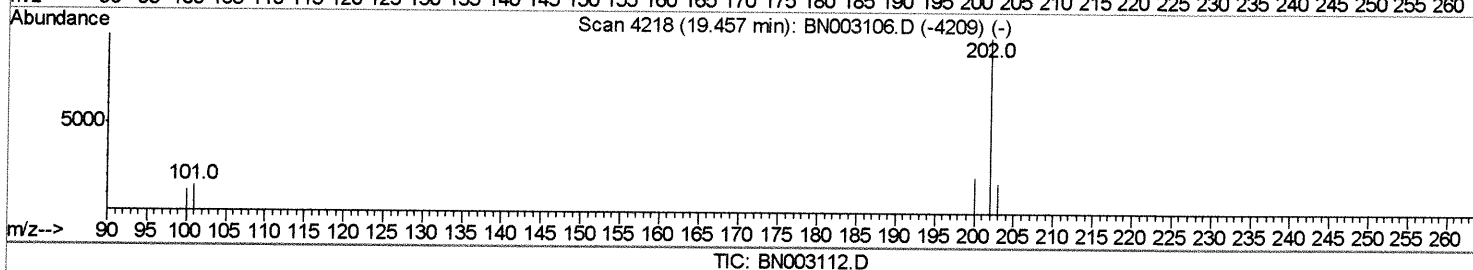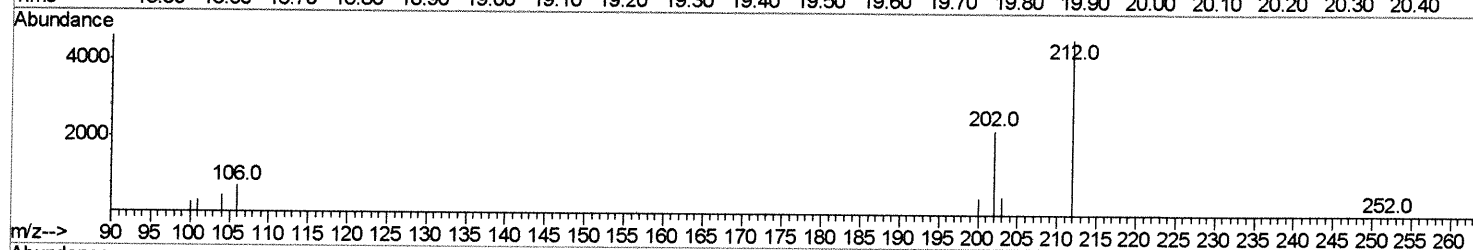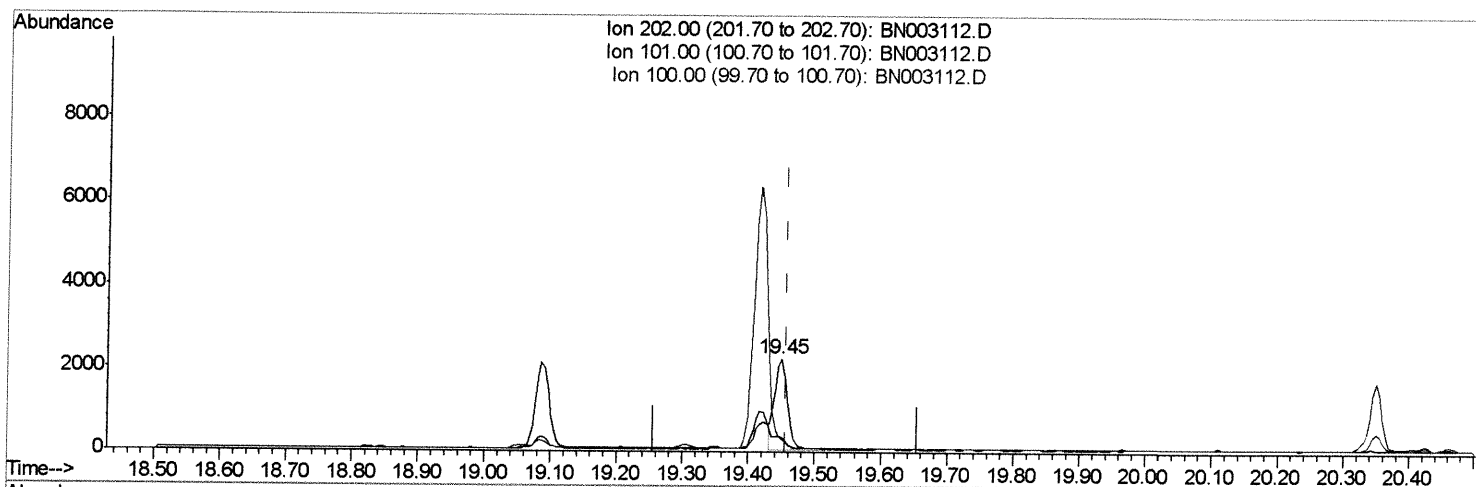

(17) Pyrene

19.448min (-0.009) 0.12ng/ul m> SJ 10/12/18

response 2910

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	16.39
100.00	12.40	14.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

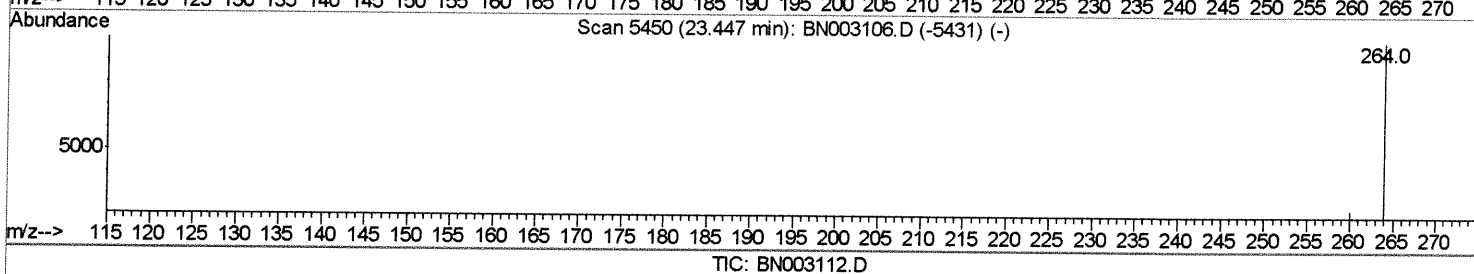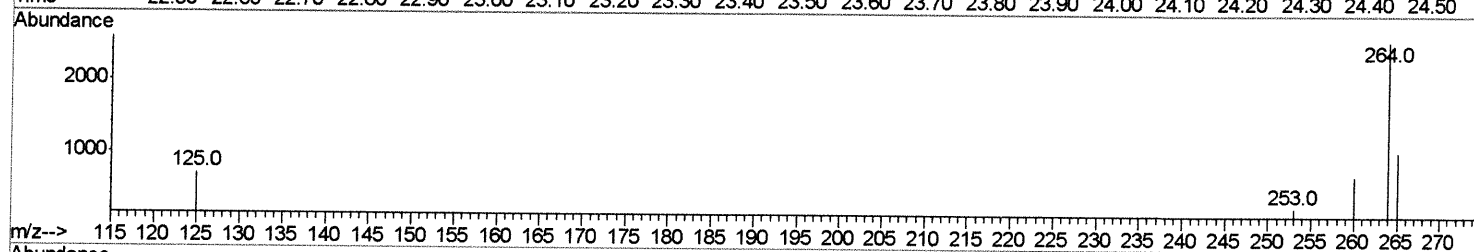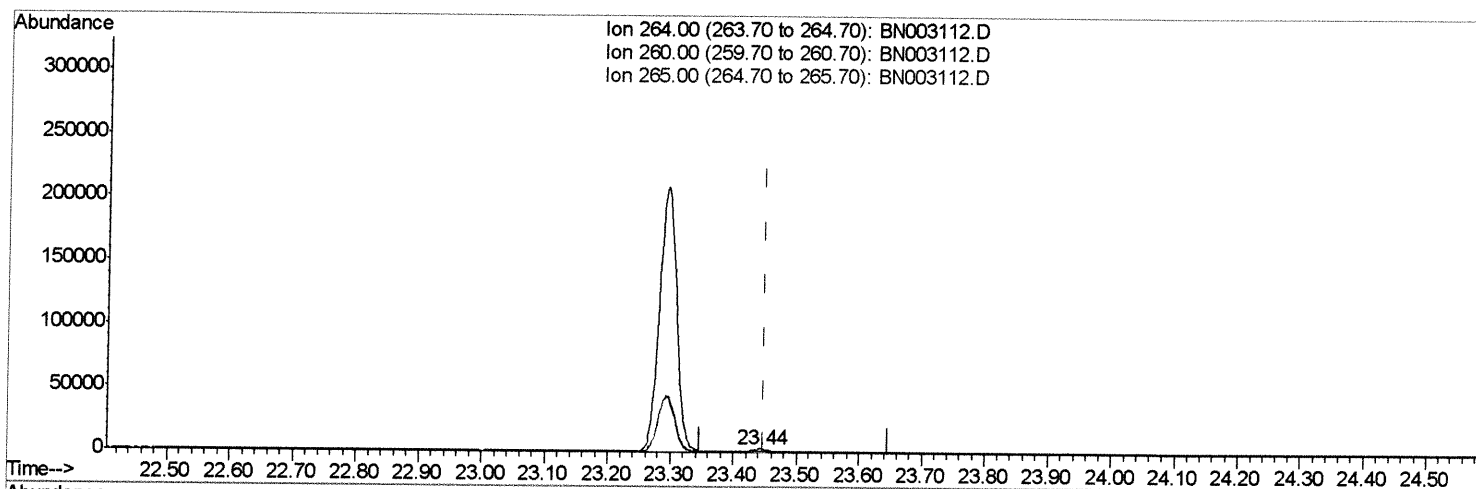

(20) Perylene-d12 (I)

23.443min (-0.005) 0.40ng/ul

response 5319

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	27.74
265.00	45.40	40.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003112.D
 Acq On : 11 Oct 2018 20:36
 Operator : MJ/SJ
 Sample : J5368-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3Z01

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

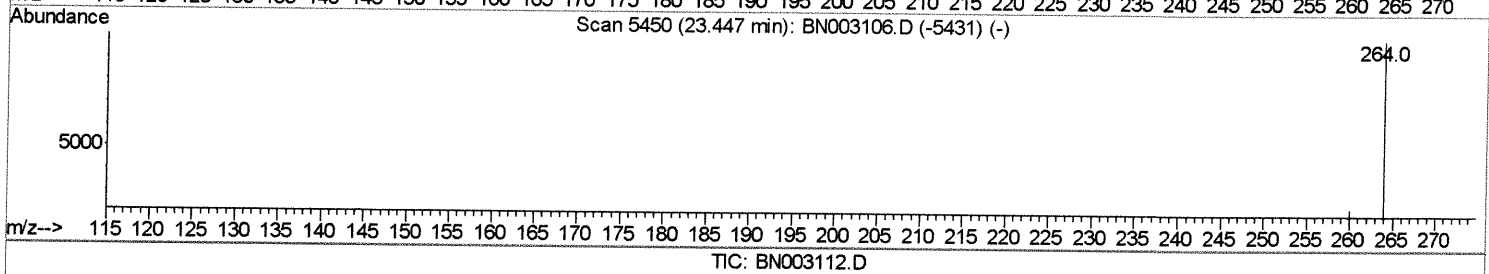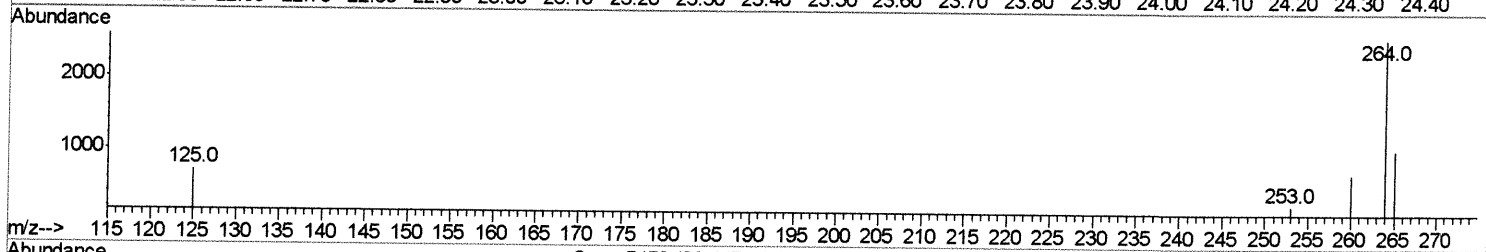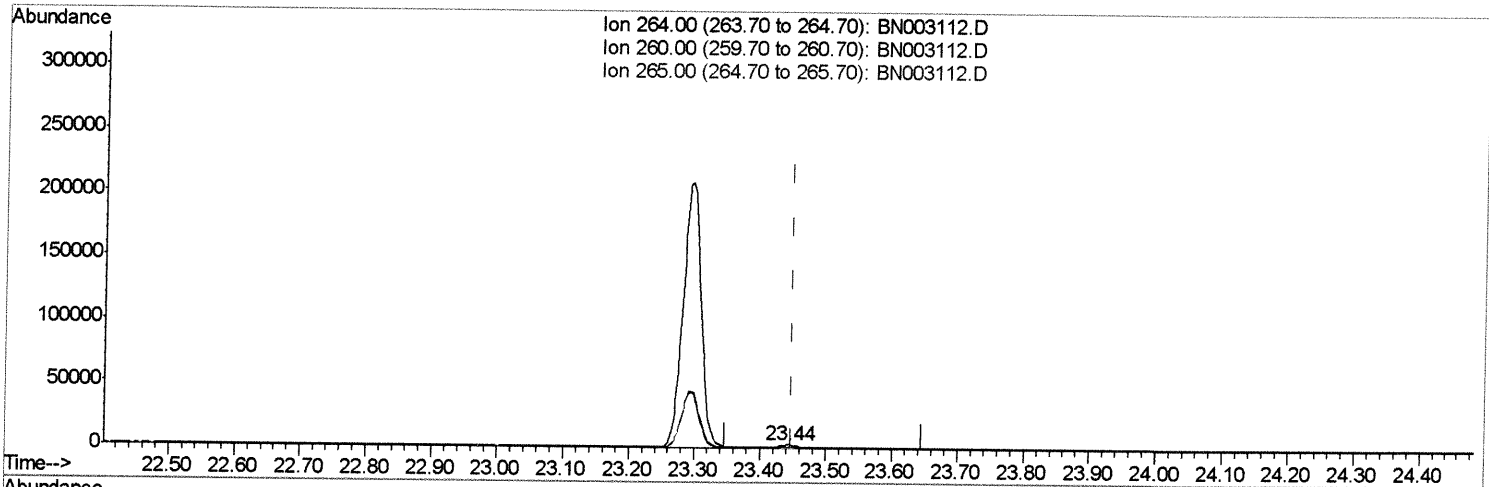

(20) Perylene-d12 (I)

23.443min (-0.005) 0.40ng/ul m > SJ 10/12/18

response 4527

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	27.74
265.00	45.40	40.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003112.D
 Acq On : 11 Oct 2018 20:36
 Operator : MJ/SJ
 Sample : J5368-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z01

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

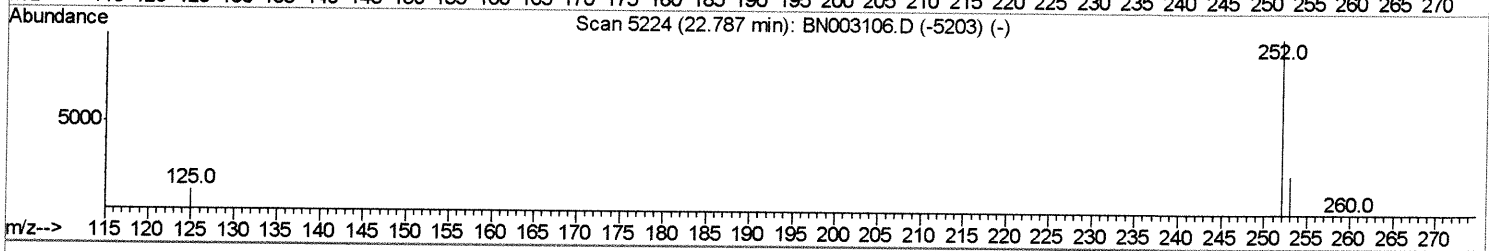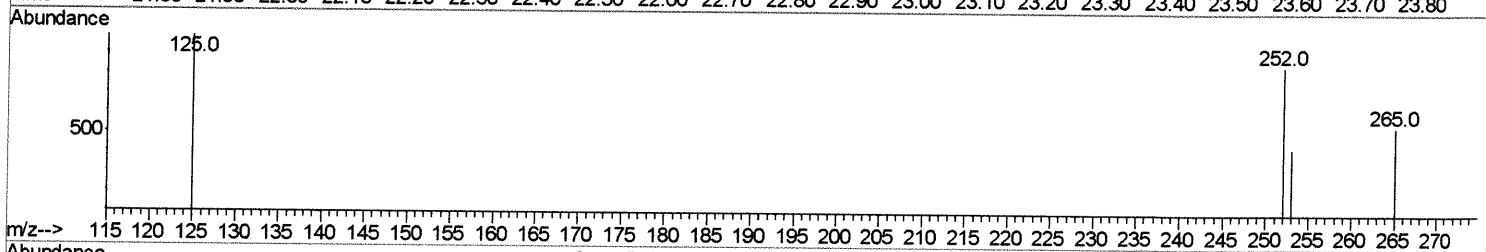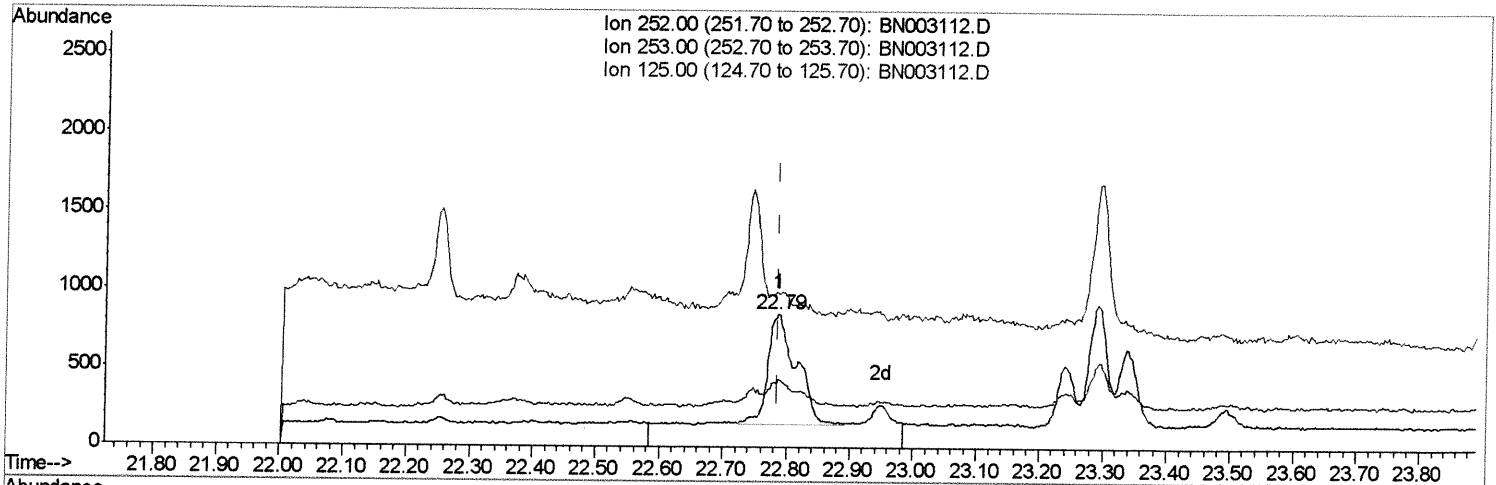

TIC: BN003112.D

(21) Benzo(b)fluoranthene

22.785min (-0.002) 0.14ng/ul

response 2208

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	50.53
125.00	17.10	116.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

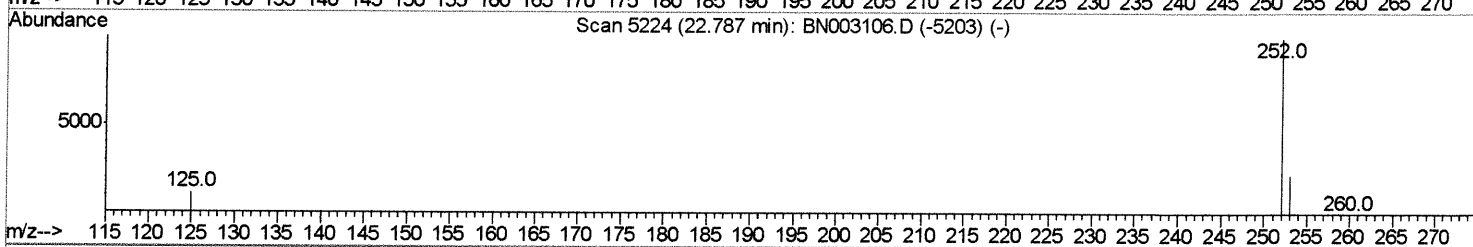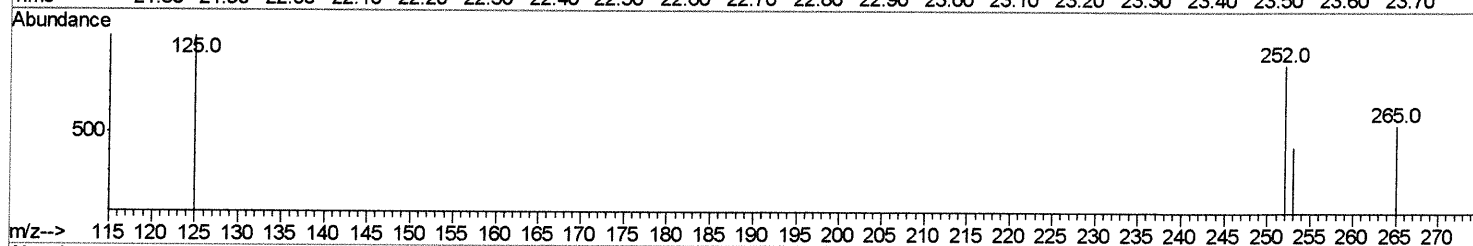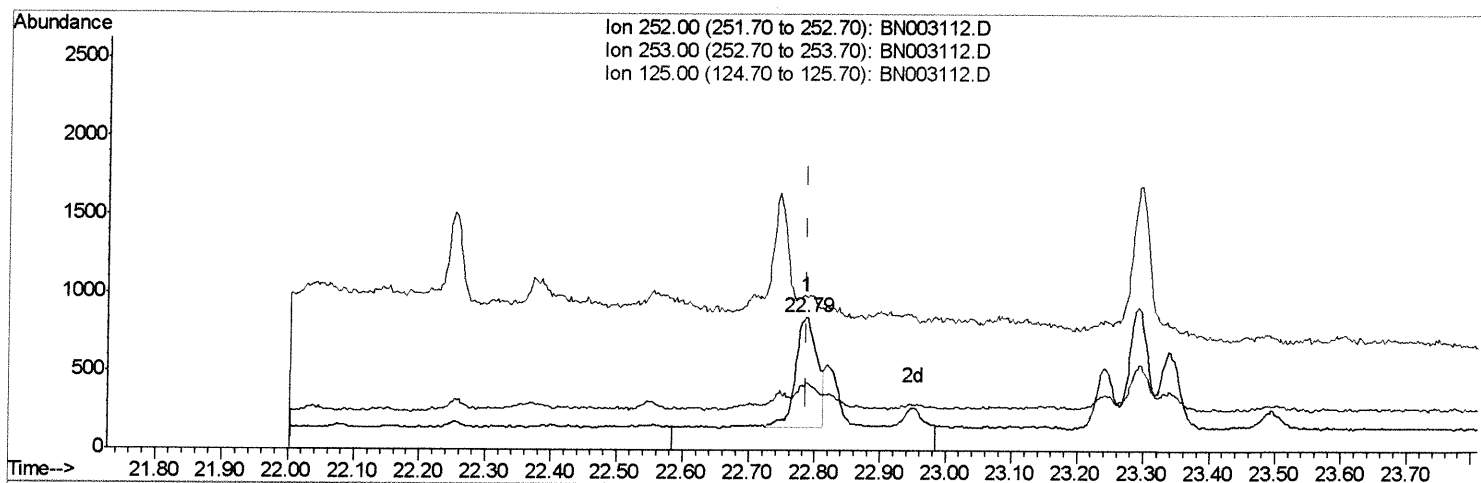

TIC: BN003112.D

(21) Benzo(b)fluoranthene

22.785min (-0.002) 0.10ng/ul m

> 50 10/12/18

response 1643

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	50.53
125.00	17.10	116.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

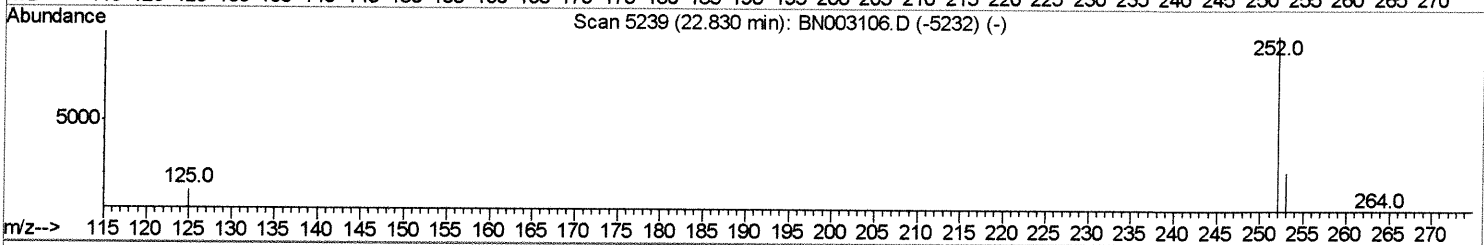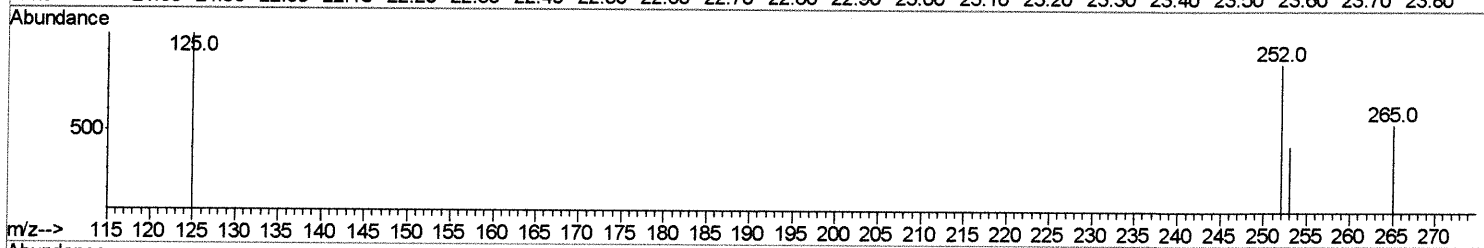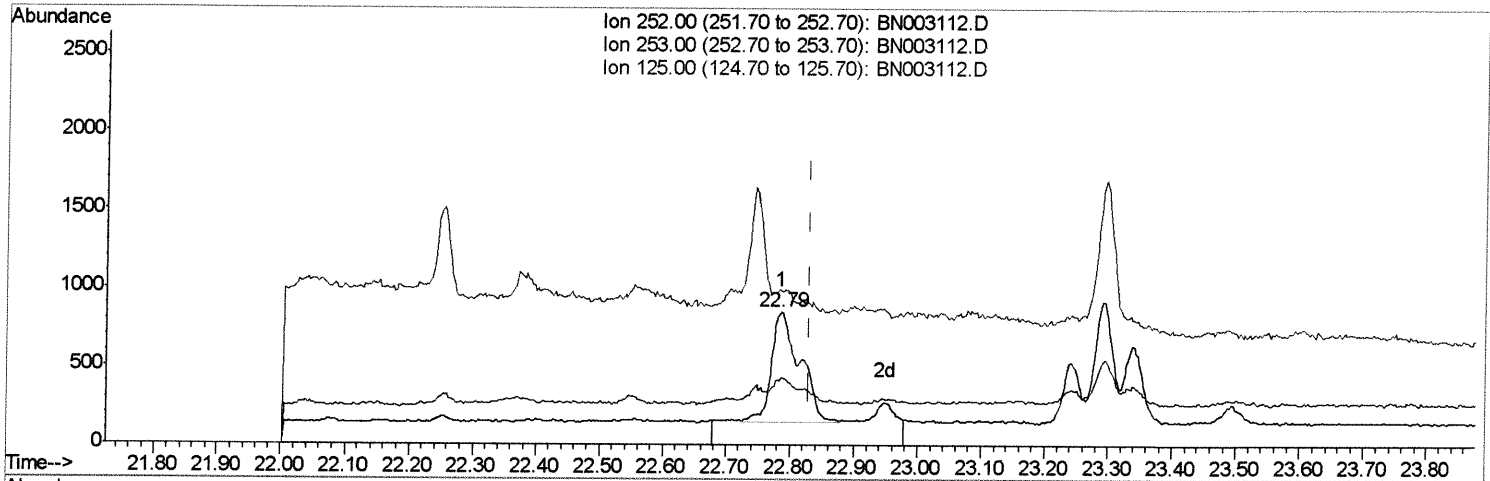

TIC: BN003112.D

(22) Benzo(k)fluoranthene

22.785min (-0.045) 0.13ng/ul

response 2202

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	50.53#
125.00	17.60	116.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z01

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:46:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

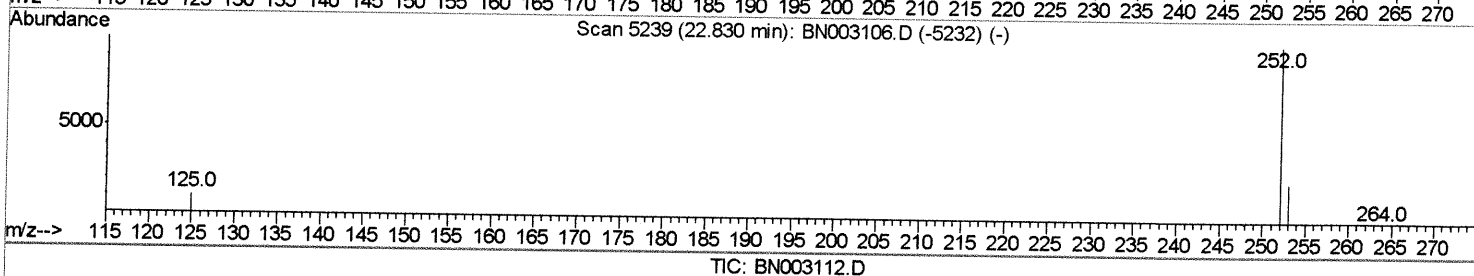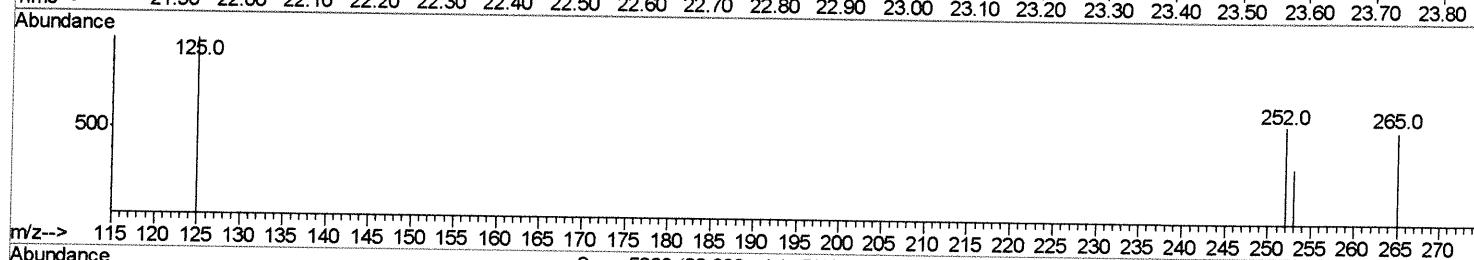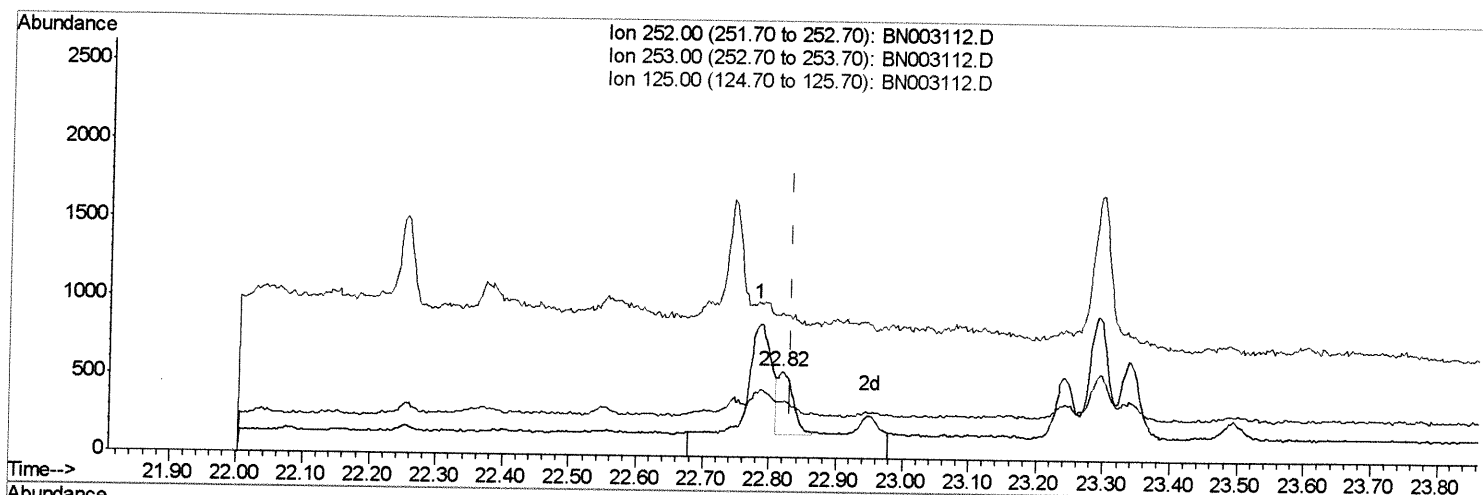

(22) Benzo(k)fluoranthene

22.817min (-0.013) 0.04ng/ul m> SJ 10/12/18

response 656

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	64.48#
125.00	17.60	167.76#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003112.D
 Acq On : 11 Oct 2018 20:36
 Operator : MJ/SJ
 Sample : J5368-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z01

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:47:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1534	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6626	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3986	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	8785m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	6472m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4527m	0.40	ng/ul	0.00

SJ 10/12/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.00	152	3810	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	9367m	0.37	ng/ul	0.00

SJ 10/12/18

Target Compounds

					Ovalue	
3) Naphthalene	10.44	128	753	0.044	ng/ul#	80
5) 2-Methylnaphthalene	12.08	142	2797	0.239	ng/ul	97
8) Acenaphthene	14.32	153	1021	0.074	ng/ul	96
12) Phenanthrene	17.06	178	1441m	0.059	ng/ul	
15) Fluoranthene	19.09	202	2944m	0.102	ng/ul	
17) Pyrene	19.45	202	2910m	0.116	ng/ul	
18) Benzo(a)anthracene	21.22	228	1658	0.080	ng/ul#	86
19) Chrysene	21.27	228	1813	0.086	ng/ul#	88
21) Benzo(b)fluoranthene	22.79	252	1643m	0.101	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	656m	0.039	ng/ul	
23) Benzo(a)pyrene	23.34	252	922	0.063	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	25.68	276	629	0.037	ng/ul#	86
26) Benzo(g,h,i)perylene	26.36	276	587	0.041	ng/ul#	29

SJ 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed