


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:51:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

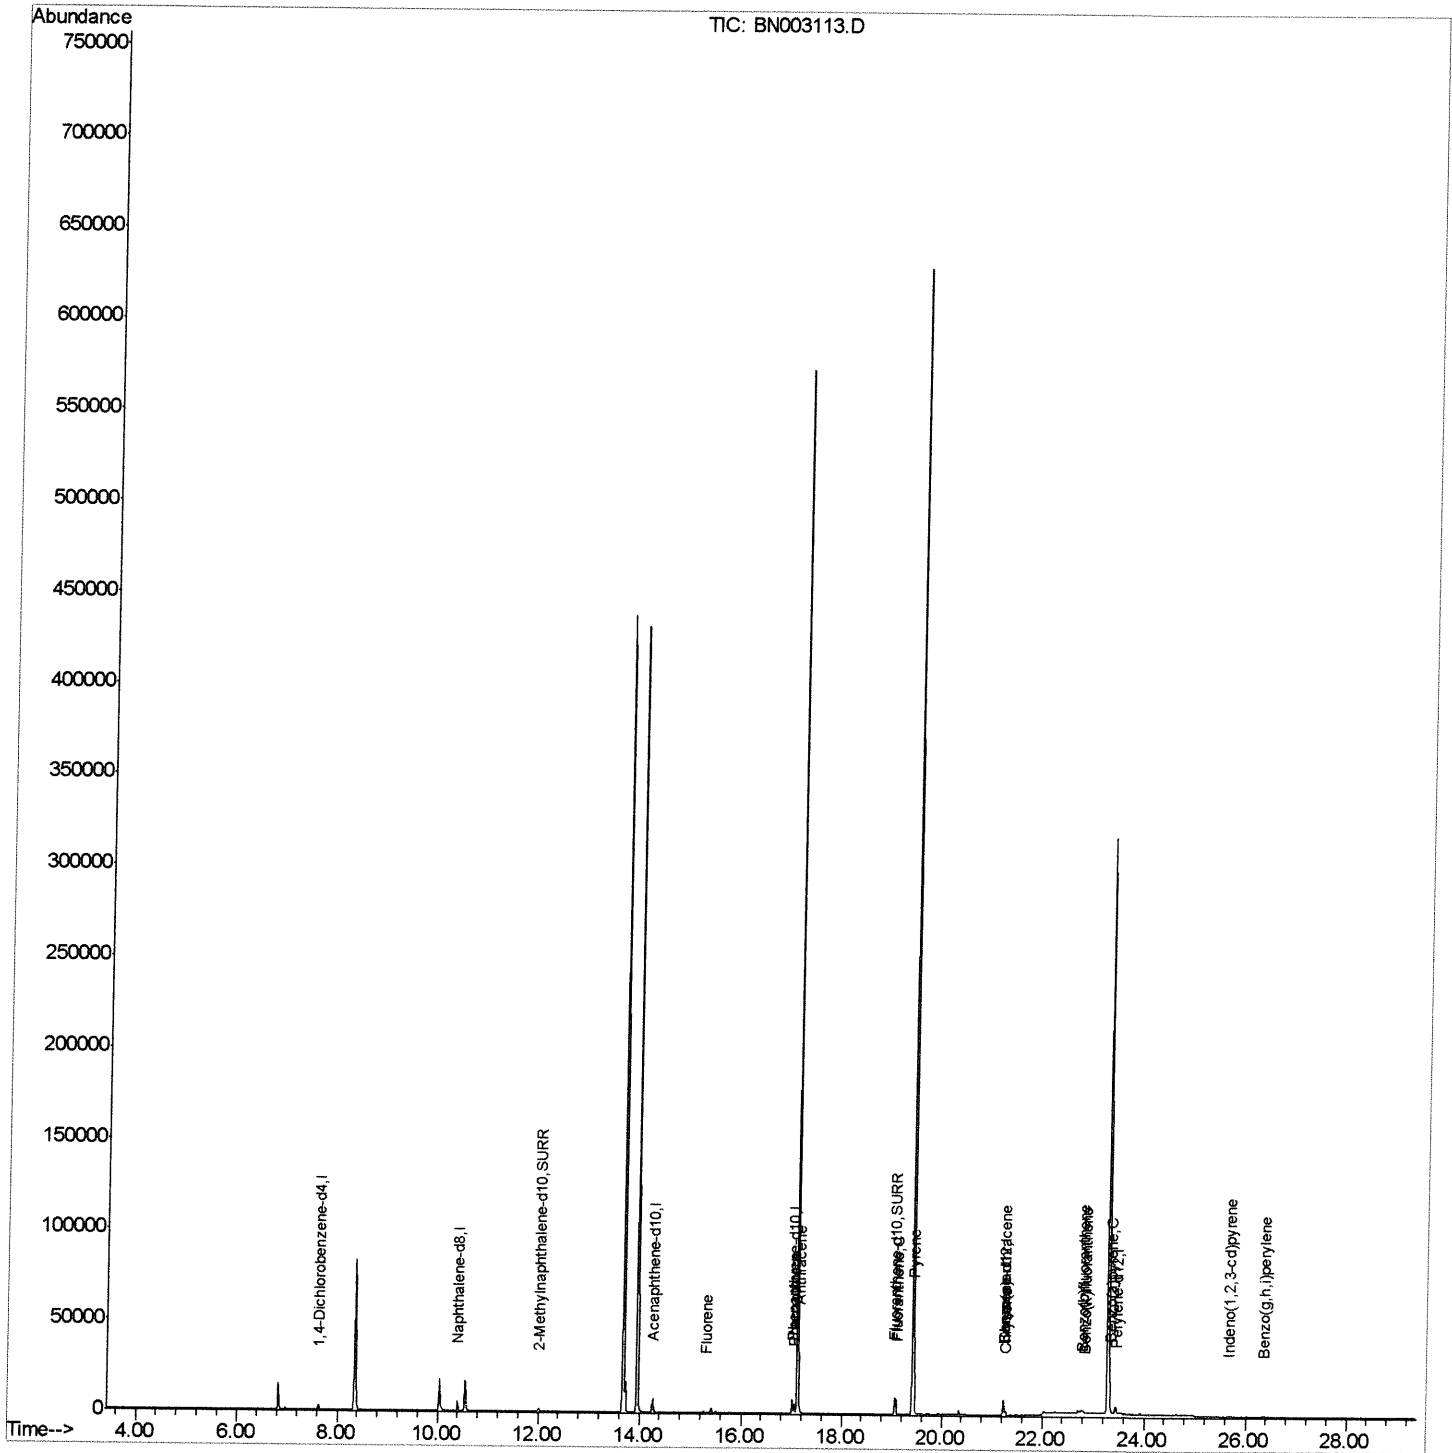

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 05:37:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

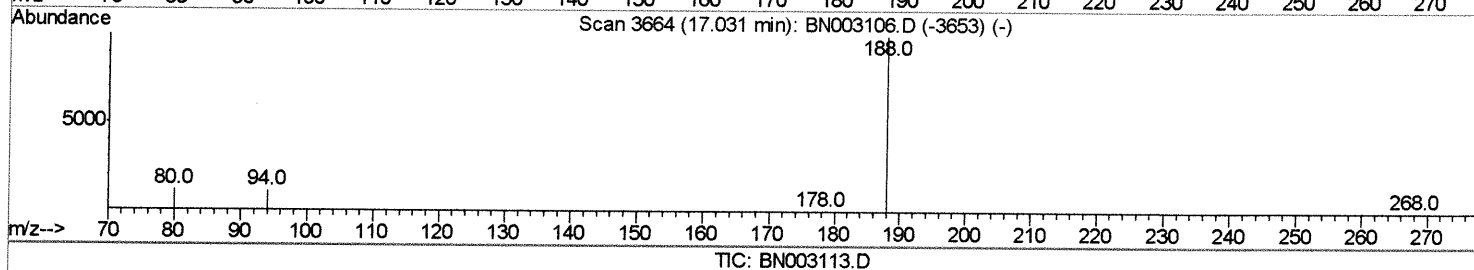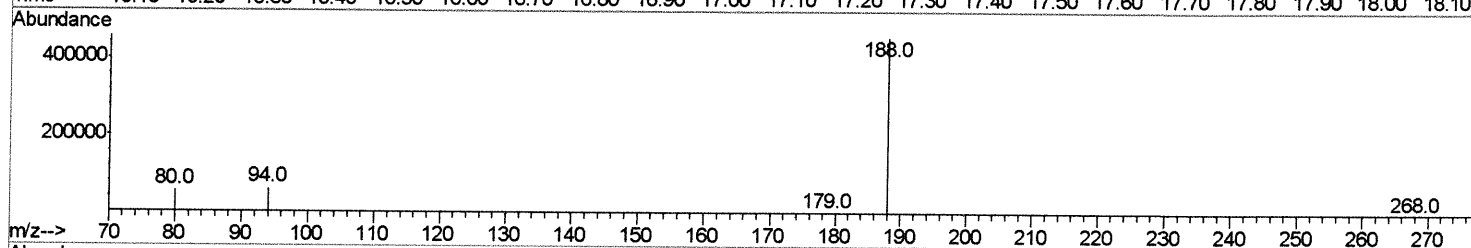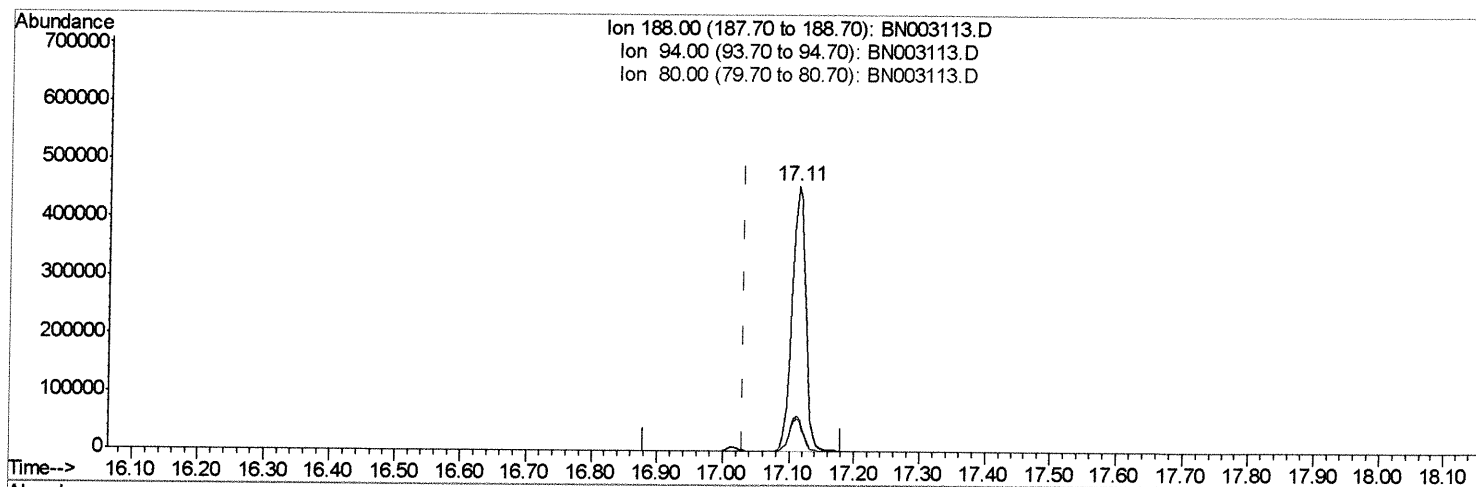

(10) Phenanthrene-d10 (I)

17.111min (+0.080) 0.40ng/ul

response 661087

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.28
80.00	12.70	12.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 05:37:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

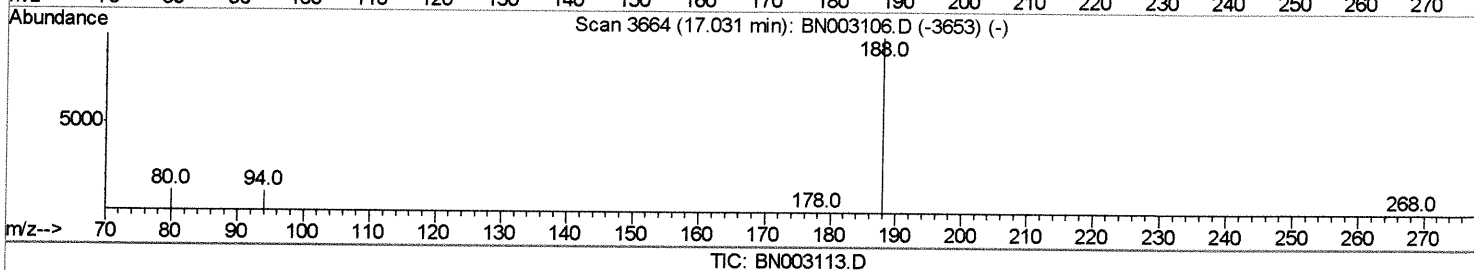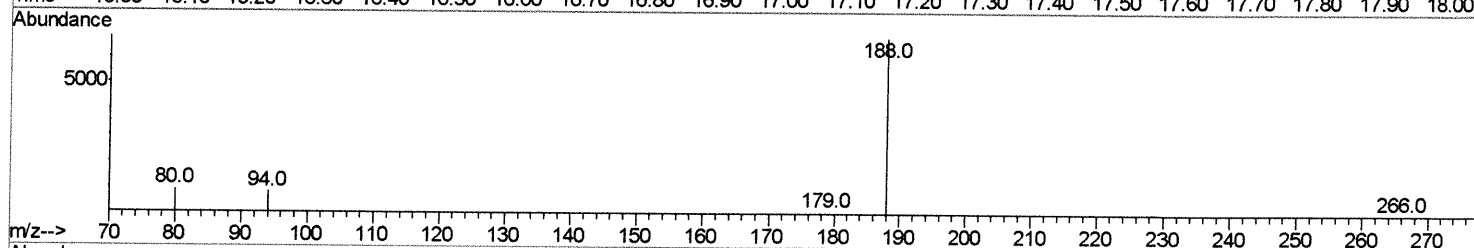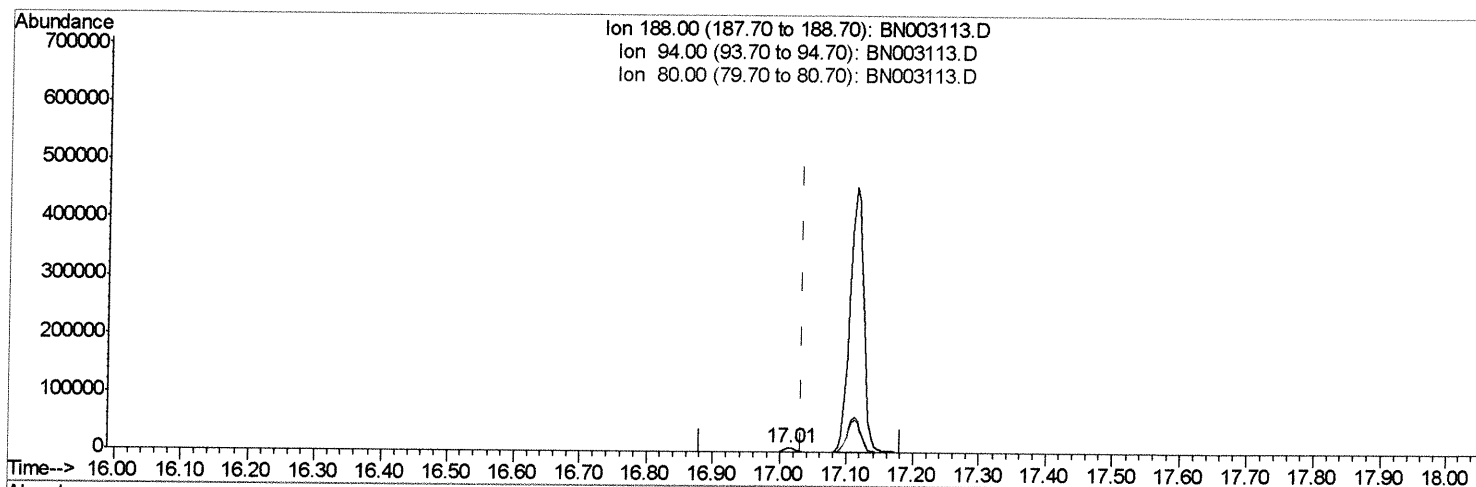

TIC: BN003113.D

(10) Phenanthrene-d10 (I)

17.014min (-0.017) 0.40ng/ul m > 50 10/12/18

response 9500

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.06
80.00	12.70	13.59
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update: Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

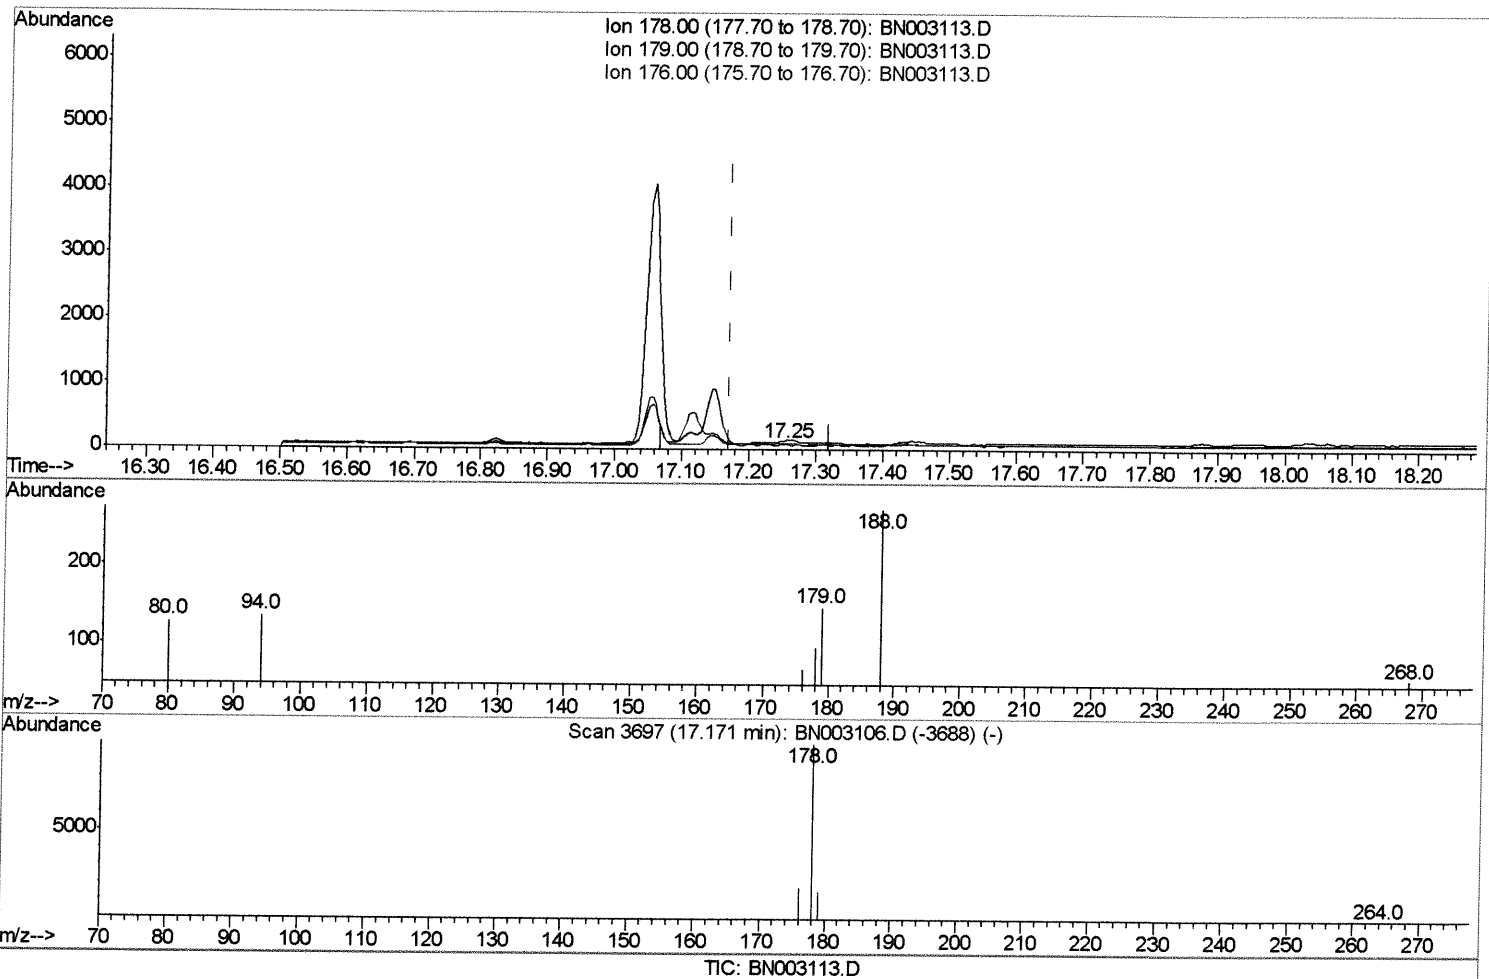

(13) Anthracene

17.255min (+0.084) 0.00ng/ul

response 26

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	154.74#
176.00	19.10	71.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

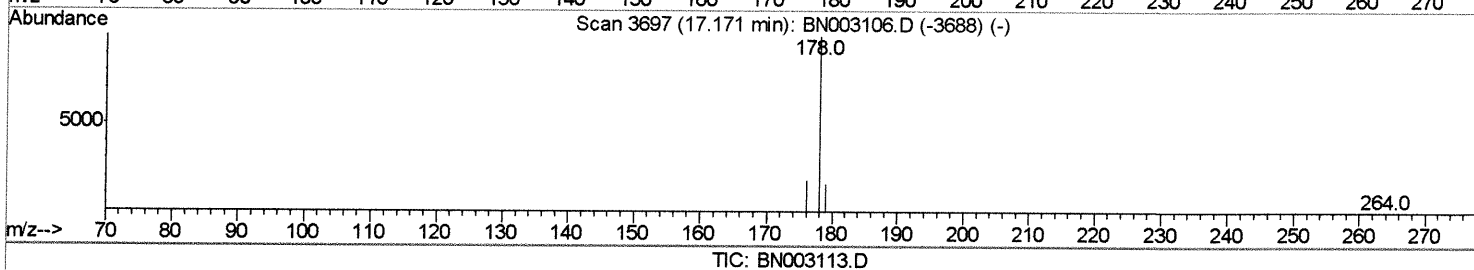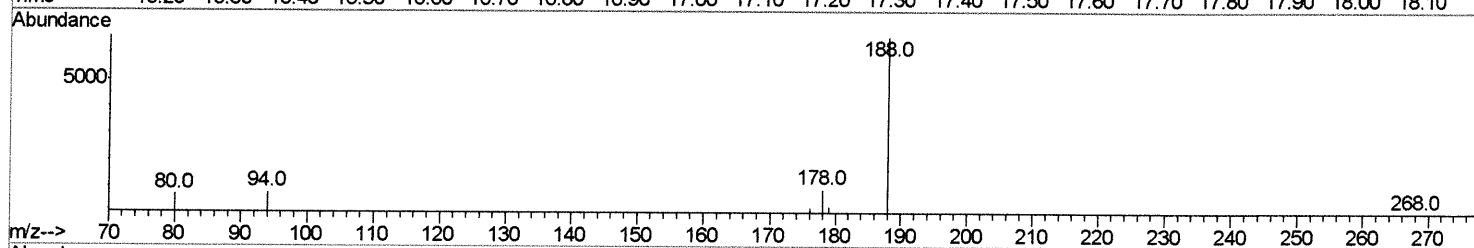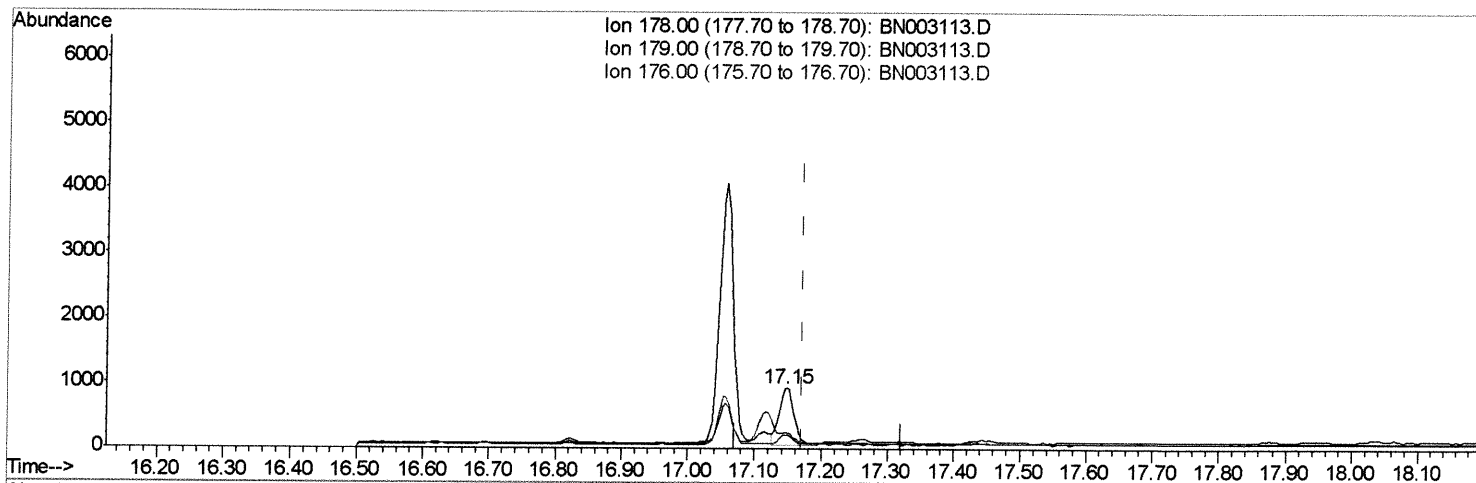

(13) Anthracene

17.145min (-0.025) 0.06ng/ul m

> 50 10/12/18

response 1408

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	27.49#
176.00	19.10	22.84
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

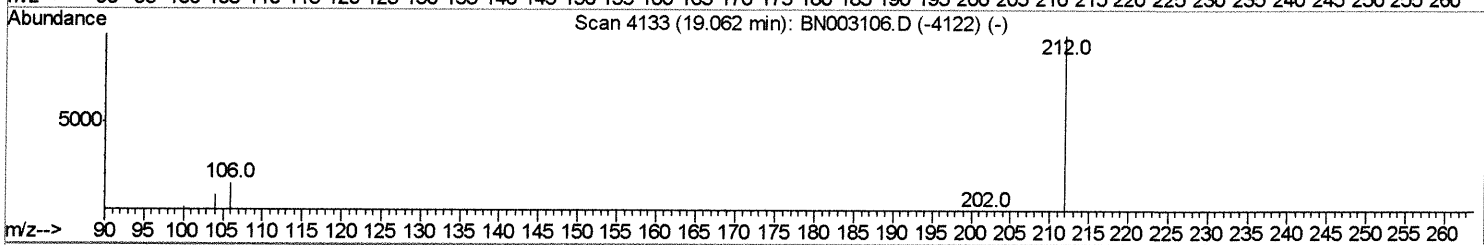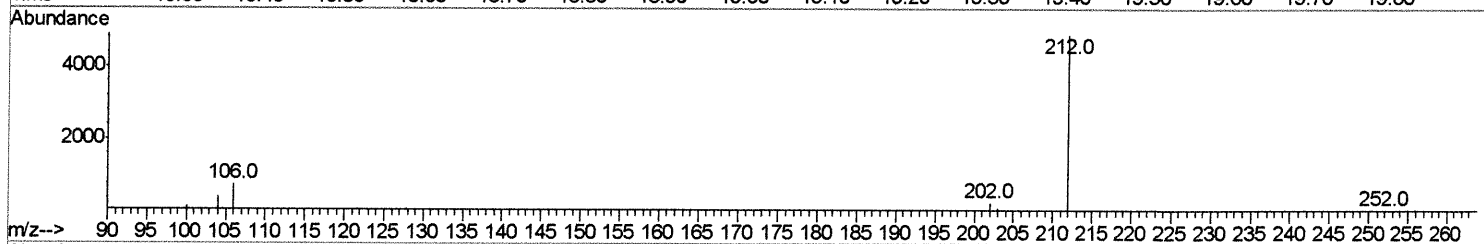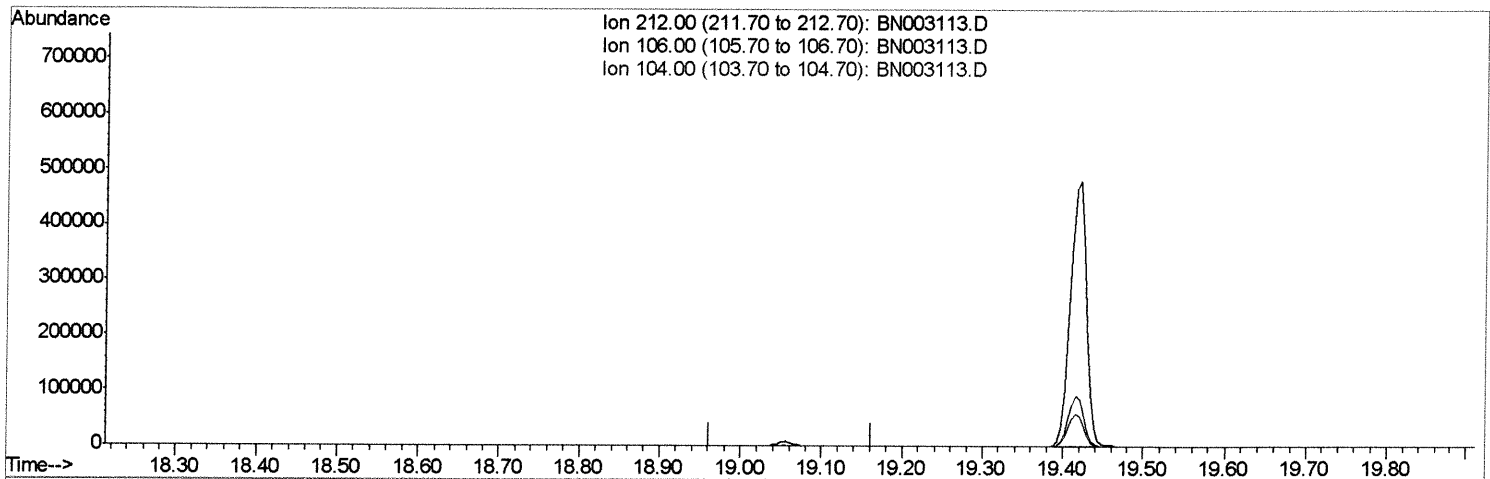

TIC: BN003113.D

(14) Fluoranthene-d10 (SURR)

19.062min (-19.062) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

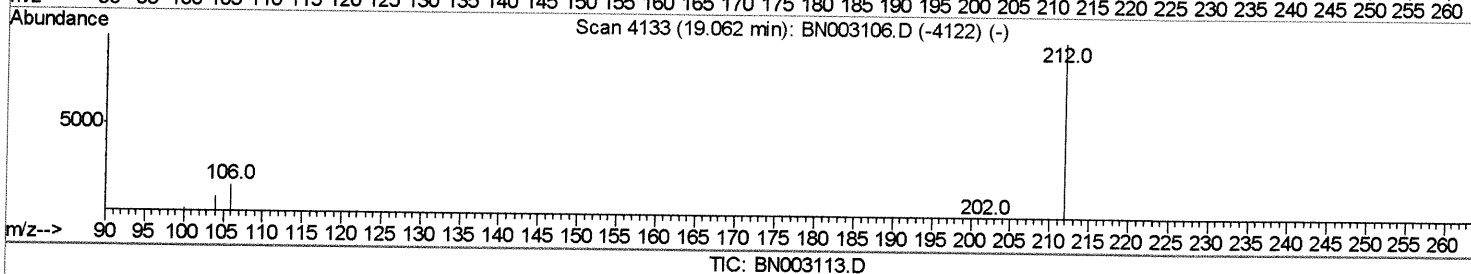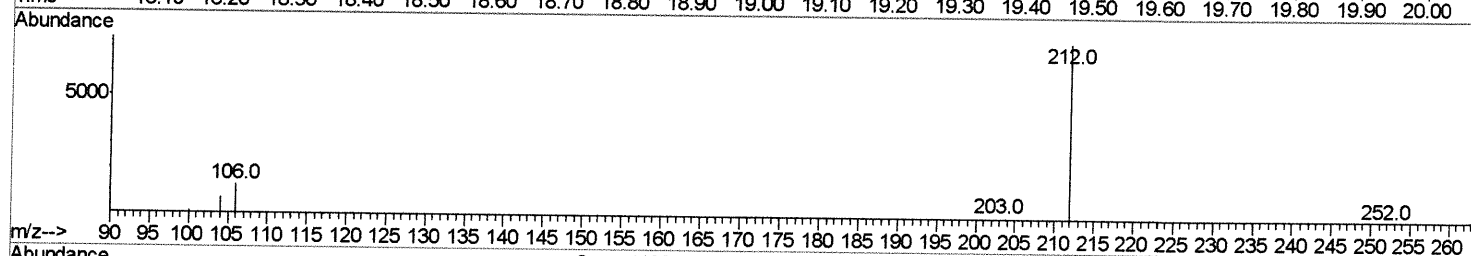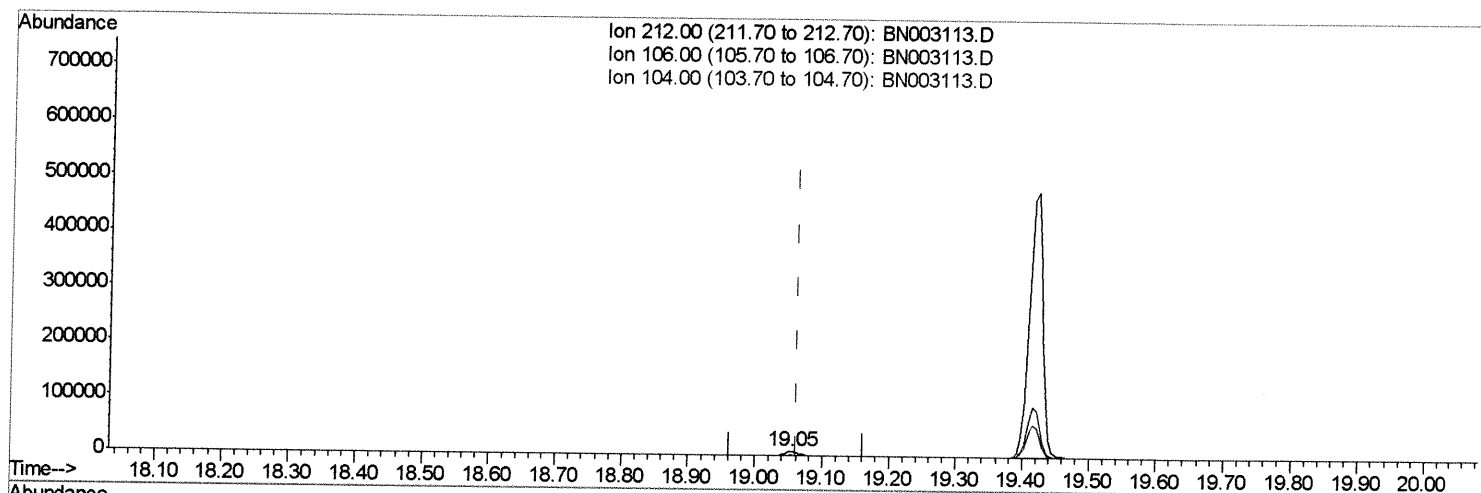

(14) Fluoranthene-d10 (SURR)

19.053min (-0.009) 0.36ng/ul m > SJ 10/12/18

response 9750

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

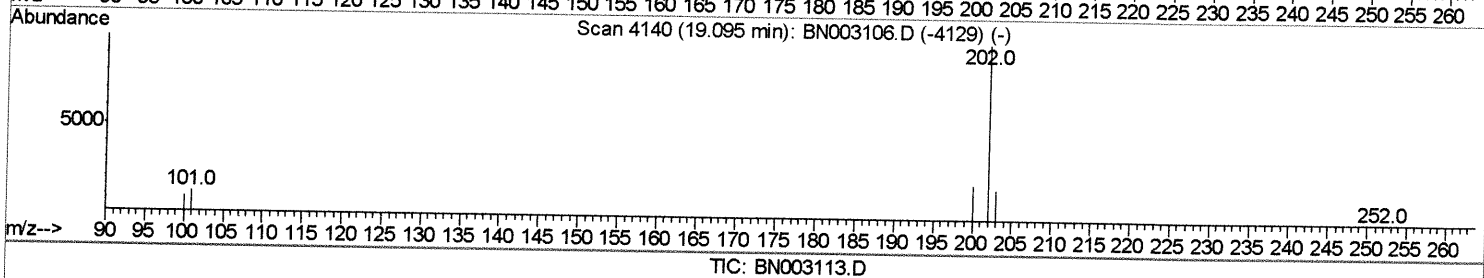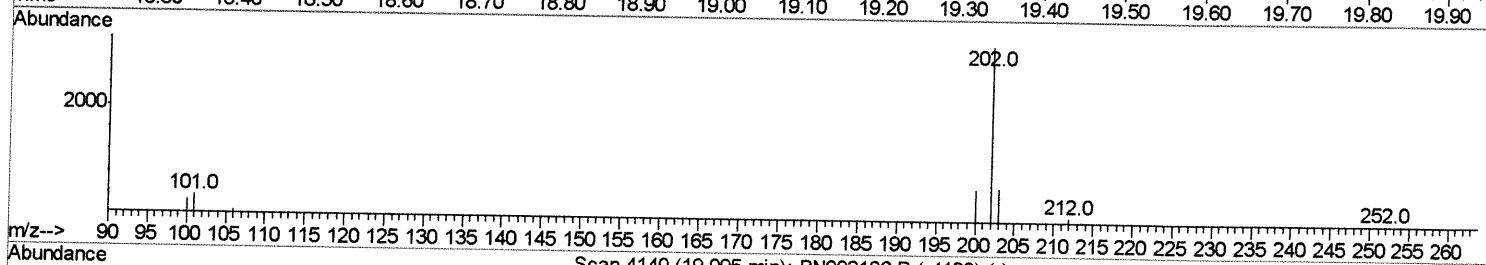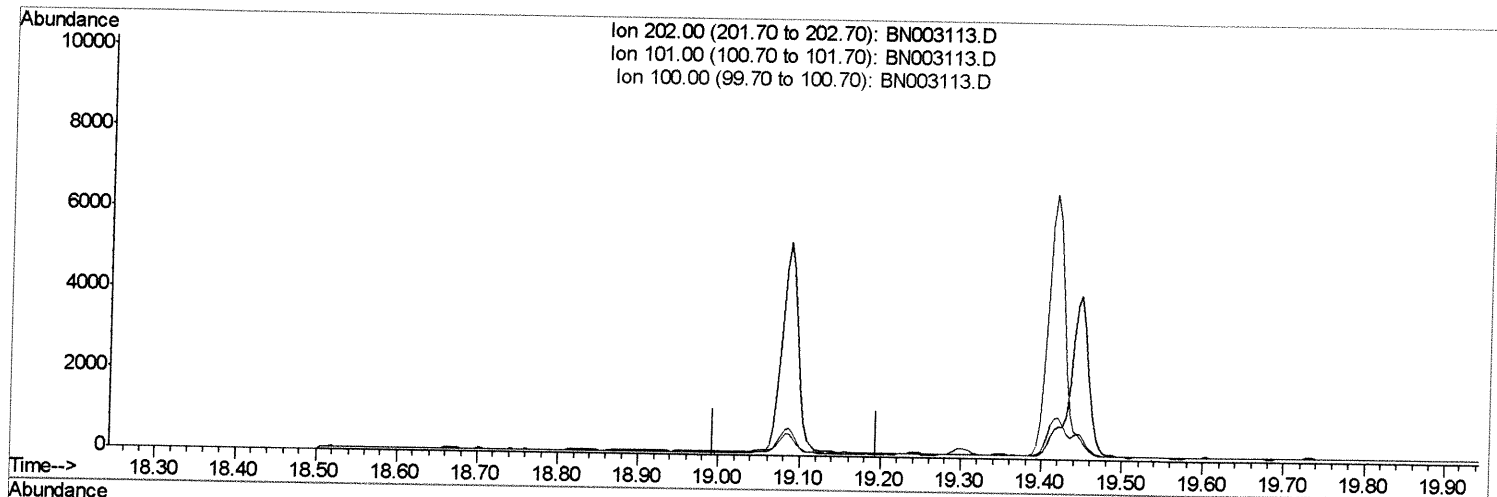

TIC: BN003113.D

(15) Fluoranthene (C)

19.095min (-19.095) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

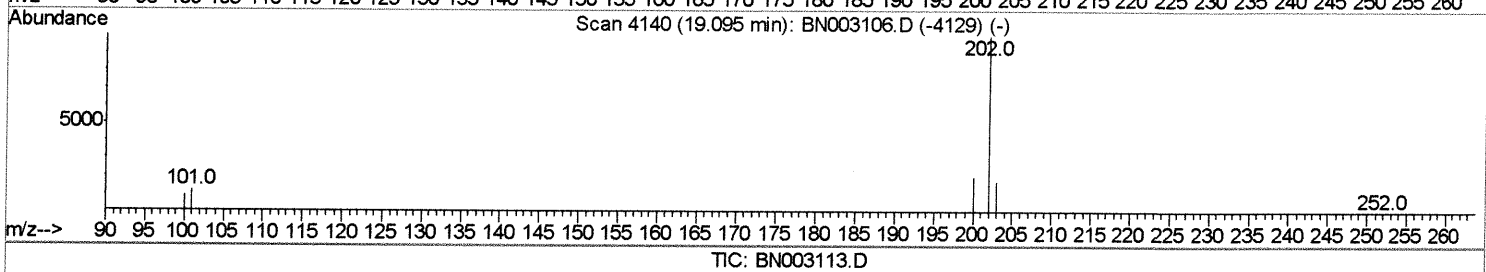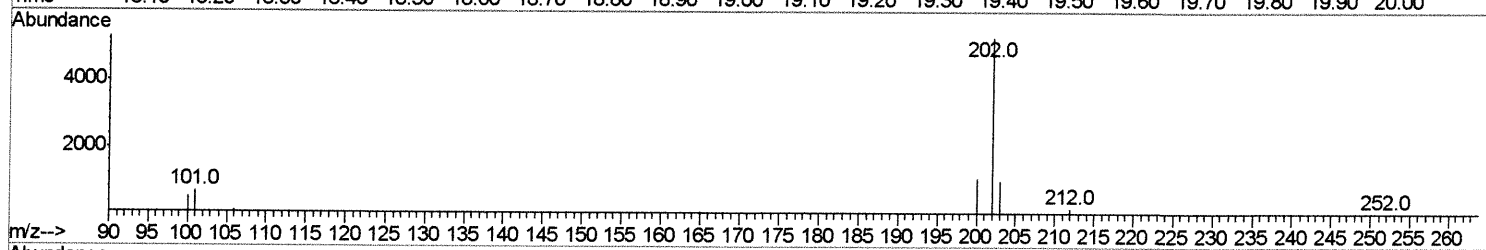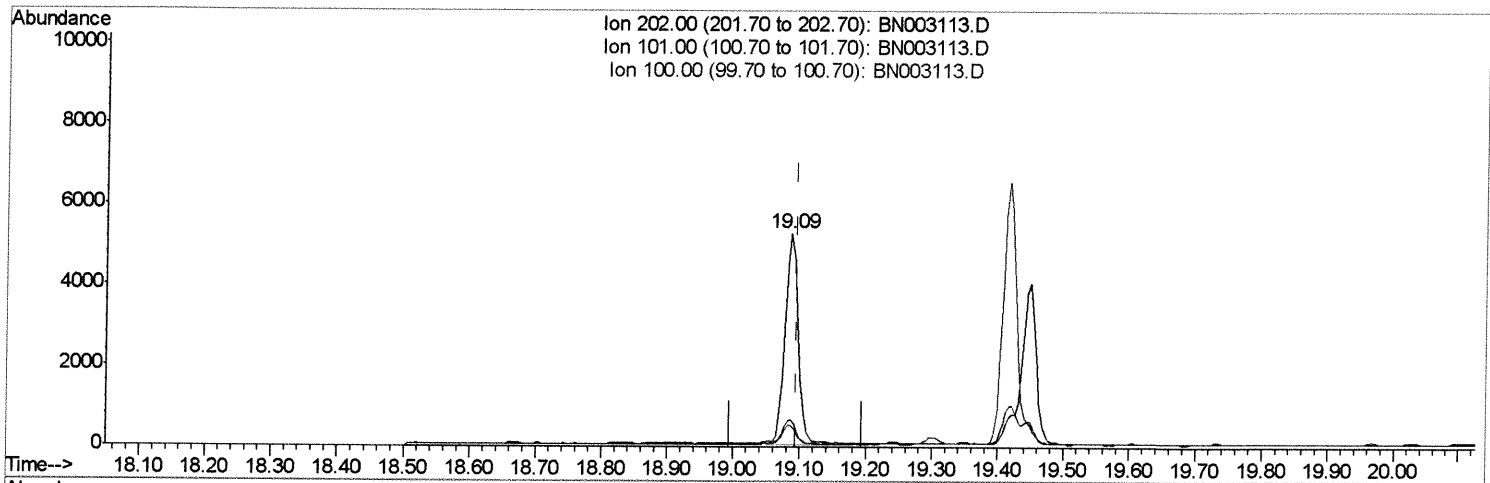

(15) Fluoranthene (C)

19.085min (-0.009) 0.24ng/ul m > SD 10/12/18

response 7332

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.19
100.00	9.10	10.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

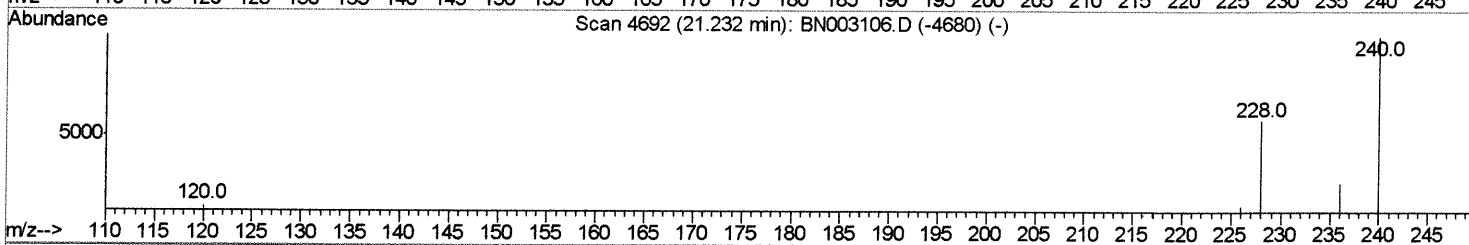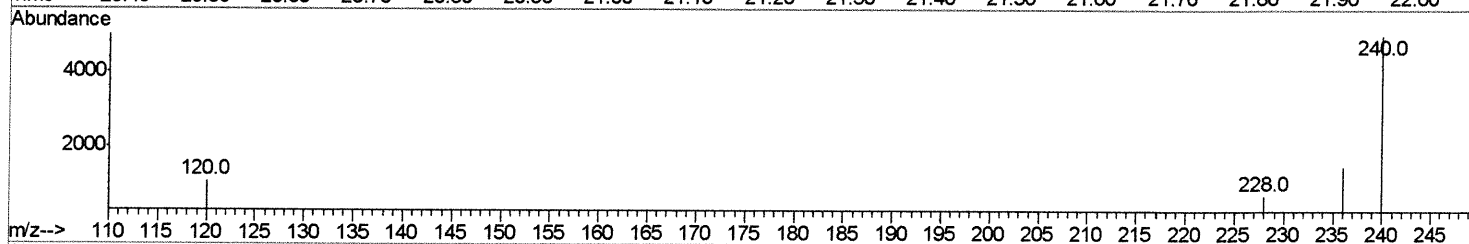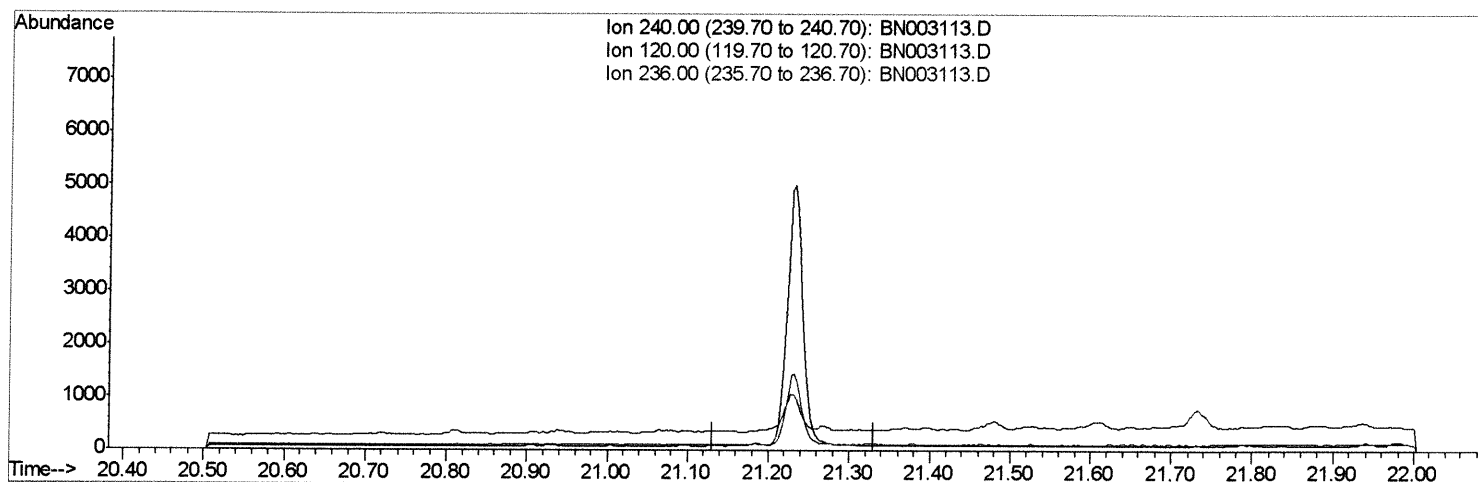

TIC: BN003113.D

(16) Chrysene-d12 (I)

21.232min (-21.232) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

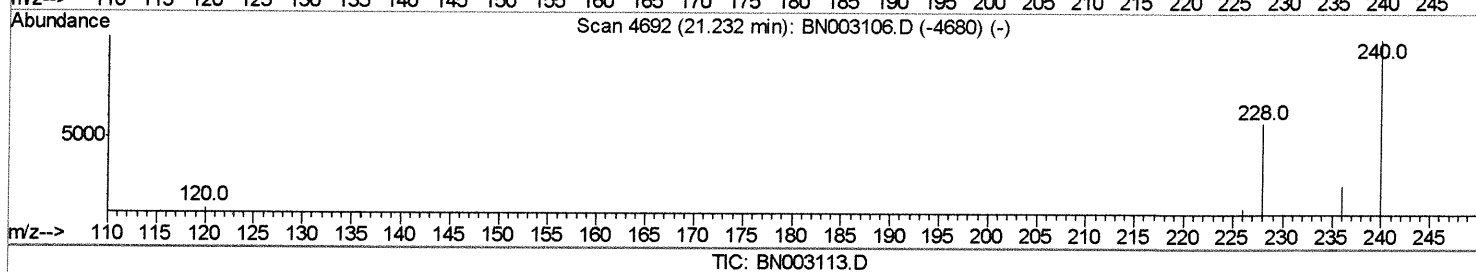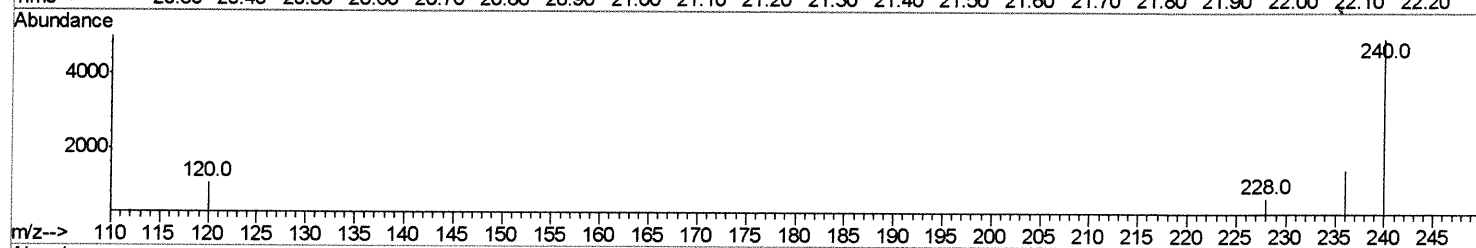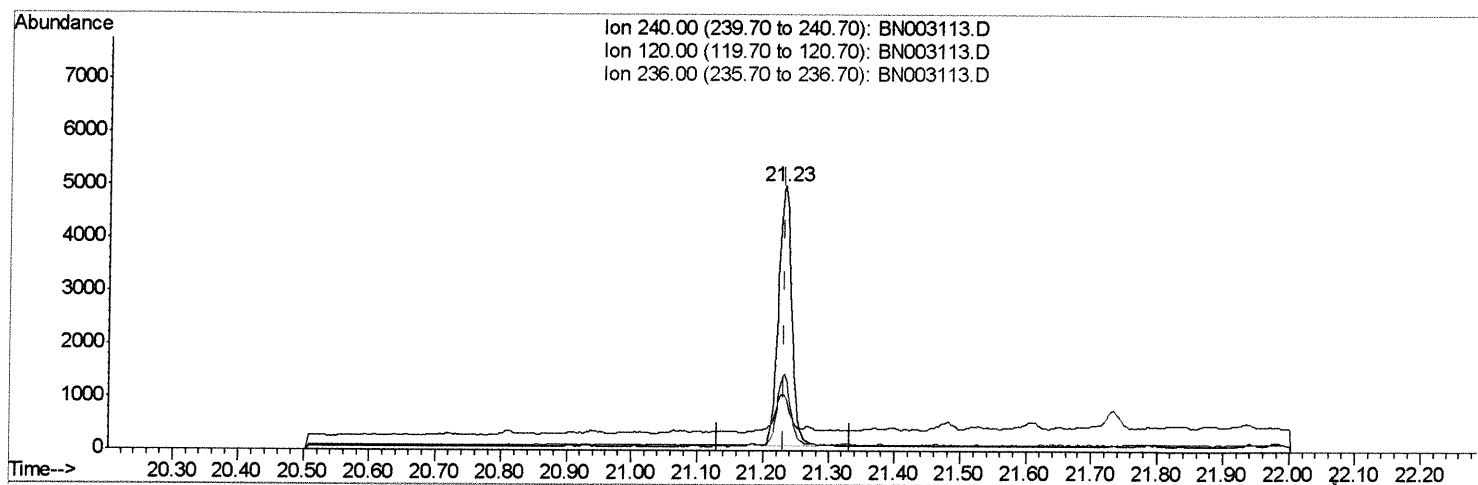

(16) Chrysene-d12 (I)

21.232min (-0.000) 0.40ng/ul m > SJ 10/12/18

response 6810

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	21.14#
236.00	28.10	29.21
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

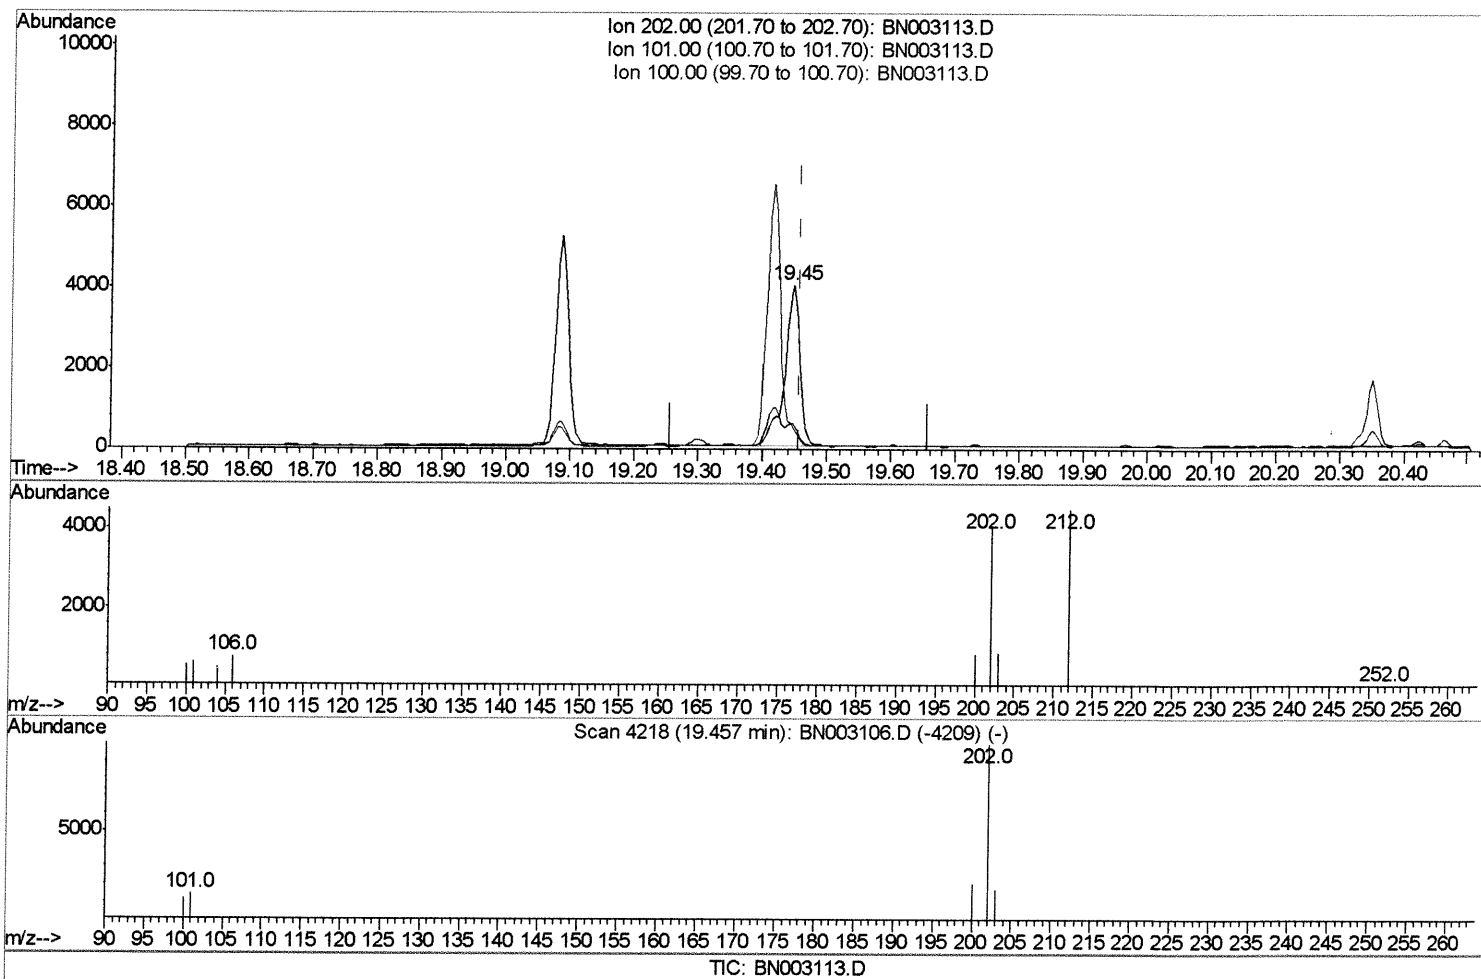

(17) Pyrene

19.448min (-0.009) 0.25ng/ul

response 6533

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	15.40
100.00	12.40	13.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:49:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

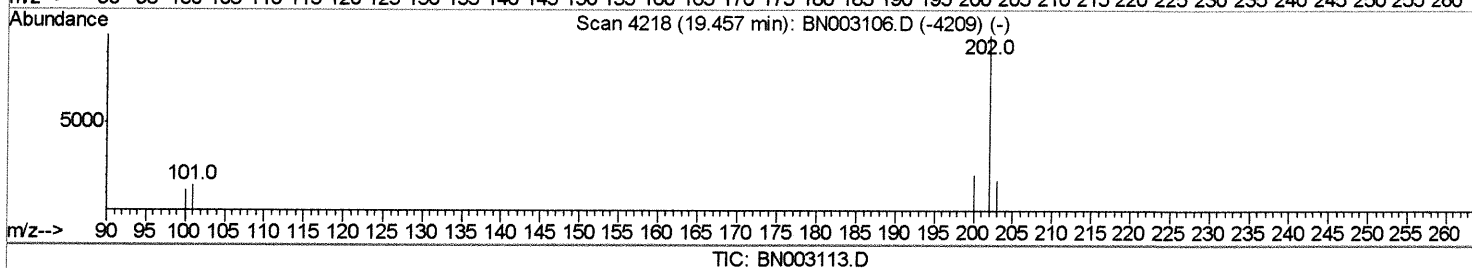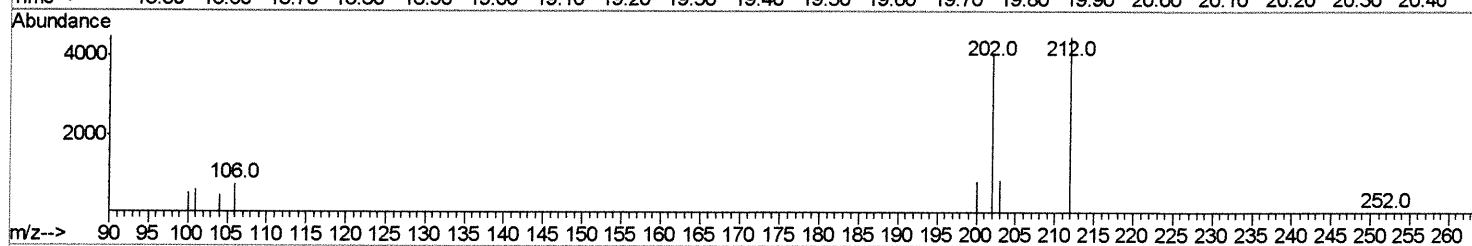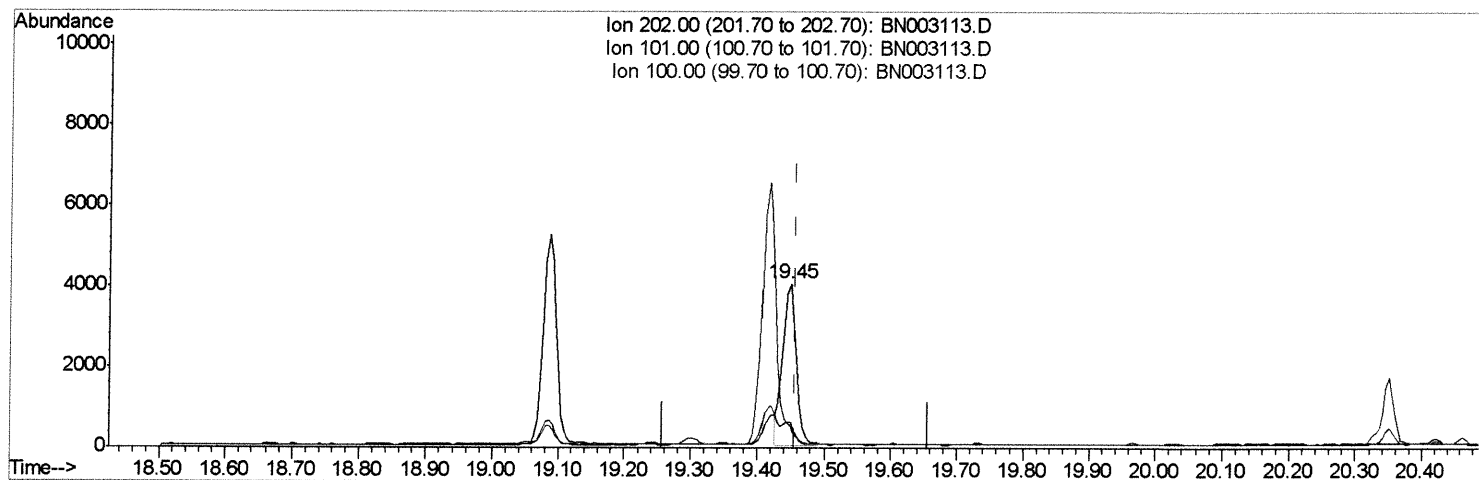

(17) Pyrene

19.448min (-0.009) 0.22ng/ul m > SJ 10/12/18

response 5822

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	15.40
100.00	12.40	13.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:49:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

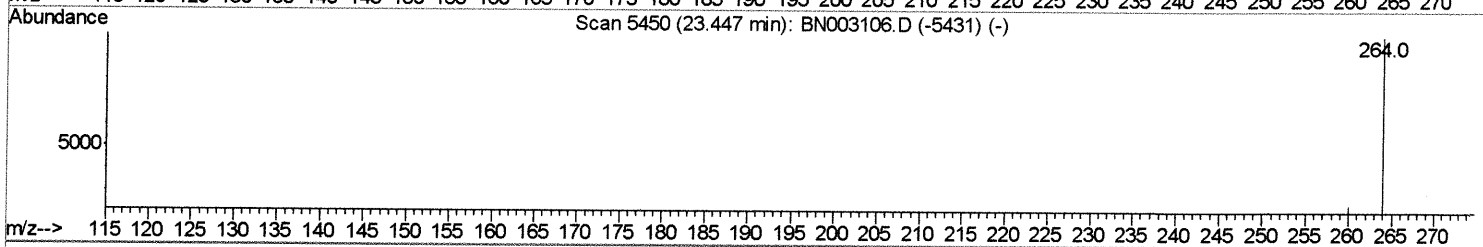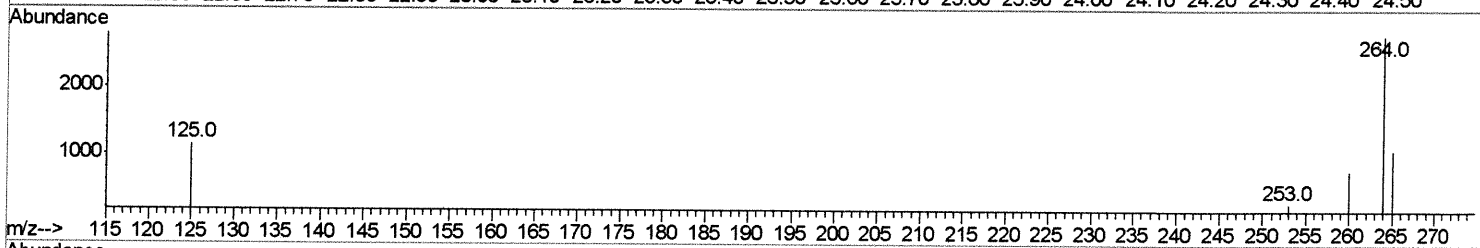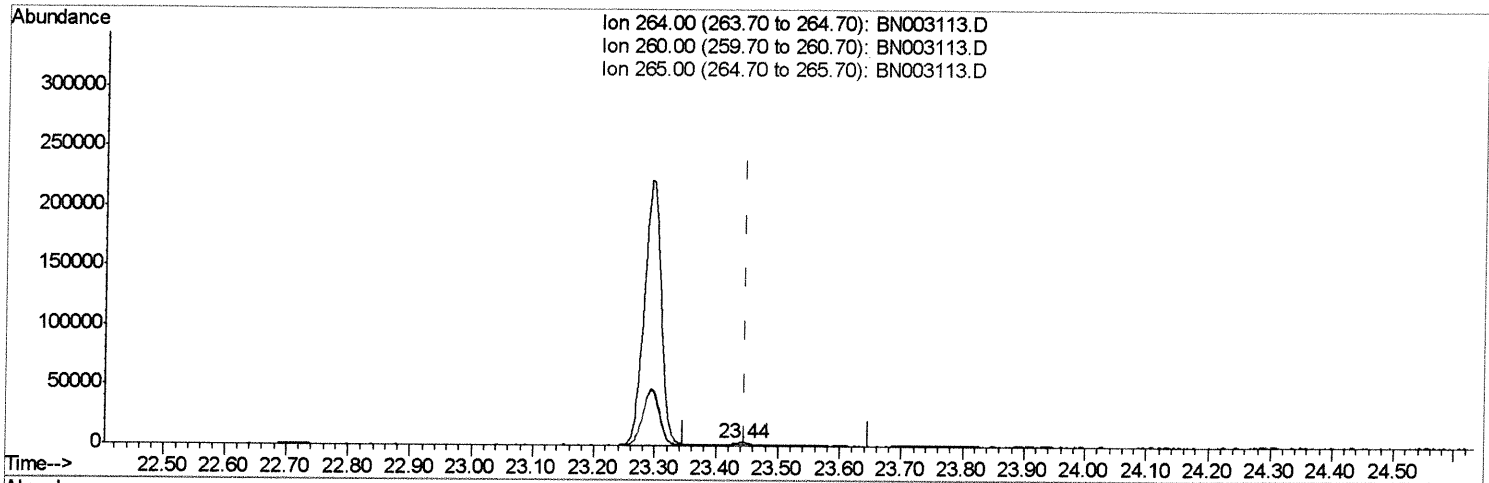

TIC: BN003113.D

(20) Perylene-d12 (I)
 23.441min (-0.006) 0.40ng/ul
 response 6026

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	28.00
265.00	45.40	38.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:49:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

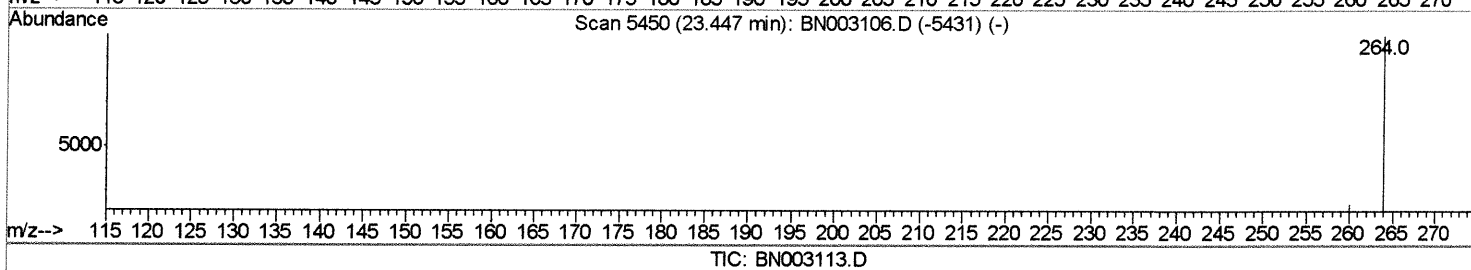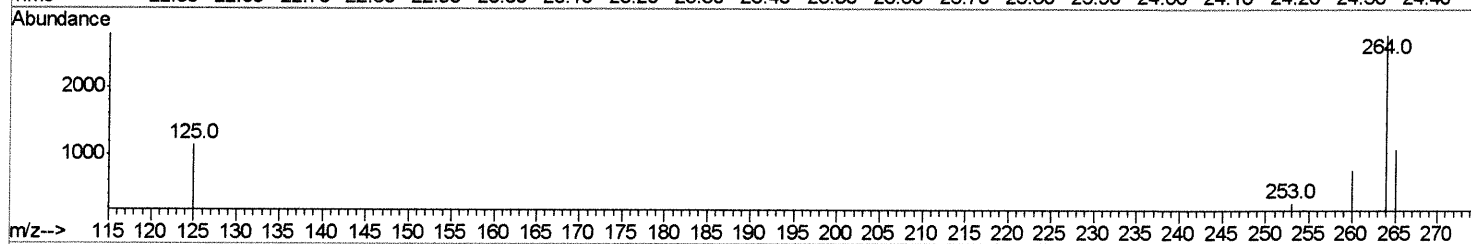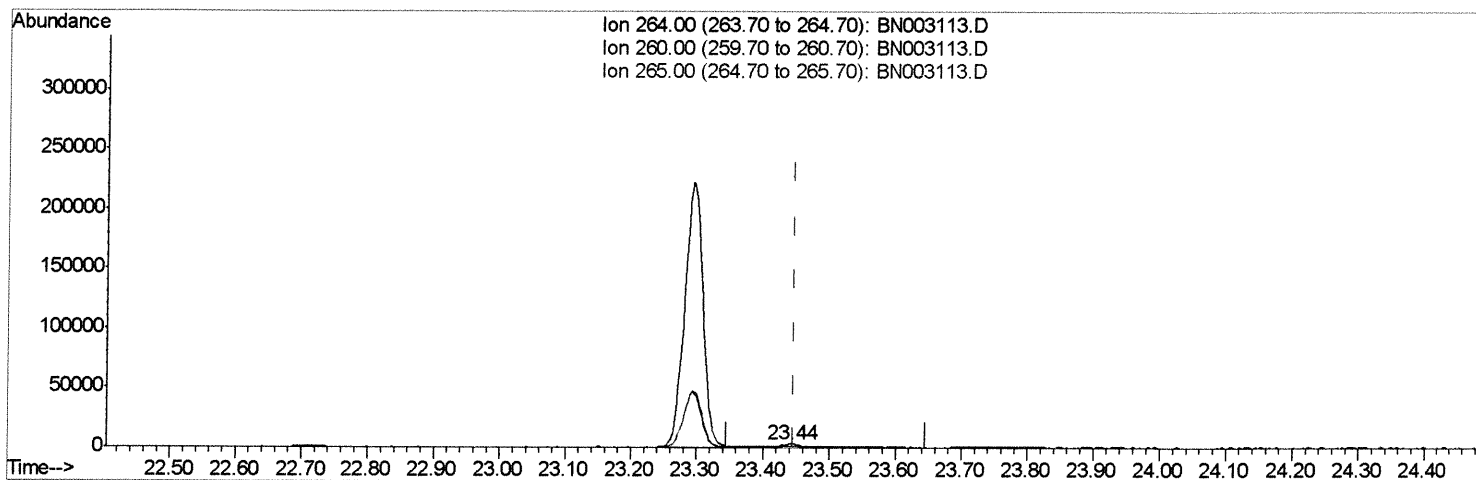

(20) Perylene-d12 (I)

23.441min (-0.006) 0.40ng/ul m

SJ 10/12/18

response 4937

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	28.00
265.00	45.40	38.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:50:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

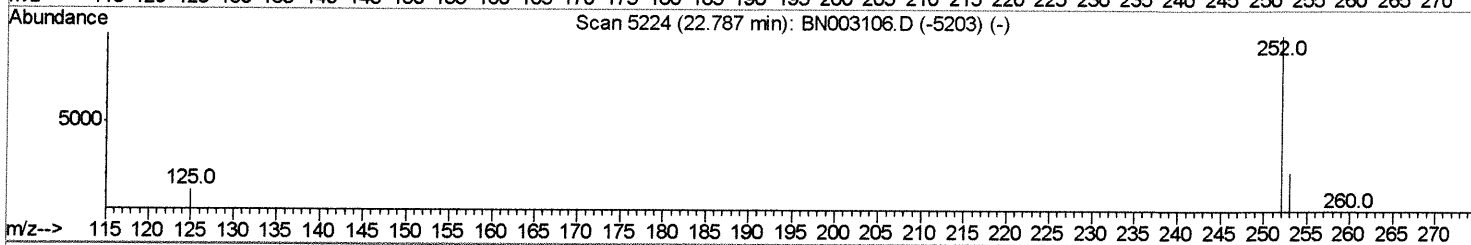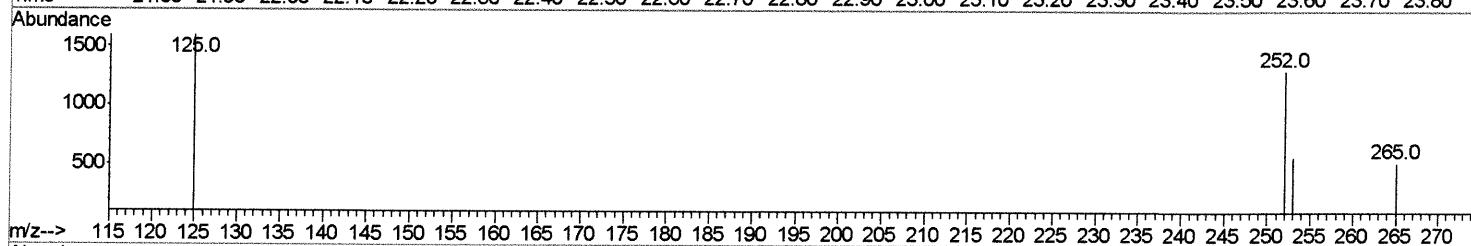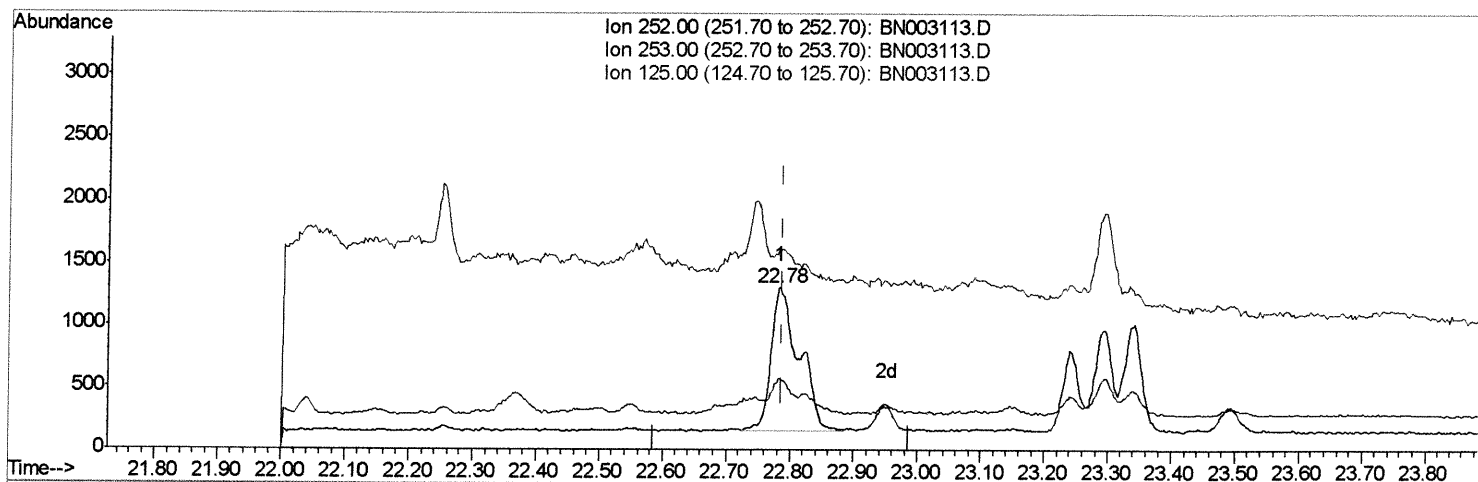

TIC: BN003113.D

(21) Benzo(b)fluoranthene

22.784min (-0.003) 0.20ng/ul

response 3490

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	43.75
125.00	17.10	122.26#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3YZ8

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:50:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

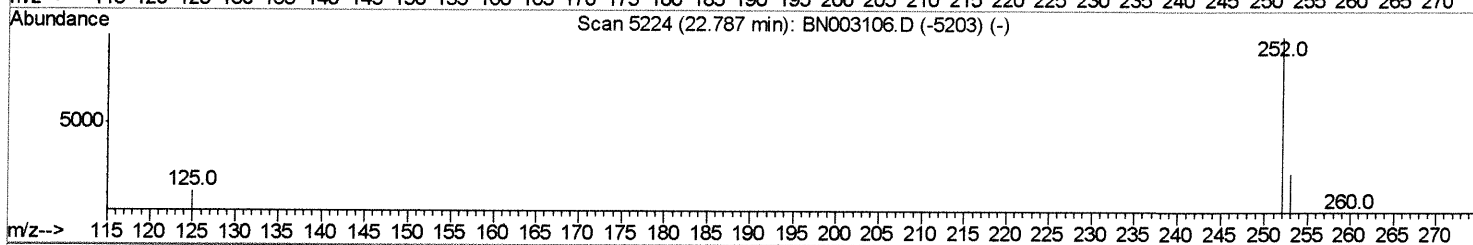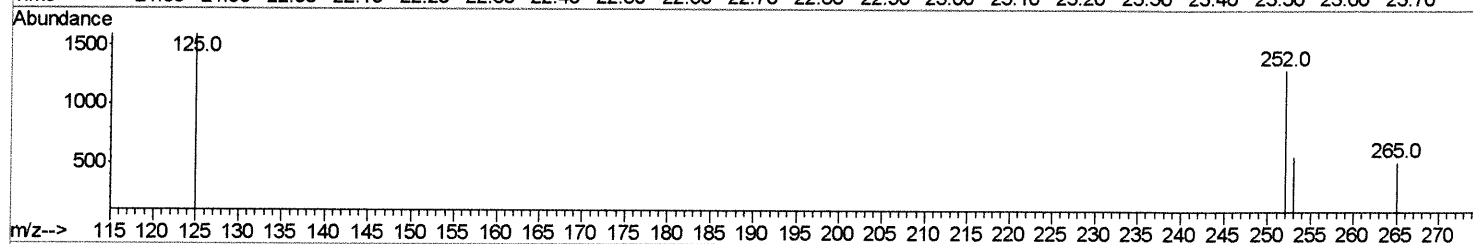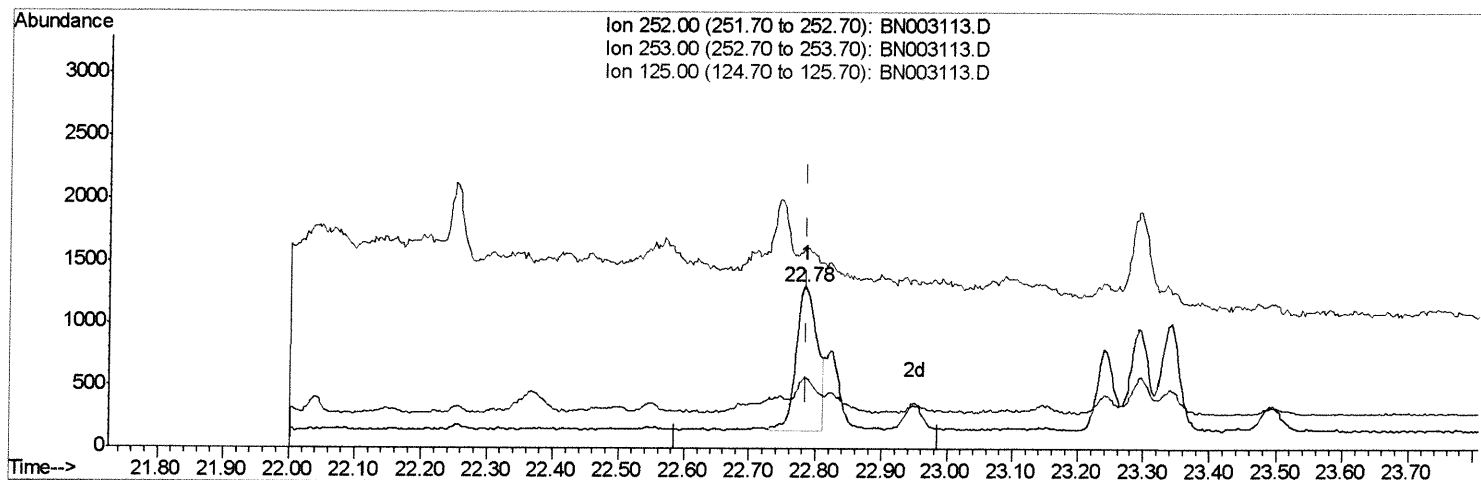

TIC: BN003113.D

(21) Benzo(b)fluoranthene

22.784min (-0.003) 0.14ng/ul m> SJ 10/12/18

response 2548

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	43.75
125.00	17.10	122.26#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:50:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

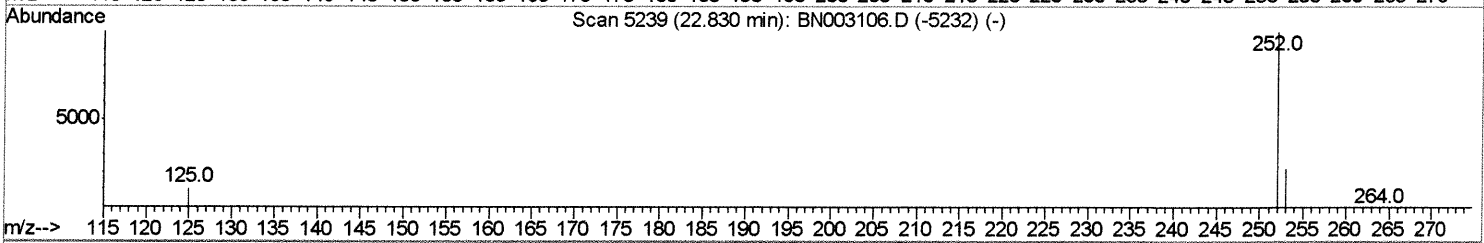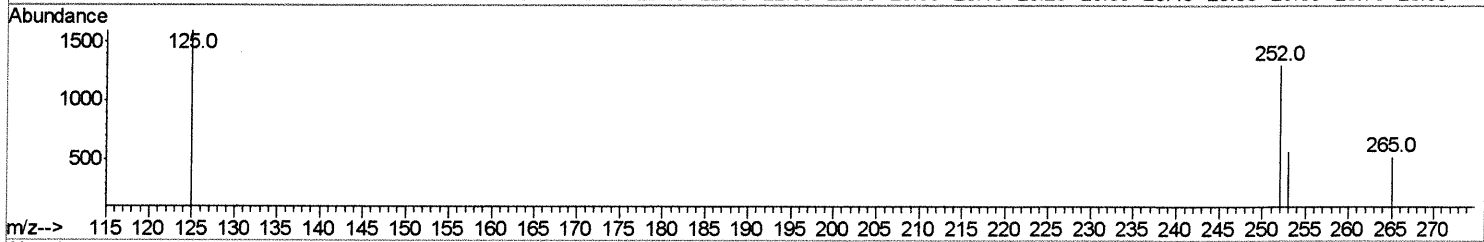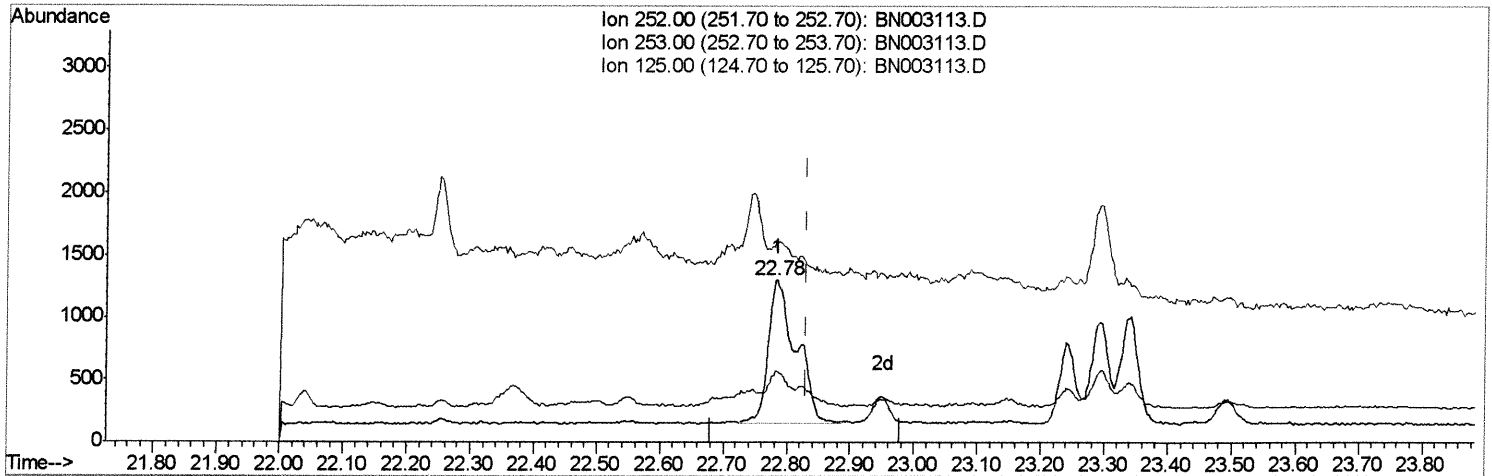

TIC: BN003113.D

(22) Benzo(k)fluoranthene
 22.784min (-0.047) 0.19ng/ul
 response 3490

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	43.75#
125.00	17.60	122.26#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:50:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

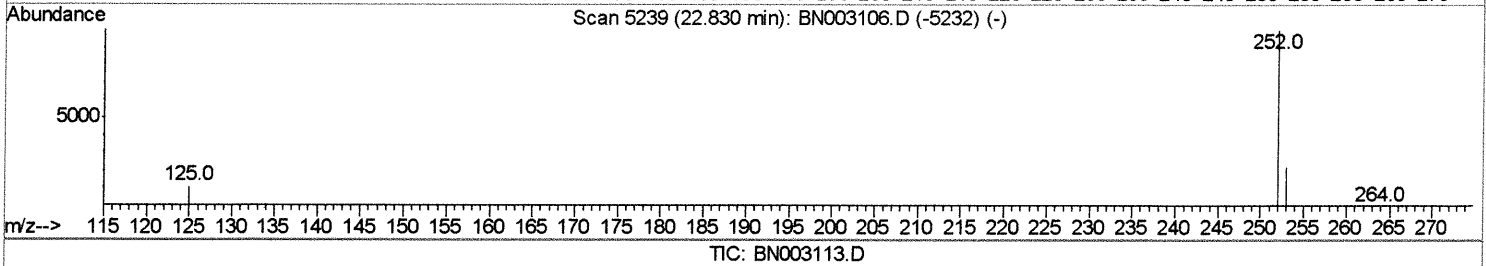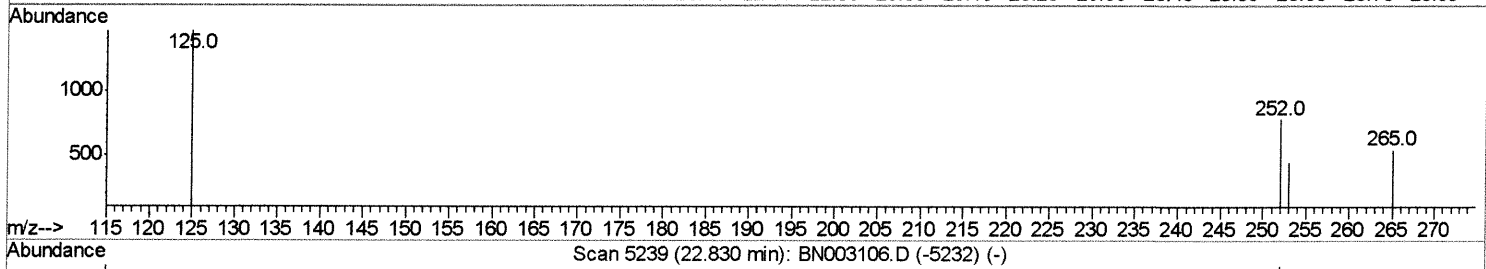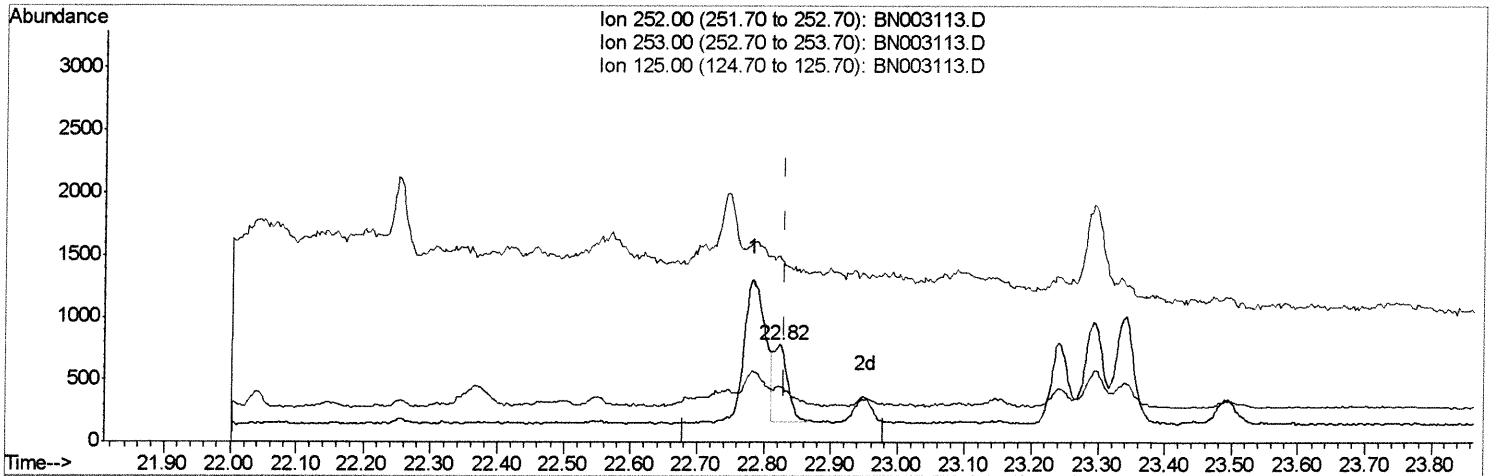

(22) Benzo(k)fluoranthene

22.825min (-0.006) 0.05ng/ul m) SJ 10/12/18

response 940

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	57.03#
125.00	17.60	187.98#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003113.D
 Acq On : 11 Oct 2018 21:12
 Operator : MJ/SJ
 Sample : J5368-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YZ8

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:21 PM

Quant Time: Oct 12 06:51:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1685	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	7290	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4335	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	9500m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	6810m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4937m	0.40	ng/ul	0.00

SJ 10/12/18

System Monitoring Compounds
 4) 2-Methylnaphthalene-d10
 14) Fluoranthene-d10

12.01	152	3980	0.35	ng/ul	0.00
19.05	212	9750m	0.36	ng/ul	0.00

SJ 10/12/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
9) Fluorene	15.32	166	354	0.021	ng/ul#	87
12) Phenanthrene	17.06	178	5674	0.214	ng/ul	98
13) Anthracene	17.15	178	1408m	0.056	ng/ul	
15) Fluoranthene	19.09	202	7332m	0.236	ng/ul	
17) Pyrene	19.45	202	5822m	0.220	ng/ul	
18) Benzo(a)anthracene	21.22	228	2641	0.121	ng/ul#	88
19) Chrysene	21.27	228	2384	0.107	ng/ul#	88
21) Benzo(b)fluoranthene	22.78	252	2548m	0.143	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	940m	0.051	ng/ul	
23) Benzo(a)pyrene	23.34	252	1652	0.104	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	25.68	276	1137	0.062	ng/ul#	49
26) Benzo(g,h,i)perylene	26.35	276	1073	0.069	ng/ul#	50

SJ 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed