


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z10DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:31 PM

Quant Time: Oct 12 07:27:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

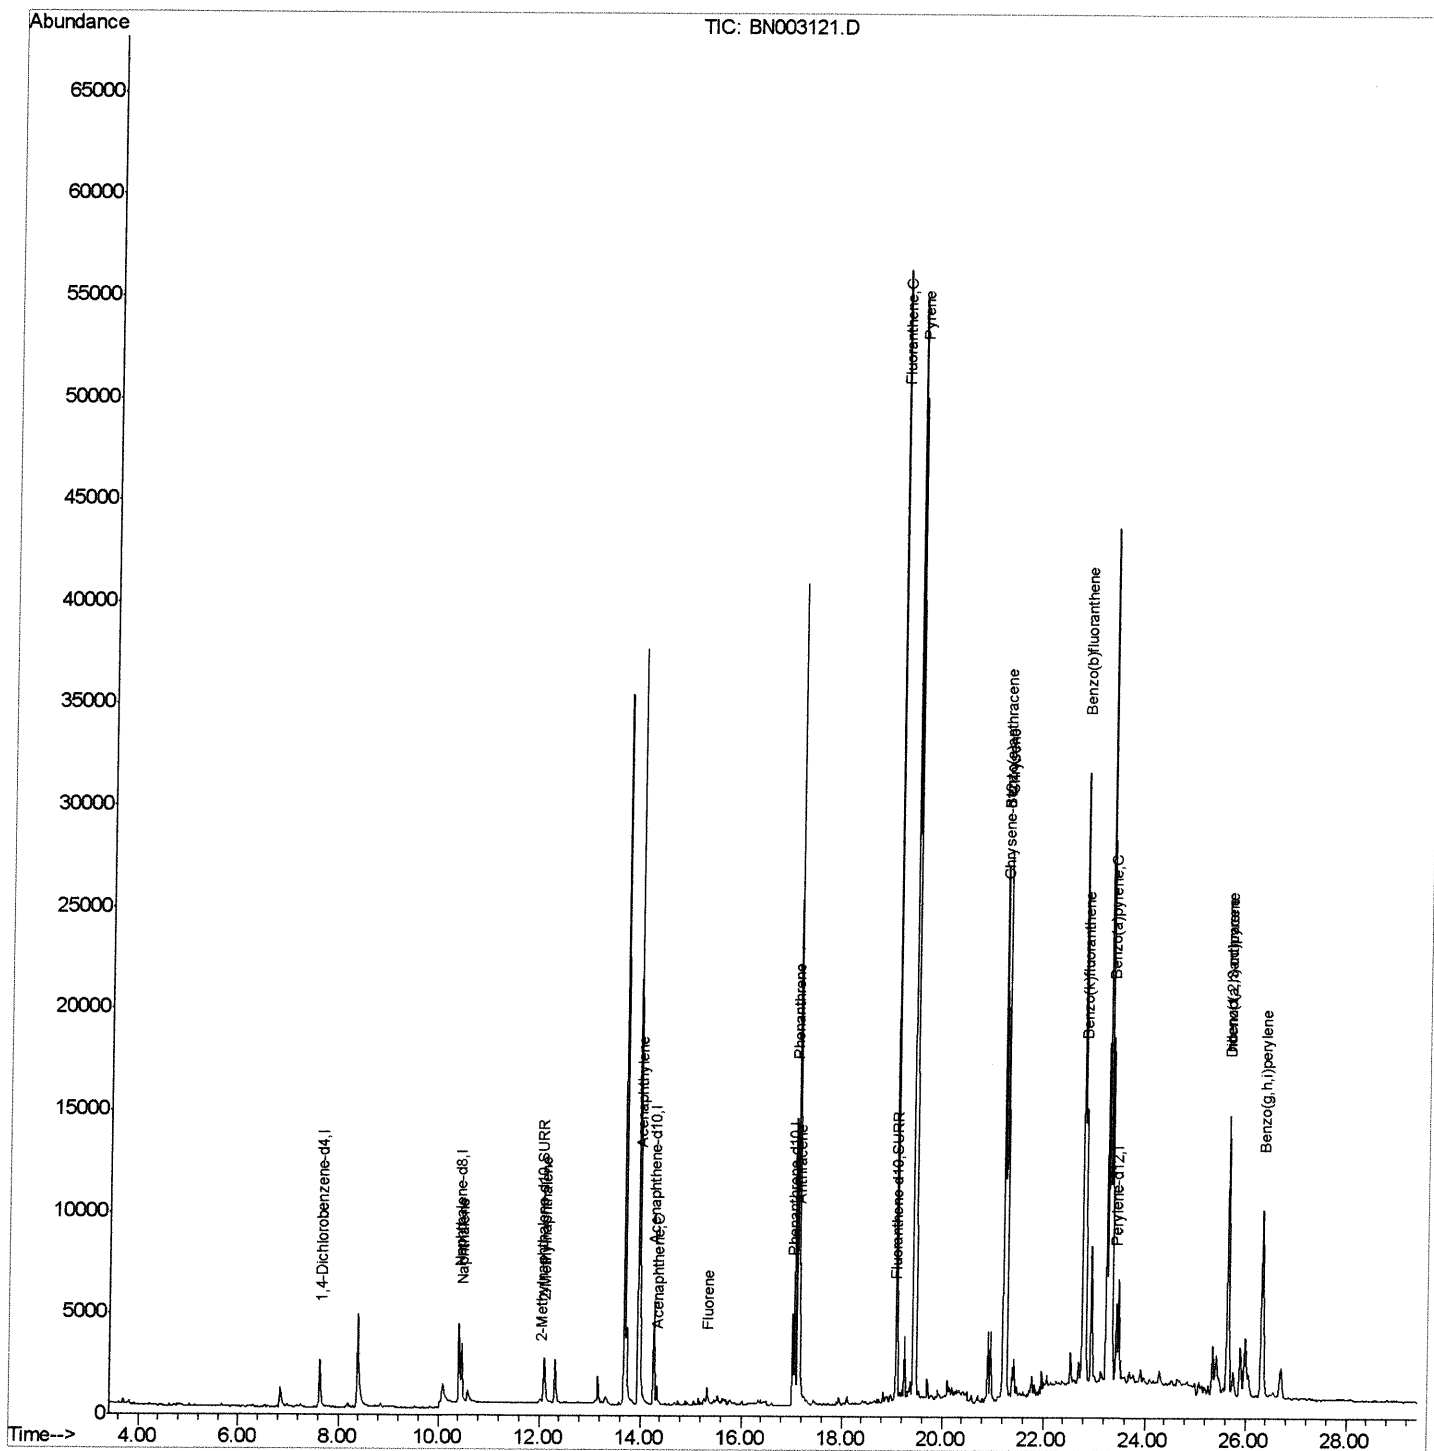

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3Z10DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:31 PM

Quant Time: Oct 12 05:38:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

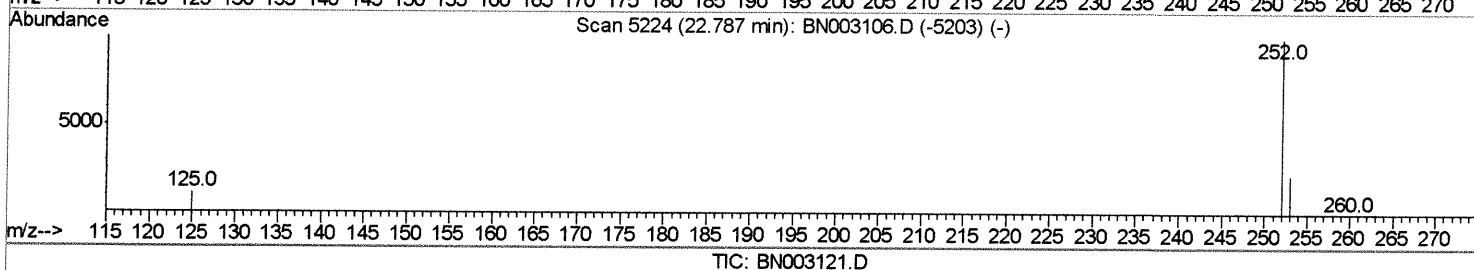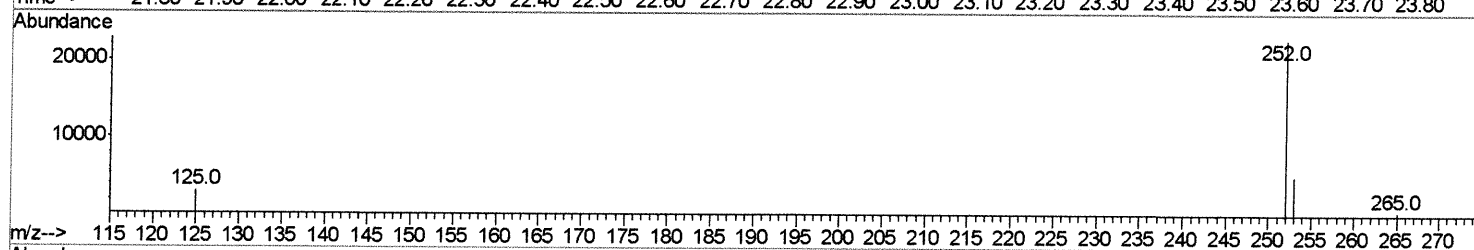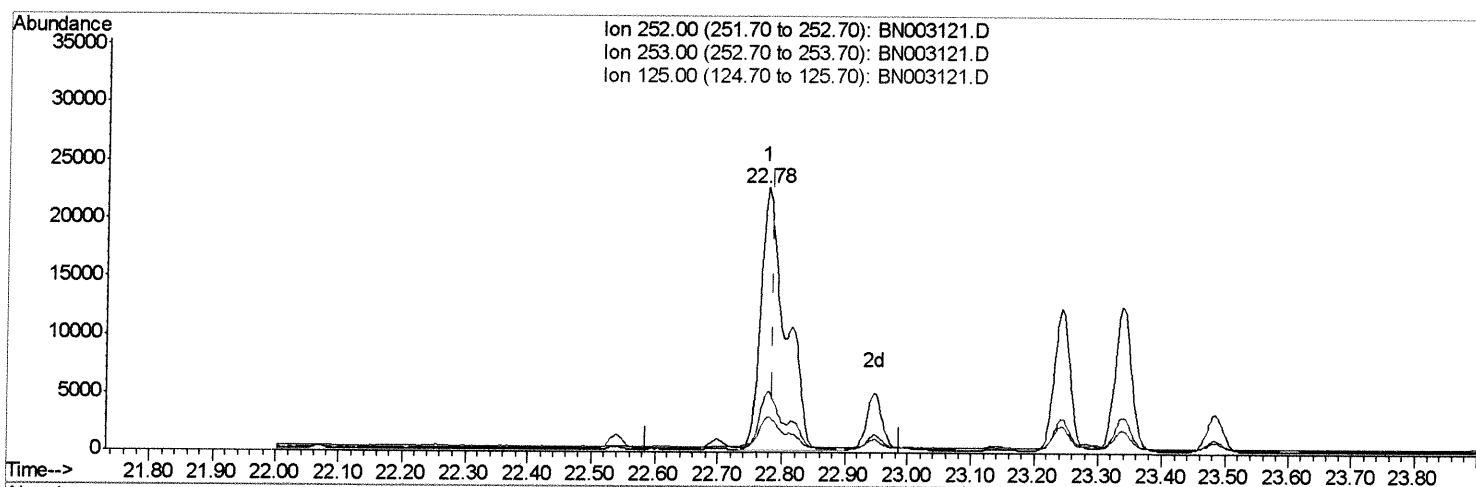

(21) Benzo(b)fluoranthene

22.775min (-0.012) 3.01ng/ul

response 61496

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.60
125.00	17.10	13.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z10DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:31 PM

Quant Time: Oct 12 05:38:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

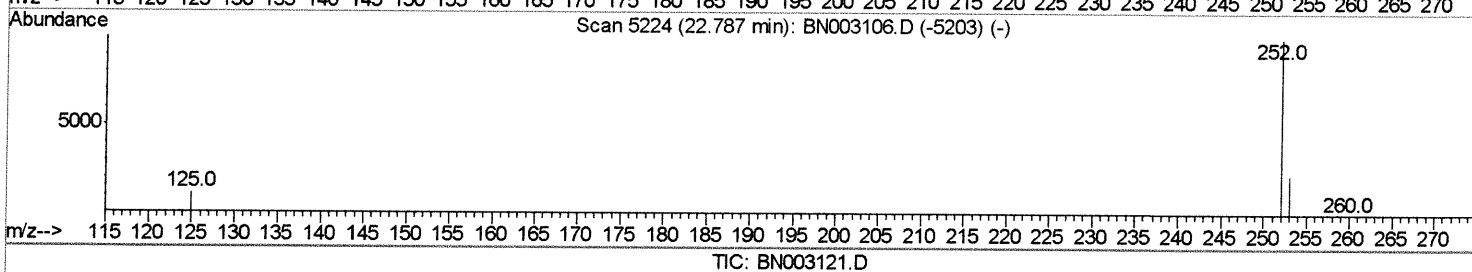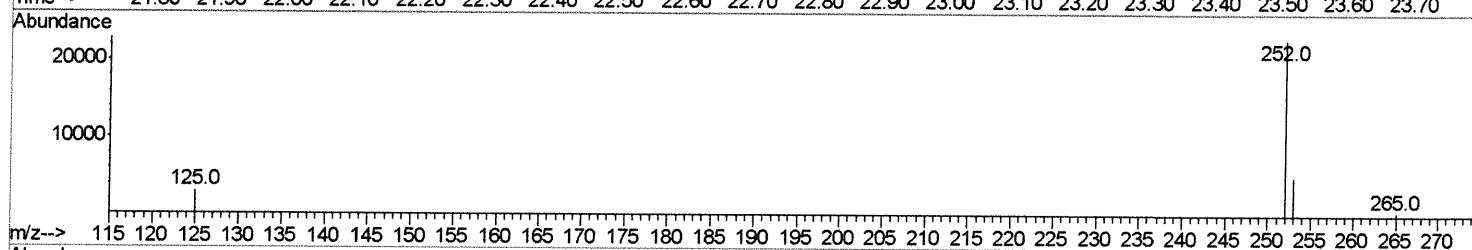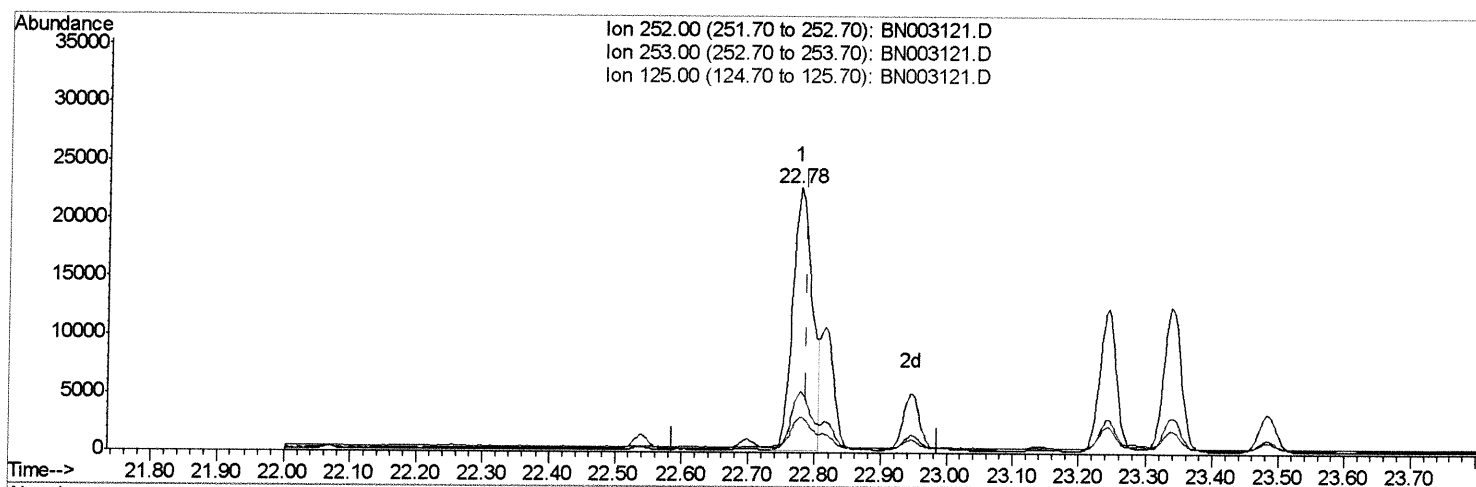

(21) Benzo(b)fluoranthene

22.775min (-0.012) 2.27ng/ul m) 50 10/14/18

response 46304

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.60
125.00	17.10	13.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z10DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:31 PM

Quant Time: Oct 12 05:38:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

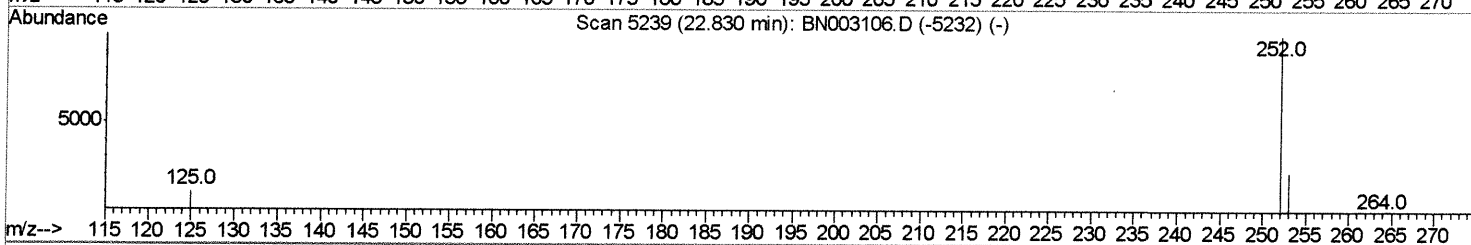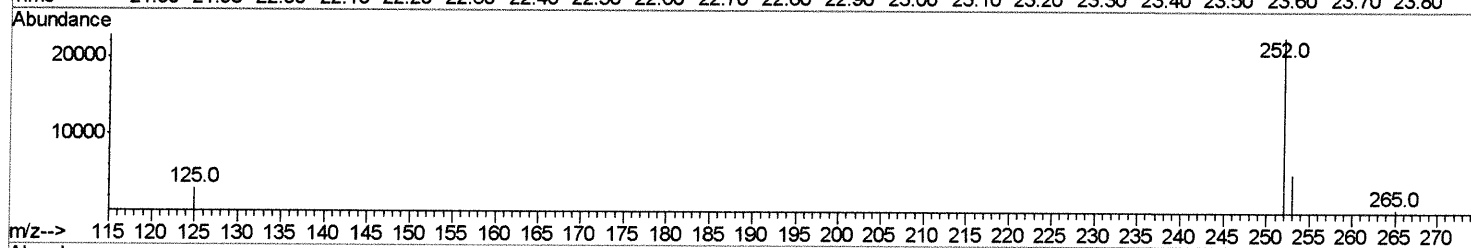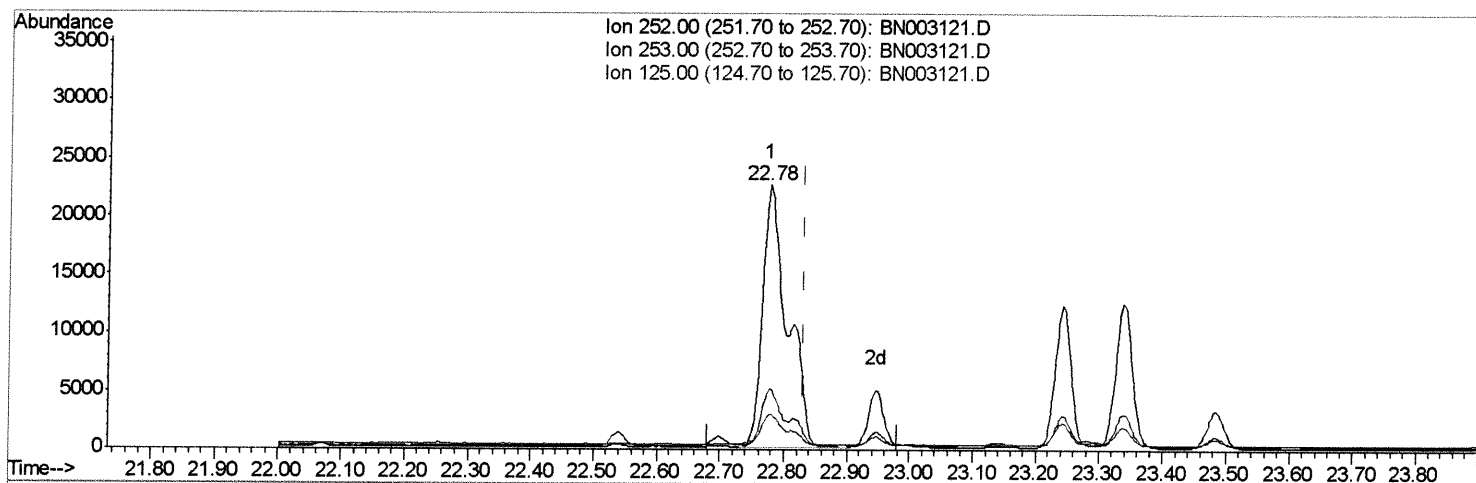

TIC: BN003121.D

(22) Benzo(k)fluoranthene

22.775min (-0.055) 2.90ng/ul

response 61496

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.60
125.00	17.60	13.34#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003121.D
Acq On : 12 Oct 2018 01:53
Operator : MJ/SJ
Sample : J5230-13DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A3Z10DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:38:31 PM

Quant Time: Oct 12 05:38:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

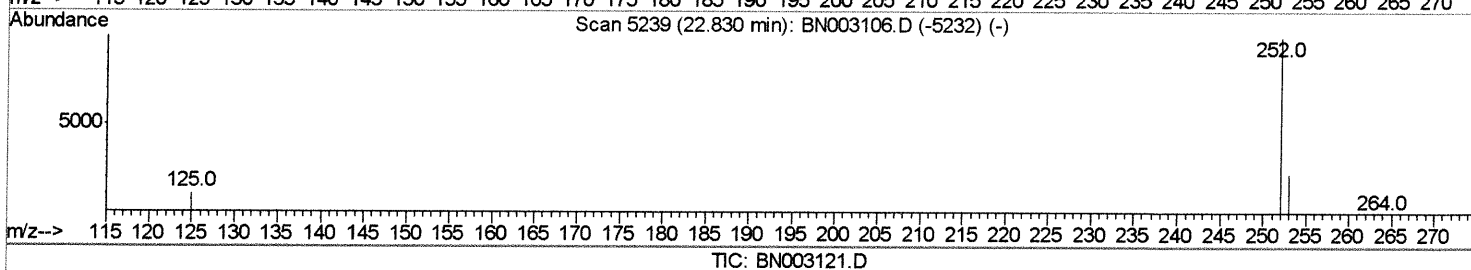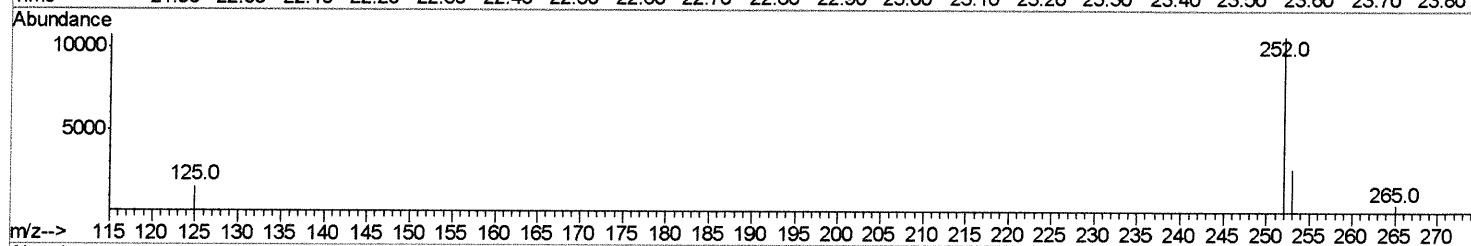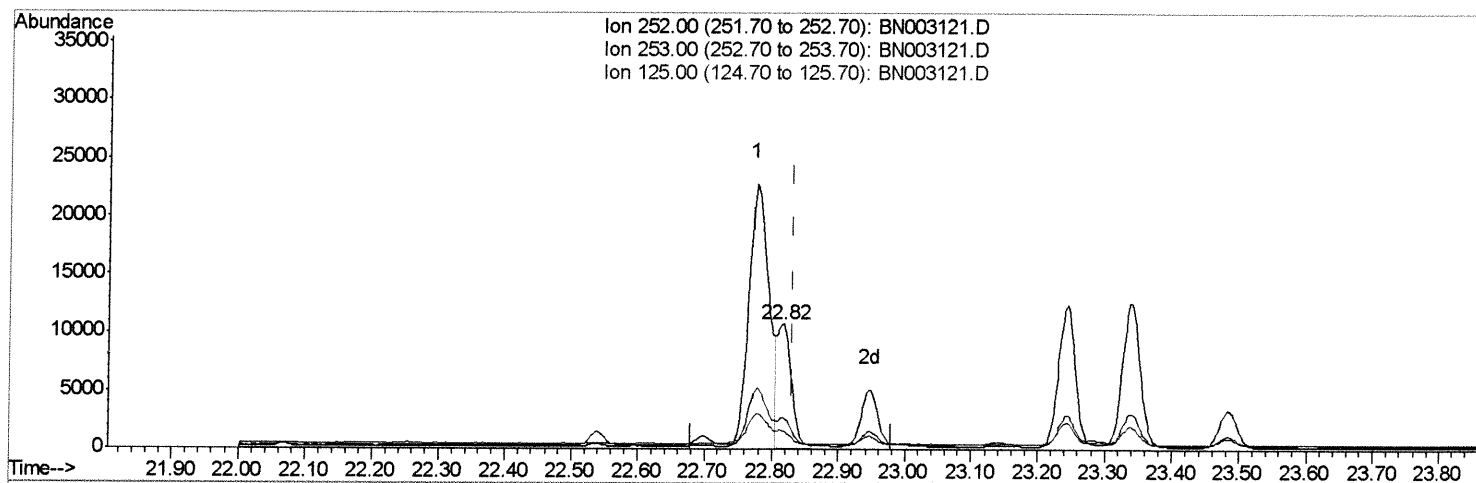

(22) Benzo(k)fluoranthene

22.816min (-0.014) 0.75ng/ul m

response 15877

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.21
125.00	17.60	14.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003121.D
 Acq On : 12 Oct 2018 01:53
 Operator : MJ/SJ
 Sample : J5230-13DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z10DL

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:38:31 PM

Quant Time: Oct 12 07:27:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1574	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.40	136	6161	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	2960	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	5447	0.40	ng/ul	-0.01
16) Chrysene-d12	21.22	240	4739	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	5671	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.01	152	420	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	740	0.05	ng/ul	0.00

Target Compounds

						Ovalue
3) Naphthalene	10.45	128	4656	0.294	ng/ul	99
5) 2-Methylnaphthalene	12.08	142	2541	0.233	ng/ul	97
7) Acenaphthylene	13.98	152	8255	0.610	ng/ul	99
8) Acenaphthene	14.32	153	587	0.057	ng/ul	96
9) Fluorene	15.32	166	675	0.057	ng/ul#	89
12) Phenanthrene	17.06	178	16208	1.067	ng/ul	100
13) Anthracene	17.15	178	7545	0.526	ng/ul	99
15) Fluoranthene	19.09	202	47851	2.686	ng/ul	99
17) Pyrene	19.45	202	41806	2.271	ng/ul	97
18) Benzo(a)anthracene	21.21	228	22293	1.462	ng/ul	98
19) Chrysene	21.26	228	28007	1.809	ng/ul	99
21) Benzo(b)fluoranthene	22.78	252	46304m	2.267	ng/ul	90
22) Benzo(k)fluoranthene	22.82	252	15877m	0.750	ng/ul	
23) Benzo(a)pyrene	23.34	252	23138	1.264	ng/ul#	
24) Indeno(1,2,3-cd)pyrene	25.65	276	21474	1.021	ng/ul#	94
25) Dibenzo(a,h)anthracene	25.64	278	6007	0.357	ng/ul	94
26) Benzo(a,h,i)perylene	26.32	276	18572	1.047	ng/ul	95

SD 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed