
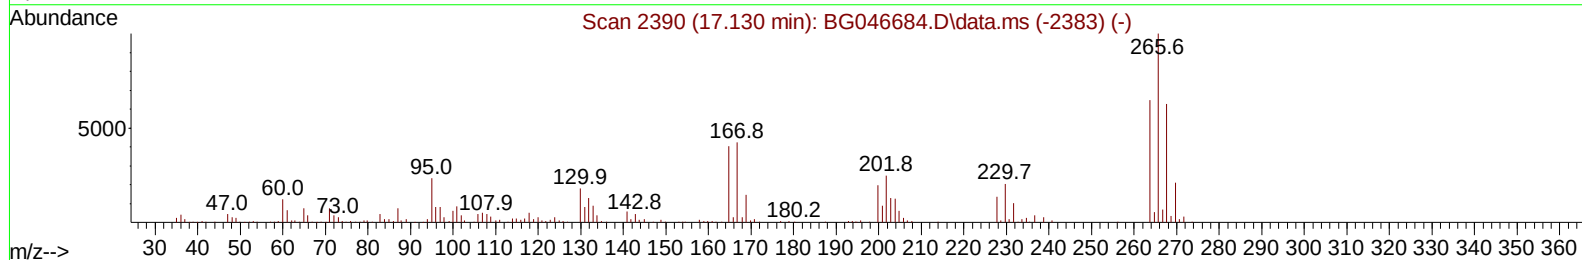
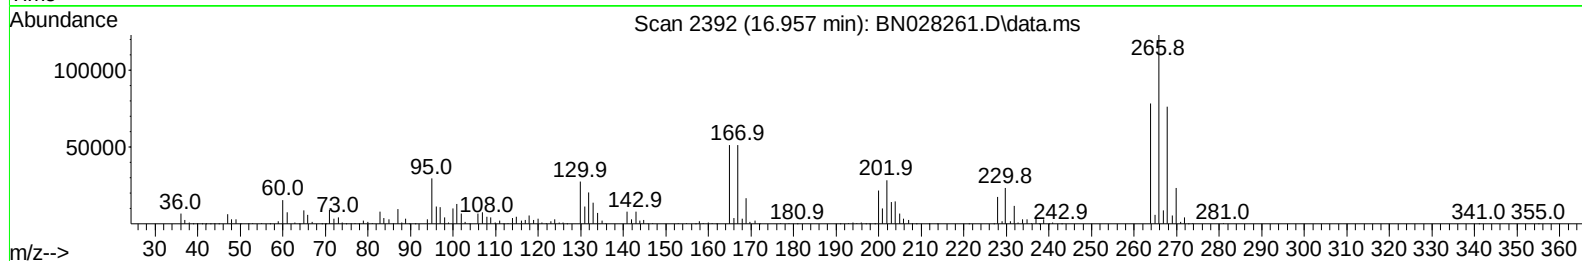


Quant Time: Oct 13 02:49:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 13 02:49:55 2023
Response via : Initial Calibration

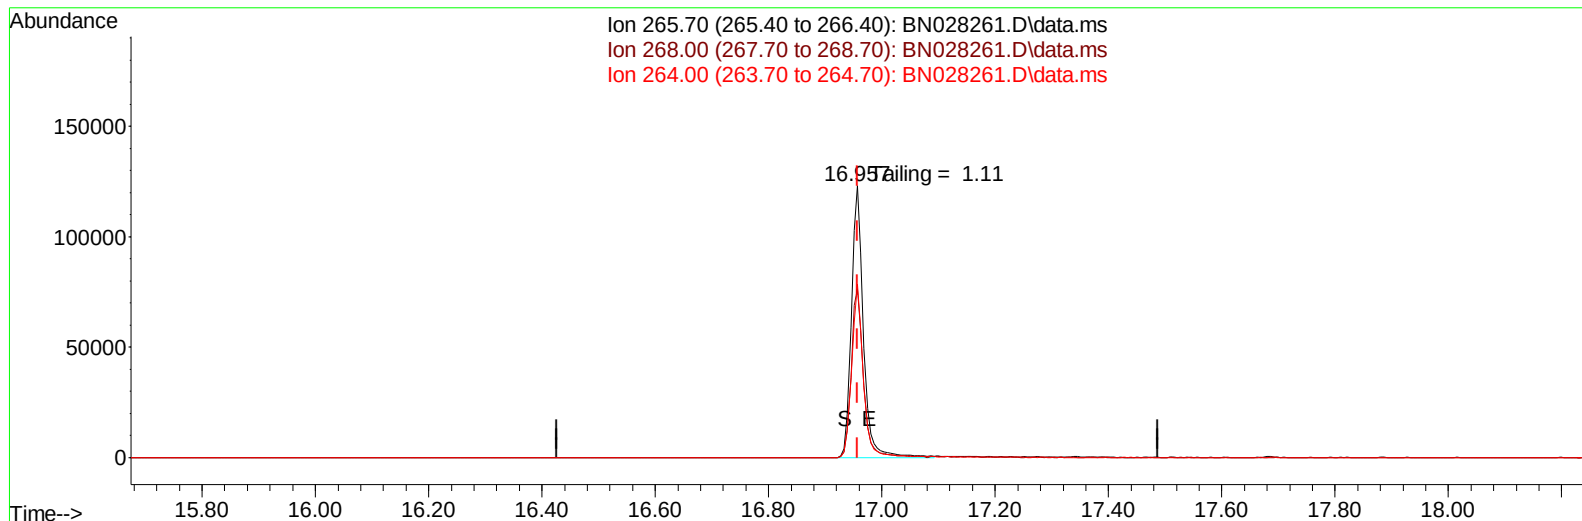

TIC: BN028261.D\data.ms




16.957min (0.000) 23122.20 ng

response **182183**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
Data File : BN028261.D
Acq On : 12 Oct 2023 14:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 02:49:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 13 02:49:55 2023
Response via : Initial Calibration

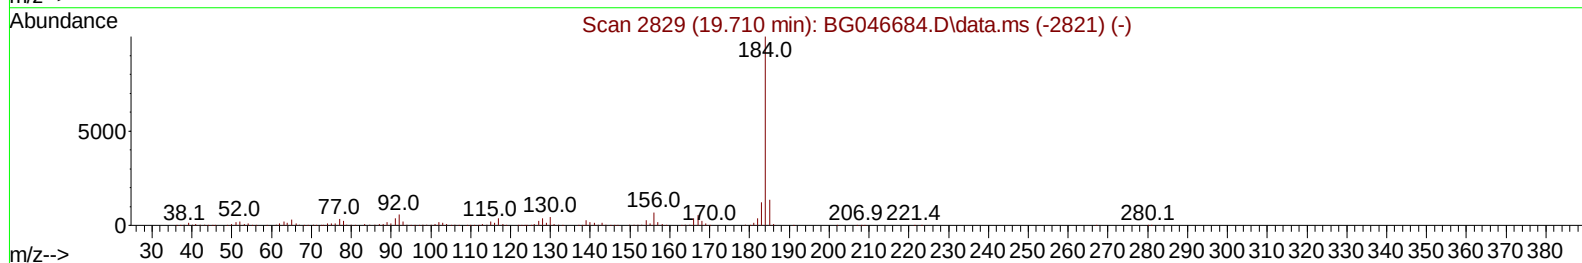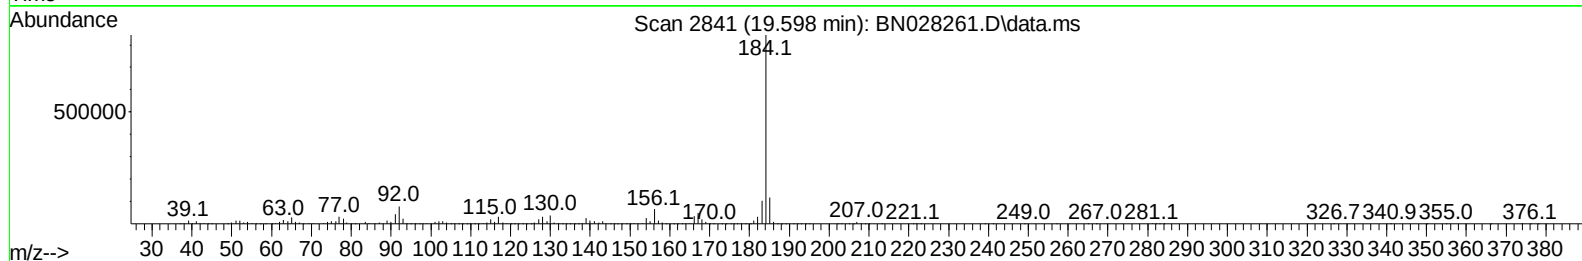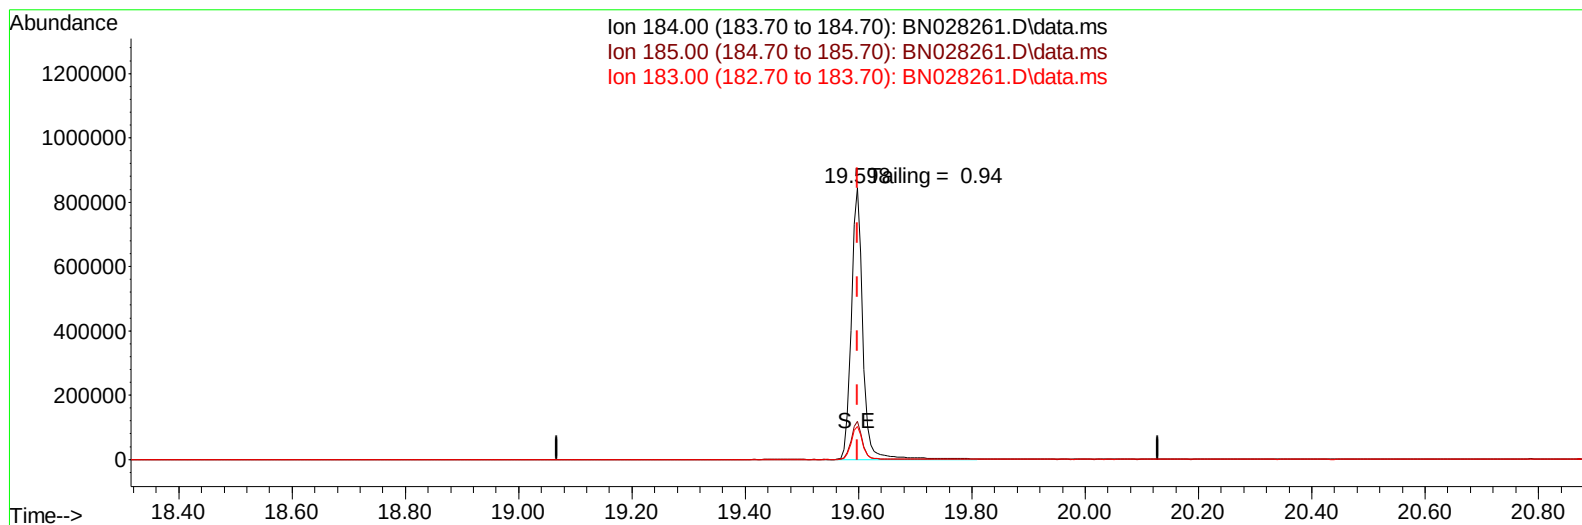

TIC: BN028261.D\data.ms

(77) Benzidine

19.598min (0.000) 340747.54 ng

response 1207922

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.14
0.00	0.00	0.00