

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
 Data File : BN028263.D
 Acq On : 12 Oct 2023 16:33
 Operator : MA/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Oct 13 02:10:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 13 02:03:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	2181	0.400	ng	0.00
7) Naphthalene-d8	10.714	136	7498	0.400	ng	# 0.00
13) Acenaphthene-d10	14.544	164	4688	0.400	ng	0.00
19) Phenanthrene-d10	17.306	188	10503	0.400	ng	0.00
29) Chrysene-d12	21.498	240	11351	0.400	ng	0.00
35) Perylene-d12	23.955	264	13222	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.423	112	807	0.119	ng	0.00
5) Phenol-d6	7.062	99	959	0.115	ng	0.00
8) Nitrobenzene-d5	9.102	82	762	0.115	ng	0.00
11) 2-Methylnaphthalene-d10	12.298	152	1128	0.100	ng	0.00
14) 2,4,6-Tribromophenol	16.053	330	264	0.115	ng	0.00
15) 2-Fluorobiphenyl	13.165	172	1742	0.106	ng	0.00
27) Fluoranthene-d10	19.337	212	2841	0.101	ng	0.00
31) Terphenyl-d14	19.923	244	2777	0.115	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.299	88	323	0.123	ng	# 74
3) n-Nitrosodimethylamine	3.661	42	270	0.094	ng	# 90
6) bis(2-Chloroethyl)ether	7.329	93	674	0.105	ng	96
9) Naphthalene	10.757	128	1987	0.102	ng	# 89
10) Hexachlorobutadiene	10.970	225	349	0.105	ng	# 97
12) 2-Methylnaphthalene	12.374	142	1402	0.101	ng	# 93
16) Acenaphthylene	14.266	152	2326	0.110	ng	97
17) Acenaphthene	14.609	154	1362	0.103	ng	99
18) Fluorene	15.593	166	1768	0.101	ng	93
21) 4-Bromophenyl-phenylether	16.487	248	534	0.099	ng	# 92
22) Hexachlorobenzene	16.574	284	562	0.101	ng	96
23) Atrazine	16.760	200	519	0.102	ng	# 84
24) Pentachlorophenol	16.946	266	289	0.114	ng	94
25) Phenanthrene	17.344	178	3037	0.106	ng	98
26) Anthracene	17.443	178	2948	0.107	ng	99
28) Fluoranthene	19.365	202	4045	0.112	ng	98
30) Pyrene	19.732	202	4457	0.115	ng	99
32) Benzo(a)anthracene	21.480	228	4527	0.112	ng	# 90
33) Chrysene	21.533	228	4218	0.109	ng	# 89
36) Indeno(1,2,3-cd)pyrene	26.536	276	6022	0.113	ng	99
37) Benzo(b)fluoranthene	23.198	252	4703	0.114	ng	# 51
38) Benzo(k)fluoranthene	23.247	252	4615	0.110	ng	# 50
39) Benzo(a)pyrene	23.847	252	4519	0.110	ng	# 42
40) Dibenzo(a,h)anthracene	26.548	278	4687	0.108	ng	# 60
41) Benzo(g,h,i)perylene	27.343	276	5020	0.112	ng	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
 Data File : BN028263.D
 Acq On : 12 Oct 2023 16:33
 Operator : MA/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Quant Time: Oct 13 02:10:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 13 02:03:40 2023
 Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.893 min Scan# 694
 Delta R.T. -0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument : BNA_N
 ClientSampleId : SSTDICC0.1



Tgt Ion: 152 Resp: 2181




Ion	Ratio	Lower	Upper
152	100		
150	150.1	121.6	182.4
115	71.3	54.3	81.5




#2
 1,4-Dioxane
 Concen: 0.123 ng
 RT: 3.299 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion: 88 Resp: 323

Ion	Ratio	Lower	Upper
88	100		
43	66.9	26.6	39.8
58	60.7	55.4	83.0









#3
 n-Nitrosodimethylamine
 Concen: 0.094 ng
 RT: 3.661 min Scan# 108
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument : BNA_N
 ClientSampleId : SSTDICC0.1

Tgt Ion: 42 Resp: 270




Ion	Ratio	Lower	Upper
42	100		
74	147.0	112.6	168.8
44	36.7	7.8	11.6




#4
 2-Fluorophenol
 Concen: 0.119 ng
 RT: 5.423 min Scan# 352
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion: 112 Resp: 807

Ion	Ratio	Lower	Upper
112	100		
64	57.4	46.9	70.3
63	31.8	25.0	37.4









#5
 Phenol-d6
 Concen: 0.115 ng
 RT: 7.062 min Scan# 579
 Delta R.T. 0.007 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion	Resp	Ion Ratio	Lower	Upper
99	959	100		
42	17.6	15.9	23.9	
71	42.3	28.6	42.8	



#6
 bis(2-Chloroethyl)ether
 Concen: 0.105 ng
 RT: 7.329 min Scan# 616
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Ion Ratio	Lower	Upper
93	674	100		
63	73.4	62.6	93.8	
95	35.3	27.2	40.8	







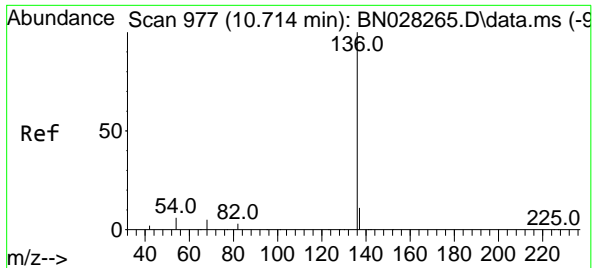

#7
 Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.714 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument : BNA_N
 ClientSampleId : SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
136	7498		
137	12.4	9.8	14.8
54	9.0	6.2	9.4
68	8.8	5.7	8.5

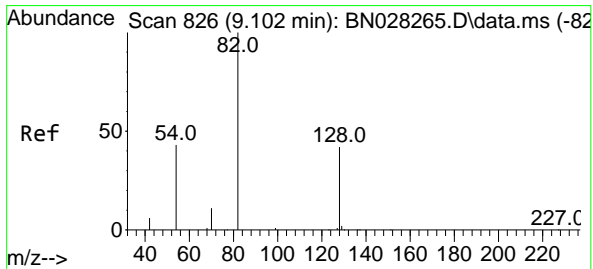

#8
 Nitrobenzene-d5
 Concen: 0.115 ng
 RT: 9.102 min Scan# 826
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
82	762		
128	54.2	36.8	55.2
54	61.0	37.4	56.2









#9
 Naphthalene
 Concen: 0.102 ng
 RT: 10.757 min Scan# 981
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:128 Resp: 1987
 Ion Ratio Lower Upper
 128 100
 129 16.9 9.8 14.6#
 127 18.4 11.4 17.0#



#10
 Hexachlorobutadiene
 Concen: 0.105 ng
 RT: 10.970 min Scan# 1001
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:225 Resp: 349
 Ion Ratio Lower Upper
 225 100
 223 0.0 0.0 0.0
 227 66.8 51.6 77.4







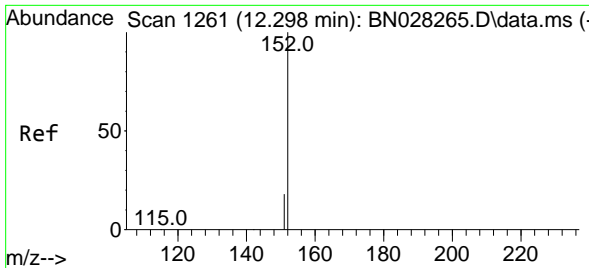

#11
 2-Methylnaphthalene-d10
 Concen: 0.100 ng
 RT: 12.298 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 1128
 Ion Ratio Lower Upper
 152 100
 151 20.1 16.1 24.1



#12
 2-Methylnaphthalene
 Concen: 0.101 ng
 RT: 12.374 min Scan# 1281
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:142 Resp: 1402
 Ion Ratio Lower Upper
 142 100
 141 91.4 71.1 106.7
 115 48.7 29.9 44.9#









#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.544 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
164	4688		
162	101.7	81.1	121.7
160	47.7	36.6	54.8



#14
 2,4,6-Tribromophenol
 Concen: 0.115 ng
 RT: 16.053 min Scan# 1726
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
330	264		
332	90.9	74.1	111.1
141	40.2	32.1	48.1









#15
 2-Fluorobiphenyl
 Concen: 0.106 ng
 RT: 13.165 min Scan# 1463
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument : BNA_N
 ClientSampleId : SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
172	100		
171	39.8	28.3	42.5
170	26.9	18.7	28.1



#16
 Acenaphthylene
 Concen: 0.110 ng
 RT: 14.266 min Scan# 1566
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
152	100		
151	21.2	15.6	23.4
153	13.7	10.6	16.0









#17
 Acenaphthene
 Concen: 0.103 ng
 RT: 14.609 min Scan# 11
 Delta R.T. 0.011 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:154 Resp: 1362




Ion	Ratio	Lower	Upper
154	100		
153	112.8	90.7	136.1
152	56.1	43.6	65.4




#18
 Fluorene
 Concen: 0.101 ng
 RT: 15.593 min Scan# 1689
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:166 Resp: 1768


Ion	Ratio	Lower	Upper
166	100		
165	106.7	79.3	118.9
167	15.2	10.9	16.3








#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.306 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1



Tgt Ion:188 Resp: 10503




Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	9.4	7.1	10.7




#21
 4-Bromophenyl-phenylether
 Concen: 0.099 ng
 RT: 16.487 min Scan# 1761
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:248 Resp: 534

Ion	Ratio	Lower	Upper
248	100		
250	102.4	80.5	120.7
141	63.6	38.9	58.3









#22
 Hexachlorobenzene
 Concen: 0.101 ng
 RT: 16.574 min Scan# 1768
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
284	100		
142	42.2	32.1	48.1
249	34.5	25.5	38.3



#23
 Atrazine
 Concen: 0.102 ng
 RT: 16.760 min Scan# 1783
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
200	100		
173	38.7	21.6	32.4
215	57.4	39.0	58.6









#24
 Pentachlorophenol
 Concen: 0.114 ng
 RT: 16.946 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument : BNA_N
 ClientSampleId : SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
266	100		
264	59.9	51.5	77.3
268	76.1	56.6	84.8



#25
 Phenanthrene
 Concen: 0.106 ng
 RT: 17.344 min Scan# 1830
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
178	100		
176	20.0	15.3	22.9
179	16.2	12.5	18.7









#26
 Anthracene
 Concen: 0.107 ng
 RT: 17.443 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument : BNA_N
 ClientSampleId : SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
178	100		
176	18.0	14.6	22.0
179	14.3	12.2	18.4



#27
 Fluoranthene-d10
 Concen: 0.101 ng
 RT: 19.337 min Scan# 2102
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33


Tgt Ion	Resp	Lower	Upper
212	100		
106	15.5	11.5	17.3
104	10.2	6.7	10.1








#28
 Fluoranthene
 Concen: 0.112 ng
 RT: 19.365 min Scan# 2108
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument : BNA_N
 ClientSampleId : SSTDICC0.1




Tgt Ion: 202 Resp: 4045

Ion	Ratio	Lower	Upper
202	100		
101	11.4	10.1	15.1
203	17.8	13.9	20.9






#29
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.498 min Scan# 2516
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33



Tgt Ion: 240 Resp: 11351


Ion	Ratio	Lower	Upper
240	100		
120	16.6	13.4	20.0
236	28.7	22.7	34.1








#30
 Pyrene
 Concen: 0.115 ng
 RT: 19.732 min Scan# 2187
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1




Tgt Ion: 202 Resp: 4457

Ion	Ratio	Lower	Upper
202	100		
200	20.7	16.7	25.1
203	19.0	14.5	21.7






#31
 Terphenyl-d14
 Concen: 0.115 ng
 RT: 19.923 min Scan# 2228
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33



Tgt Ion: 244 Resp: 2777

Ion	Ratio	Lower	Upper
244	100		
212	12.2	6.6	10.0#
122	19.0	11.7	17.5#









#32
 Benzo(a)anthracene
 Concen: 0.112 ng
 RT: 21.480 min Scan# 2148
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33




Instrument : BNA_N
 ClientSampleId : SSTDICC0.1


Tgt Ion	Resp	Lower	Upper
228	4527		
226	32.8	22.9	34.3
229	27.2	16.6	24.8



#33
 Chrysene
 Concen: 0.109 ng
 RT: 21.533 min Scan# 2520
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion	Resp	Lower	Upper
228	4218		
226	36.3	25.2	37.8
229	27.4	16.6	25.0









#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.955 min Scan# 3146
 Delta R.T. -0.006 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument : BNA_N
 ClientSampleId : SSTDICC0.1

Tgt Ion:264 Resp: 13222




Ion	Ratio	Lower	Upper
264	100		
260	27.4	20.7	31.1
265	58.6	38.3	57.5#




#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.113 ng
 RT: 26.536 min Scan# 4029
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:276 Resp: 6022

Ion	Ratio	Lower	Upper
276	100		
138	26.1	21.3	31.9
277	25.5	20.0	30.0









#37
 Benzo(b)fluoranthene
 Concen: 0.114 ng
 RT: 23.198 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument : BNA_N
 ClientSampleId : SSTDICC0.1

Tgt Ion:252 Resp: 4703




Ion	Ratio	Lower	Upper
252	100		
253	47.6	21.8	32.8#
125	48.0	15.6	23.4#




#38
 Benzo(k)fluoranthene
 Concen: 0.110 ng
 RT: 23.247 min Scan# 2904
 Delta R.T. -0.003 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Tgt Ion:252 Resp: 4615


Ion	Ratio	Lower	Upper
252	100		
253	47.0	22.0	33.0#
125	50.1	15.3	22.9#








#39
 Benzo(a)pyrene
 Concen: 0.110 ng
 RT: 23.847 min Scan# 3109
 Delta R.T. -0.003 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1







Tgt Ion:252 Resp: 4519
 Ion Ratio Lower Upper
 252 100
 253 51.6 22.7 34.1#
 125 57.6 17.0 25.6#



#40
 Dibenzo(a,h)anthracene
 Concen: 0.108 ng
 RT: 26.548 min Scan# 4033
 Delta R.T. -0.003 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33


Tgt Ion:278 Resp: 4687
 Ion Ratio Lower Upper
 278 100
 139 47.5 18.8 28.2#
 279 46.9 23.5 35.3#





#41
 Benzo(g,h,i)perylene
 Concen: 0.112 ng
 RT: 27.343 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN028263.D
 Acq: 12 Oct 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1



Tgt Ion: 276 Resp: 5020

Ion	Ratio	Lower	Upper
276	100		
277	37.5	21.7	32.5#
138	40.1	21.7	32.5#

