
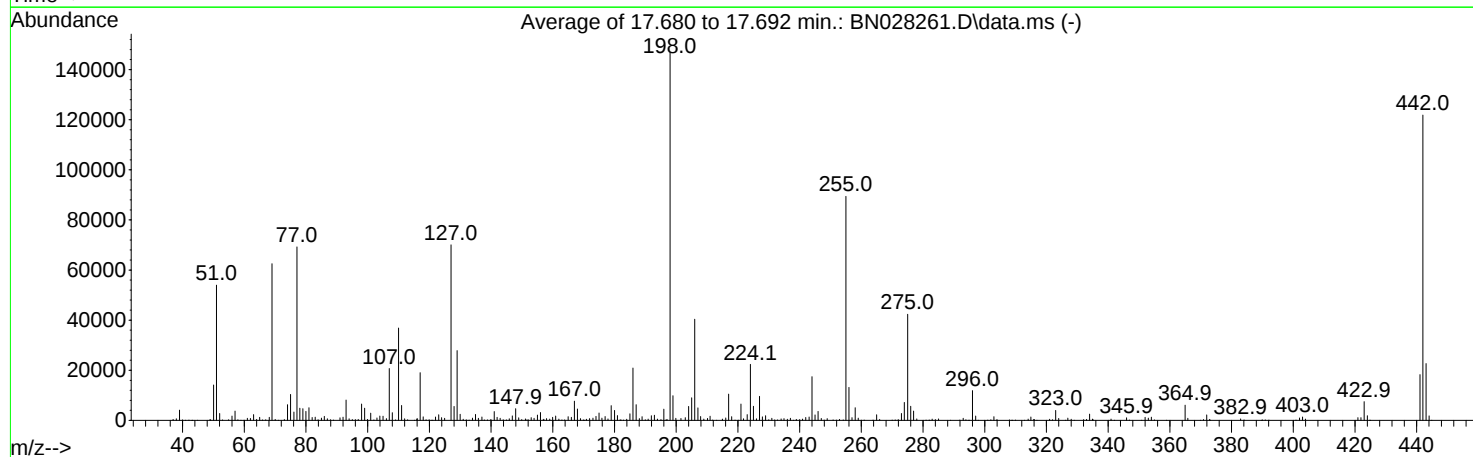


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
Data File : BN028261.D
Acq On : 12 Oct 2023 14:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 13 02:17:11 2023

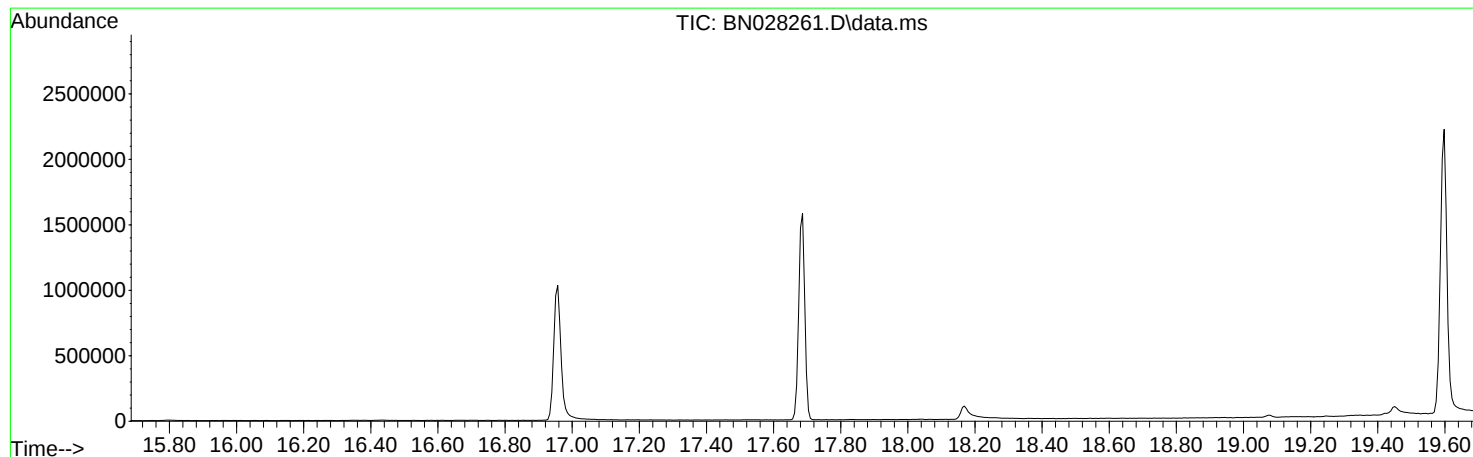




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	54005	PASS
68	69	0.00	2	1.9	1215	PASS
69	198	0.00	100	42.6	62509	PASS
70	69	0.00	2	0.6	404	PASS
127	198	10	80	47.7	70080	PASS
197	198	0.00	2	0.2	366	PASS
198	198	100	100	100.0	146837	PASS
199	198	5	9	6.7	9844	PASS
275	198	10	60	28.8	42344	PASS
365	198	1	100	4.1	6075	PASS
441	198	0.01	100	12.4	18269	PASS
442	442	50	100	100.0	121872	PASS
443	442	15	24	18.6	22704	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
Data File : BN028261.D
Acq On : 12 Oct 2023 14:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 13 02:49:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 13 02:49:55 2023
Response via : Initial Calibration

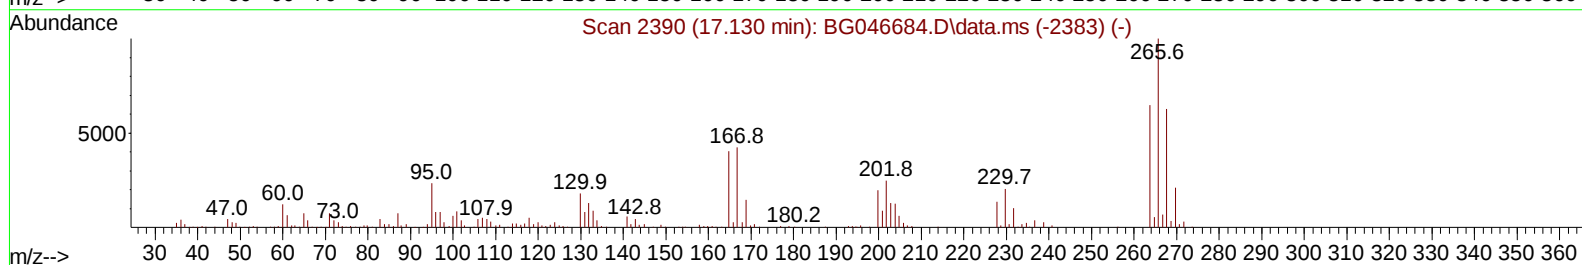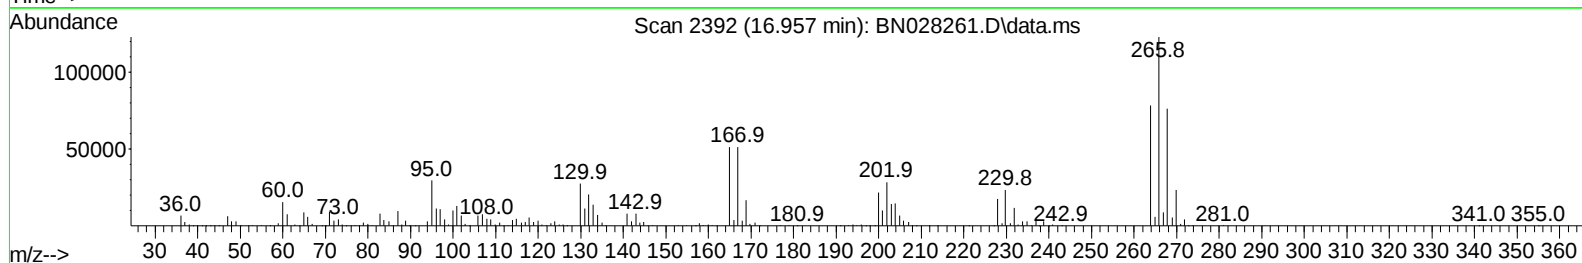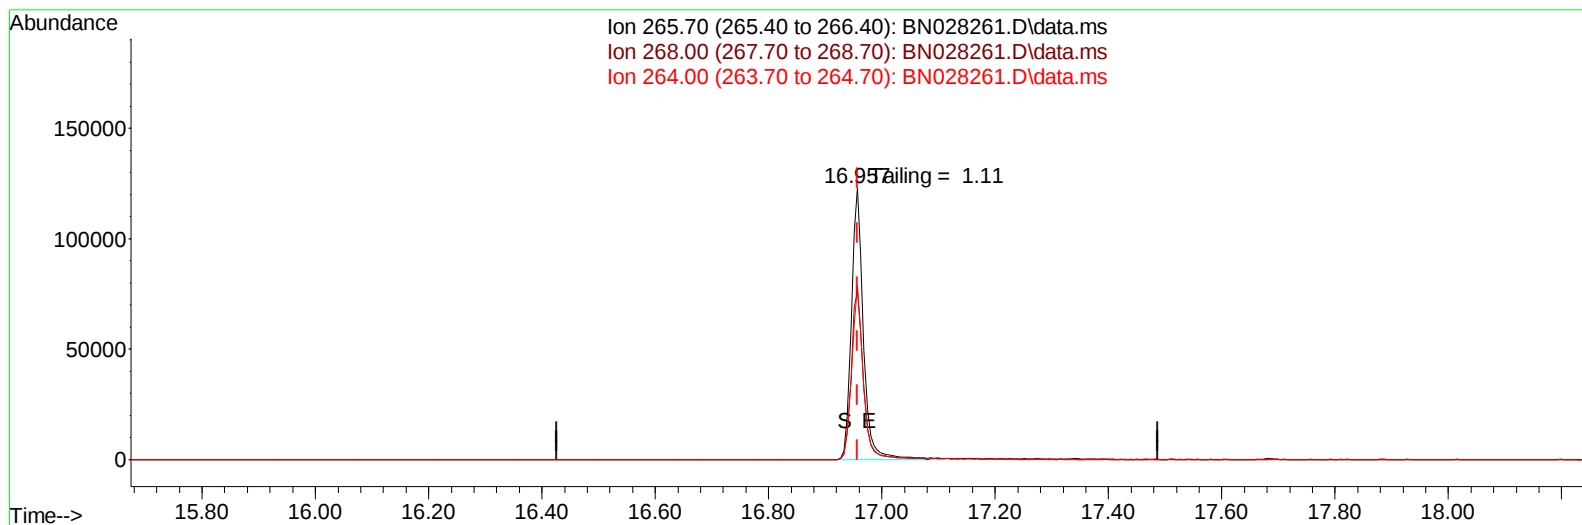

TIC: BN028261.D\data.ms

(70) Pentachlorophenol (C)

16.957min (0.000) 23122.20 ng




response 182183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101223\
Data File : BN028261.D
Acq On : 12 Oct 2023 14:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 13 02:49:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 13 02:49:55 2023
Response via : Initial Calibration

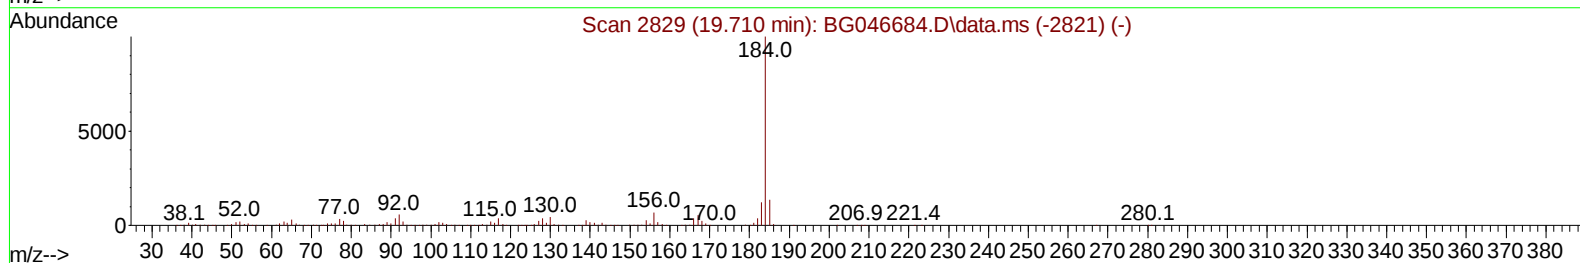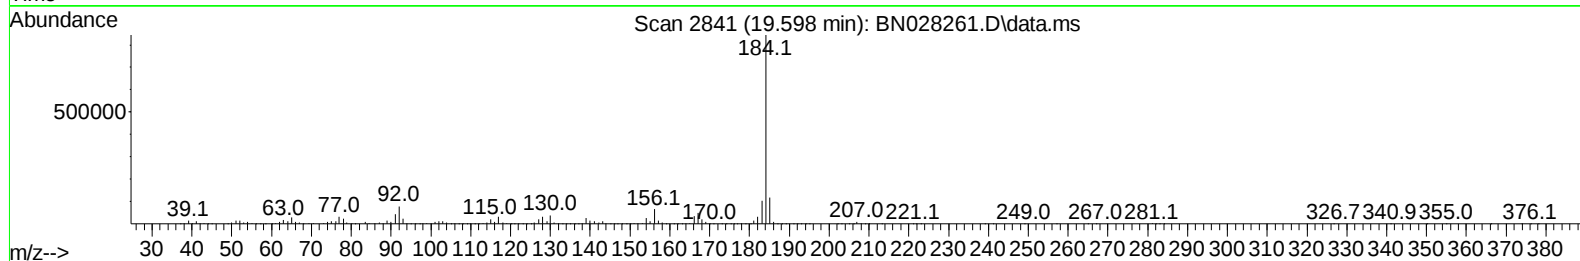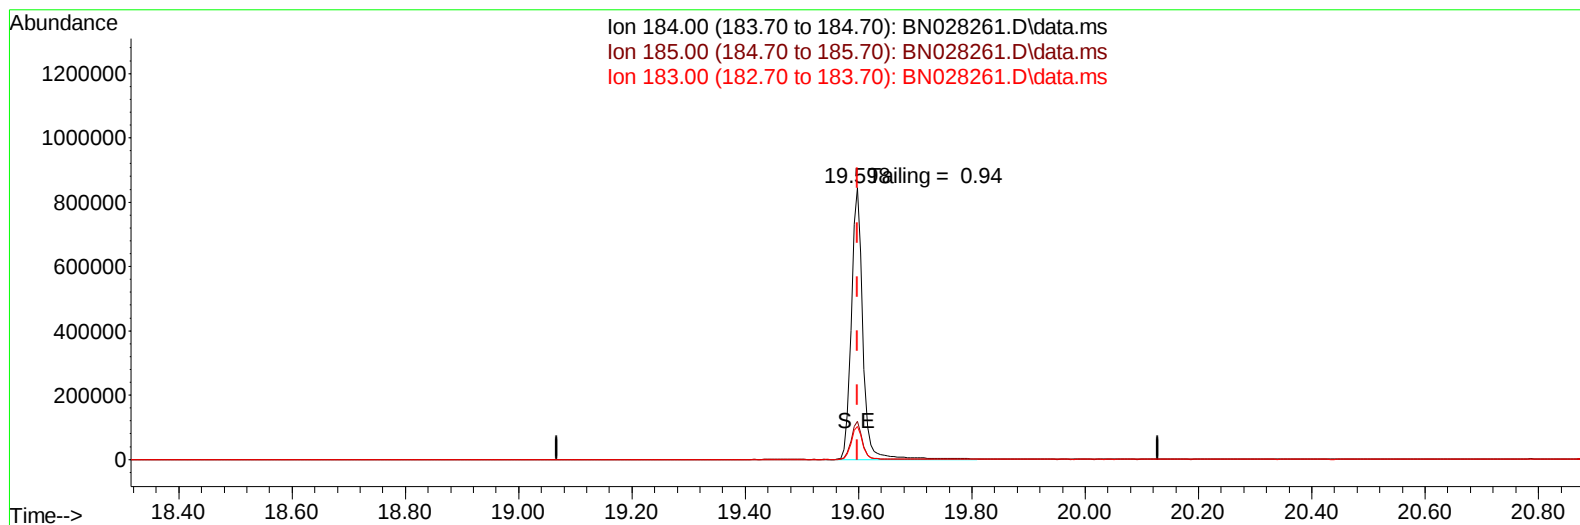

TIC: BN028261.D\data.ms

(77) Benzidine

19.598min (0.000) 340747.54 ng

response 1207922

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2023	BNA_N	<u>BN028261.D</u>
Compound Name	Response	Retention Time
DDT	533898	20.786
DDD	43809	20.351
DDE	1007	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44816	578714	7.74

p

Instrument :
BNA_N
ClientSampleId :
DFTPP