
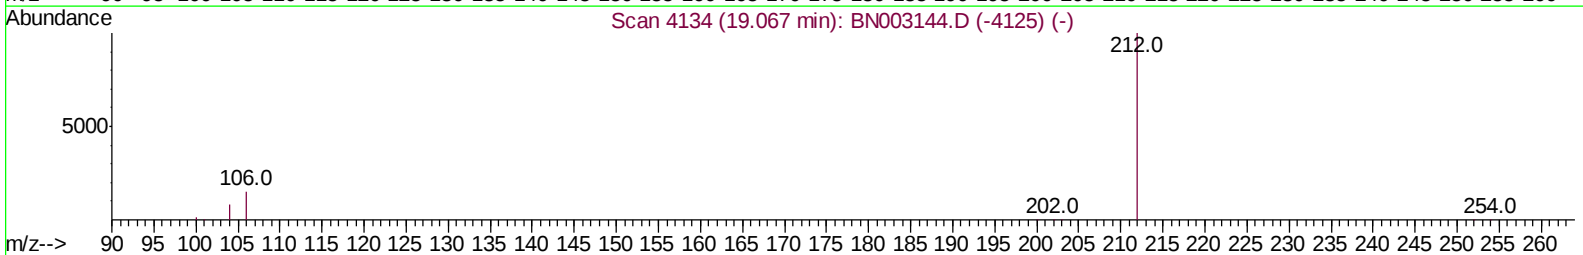
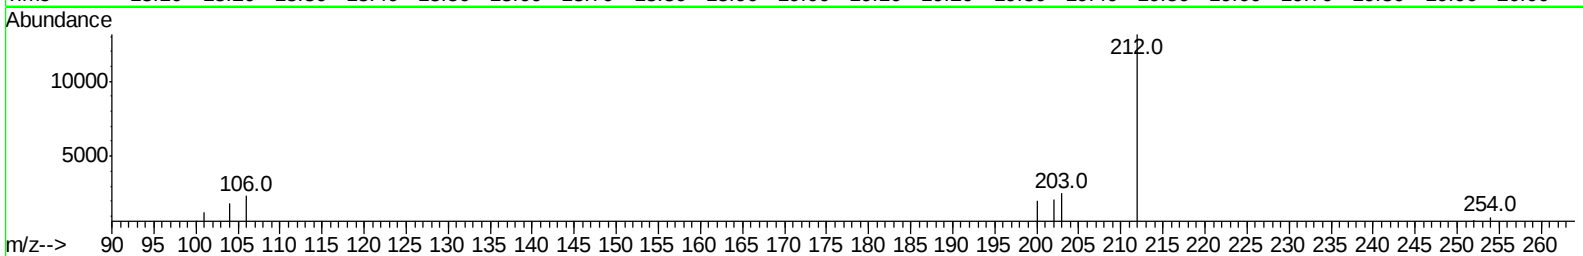


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003146.D
Acq On : 12 Oct 2018 19:15
Operator : MJ/SJ
Sample : J5234-16RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:05:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

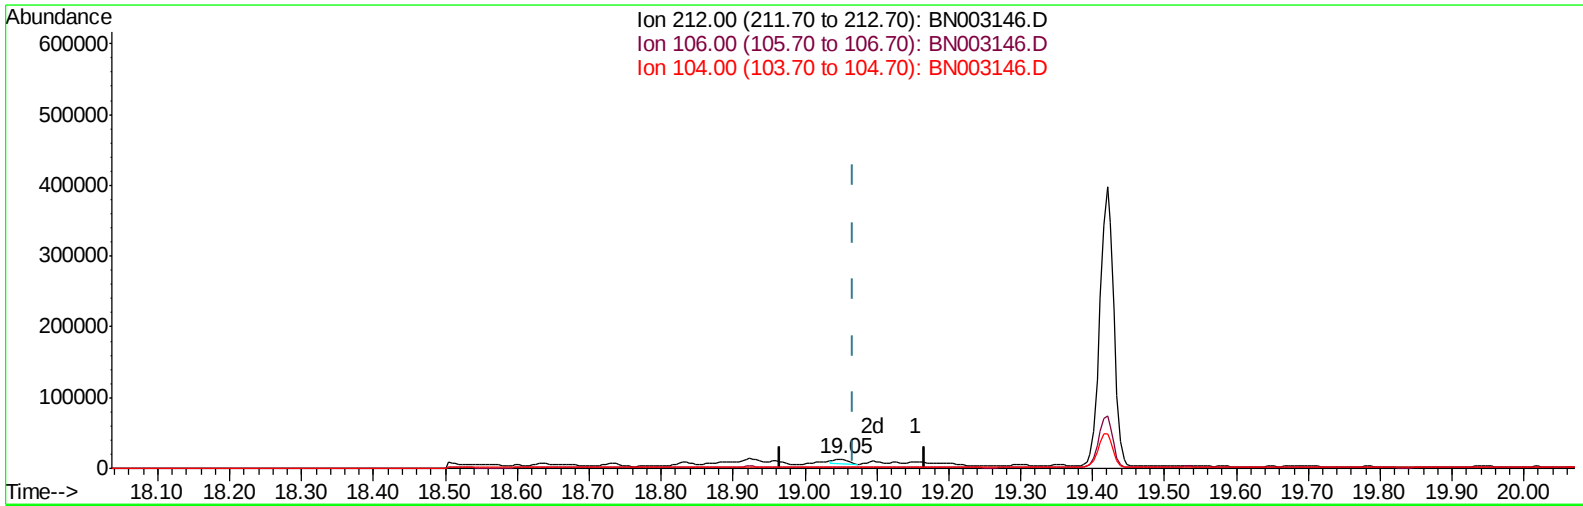

TIC: BN003146.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.014) 0.33ng/ul m

response 8638

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	2.69#
0.00	0.00	0.00