
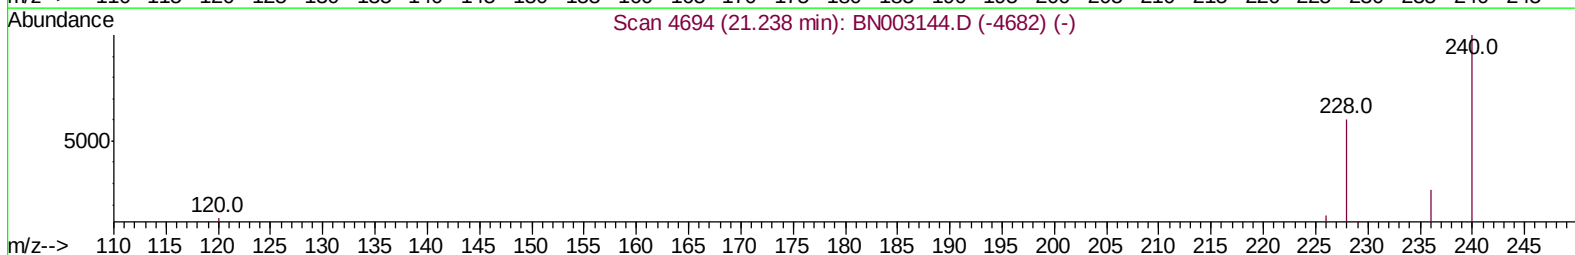
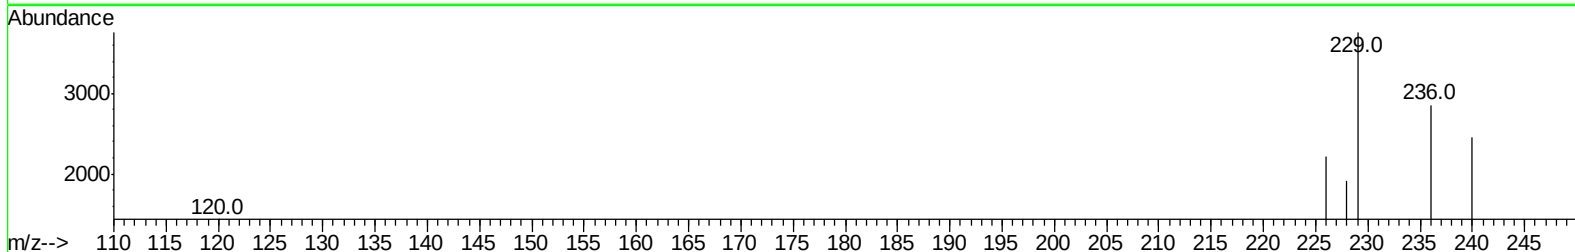


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\  
Data File : BN003146.D  
Acq On : 12 Oct 2018 19:15  
Operator : MJ/SJ  
Sample : J5234-16RE  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:08:29 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 13 04:51:37 2018  
Response via : Initial Calibration

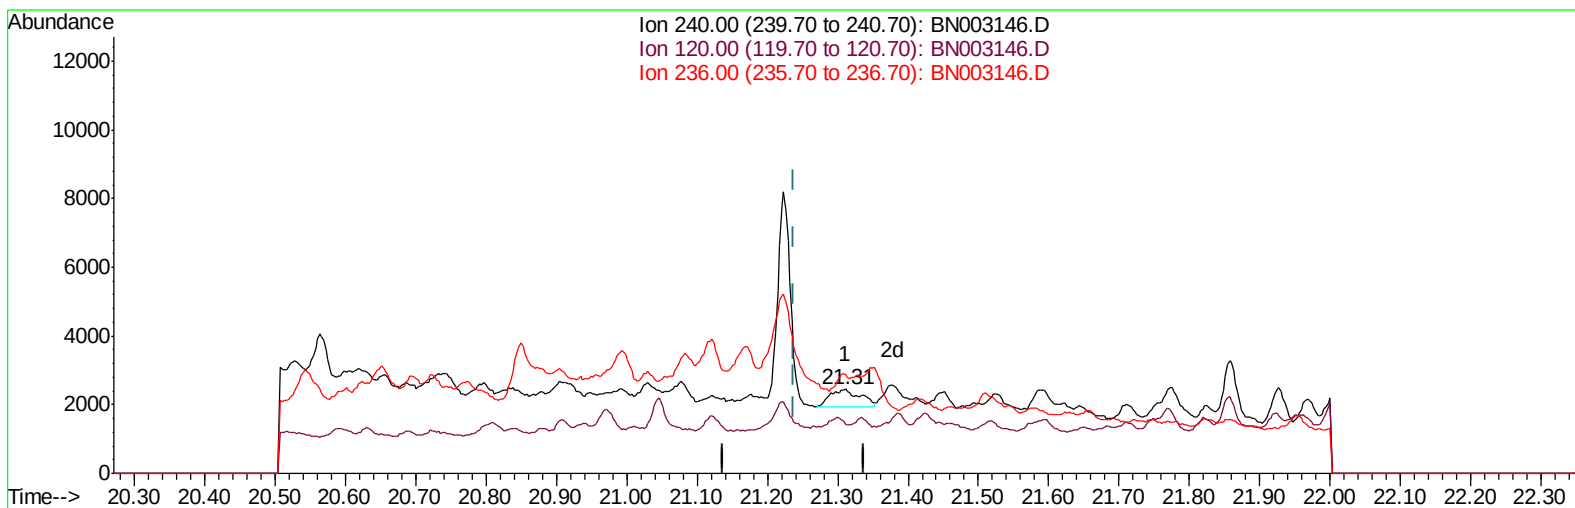

TIC: BN003146.D

(16) Chrysene-d12 (I)

21.311min (+0.073) 0.40ng/ul

response 1524

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 240.00 | 100   | 100     |
| 120.00 | 16.40 | 58.45#  |
| 236.00 | 28.10 | 116.25# |
| 0.00   | 0.00  | 0.00    |