
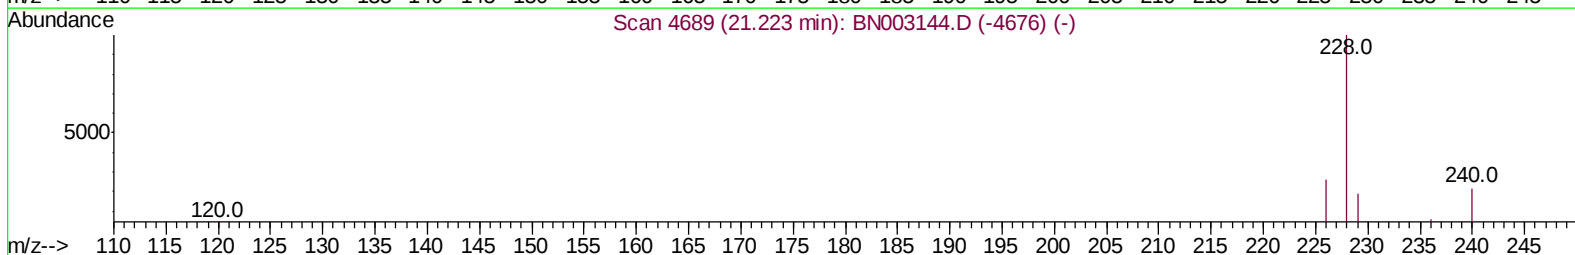
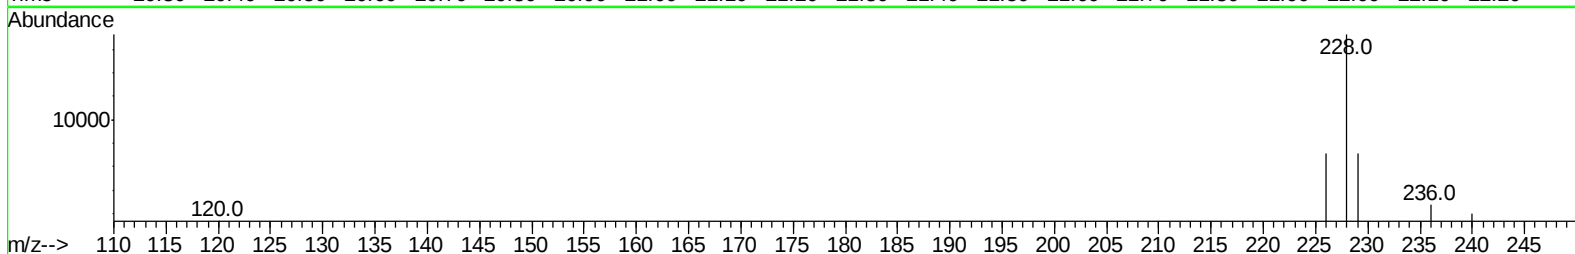


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\  
Data File : BN003146.D  
Acq On : 12 Oct 2018 19:15  
Operator : MJ/SJ  
Sample : J5234-16RE  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:08:57 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 13 04:51:37 2018  
Response via : Initial Calibration

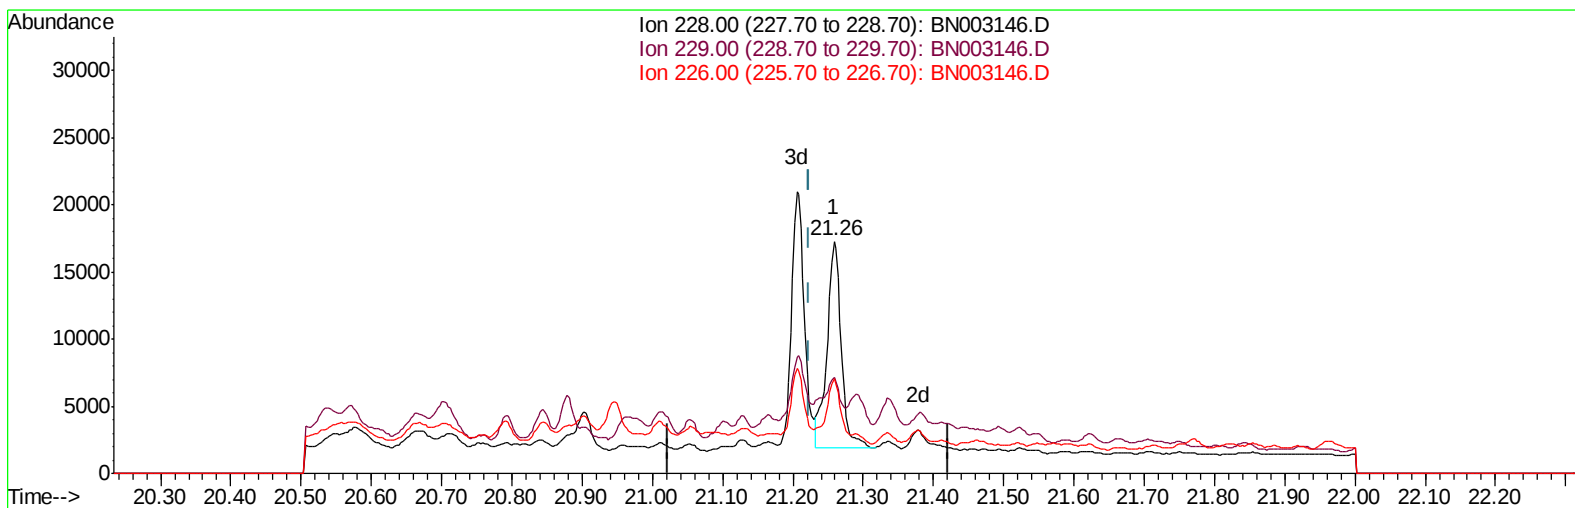

TIC: BN003146.D

(18) Benzo(a)anthracene  
21.258min (+0.035) 0.89ng/ul  
response 21809

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 229.00 | 20.20 | 41.45# |
| 226.00 | 27.90 | 41.00# |
| 0.00   | 0.00  | 0.00   |