
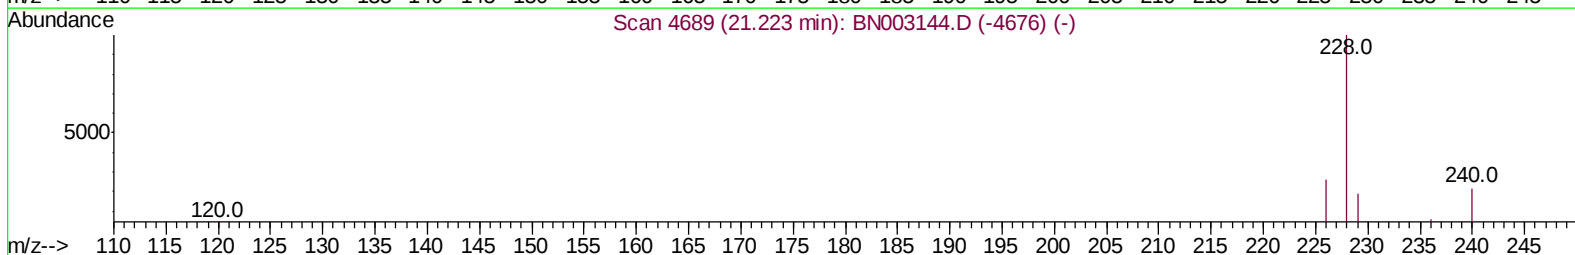
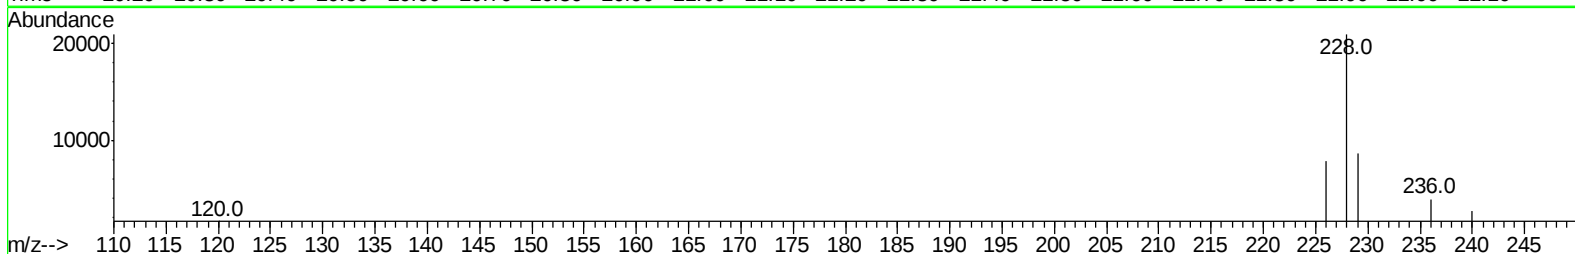


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003146.D
Acq On : 12 Oct 2018 19:15
Operator : MJ/SJ
Sample : J5234-16RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:08:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

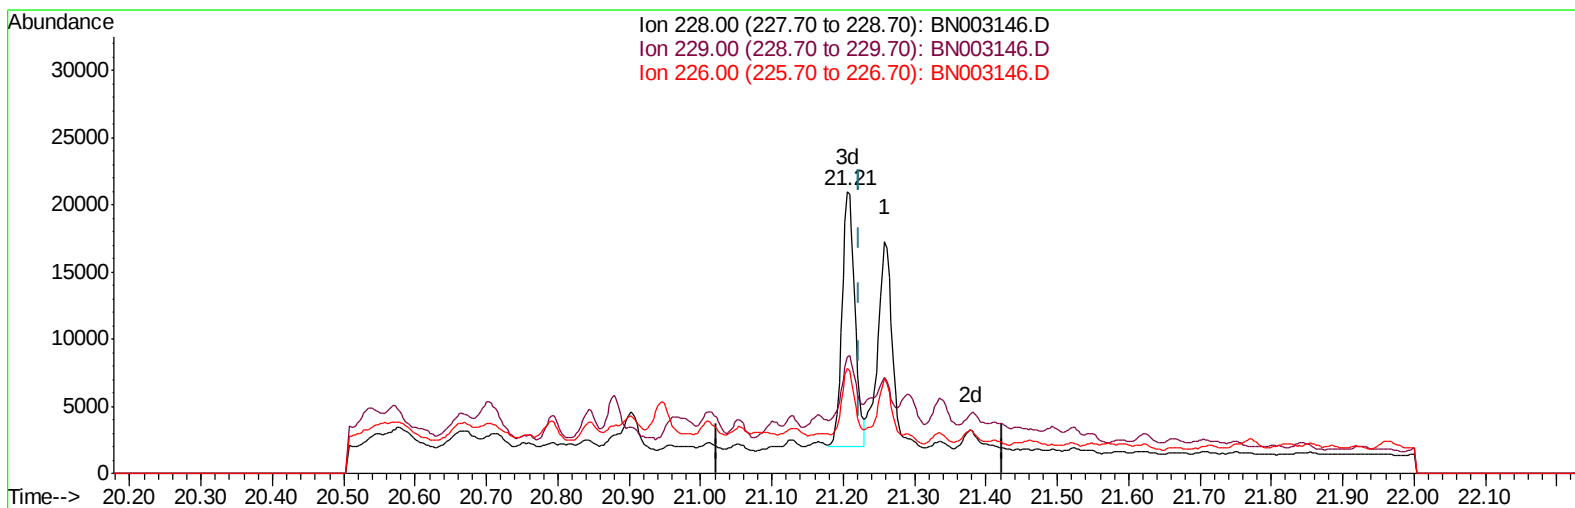

TIC: BN003146.D

(18) Benzo(a)anthracene

21.206min (-0.017) 0.96ng/ul m

response 23553

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	41.22#
226.00	27.90	37.32#
0.00	0.00	0.00