
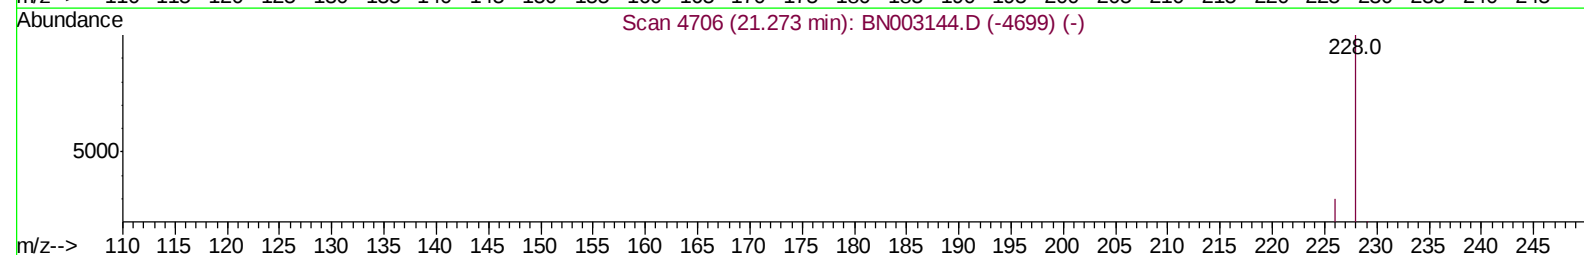
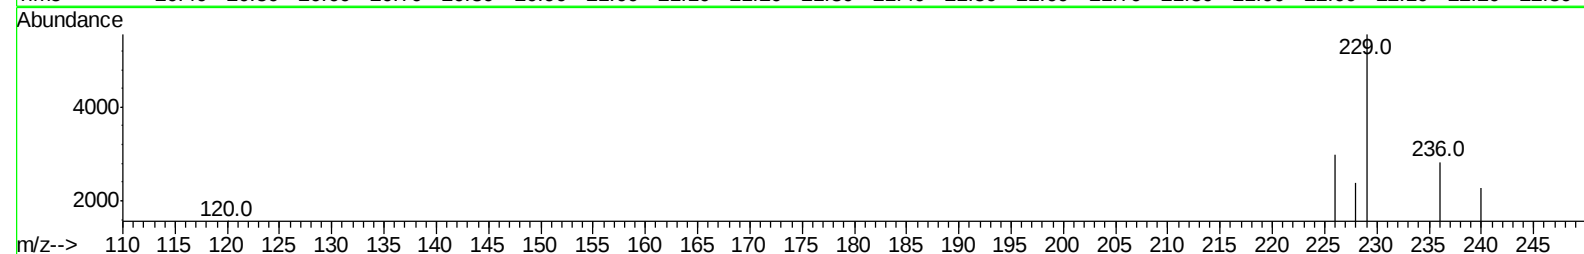


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\  
 Data File : BN003146.D  
 Acq On : 12 Oct 2018 19:15  
 Operator : MJ/SJ  
 Sample : J5234-16RE  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:08:57 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Oct 13 04:51:37 2018  
 Response via : Initial Calibration

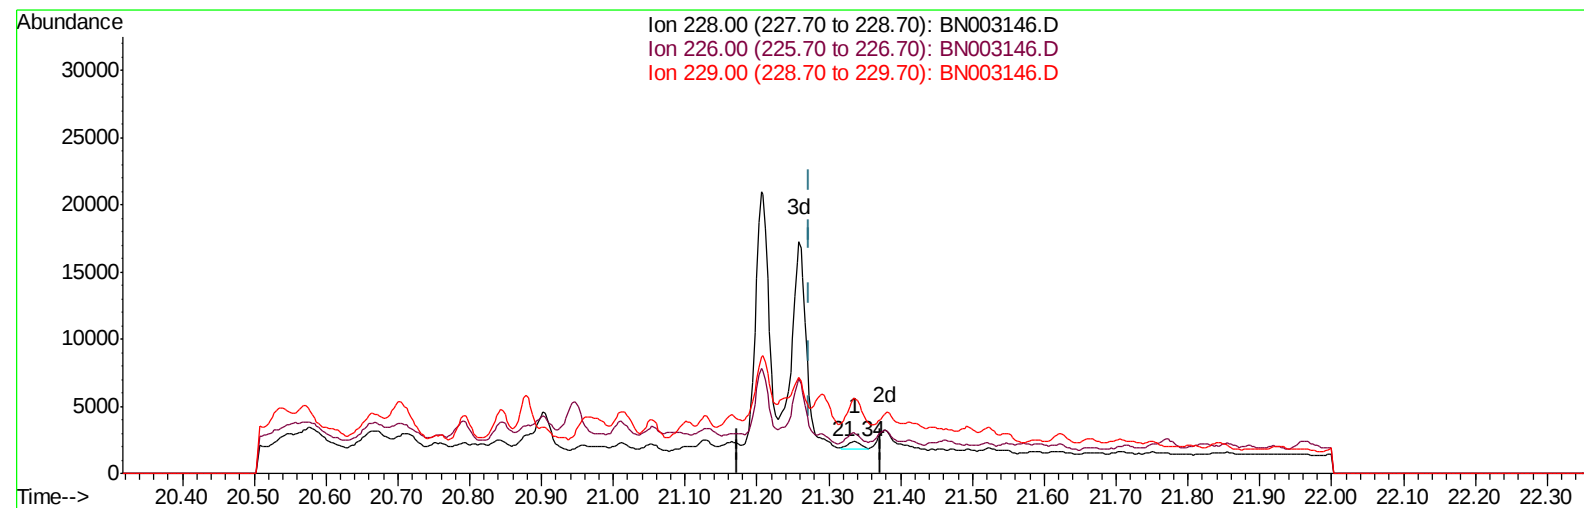

TIC: BN003146.D

(19) Chrysene

21.337min (+0.064) 0.03ng/ul

response 691

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 228.00 | 100   | 100     |
| 226.00 | 30.30 | 125.40# |
| 229.00 | 20.90 | 233.12# |
| 0.00   | 0.00  | 0.00    |