
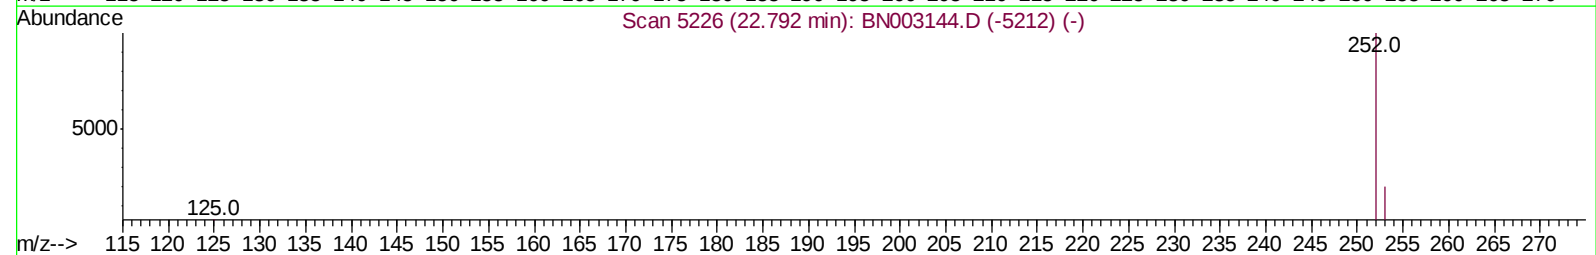
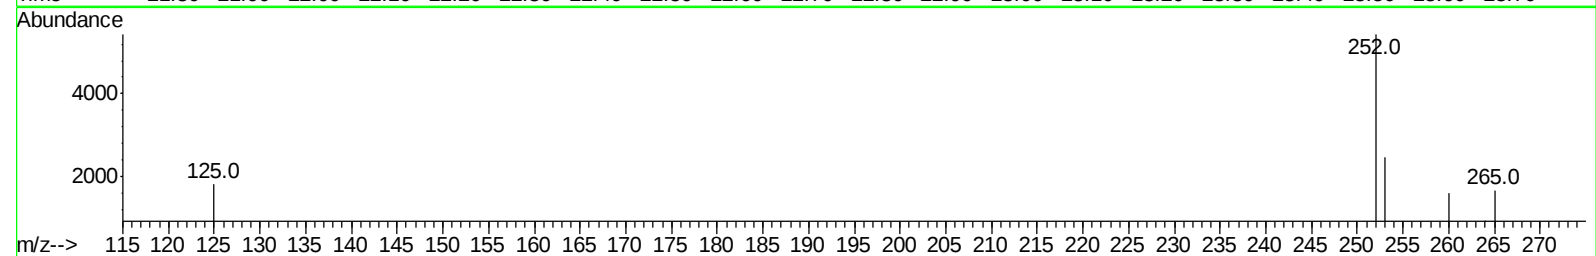


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003146.D
Acq On : 12 Oct 2018 19:15
Operator : MJ/SJ
Sample : J5234-16RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:10:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

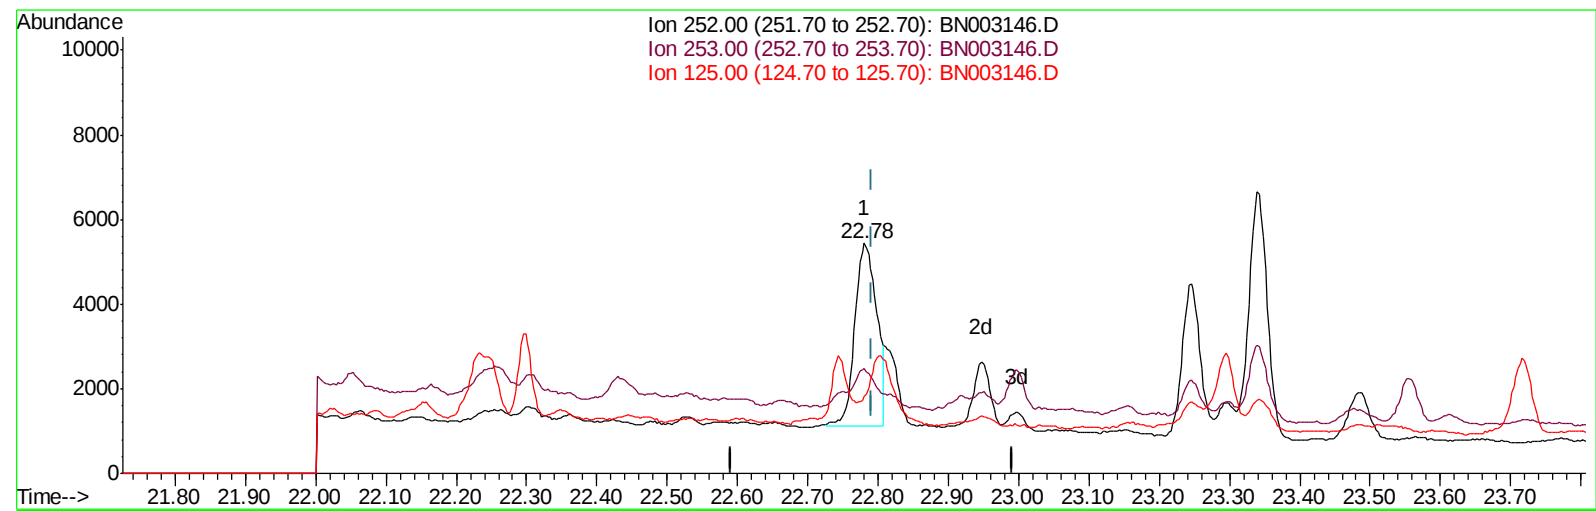

TIC: BN003146.D

(21) Benzo(b)fluoranthene

22.781min (-0.012) 0.47ng/ul m

response 9312

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	45.50
125.00	17.10	33.36
0.00	0.00	0.00