
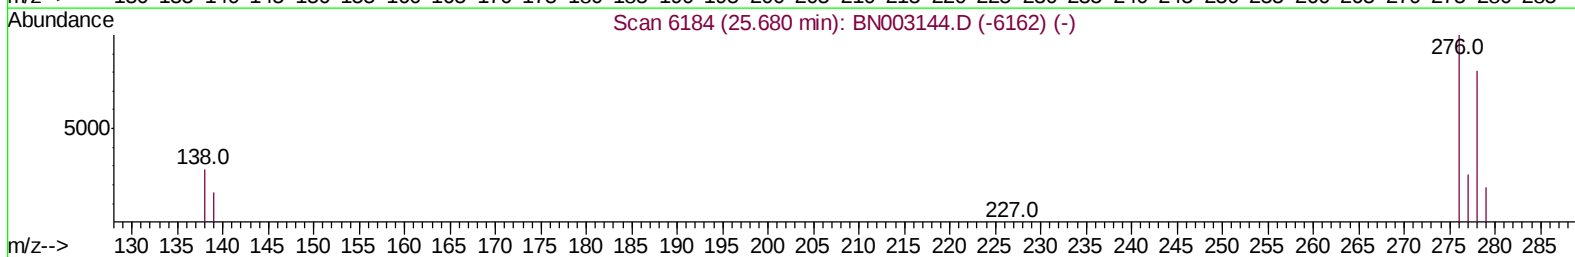
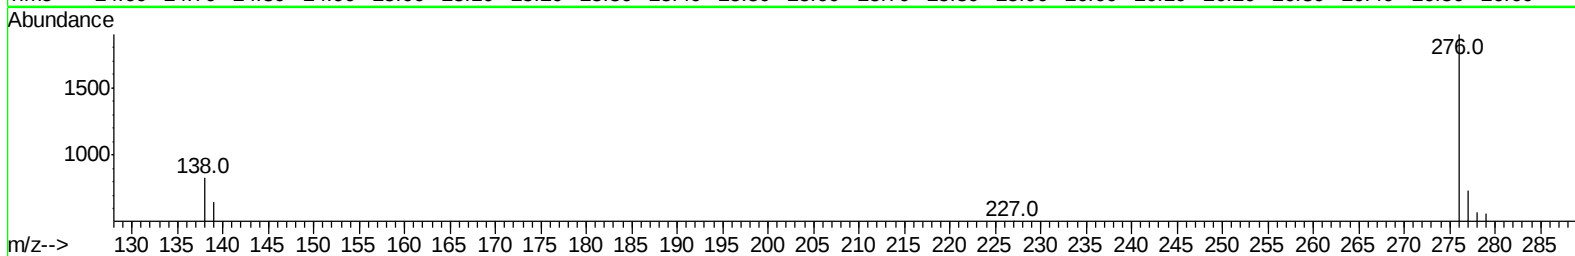


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003146.D
Acq On : 12 Oct 2018 19:15
Operator : MJ/SJ
Sample : J5234-16RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 13 05:10:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

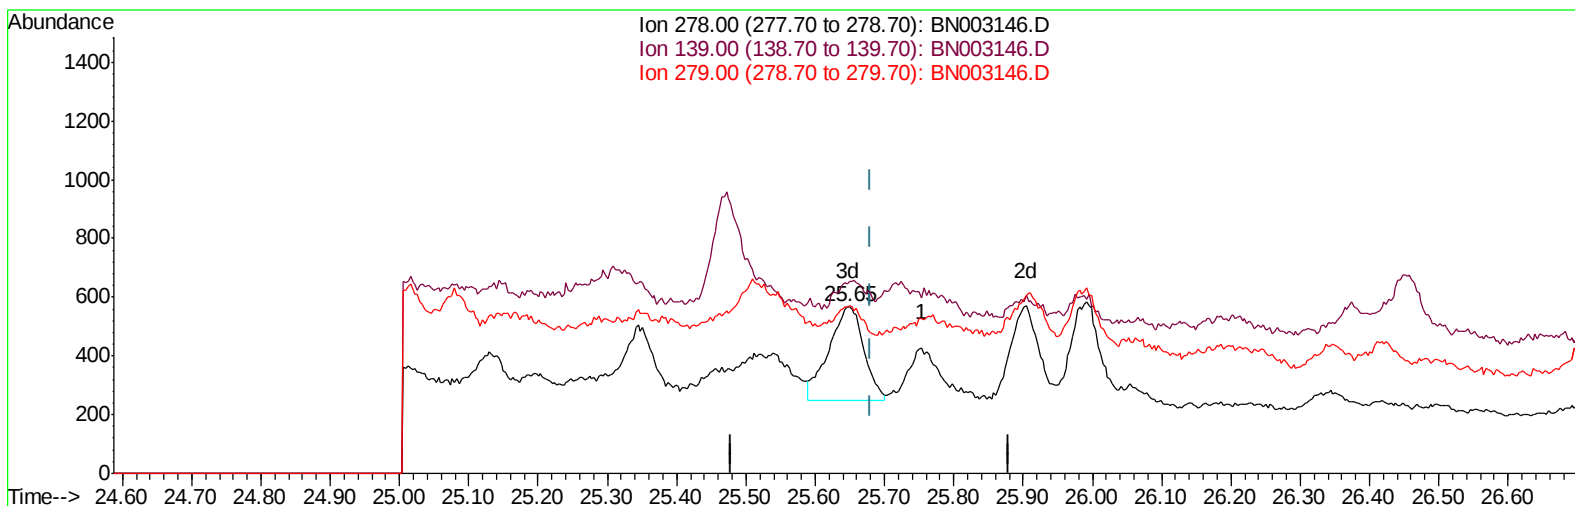

TIC: BN003146.D

(25) Dibenzo(a,h)anthracene

25.646min (-0.033) 0.07ng/ul m

response 1116

Ion	Exp%	Act%
278.00	100	100
139.00	25.30	113.56#
279.00	29.80	99.47#
0.00	0.00	0.00