
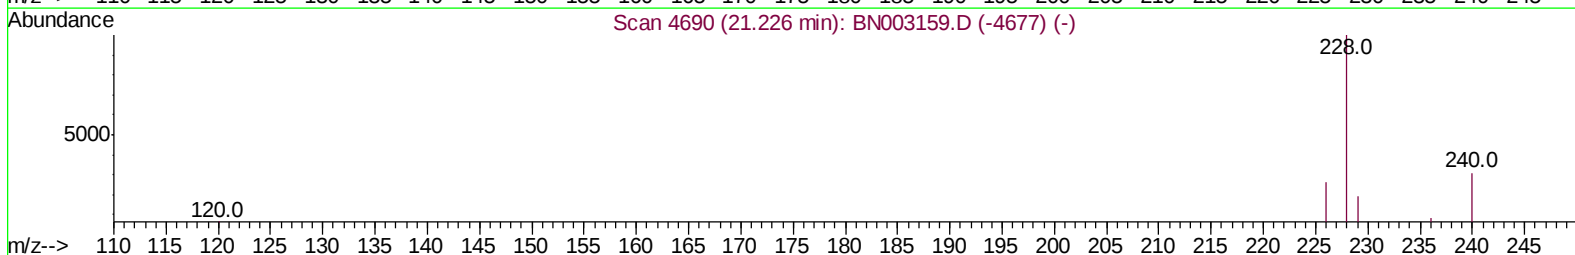
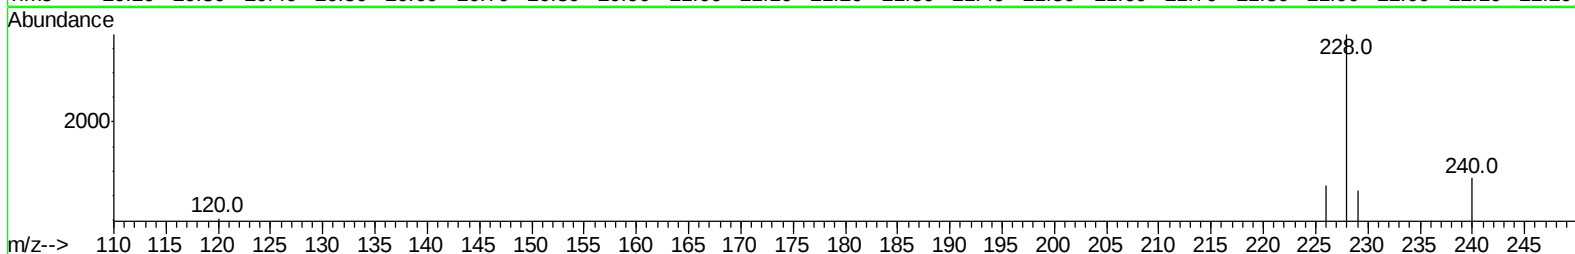


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003160.D
Acq On : 13 Oct 2018 03:43
Operator : MJ/SJ
Sample : J5368-01DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 13 06:03:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 05:59:15 2018
Response via : Initial Calibration

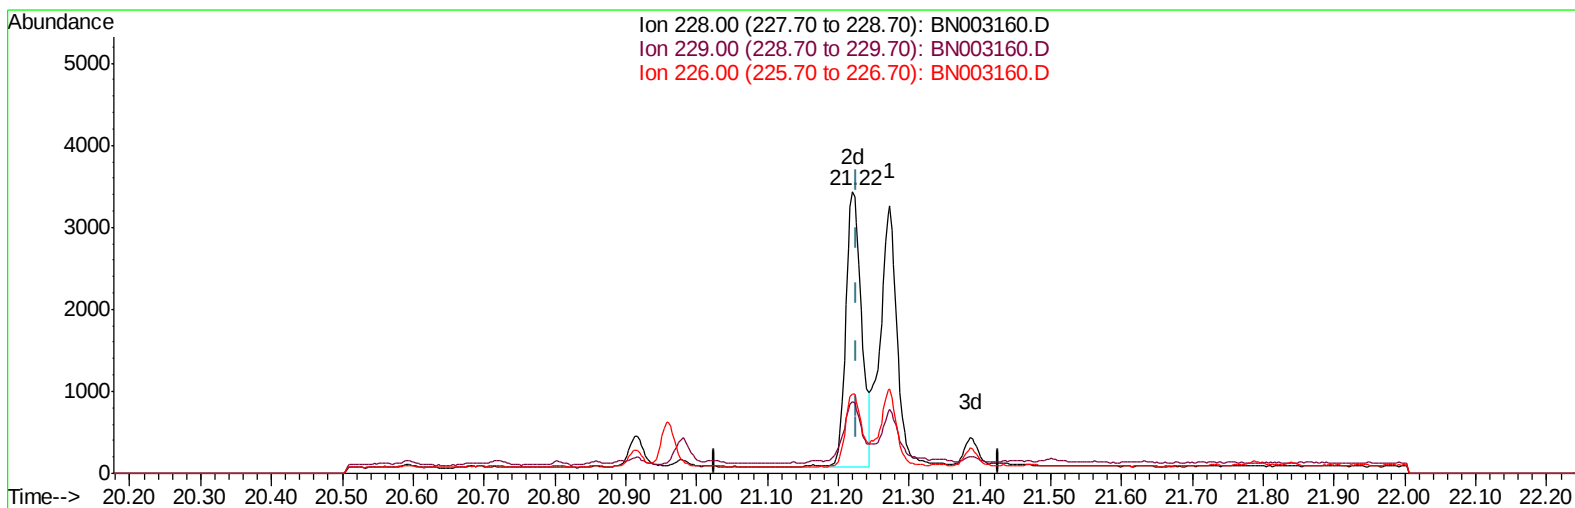

TIC: BN003160.D

(18) Benzo(a)anthracene

21.220min (-0.006) 0.25ng/ul m

response 5105

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	25.63#
226.00	27.90	28.05
0.00	0.00	0.00