
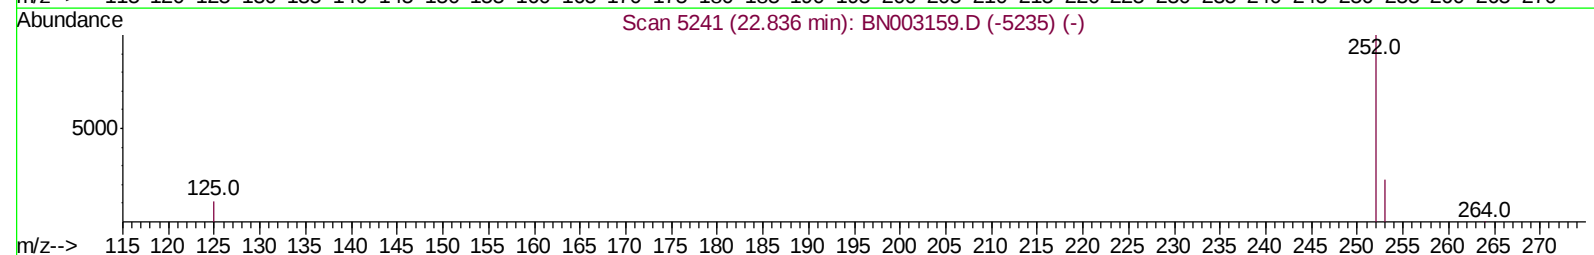
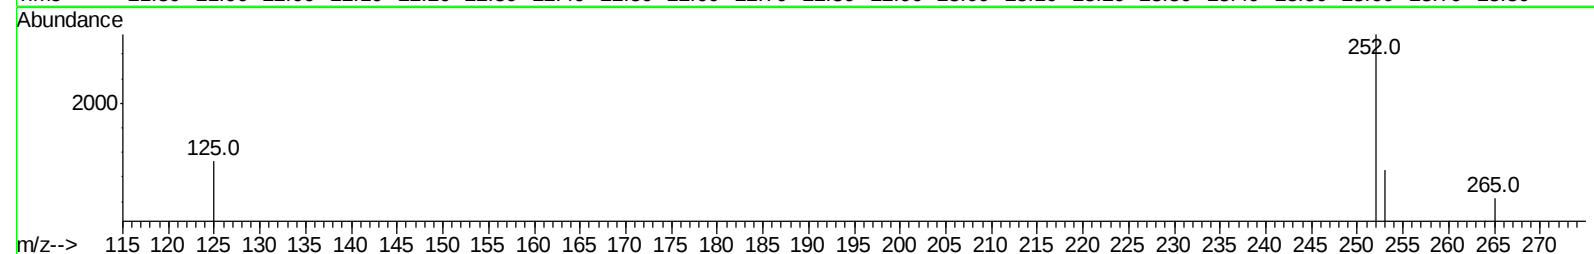


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003160.D
Acq On : 13 Oct 2018 03:43
Operator : MJ/SJ
Sample : J5368-01DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 13 06:03:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 05:59:15 2018
Response via : Initial Calibration

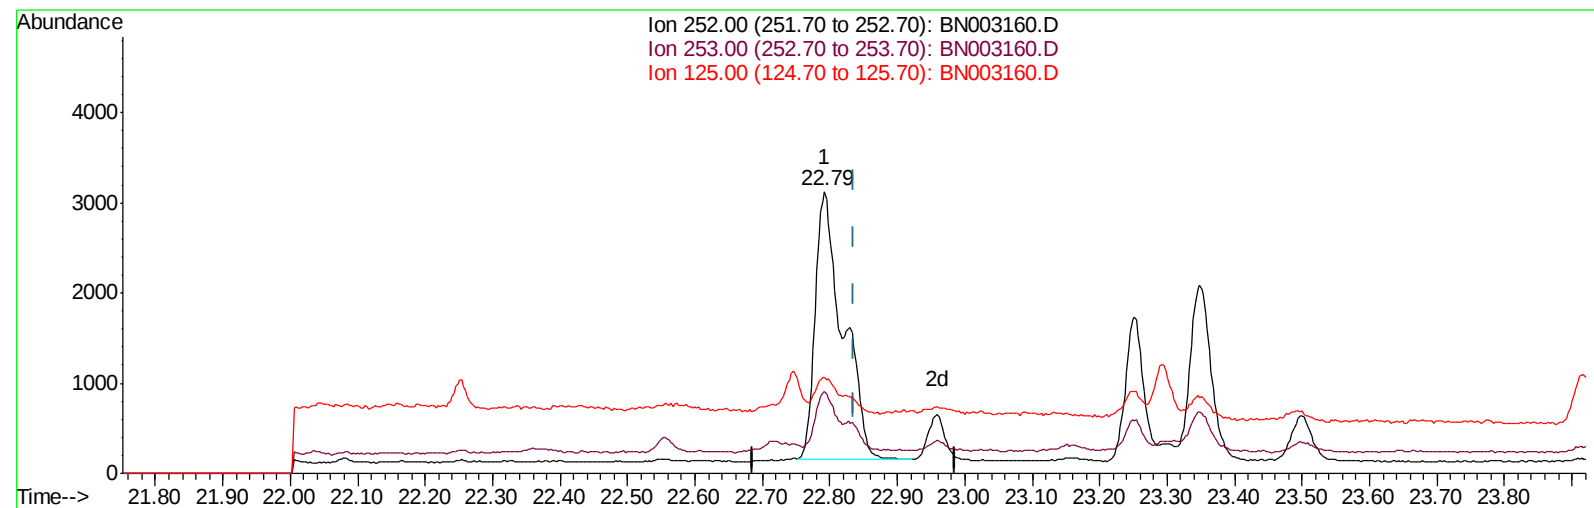

TIC: BN003160.D

(22) Benzo(k)fluoranthene

22.792min (-0.044) 0.44ng/ul

response 8468

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	28.99
125.00	17.60	34.08#
0.00	0.00	0.00