
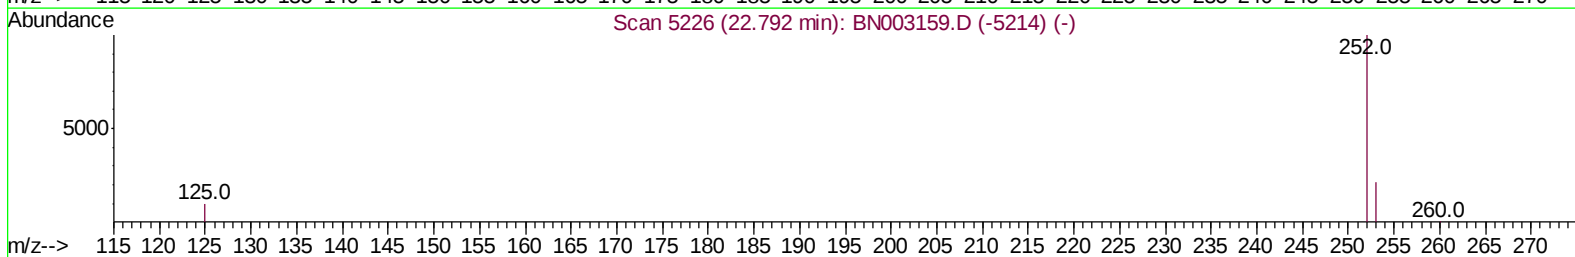
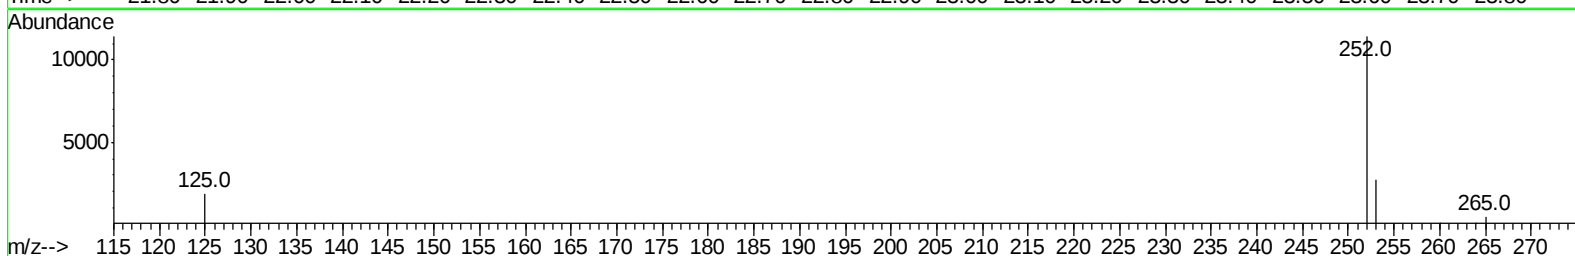


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003161.D
Acq On : 13 Oct 2018 04:18
Operator : MJ/SJ
Sample : J5368-06DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 13 06:03:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 05:59:15 2018
Response via : Initial Calibration

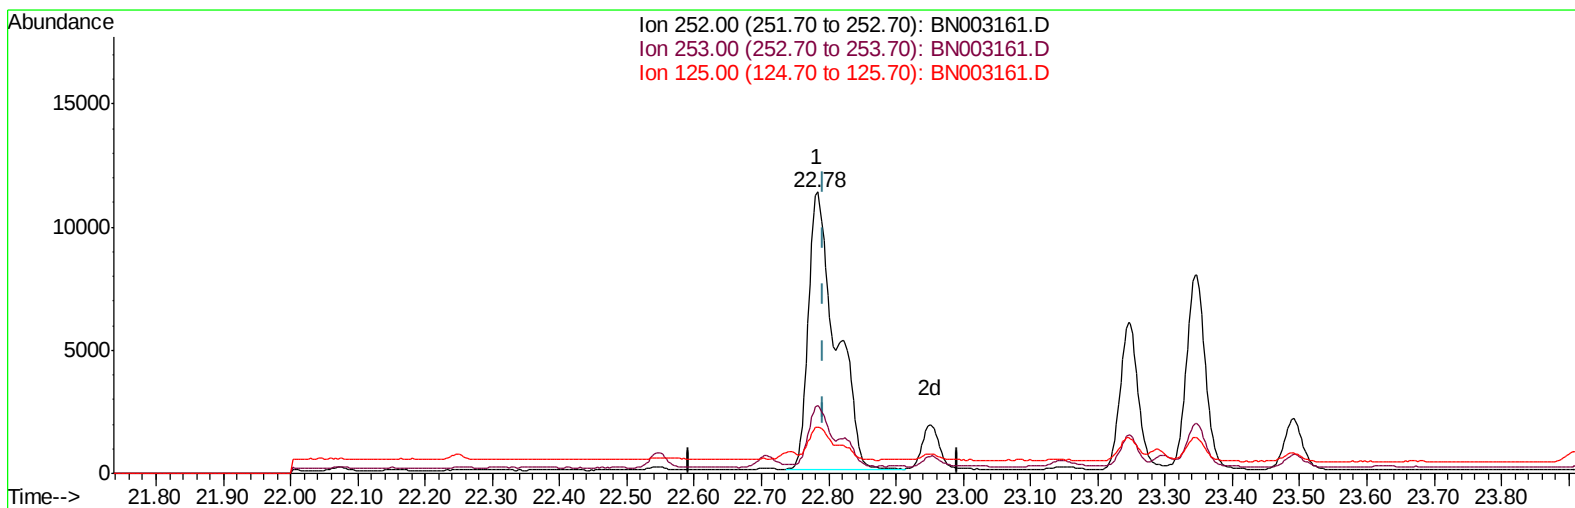

TIC: BN003161.D

(21) Benzo(b)fluoranthene
22.784min (-0.009) 1.51ng/ul
response 31746

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.93
125.00	17.10	16.32
0.00	0.00	0.00