
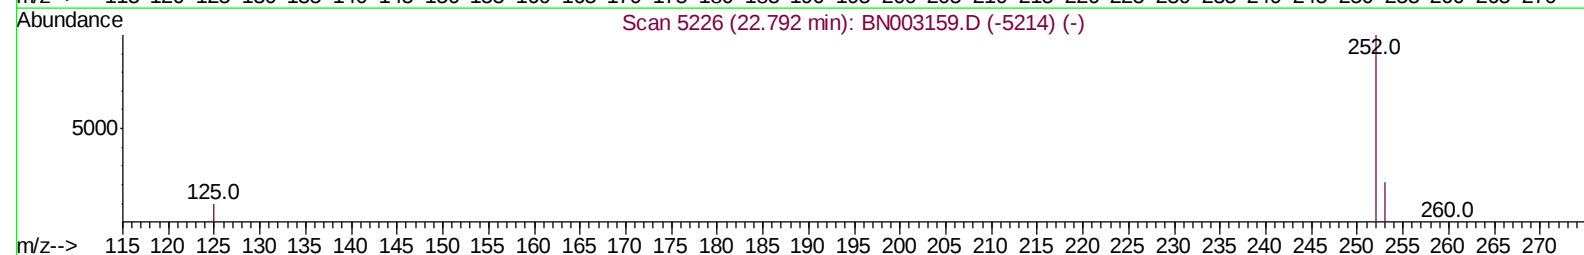
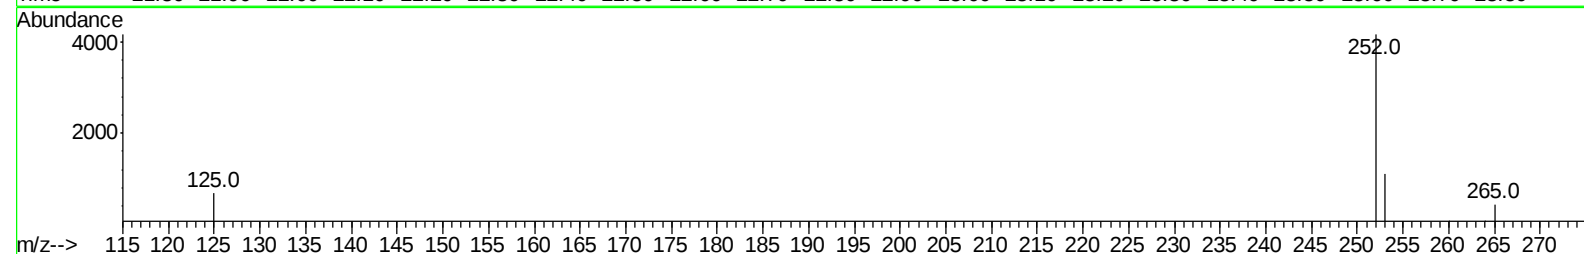


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\  
Data File : BN003162.D  
Acq On : 13 Oct 2018 04:53  
Operator : MJ/SJ  
Sample : J5368-03DL 10X  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Oct 13 06:03:48 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 13 05:59:15 2018  
Response via : Initial Calibration

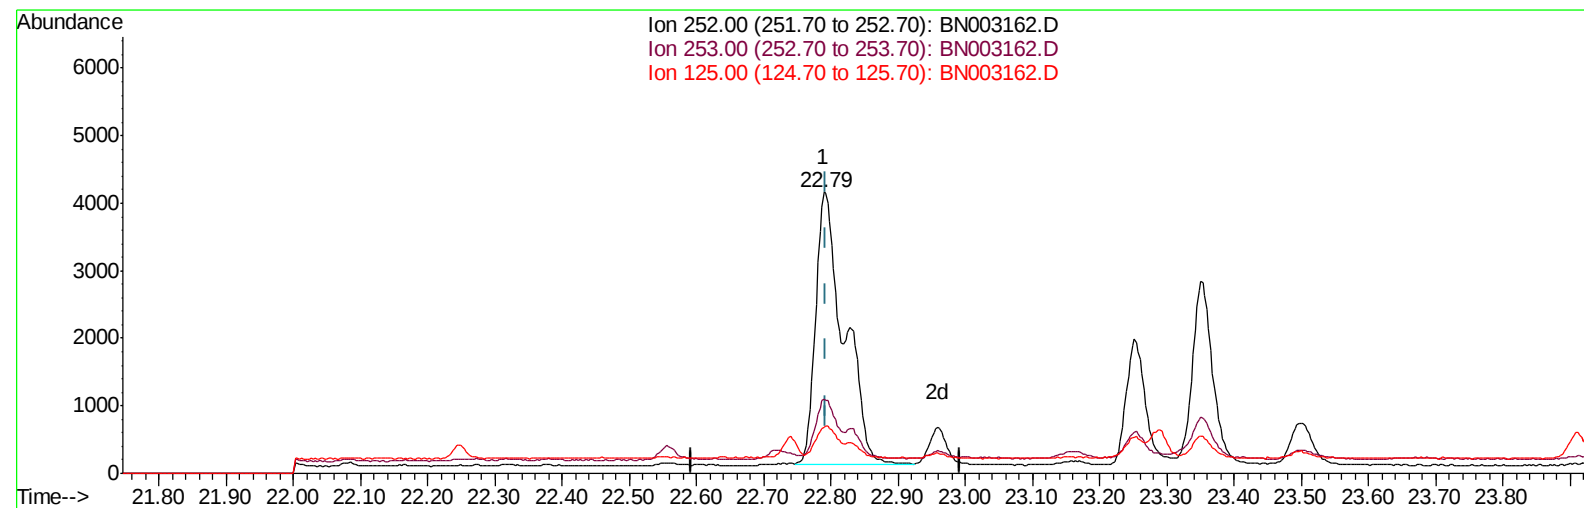

TIC: BN003162.D

(21) Benzo(b)fluoranthene  
22.789min (-0.003) 0.65ng/ul  
response 11826

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 26.60 | 26.34 |
| 125.00 | 17.10 | 16.60 |
| 0.00   | 0.00  | 0.00  |