

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
 Data File : BN003145.D
 Acq On : 12 Oct 2018 18:40
 Operator : MJ/SJ
 Sample : PB113826BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 13 04:57:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 13 04:51:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1369	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	5942	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3646	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	621402	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.44	264	5481	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3650	0.40	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.26	166	971	0.067	ng/ul#	16
23) Benzo(a)pyrene	23.29	252	1443	0.082	ng/ul#	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003145.D
Acq On : 12 Oct 2018 18:40
Operator : MJ/SJ
Sample : PB113826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 13 04:57:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

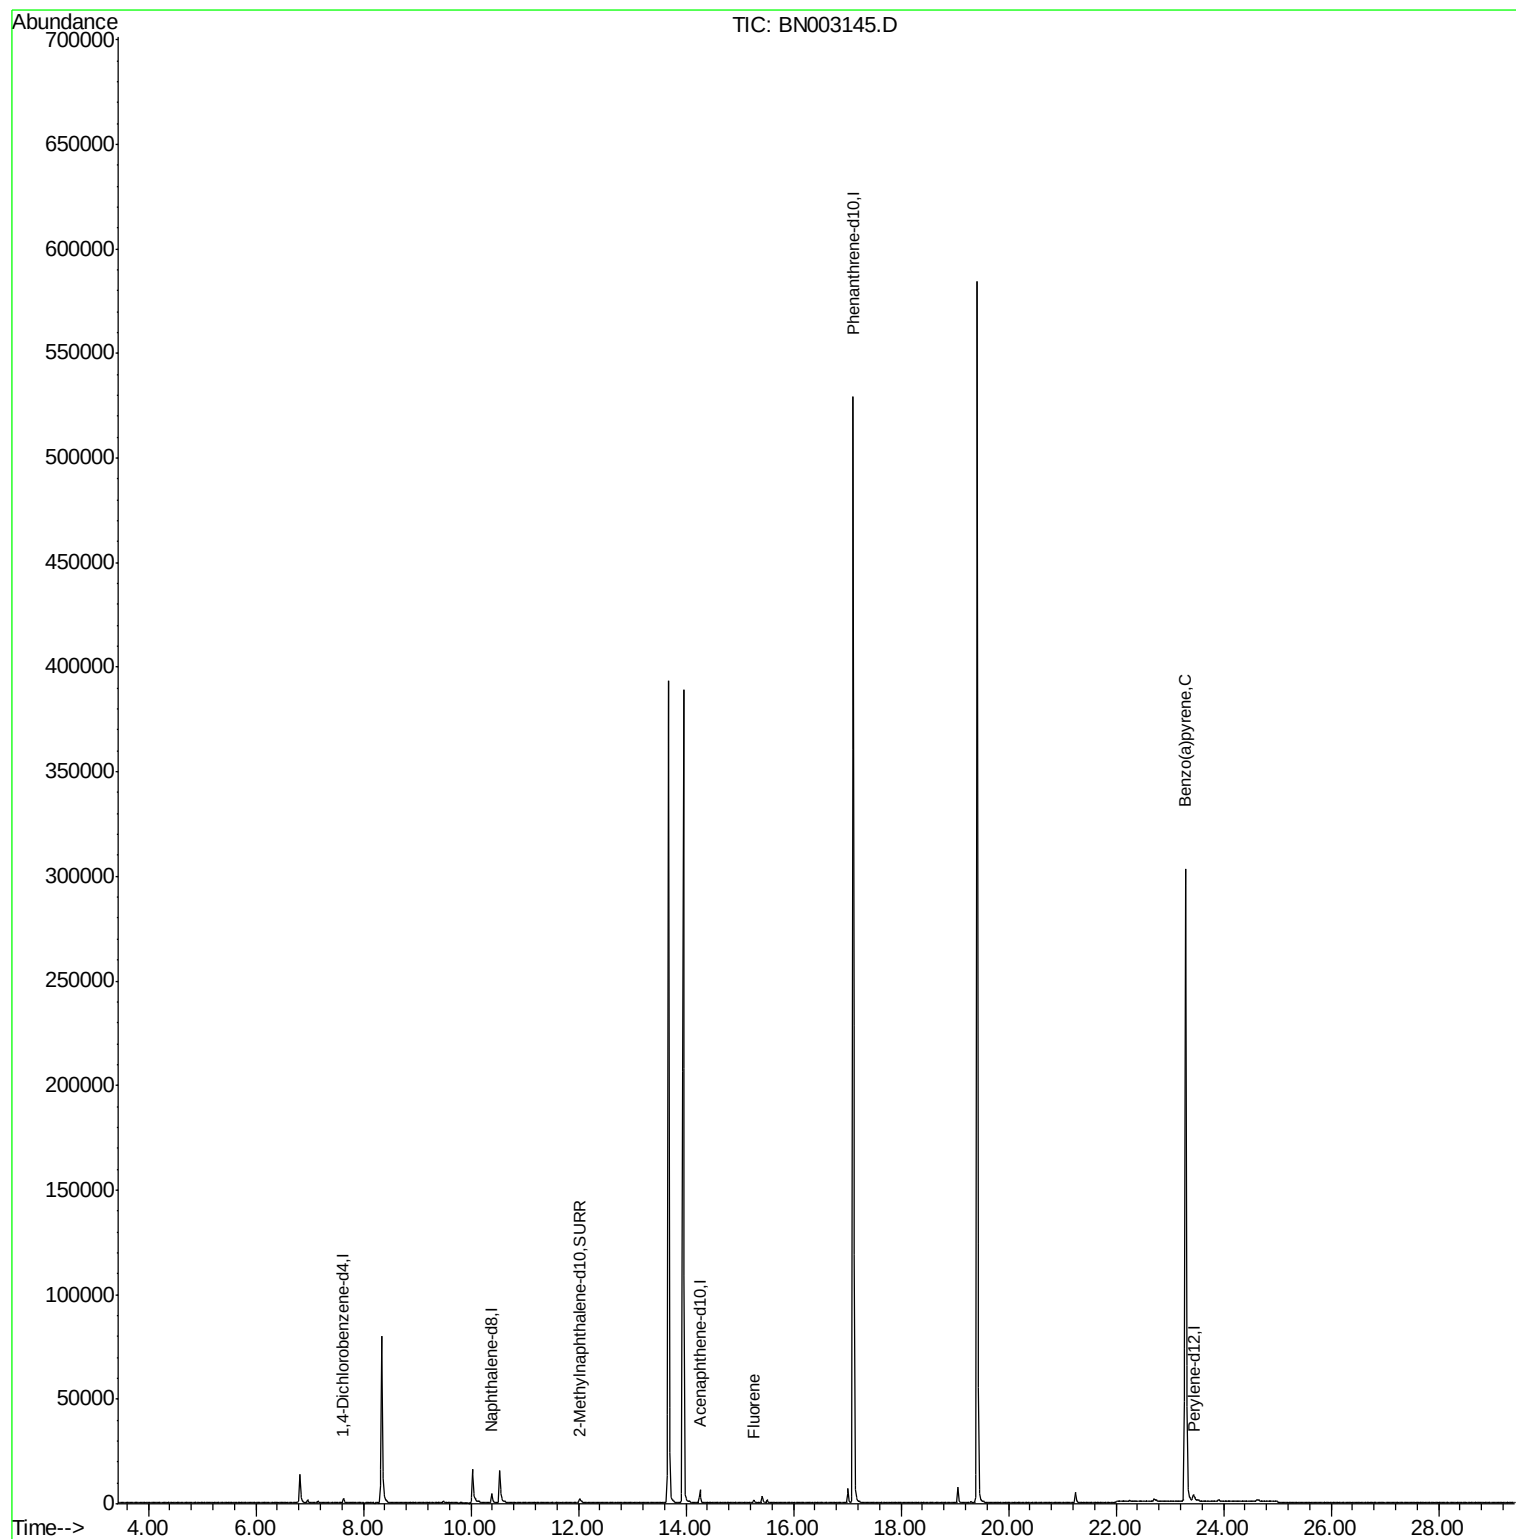

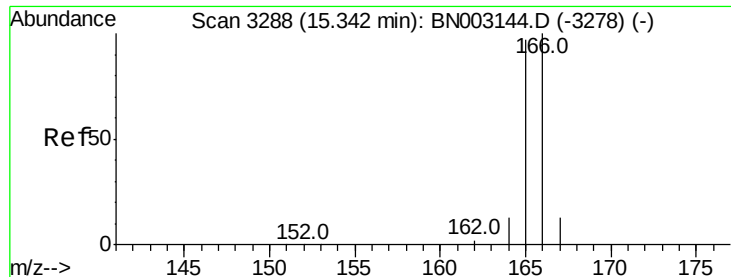

#9

Fluorene

Concen: 0.067 ng/ul

RT: 15.26 min Scan# 3270

Delta R.T. -0.08 min

Lab File: BN003145.D

Acq: 12 Oct 2018 18:40

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 971

Ion Ratio Lower Upper

166 100

165 10.1 78.5 117.7#


167 34.9 11.6 17.4#

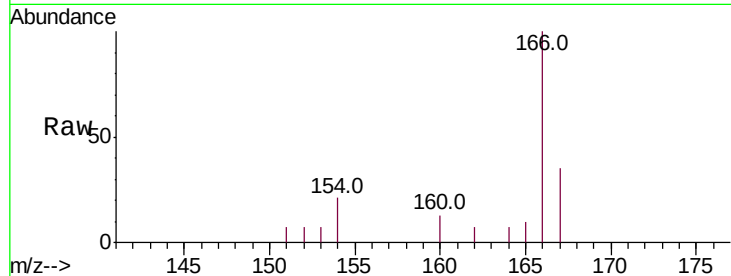



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

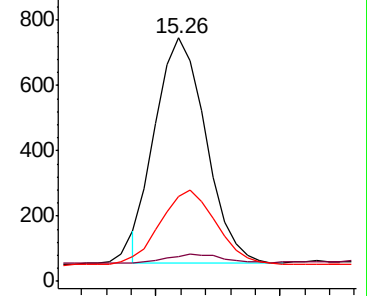

Time-->

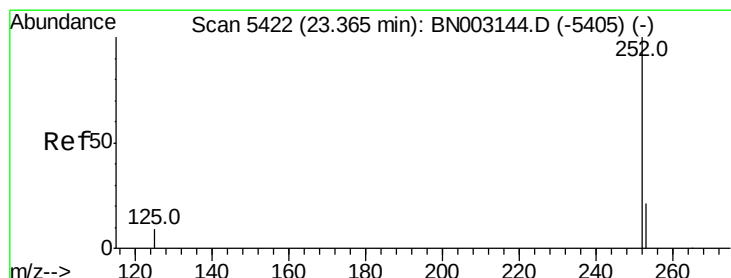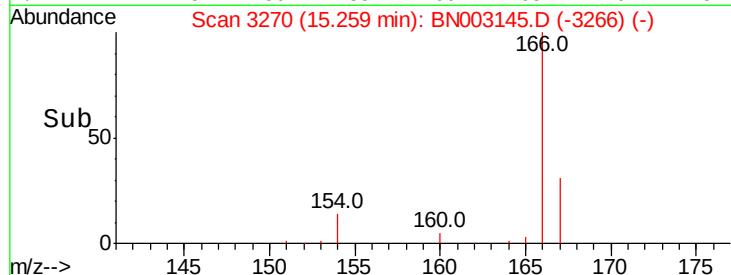

#23

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.29 min Scan# 5398

Delta R.T. -0.07 min

Lab File: BN003145.D

Acq: 12 Oct 2018 18:40


Tgt Ion:252 Resp: 1443

Ion Ratio Lower Upper

252 100

253 53.2 23.1 34.7#


125 95.3 16.9 25.3#

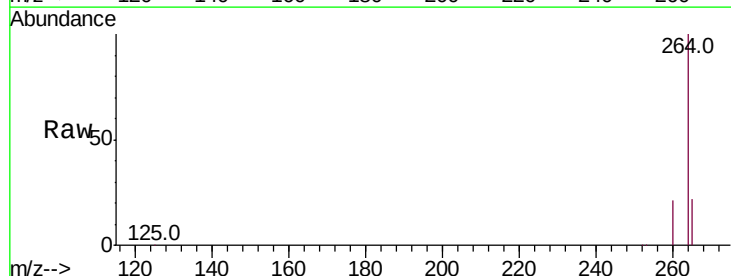

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

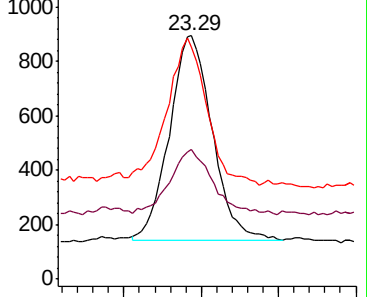

Time-->

