

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
 Data File : BN003155.D
 Acq On : 13 Oct 2018 00:32
 Operator : MJ/SJ
 Sample : J5234-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 13 04:58:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 13 04:51:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1351	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	5846	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3577	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	626085	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.44	264	5631	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3705	0.41	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.26	166	962	0.068	ng/ul#	17
23) Benzo(a)pyrene	23.29	252	1681	0.092	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003155.D
Acq On : 13 Oct 2018 00:32
Operator : MJ/SJ
Sample : J5234-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 13 04:58:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration




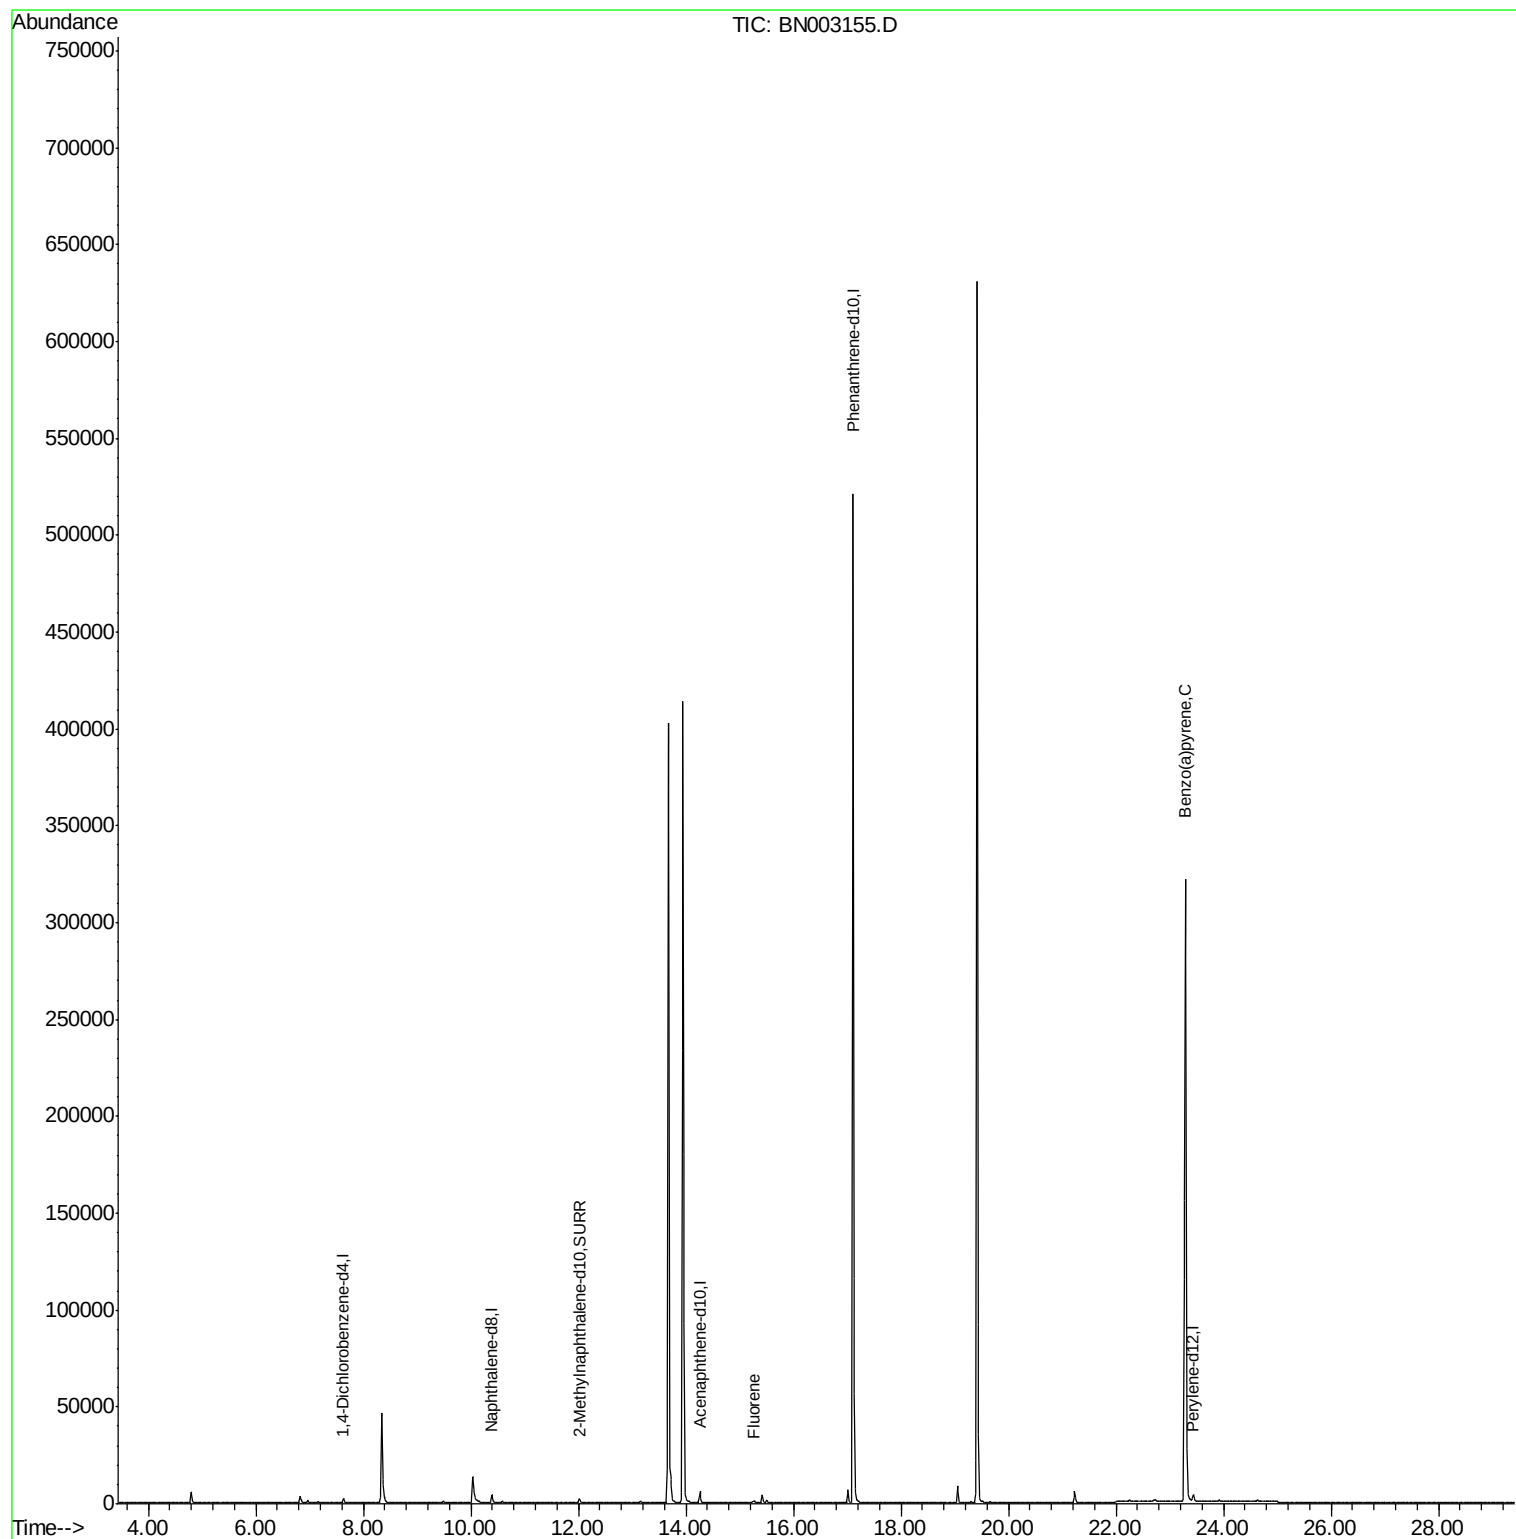


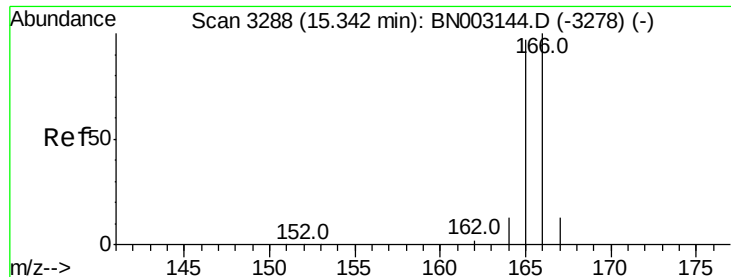

#9
Fluorene
 Concen: 0.068 ng/ul
 RT: 15.26 min Scan# 3270
 Delta R.T. -0.08 min
 Lab File: BN003155.D
 Acq: 13 Oct 2018 00:32

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 962
 Ion Ratio Lower Upper
 166 100
 165 12.0 78.5 117.7#
 167 37.6 11.6 17.4#

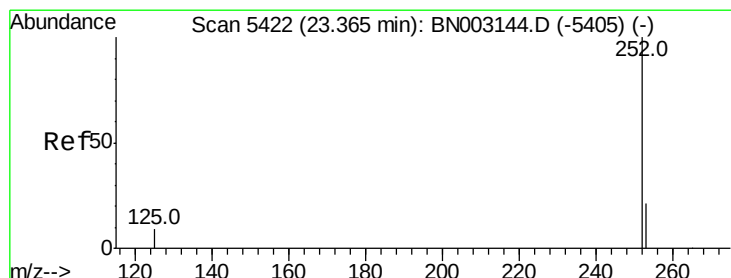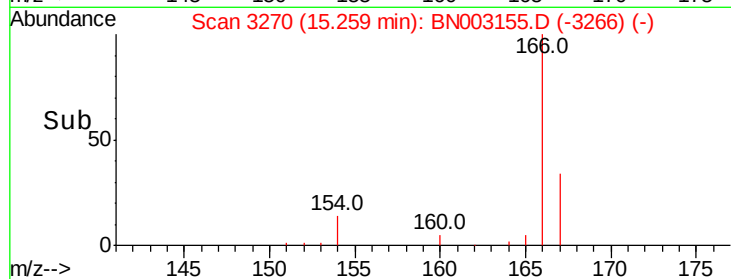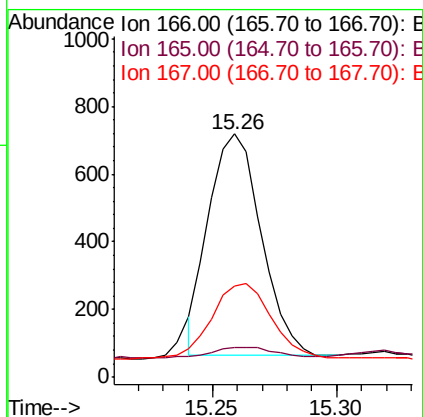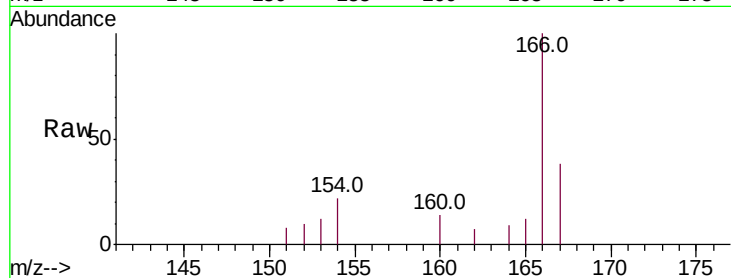

#23
Benzo(a)pyrene
 Concen: 0.092 ng/ul
 RT: 23.29 min Scan# 5396
 Delta R.T. -0.08 min
 Lab File: BN003155.D
 Acq: 13 Oct 2018 00:32

Tgt Ion:252 Resp: 1681
 Ion Ratio Lower Upper
 252 100
 253 52.4 23.1 34.7#
 125 122.3 16.9 25.3#

