

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
 Data File : BN003157.D
 Acq On : 13 Oct 2018 01:43
 Operator : MJ/SJ
 Sample : J5258-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 13 04:58:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 13 04:51:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1093	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	4822	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3086	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	636367	0.40	ng/ul	0.08
16) Chrysene-d12	21.24	240	4314	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	5560	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3634	0.49	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.42	202	1064	0.064	ng/ul#	1
23) Benzo(a)pyrene	23.29	252	1716	0.096	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003157.D
Acq On : 13 Oct 2018 01:43
Operator : MJ/SJ
Sample : J5258-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 13 04:58:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

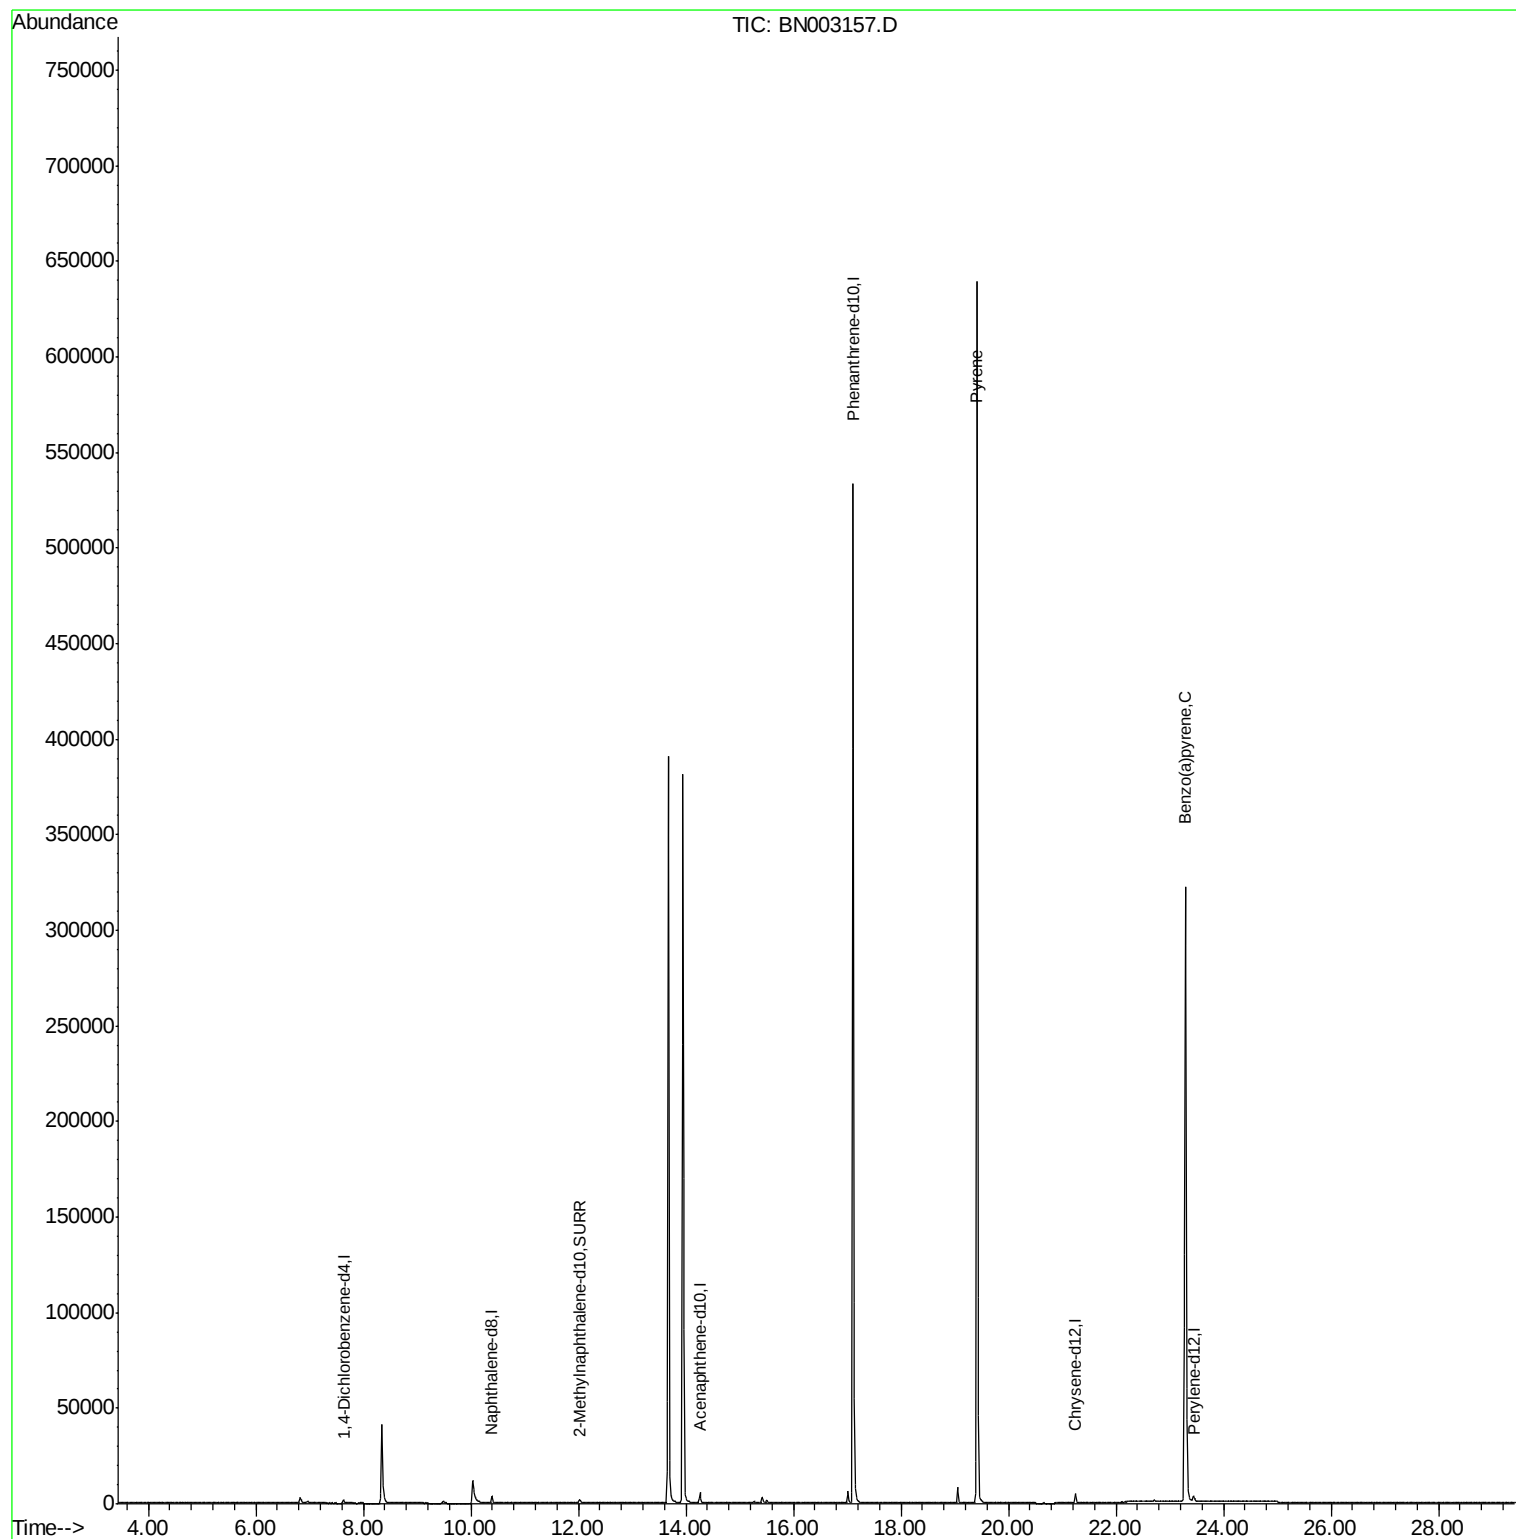

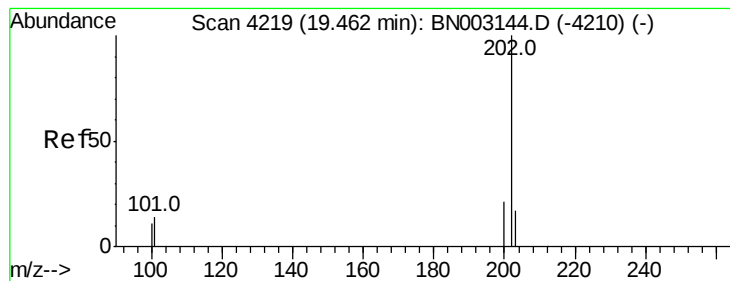

#17

Pvrene

Concen: 0.064 ng/ul

RT: 19.42 min Scan# 4209

Delta R.T. -0.05 min

Lab File: BN003157.D

Acq: 13 Oct 2018 01:43

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 1064

Ion Ratio Lower Upper

202 100

101 144.1 11.9 17.9#




100 920.2 9.9 14.9#

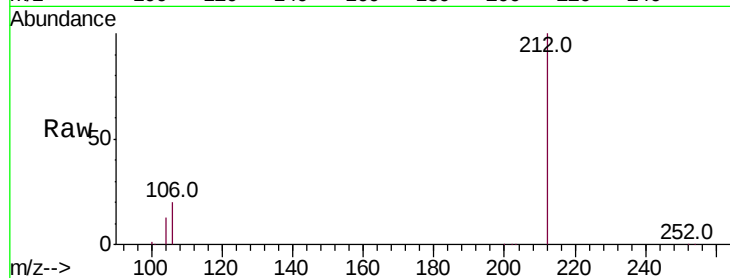

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

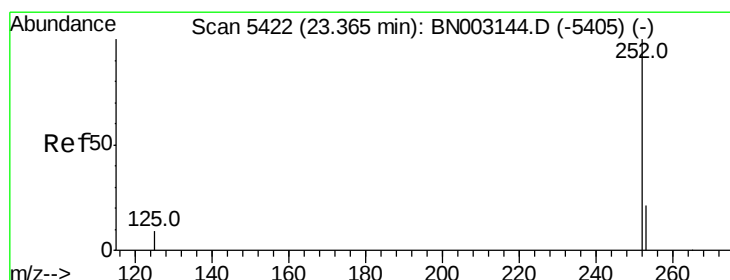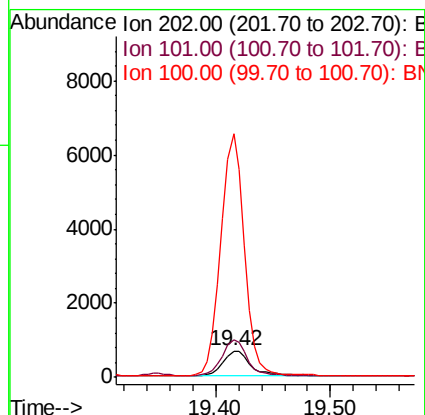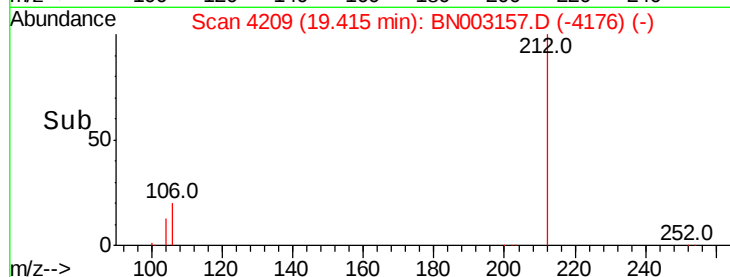

#23

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.29 min Scan# 5397

Delta R.T. -0.07 min

Lab File: BN003157.D

Acq: 13 Oct 2018 01:43


Tgt Ion:252 Resp: 1716

Ion Ratio Lower Upper

252 100

253 49.5 23.1 34.7#

125 80.0 16.9 25.3#

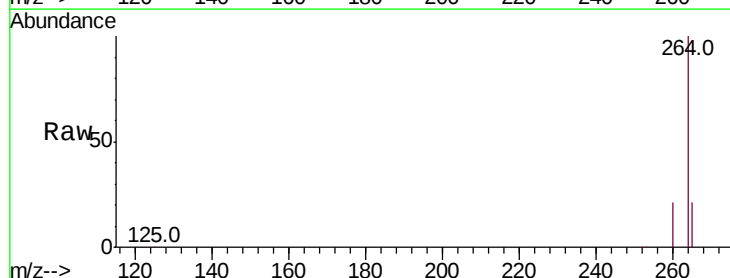

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

