

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
 Data File : BN003158.D
 Acq On : 13 Oct 2018 02:18
 Operator : MJ/SJ
 Sample : J5258-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 13 04:58:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 13 04:51:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1324	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	5698	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3471	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.11	188	444307	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.44	264	5302	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	2723	0.31	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.29	252	1211	0.071	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101318\
Data File : BN003158.D
Acq On : 13 Oct 2018 02:18
Operator : MJ/SJ
Sample : J5258-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 13 04:58:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

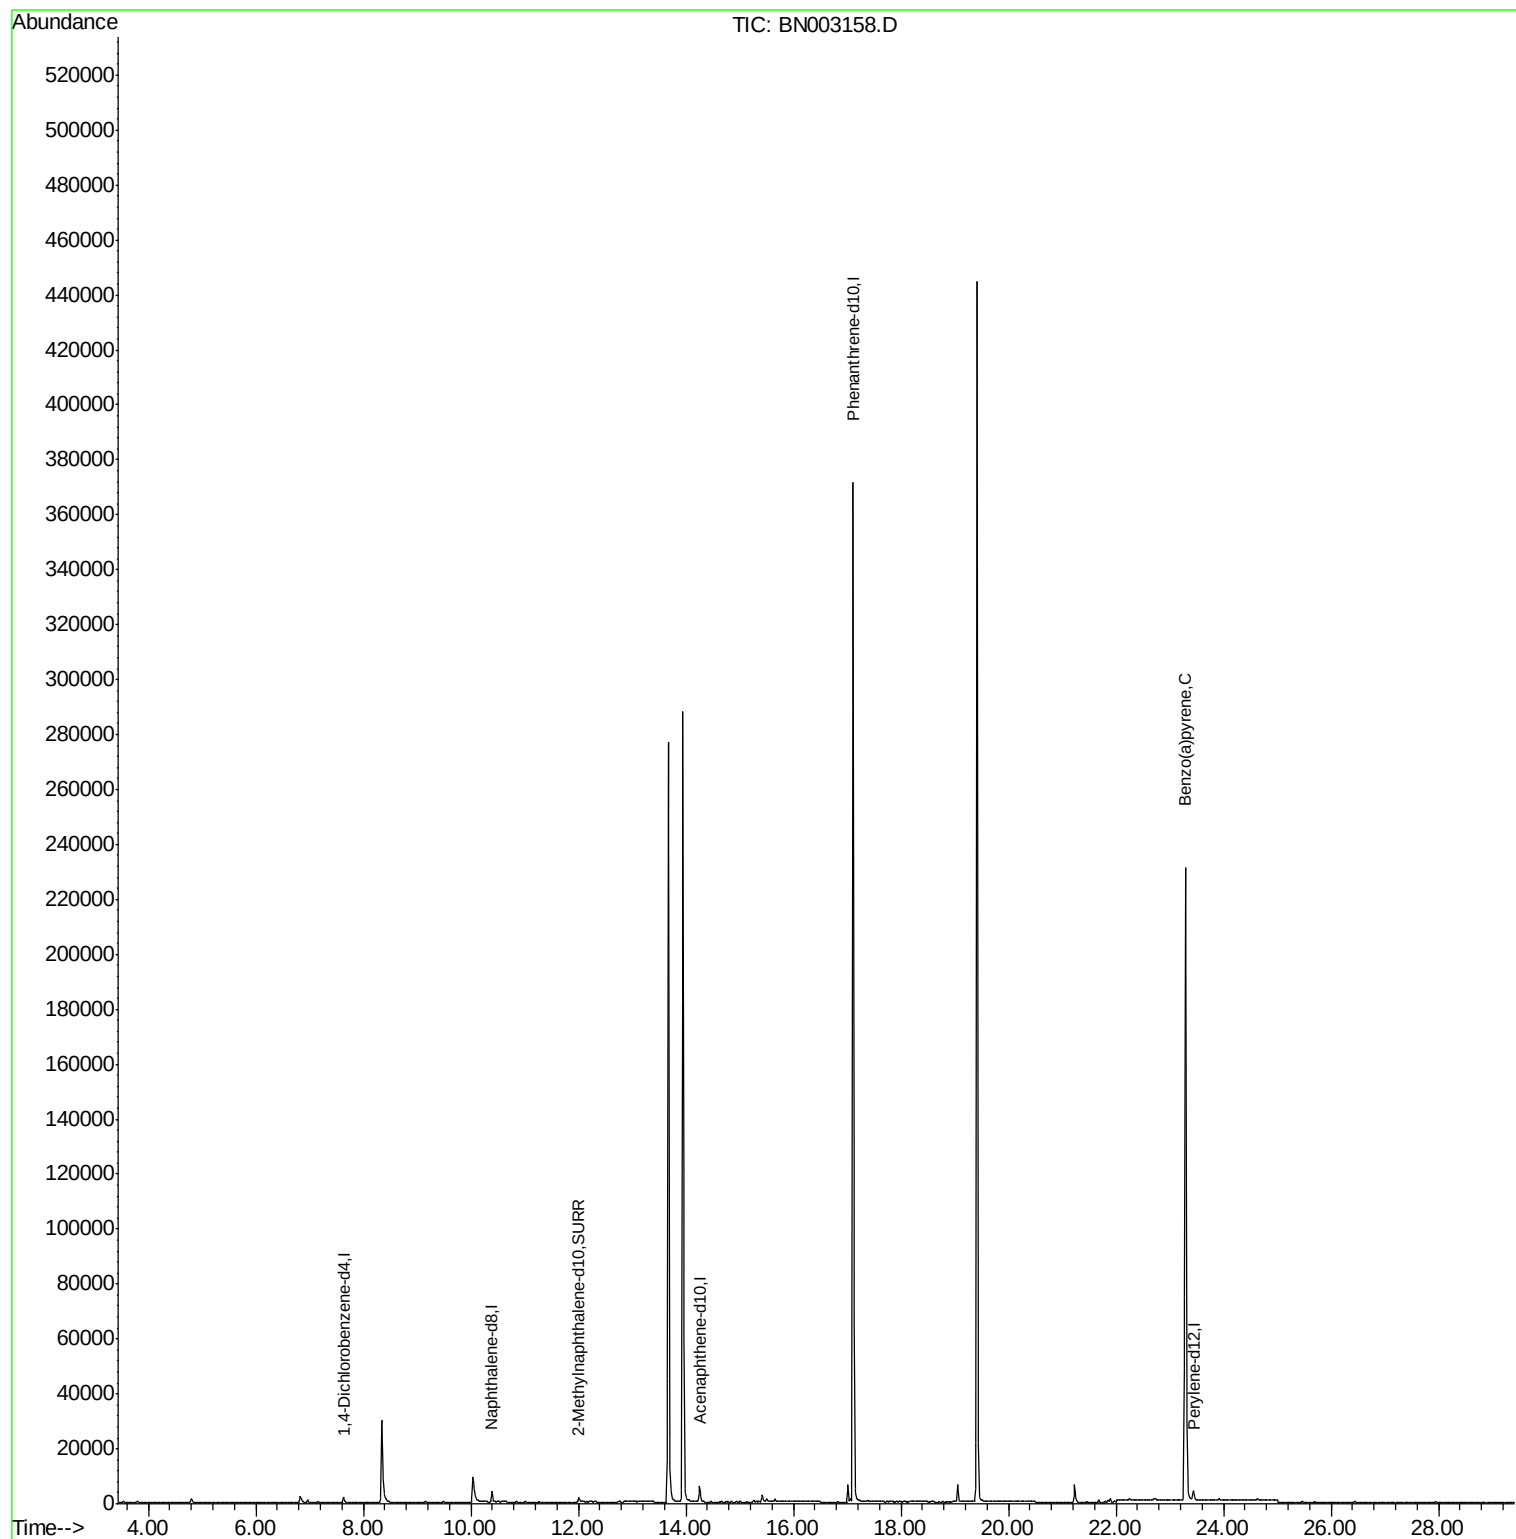

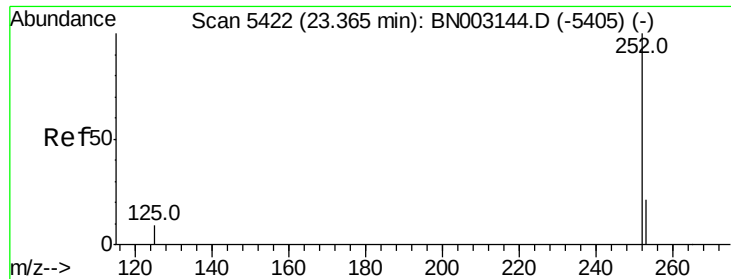

#23

Benzo(a)pyrene

Concen: 0.071 ng/ul

RT: 23.29 min Scan# 5397

Delta R.T. -0.07 min

Lab File: BN003158.D

Acq: 13 Oct 2018 02:18

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 1211

Ion Ratio Lower Upper

252 100

253 59.6 23.1 34.7#

125 107.4 16.9 25.3#

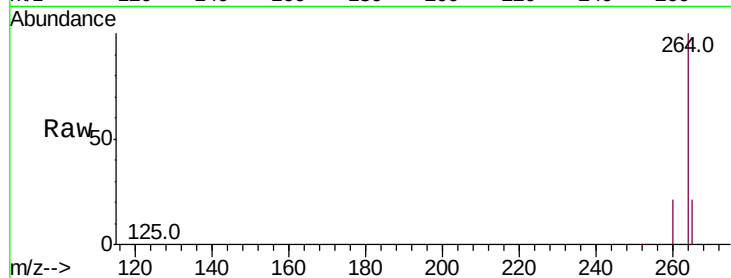

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

