

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101318\
 Data File : BN003156.D
 Acq On : 13 Oct 2018 01:07
 Operator : MJ/SJ
 Sample : J5295-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3Z49

Manual Integrations
 APPROVED

Sohil
 10/15/2018 4:15:12 PM

Quant Time: Oct 13 05:50:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 13 04:51:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1302	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	5582	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3559	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	7954m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	6567m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4468m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	3808	0.44	ng/ul	-0.02
14) Fluoranthene-d10	19.06	212	9925m	0.44	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.34	153	1396	0.113	ng/ul#	Qvalue 26

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101318\
Data File : BN003156.D
Acq On : 13 Oct 2018 01:07
Operator : MJ/SJ
Sample : J5295-01
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A3Z49

Manual Integrations
APPROVED

Sohil
10/15/2018 4:15:12 PM

Quant Time: Oct 13 05:50:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 13 04:51:37 2018
Response via : Initial Calibration

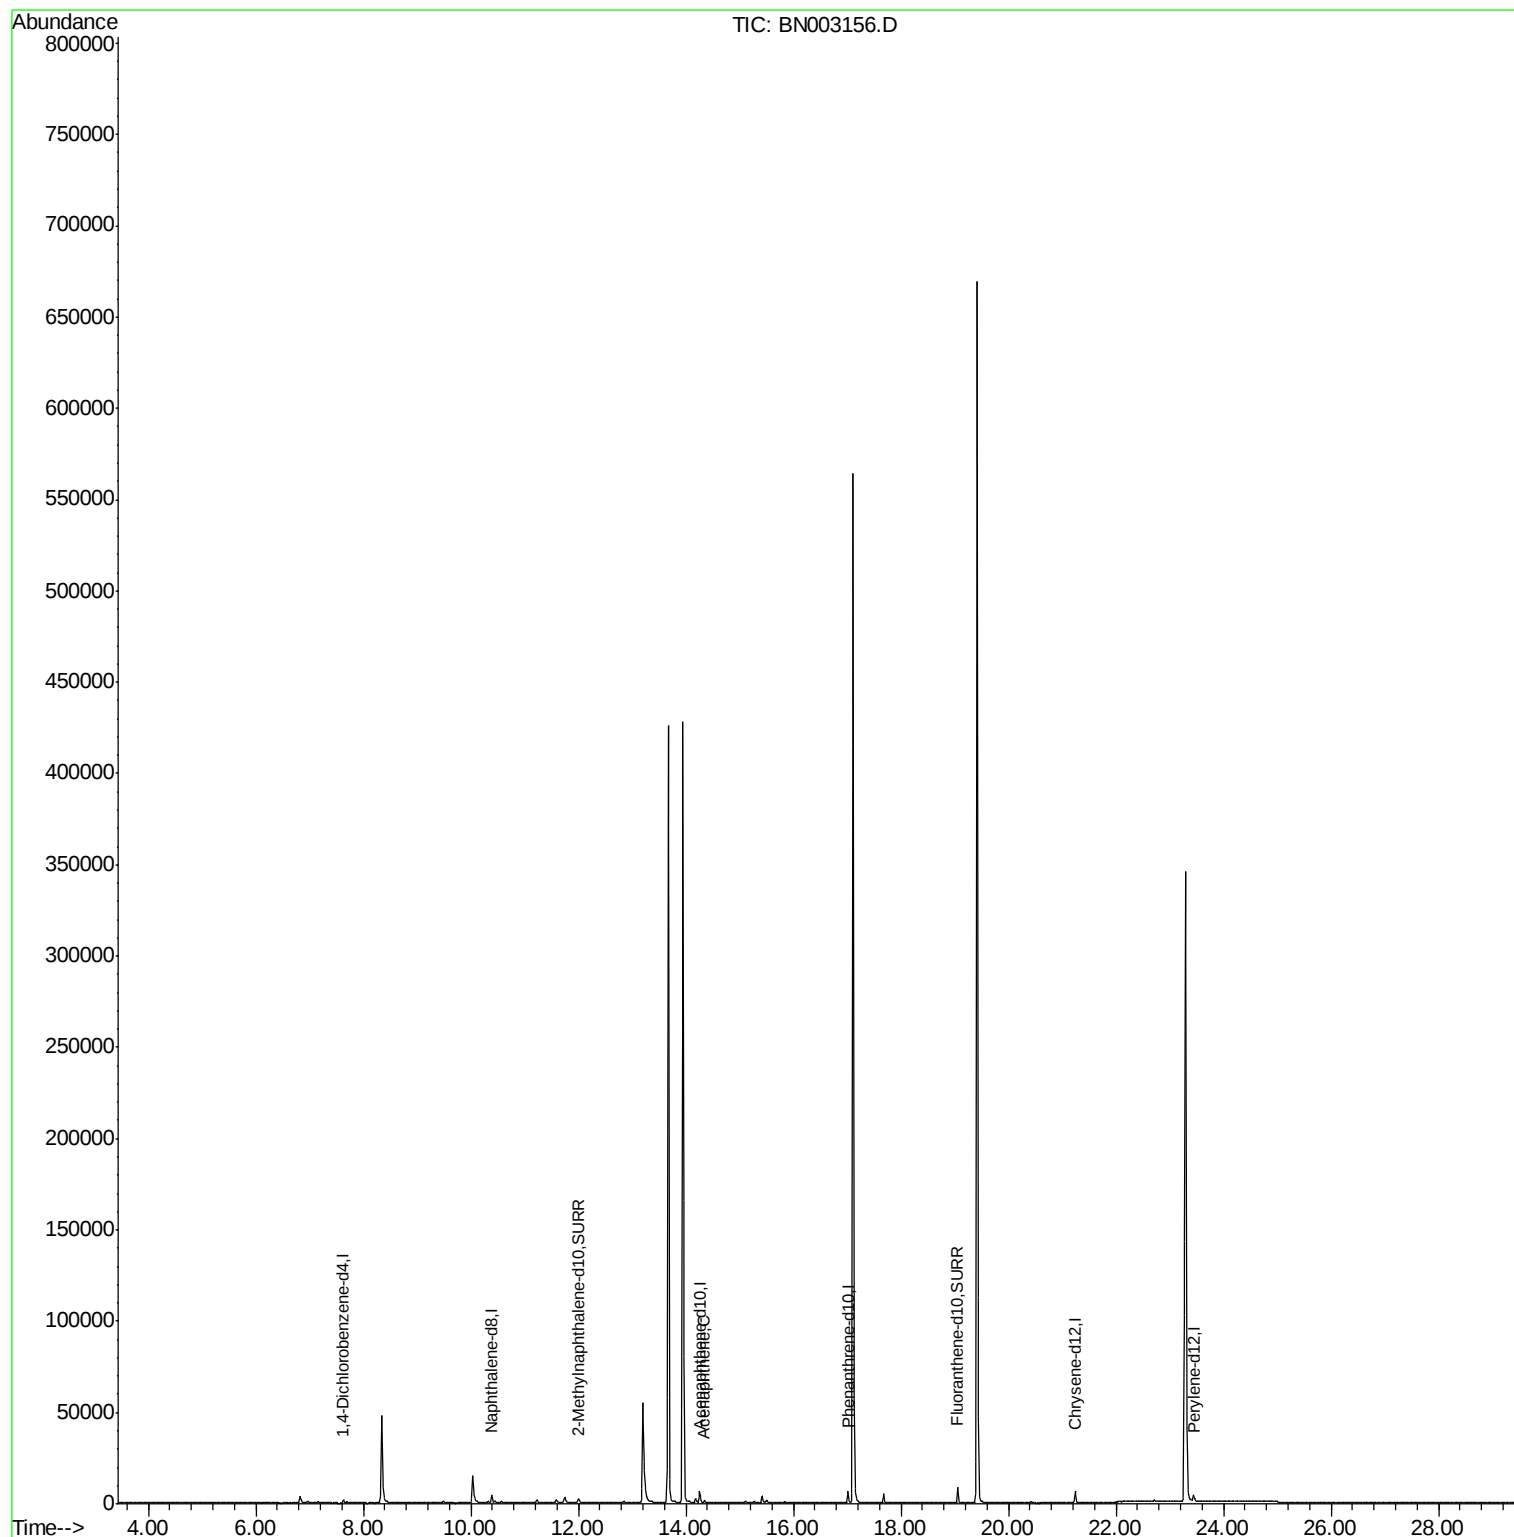

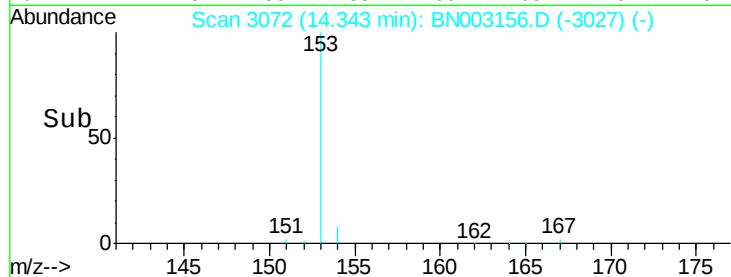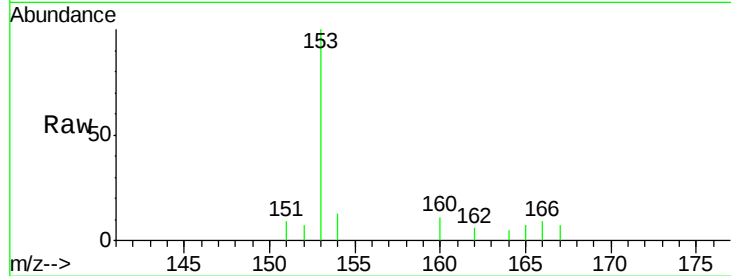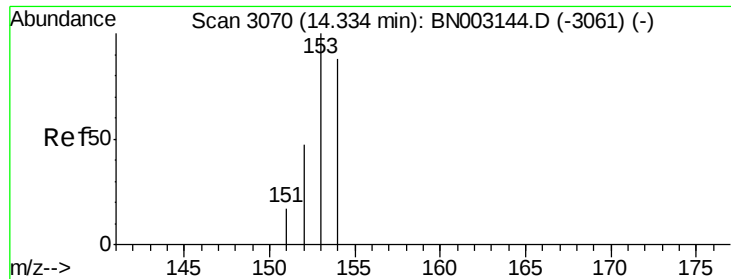

#8

Acenaphthene

Concen: 0.113 ng/ul

RT: 14.34 min Scan# 3072

Delta R.T. 0.01 min

Lab File: BN003156.D

Acq: 13 Oct 2018 01:07

Instrument :

BNA_N

ClientSampleId :

A3Z49

Tgt Ion:153 Resp: 1396

Ion Ratio Lower Upper

153 100

152 6.6 38.2 57.4#

154 13.1 70.2 105.2#

Manual Integrations

APPROVED

Sohil

10/15/2018 4:15:12 PM

