

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101320\
 Data File : BN012169.D
 Acq On : 13 Oct 2020 20:37
 Operator : CG/JU
 Sample : L4359-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7M8

Quant Time: Oct 14 00:17:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 00:15:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	226703	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	887423	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	546589	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1139971	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1151599	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1206729	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	33352	6.50	ng/uL	0.00
5) Phenol-d5	6.80	99	120887	6.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	331748	27.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	360599	23.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	220946	13.96	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	210697	29.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	236007	29.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	388587	25.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	27541	1.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1329471	29.71	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1637811	30.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	34001	4.07	ng/ul	0.01
58) Fluorene-d10	15.27	176	1151050	29.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	220027	29.13	ng/ul	0.00
71) Anthracene-d10	17.12	188	2029346	36.37	ng/ul	0.00
79) Pyrene-d10	19.42	212	2186815	36.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	2560882	37.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	47434	1.016	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101320\
Data File : BN012169.D
Acq On : 13 Oct 2020 20:37
Operator : CG/JU
Sample : L4359-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7M8

Quant Time: Oct 14 00:17:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 00:15:58 2020
Response via : Initial Calibration

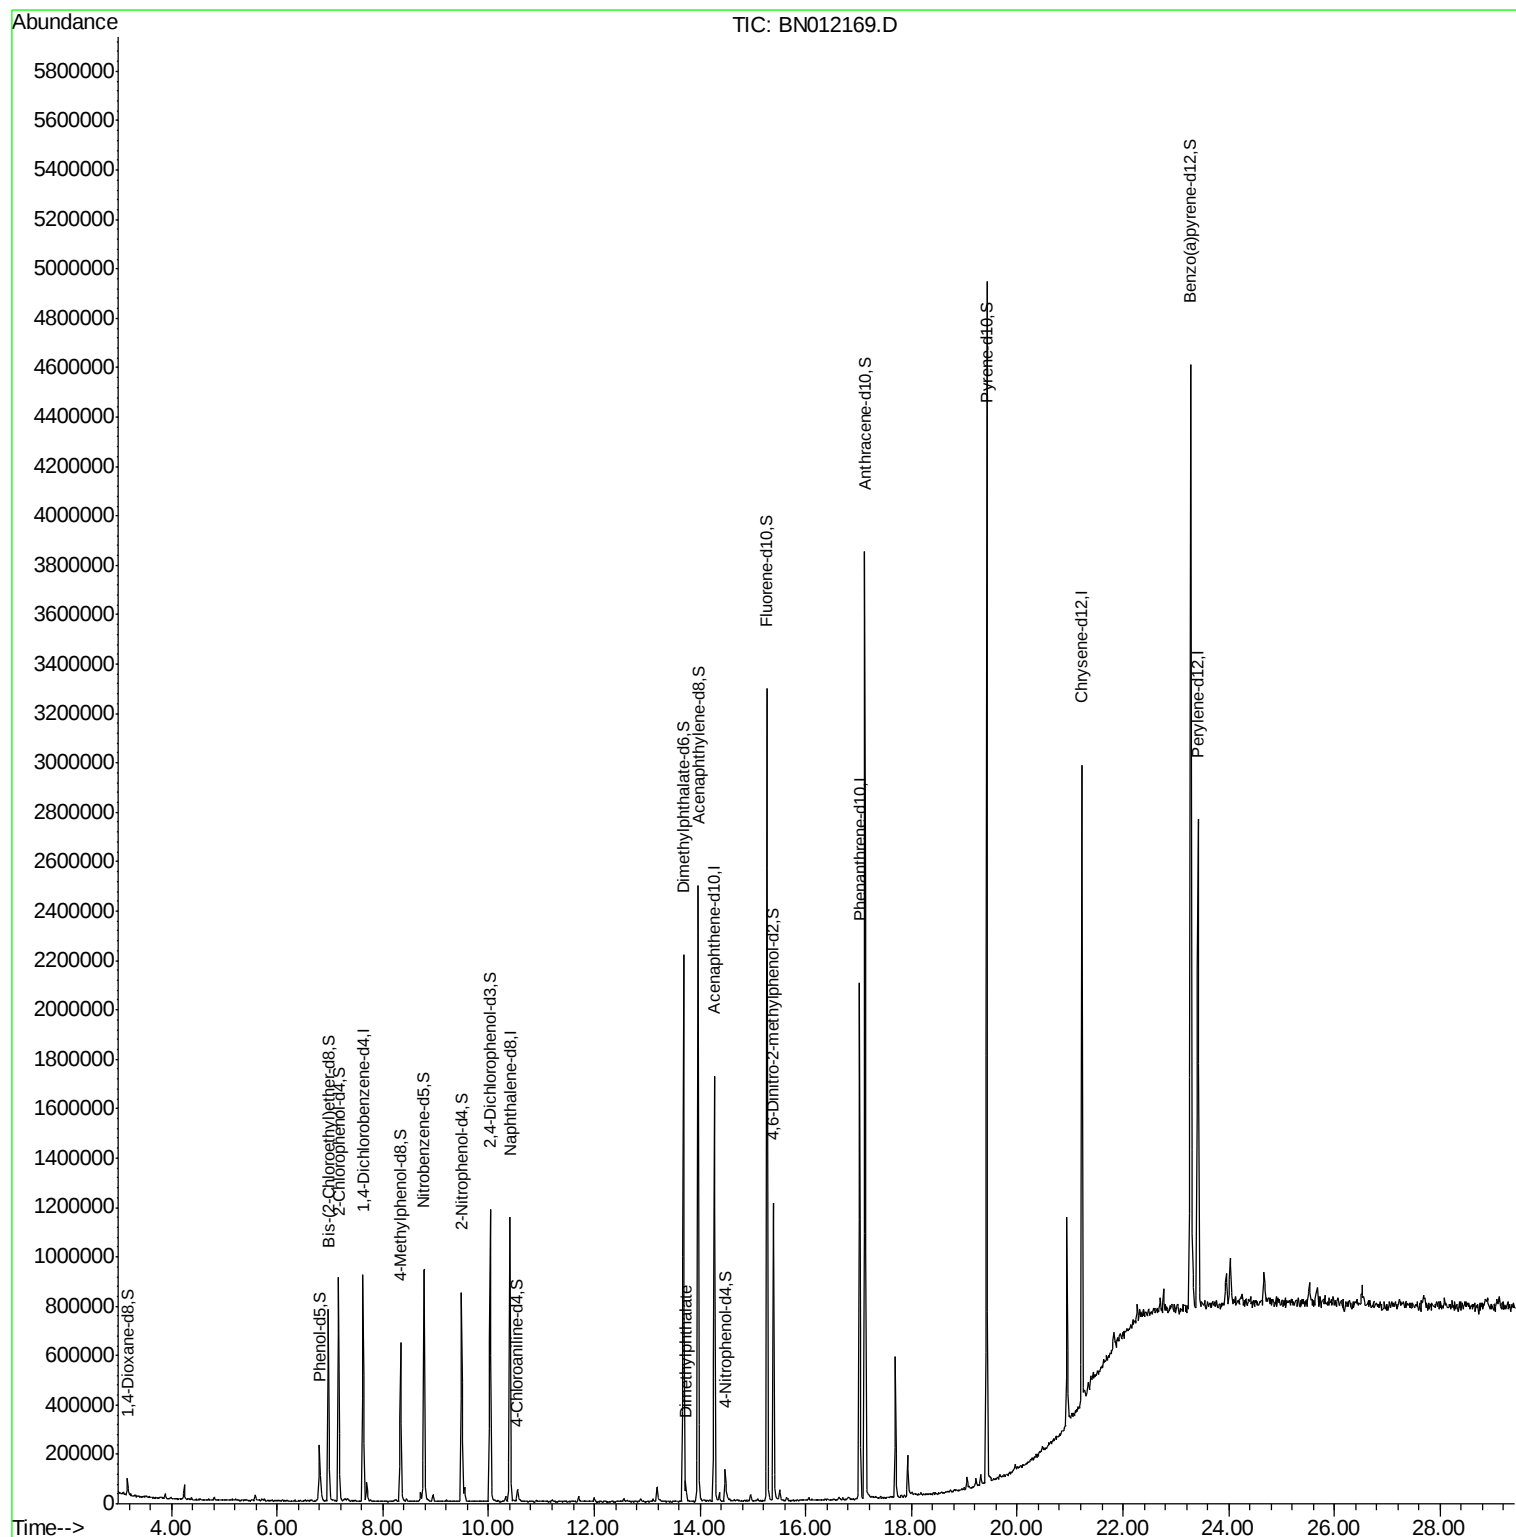

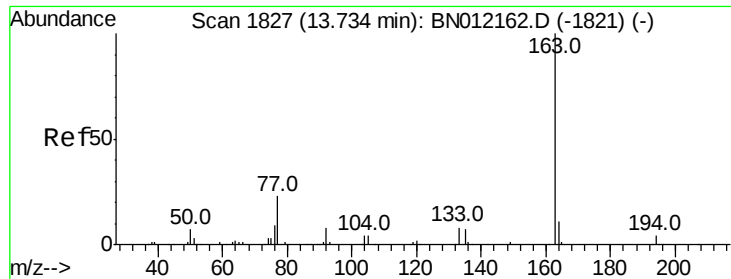

#45

Dimethylphthalate

Concen: 1.016 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BN012169.D

Acq: 13 Oct 2020 20:37

Instrument :

BNA_N

ClientSampleId :

CB7M8


Tot Ion:163 Resp: 47434

Ion Ratio Lower Upper

163 100

194 5.7 3.7 5.5#

164 11.2 8.6 12.8

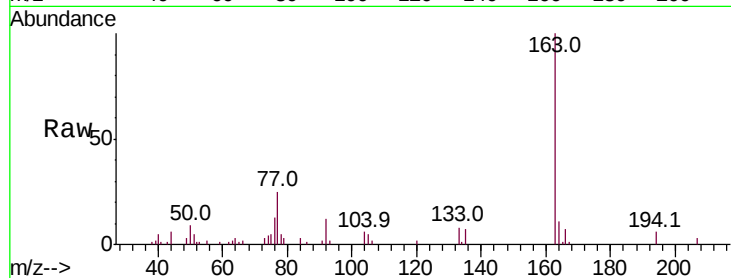

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

