

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101320\
 Data File : BN012175.D
 Acq On : 14 Oct 2020 00:15
 Operator : CG/JU
 Sample : L4359-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7P3

Quant Time: Oct 14 03:23:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 03:20:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	293025	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1183031	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	745640	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1601549	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1536506	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1565299	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	40319	6.08	ng/uL	0.00
5) Phenol-d5	6.81	99	117953	4.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	289131	18.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	332754	16.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	227305	11.11	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	189923	19.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	209834	19.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	396518	19.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	485439	19.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1349228	22.10	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1590719	22.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	42569	3.74	ng/ul	0.01
58) Fluorene-d10	15.27	176	1143026	21.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	126793	11.95	ng/ul	0.00
71) Anthracene-d10	17.12	188	1770946	22.59	ng/ul	0.00
79) Pyrene-d10	19.42	212	1986627	24.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	2070552	23.44	ng/ul	0.00

Target Compounds


					Ovalue	
2) 1,4-Dioxane	3.20	88	53338	7.110	ng/uL	95
28) Naphthalene	10.45	128	225371	3.252	ng/ul	99
34) 2-Methylnaphthalene	12.07	142	147254	3.092	ng/ul	97
35) 1-Methylnaphthalene	12.29	142	123338	2.635	ng/uL#	96
41) 1,1'-Biphenyl	13.10	154	62609	1.014	ng/ul	99
45) Dimethylphthalate	13.73	163	127697	2.004	ng/ul	97
50) Acenaphthene	14.33	153	719812	13.560	ng/ul	98
54) Dibenzofuran	14.67	168	411006	5.560	ng/ul	97
59) Fluorene	15.32	166	544459	8.758	ng/ul	97
70) Phenanthrene	17.06	178	1102907	11.284	ng/ul	99
72) Anthracene	17.15	178	189259	1.901	ng/ul	96
75) Carbazole	17.43	167	603488	7.124	ng/ul	99
77) Fluoranthene	19.09	202	358008	3.235	ng/ul	97
80) Pyrene	19.45	202	197281	1.800	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101320\
Data File : BN012175.D
Acq On : 14 Oct 2020 00:15
Operator : CG/JU
Sample : L4359-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7P3

Quant Time: Oct 14 03:23:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 03:20:27 2020
Response via : Initial Calibration

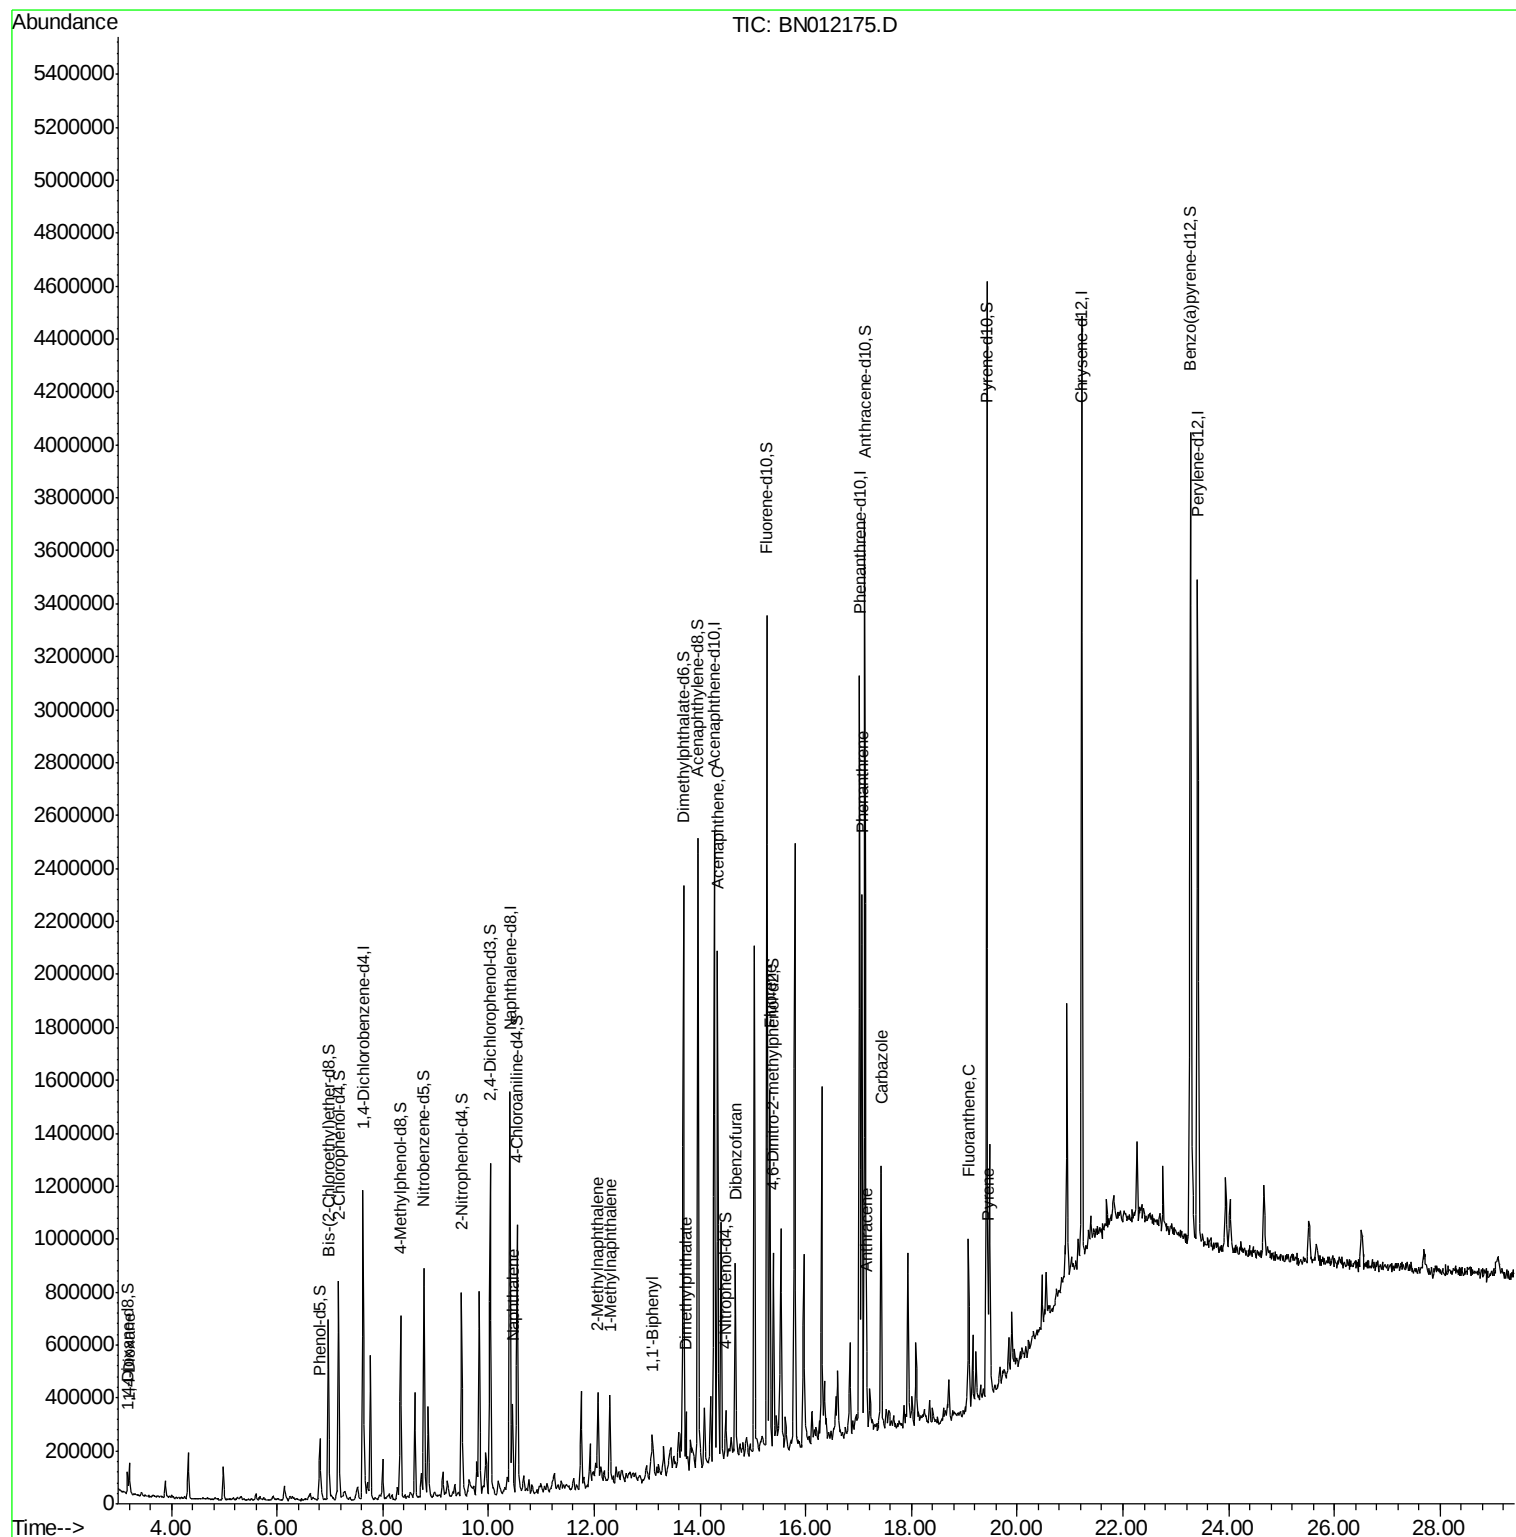

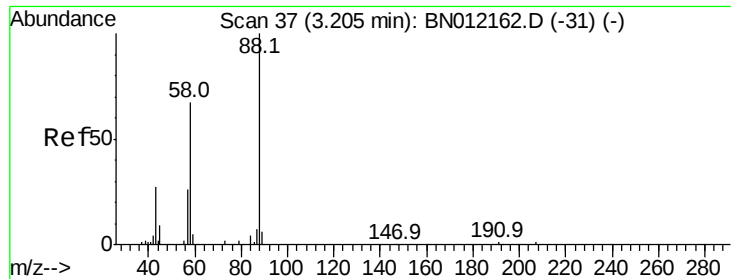

#2

1,4-Dioxane

Concen: 7.110 ng/uL

RT: 3.20 min Scan# 37

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampled :

CB7P3


Tot Ion: 88 Resp: 53338

Ion Ratio Lower Upper

88 100

43 31.2 26.5 39.7




58 70.8 61.0 91.4

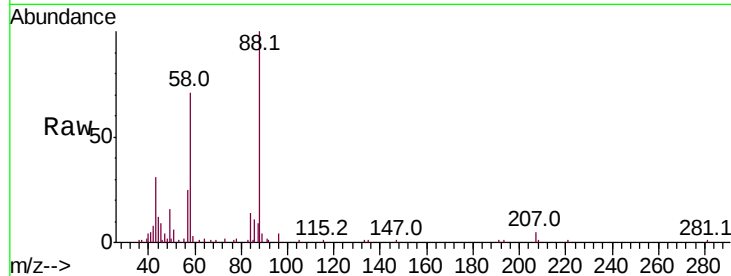

Abundance Ion 88.00 (87.70 to 88.70): BN0

Ion 43.00 (42.70 to 43.70): BN0

Ion 58.00 (57.70 to 58.70): BN0

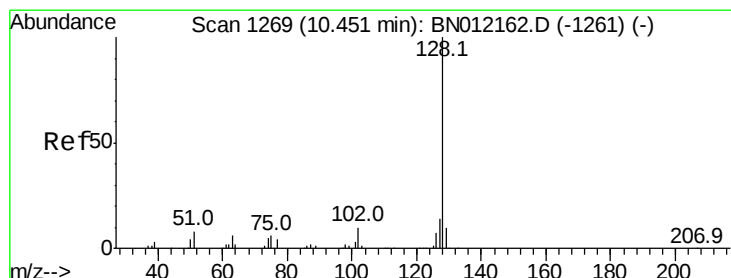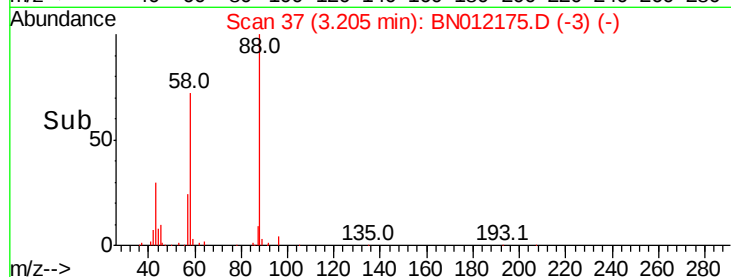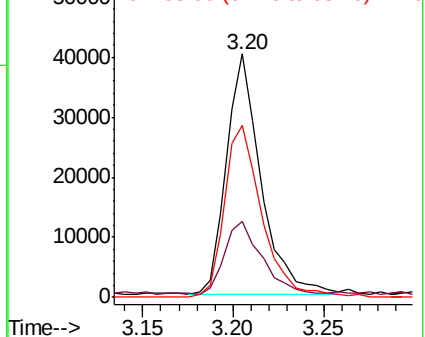

#28

Naphthalene

Concen: 3.252 ng/uL

RT: 10.45 min Scan# 1269

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion: 128 Resp: 225371

Ion Ratio Lower Upper

128 100

129 10.8 8.8 13.2



127 13.1 10.7 16.1

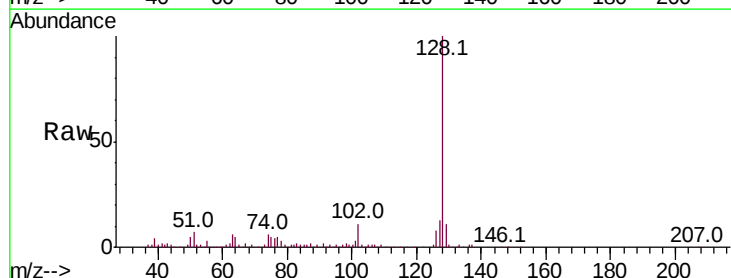


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

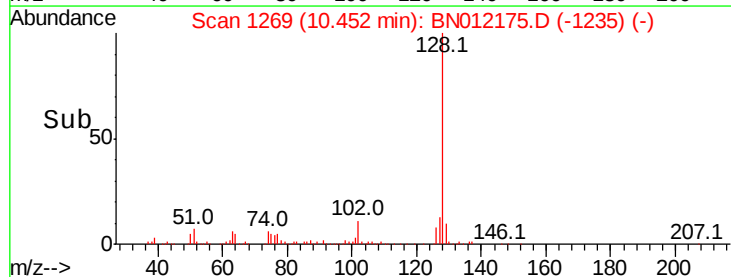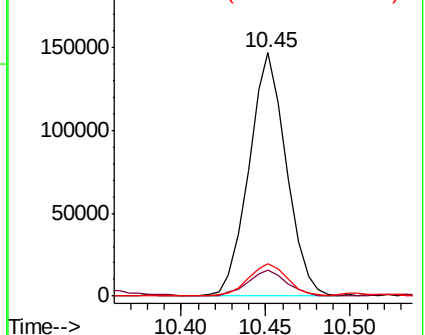

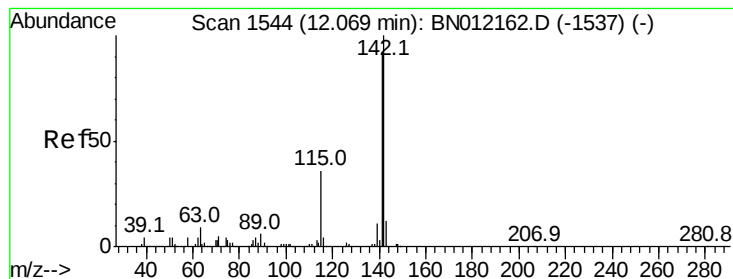

#34

2-Methylnaphthalene

Concen: 3.092 ng/ul

RT: 12.07 min Scan# 1544

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampleId :


CB7P3

Tot Ion:142 Resp: 147254

Ion Ratio Lower Upper




142 100

141 92.4 75.9 113.9

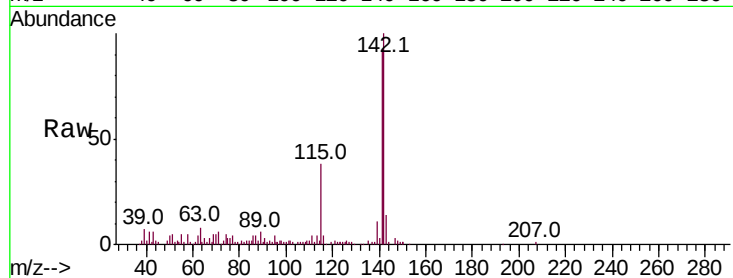

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

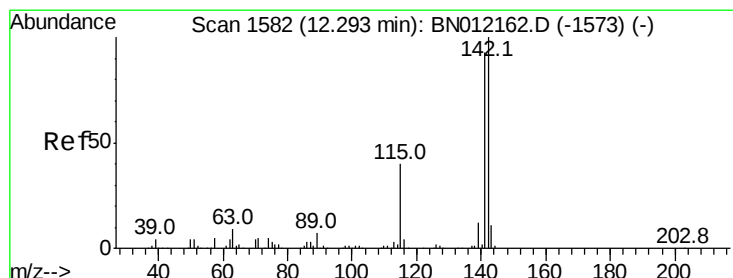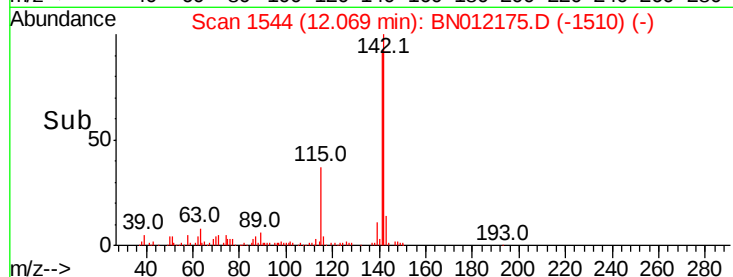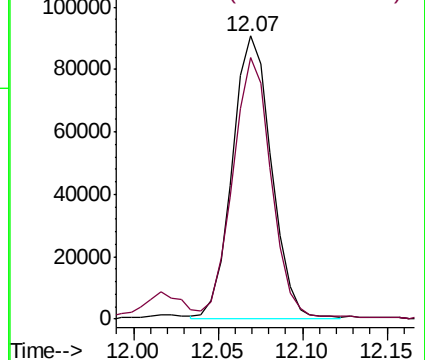

#35

1-Methylnaphthalene

Concen: 2.635 ng/uL

RT: 12.29 min Scan# 1582

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion:142 Resp: 123338

Ion Ratio Lower Upper

142 100

141 90.4 75.2 112.8



116 5.8 3.4 5.2#

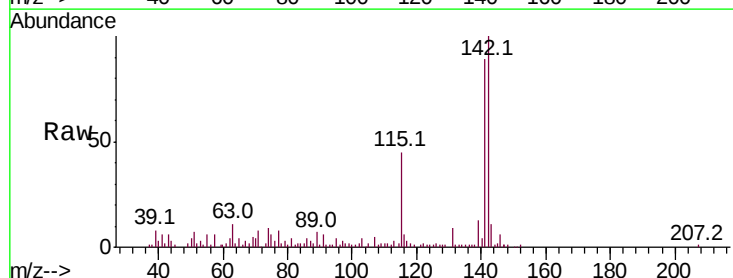


Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

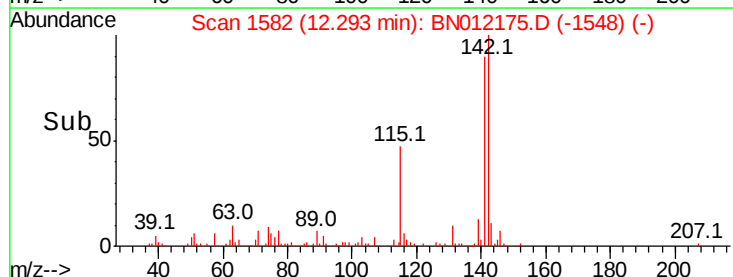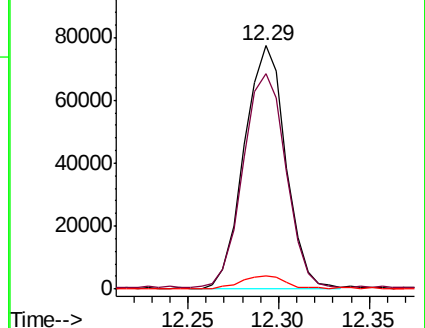

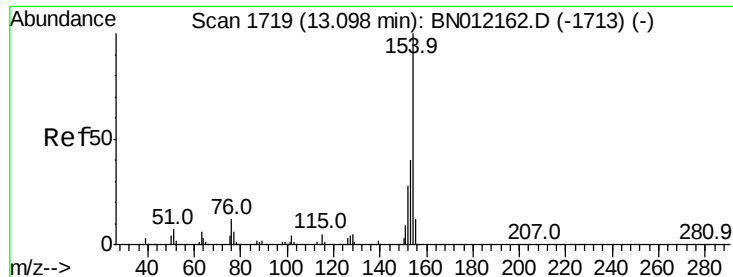

#41

1,1'-Biphenyl

Concen: 1.014 ng/ul

RT: 13.10 min Scan# 1719

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampled :

CB7P3


Tot Ion:154 Resp: 62609

Ion Ratio Lower Upper




154 100

153 42.0 33.9 50.9

76 12.7 9.8 14.8

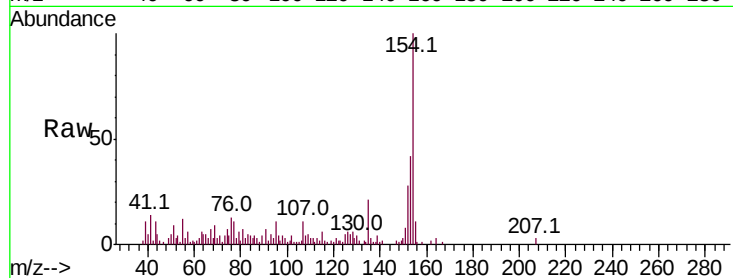

Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 76.00 (75.70 to 76.70): BNC

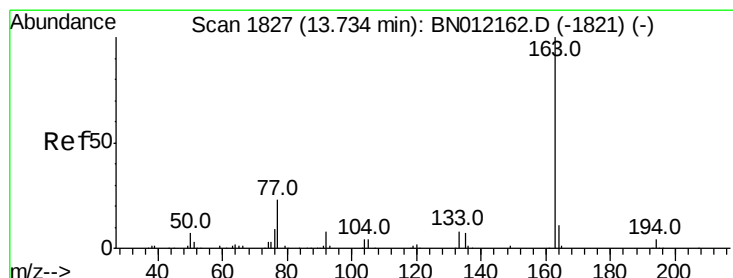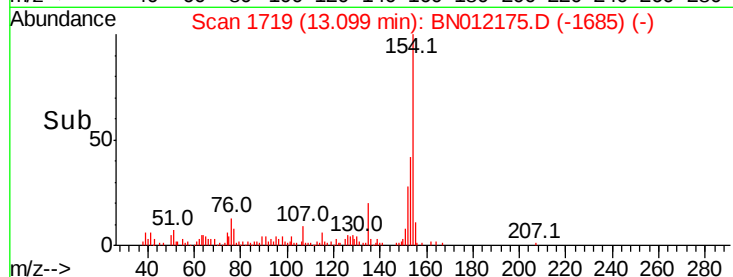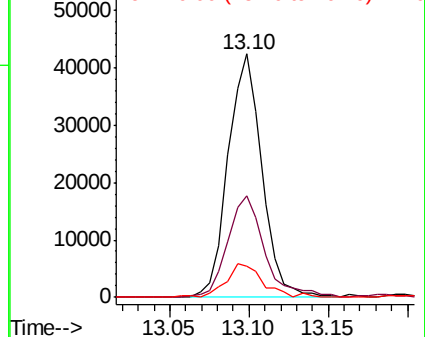

#45

Dimethylphthalate

Concen: 2.004 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion:163 Resp: 127697

Ion Ratio Lower Upper



163 100


194 3.6 3.4 5.0

164 8.8 7.8 11.8

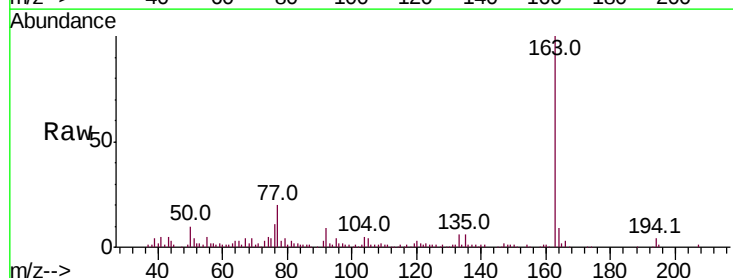

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

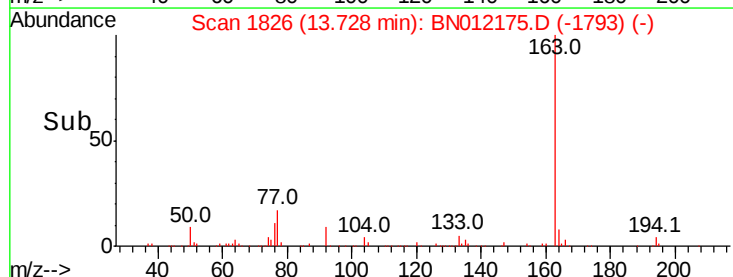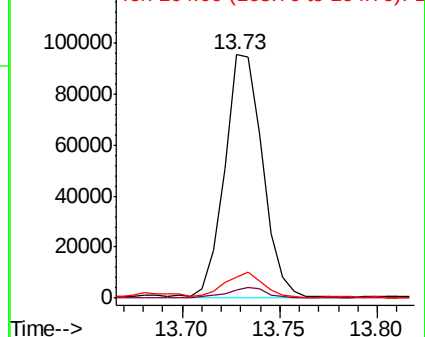

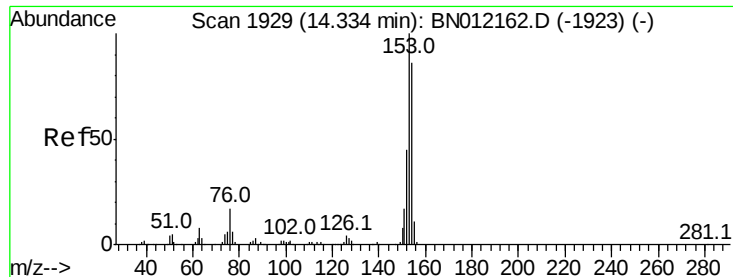

#50

Acenaphthene

Concen: 13.560 ng/ul

RT: 14.33 min Scan# 1929

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampleId :

CB7P3


Tot Ion:153 Resp: 719812

Ion Ratio Lower Upper




153 100

152 46.6 35.9 53.9

154 86.0 70.2 105.2

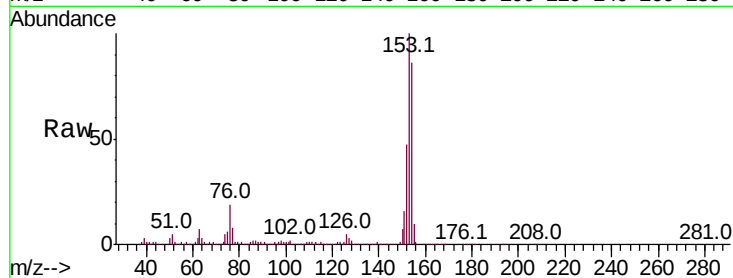

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

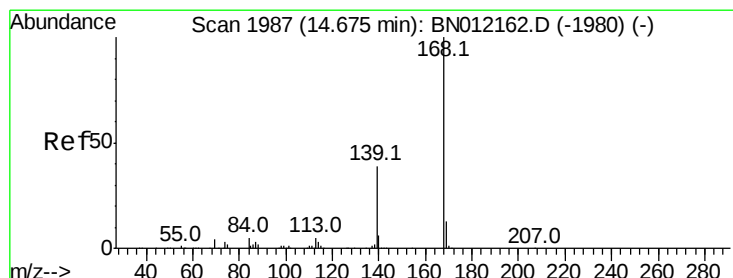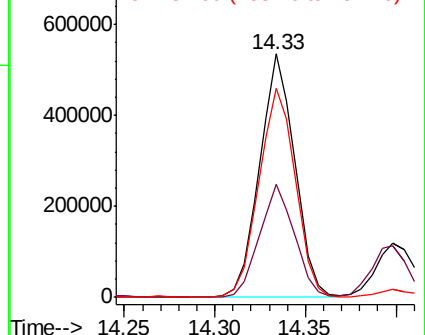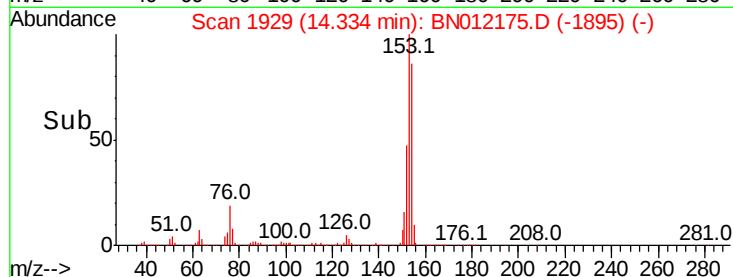

#54

Dibenzofuran

Concen: 5.560 ng/ul

RT: 14.67 min Scan# 1986

Delta R.T. -0.01 min

Lab File: BN012175.D


Acq: 14 Oct 2020 00:15

Tgt Ion:168 Resp: 411006



Ion Ratio Lower Upper


168 100

139 37.4 31.5 47.3

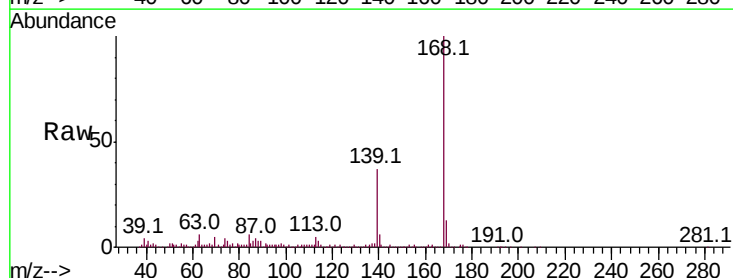

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E

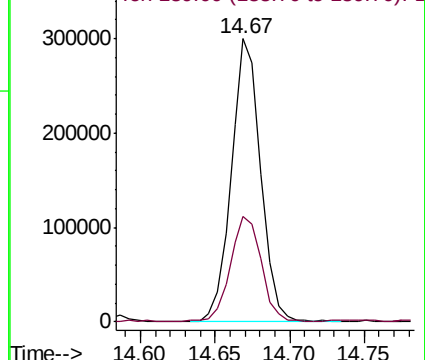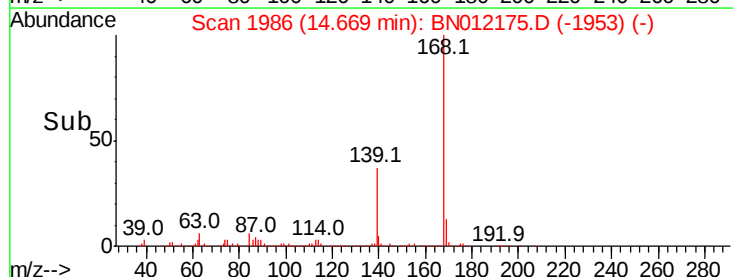

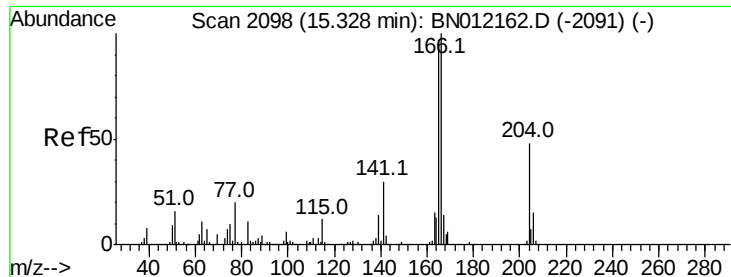

#59

Fluorene

Concen: 8.758 ng/ul

RT: 15.32 min Scan# 2097

Delta R.T. -0.01 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampled :

CB7P3


Tot Ion:166 Resp: 544459

Ion Ratio Lower Upper

166 100

165 102.5 79.0 118.6




167 13.4 10.5 15.7

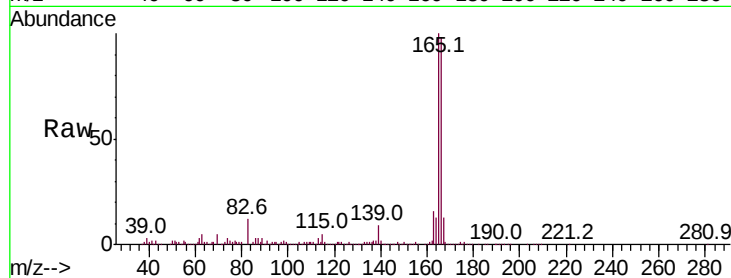

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

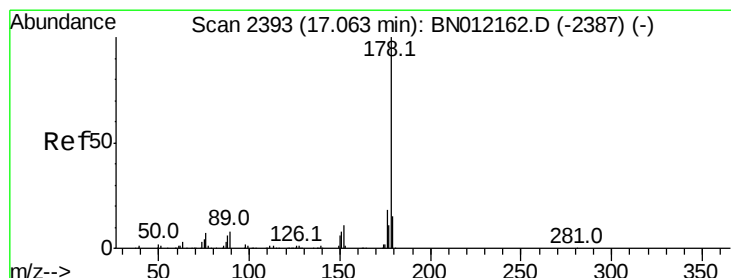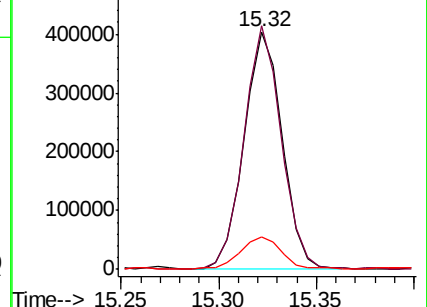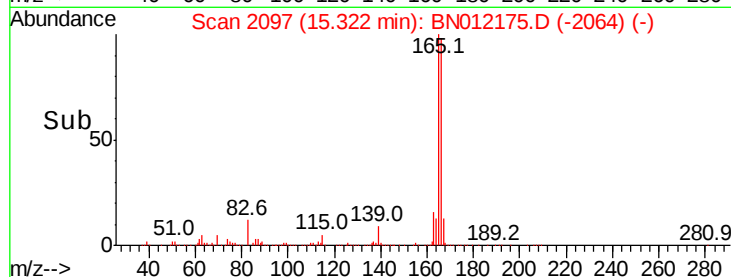

#70

Phenanthrene

Concen: 11.284 ng/ul

RT: 17.06 min Scan# 2393

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion:178 Resp: 1102907

Ion Ratio Lower Upper

178 100

179 15.7 12.2 18.2



176 19.9 15.4 23.2

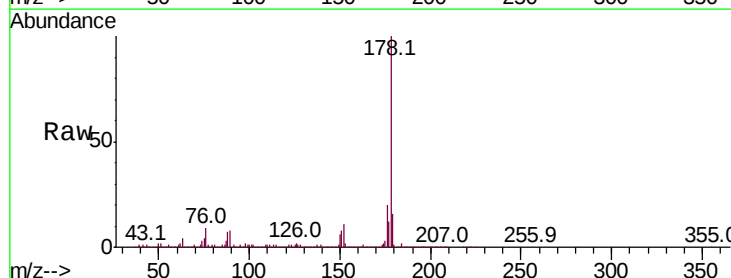


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

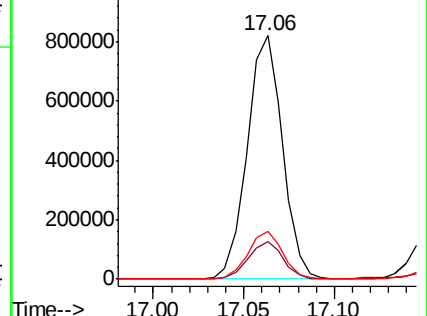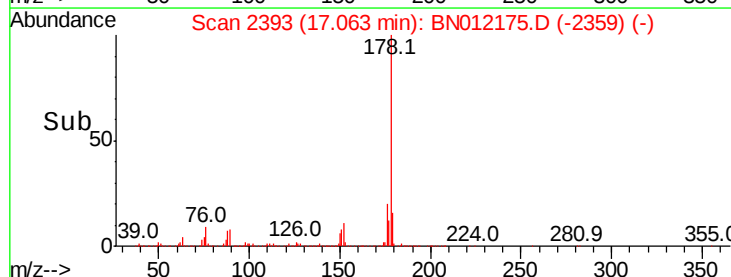

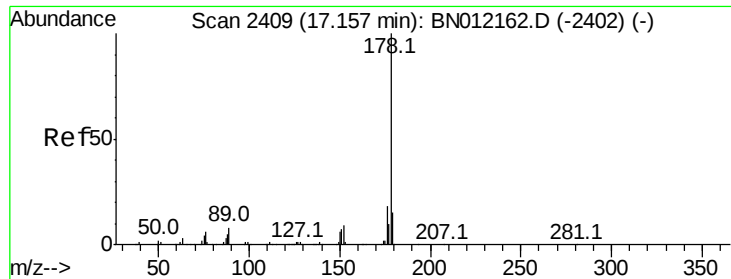

#72

Anthracene

Concen: 1.901 ng/ul

RT: 17.15 min Scan# 2408

Delta R.T. -0.01 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampleId :

CB7P3


Tot Ion:178 Resp: 189259

Ion Ratio Lower Upper

178 100

179 17.0 12.8 19.2




176 20.9 15.0 22.6

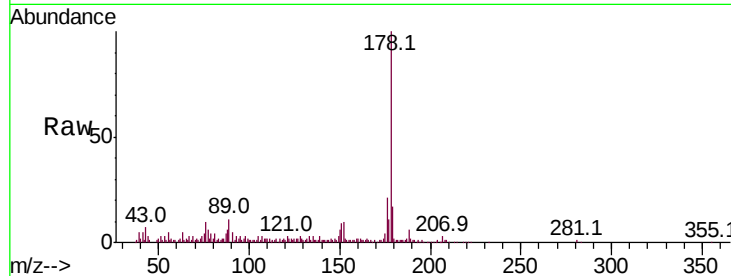

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

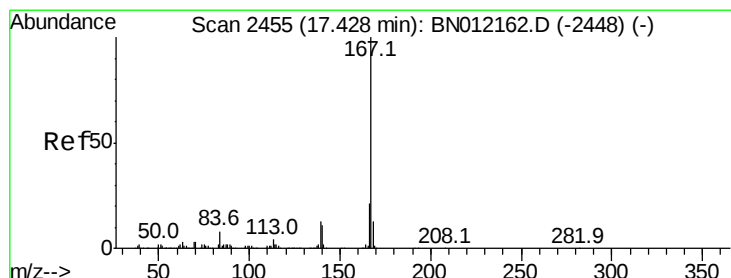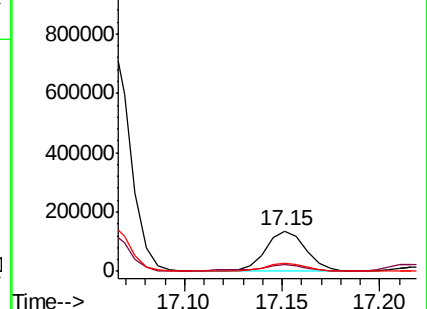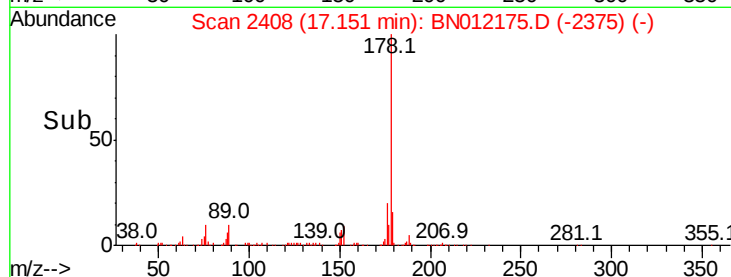

#75

Carbazole

Concen: 7.124 ng/ul

RT: 17.43 min Scan# 2455

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion:167 Resp: 603488

Ion Ratio Lower Upper

167 100

166 21.5 17.4 26.0



139 13.2 10.9 16.3

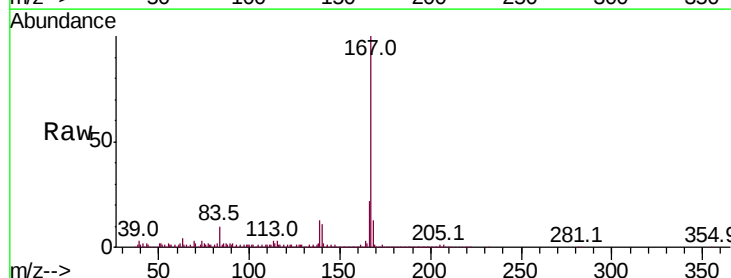


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

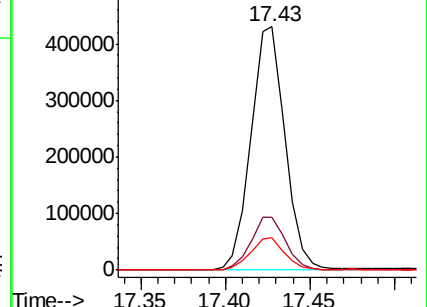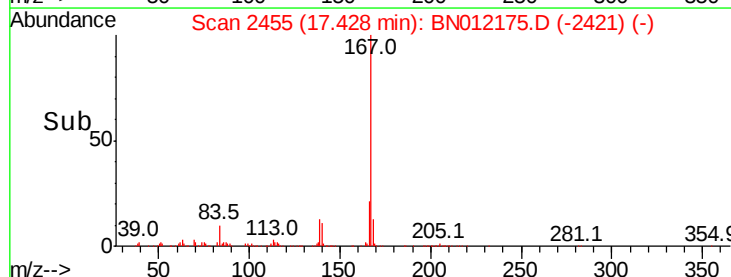

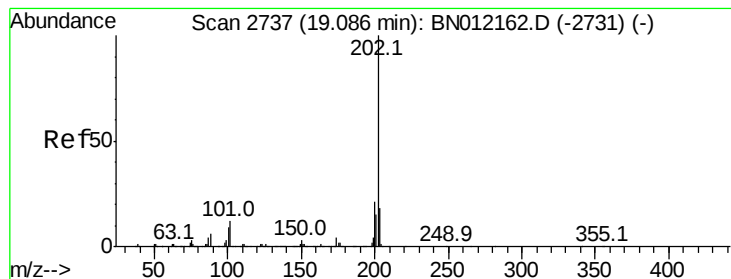

#77

Fluoranthene

Concen: 3.235 ng/ul

RT: 19.09 min Scan# 2737

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15

Instrument :

BNA_N

ClientSampleId :

CB7P3


Tot Ion:202 Resp: 358008

Ion Ratio Lower Upper

202 100

101 11.9 8.6 13.0




100 9.0 6.6 9.8

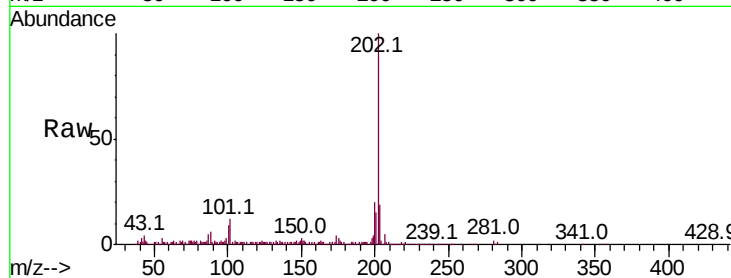

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

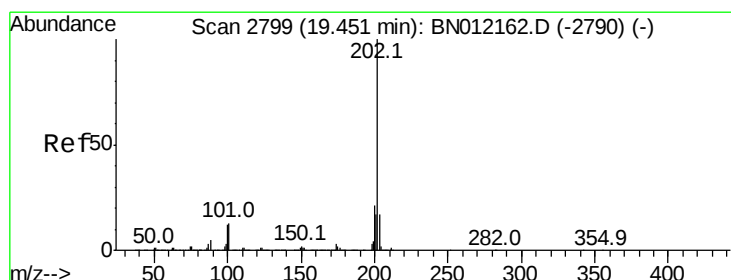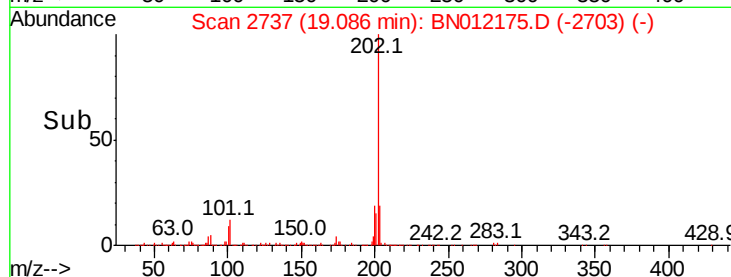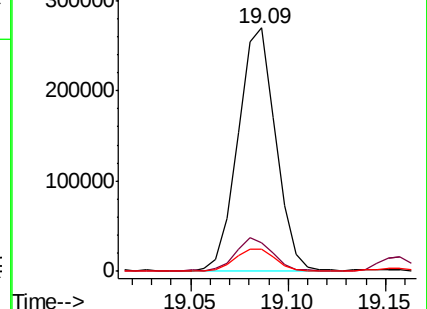

#80

Pyrene

Concen: 1.800 ng/ul

RT: 19.45 min Scan# 2799

Delta R.T. 0.00 min

Lab File: BN012175.D

Acq: 14 Oct 2020 00:15


Tgt Ion:202 Resp: 197281

Ion Ratio Lower Upper

202 100

101 13.6 10.2 15.2

100 10.7 8.8 13.2

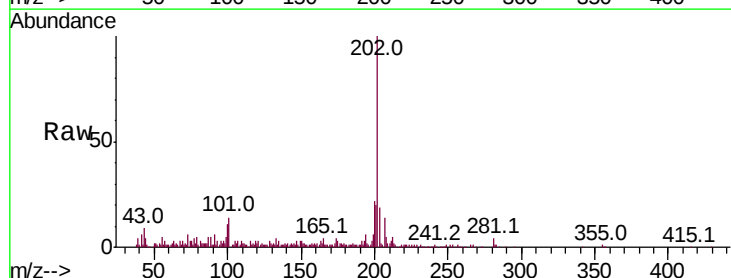

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

