

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101320\
 Data File : BN012187.D
 Acq On : 14 Oct 2020 08:05
 Operator : CG/JU
 Sample : L4360-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7X0

Quant Time: Oct 14 08:37:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 05:54:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	280418	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1142233	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	714846	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1504237	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1439375	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1434442	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	40782	6.43	ng/uL	0.00
5) Phenol-d5	6.81	99	148032	6.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	327522	22.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	400764	20.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	278577	14.23	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	225359	24.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	256909	24.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	492787	25.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	588363	24.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1613445	27.57	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1959873	28.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	45730	4.19	ng/ul	0.02
58) Fluorene-d10	15.27	176	1337806	26.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	118262	11.86	ng/ul	0.00
71) Anthracene-d10	17.12	188	2058869	27.96	ng/ul	0.00
79) Pyrene-d10	19.42	212	2287682	30.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	2401756	29.67	ng/ul	0.00

Target Compounds


					Ovalue
2) 1,4-Dioxane	3.20	88	67654	9.424	ng/uL 96
6) Phenol	6.83	94	29584	1.160	ng/ul 96
28) Naphthalene	10.45	128	102817	1.537	ng/ul 98
35) 1-Methylnaphthalene	12.29	142	68196	1.509	ng/uL# 96
45) Dimethylphthalate	13.73	163	152751	2.501	ng/ul 99
50) Acenaphthene	14.33	153	262233	5.153	ng/ul 97
54) Dibenzofuran	14.67	168	135627	1.914	ng/ul 99
59) Fluorene	15.32	166	123541	2.073	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101320\
Data File : BN012187.D
Acq On : 14 Oct 2020 08:05
Operator : CG/JU
Sample : L4360-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7X0

Quant Time: Oct 14 08:37:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 05:54:37 2020
Response via : Initial Calibration

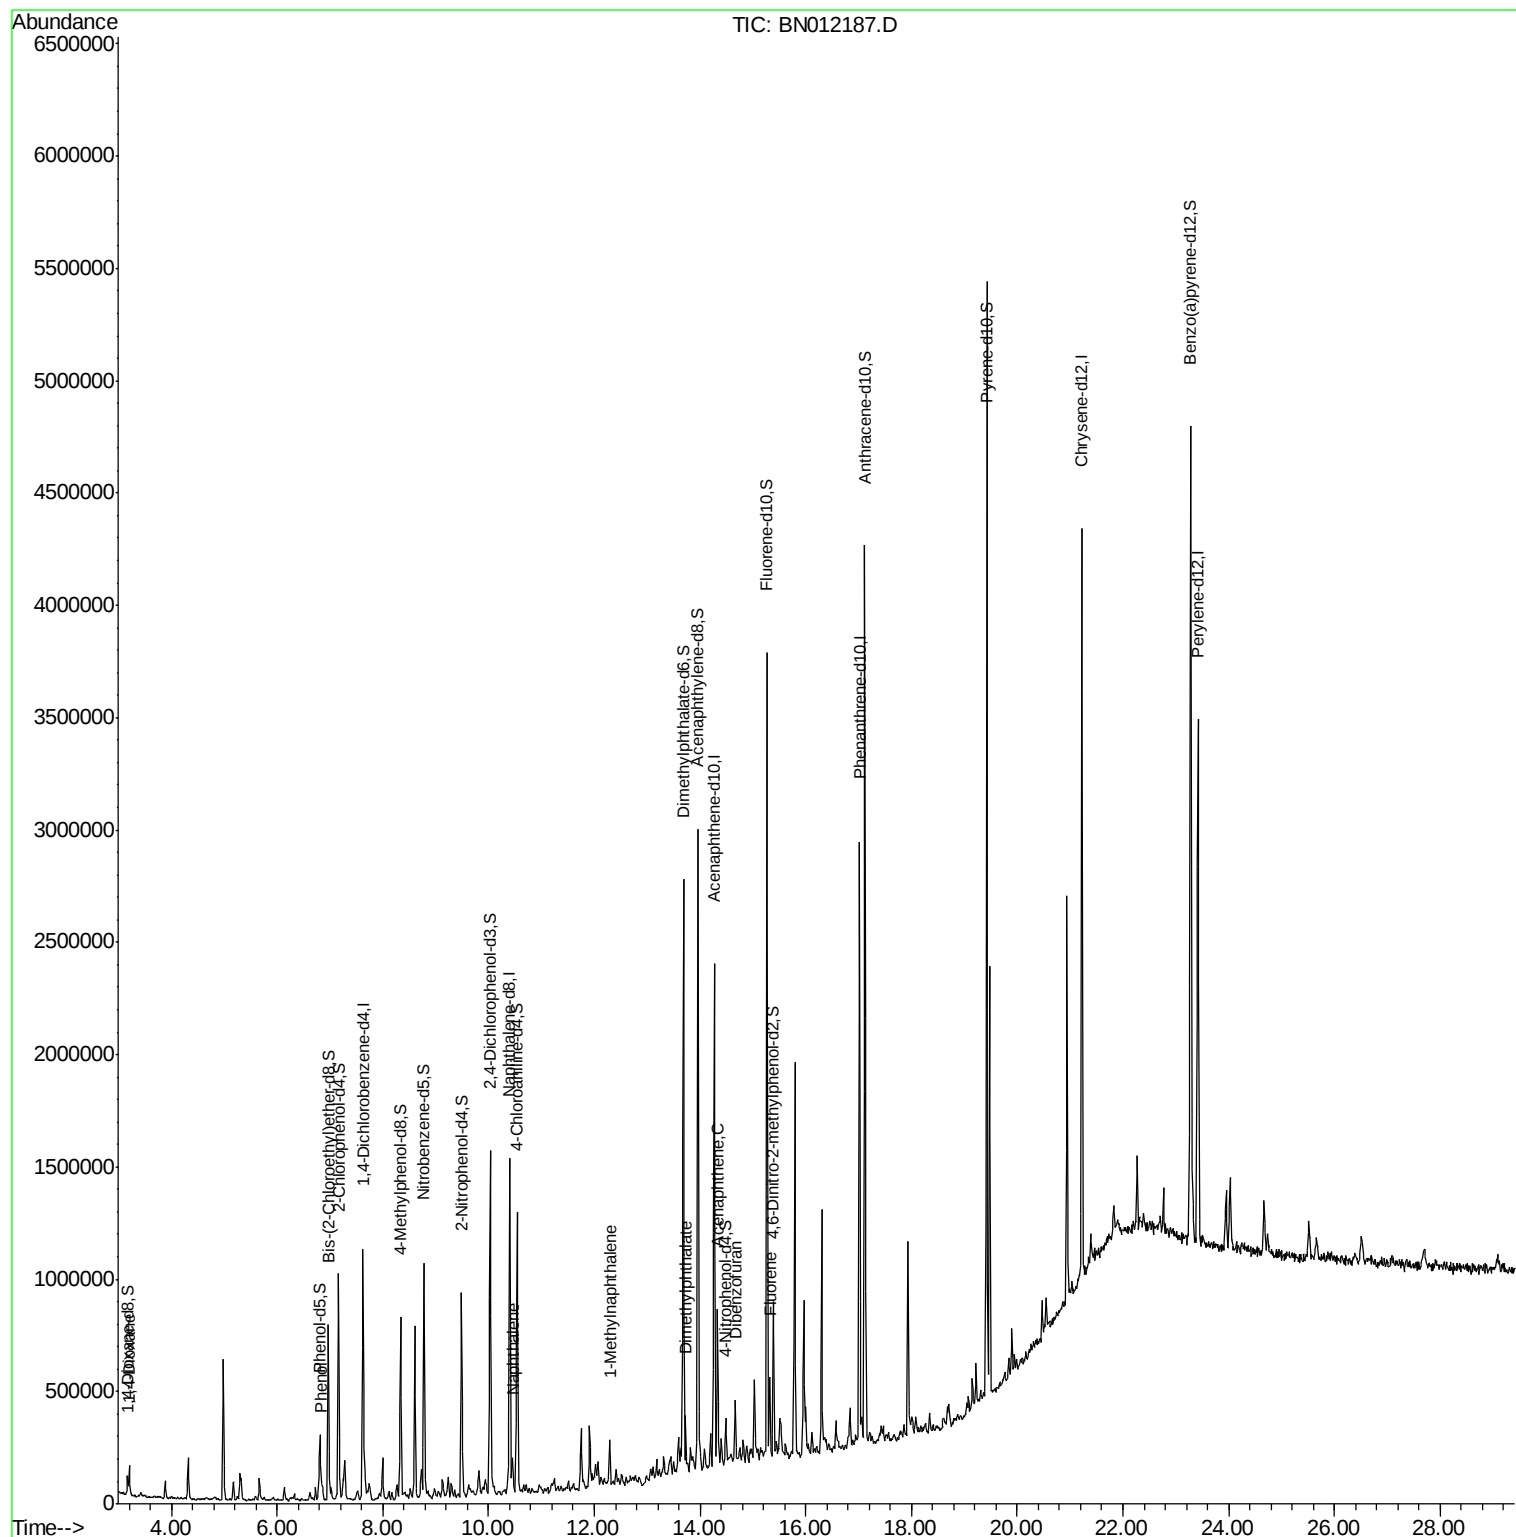

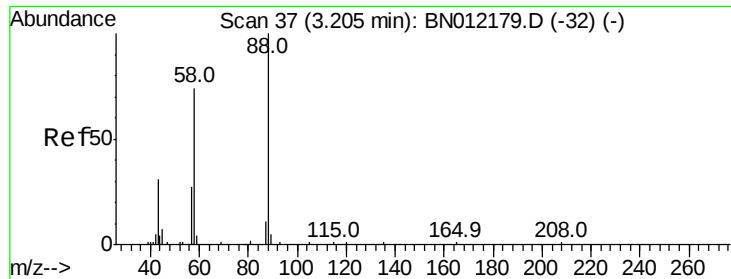

#2

1,4-Dioxane

Concen: 9.424 ng/uL

RT: 3.20 min Scan# 36

Delta R.T. -0.01 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05

Instrument :

BNA_N

ClientSampleId :

CB7X0


Tot Ion: 88 Resp: 67654

Ion Ratio Lower Upper

88 100

43 31.0 26.5 39.7




58 73.0 61.0 91.4

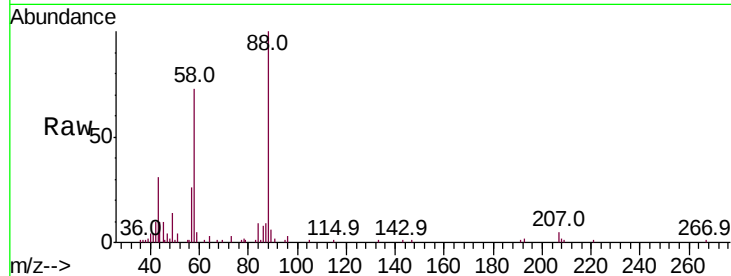

Abundance Ion 88.00 (87.70 to 88.70): BN0

Ion 43.00 (42.70 to 43.70): BN0

Ion 58.00 (57.70 to 58.70): BN0

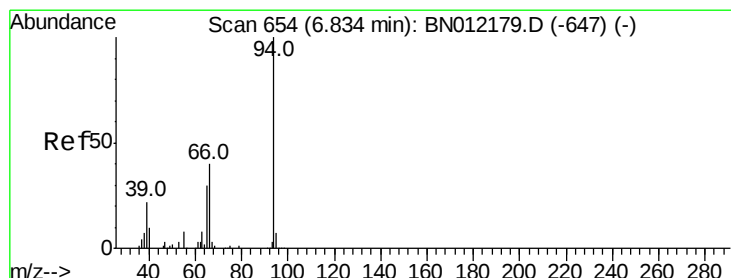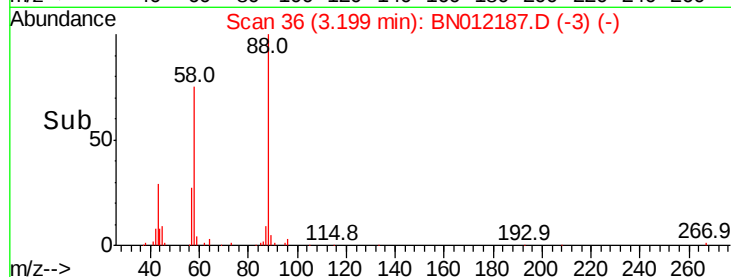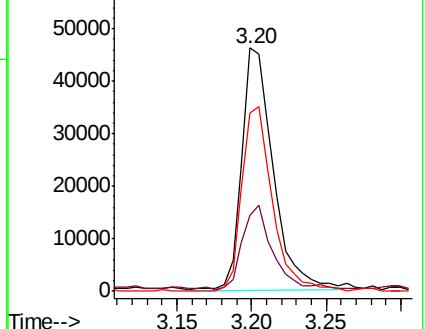

#6

Phenol

Concen: 1.160 ng/uL

RT: 6.83 min Scan# 654

Delta R.T. 0.00 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05


Tgt Ion: 94 Resp: 29584

Ion Ratio Lower Upper

94 100

65 32.3 26.8 40.2



66 51.5 37.9 56.9

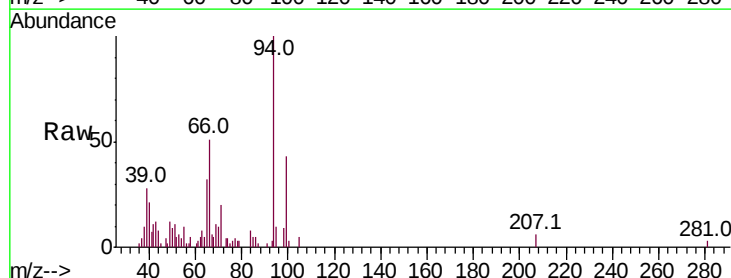


Abundance Ion 94.00 (93.70 to 94.70): BN0

Ion 65.00 (64.70 to 65.70): BN0

Ion 66.00 (65.70 to 66.70): BN0

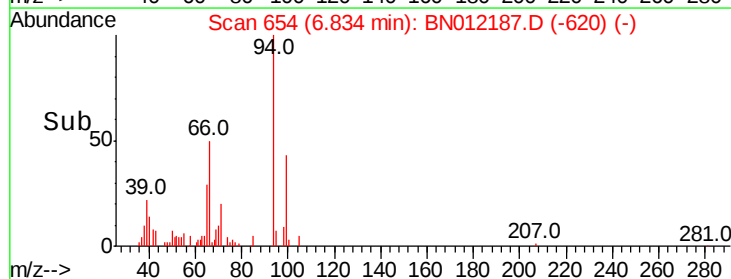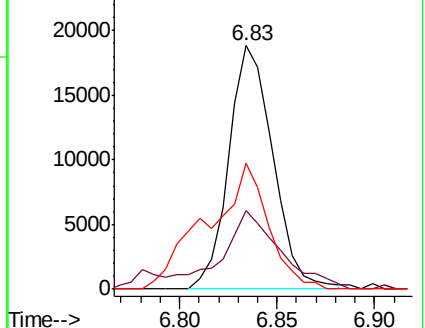

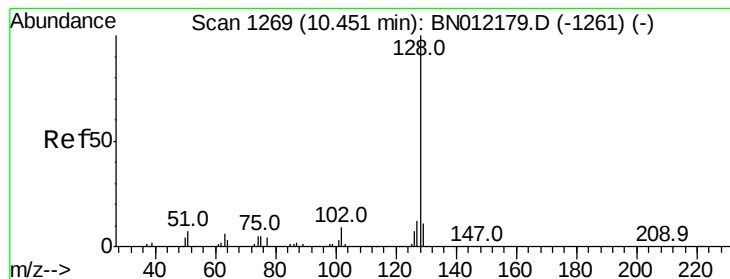

#28

Naphthalene

Concen: 1.537 ng/ul

RT: 10.45 min Scan# 1269

Delta R.T. 0.00 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05

Instrument :

BNA_N

ClientSampleId :

CB7X0


Tot Ion:128 Resp: 102817

Ion Ratio Lower Upper

128 100

129 10.8 8.8 13.2




127 12.0 10.7 16.1

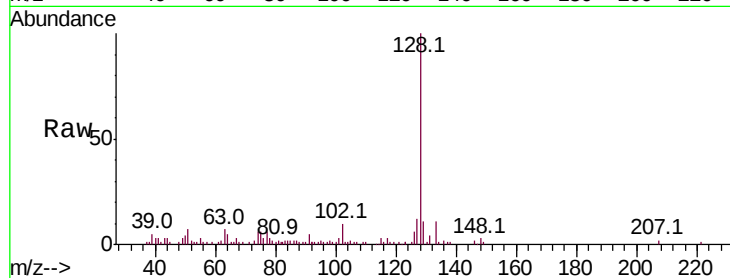

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

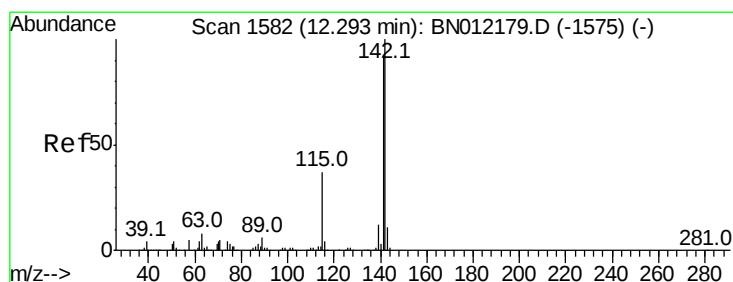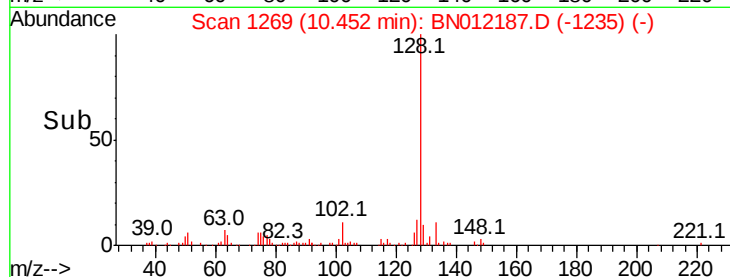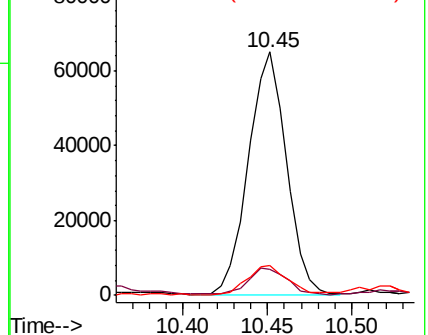

#35

1-Methylnaphthalene

Concen: 1.509 ng/uL

RT: 12.29 min Scan# 1582

Delta R.T. 0.00 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05


Tgt Ion:142 Resp: 68196

Ion Ratio Lower Upper

142 100

141 97.5 75.2 112.8



116 6.0 3.4 5.2#

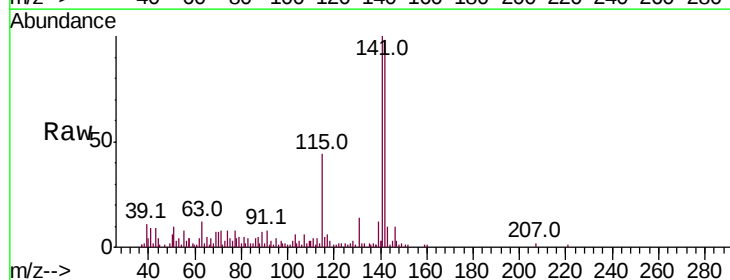


Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E



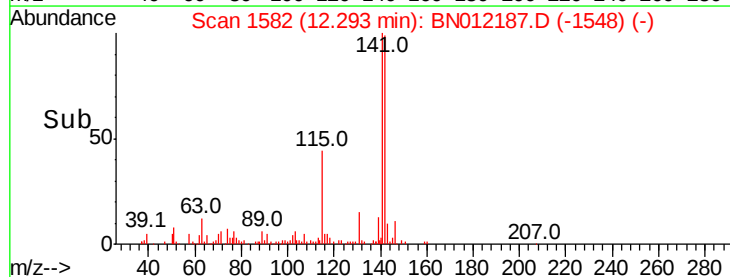
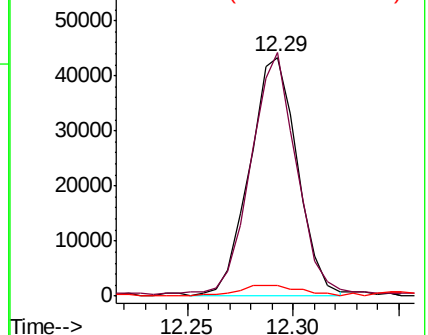


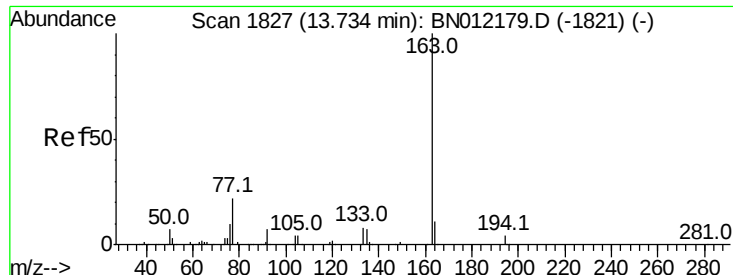

#45
Dimethylphthalate
Concen: 2.501 ng/ul
RT: 13.73 min Scan# 1827
Delta R.T. 0.00 min
Lab File: BN012187.D
Acq: 14 Oct 2020 08:05




Instrument :
BNA_N
ClientSampleId :
CB7X0


Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.0
164	10.4	7.8	11.8

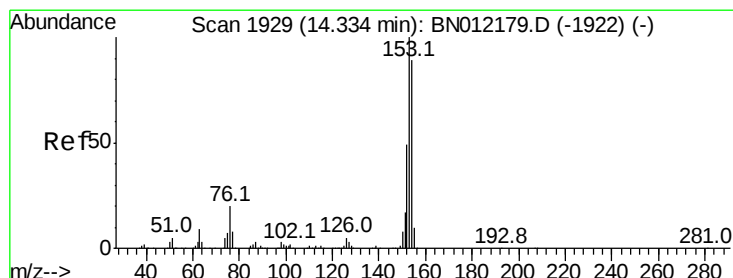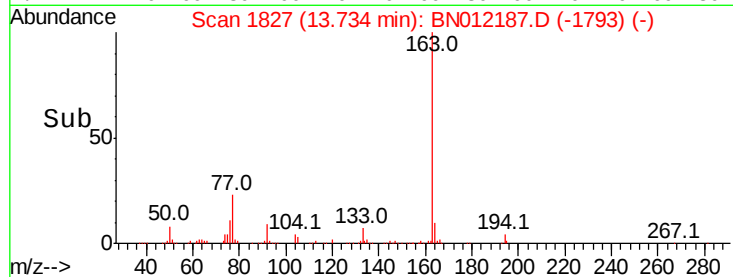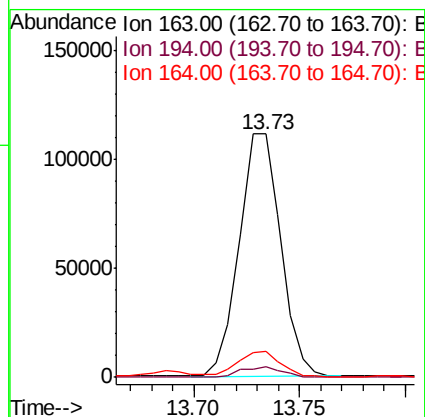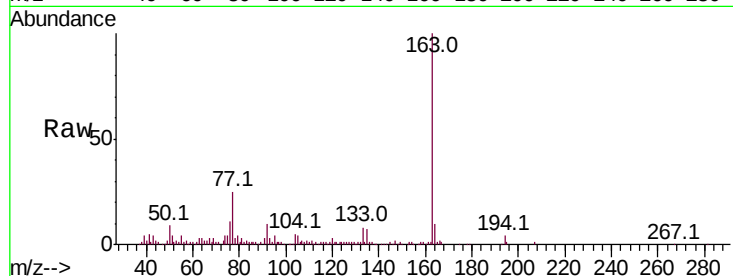

#50
Acenaphthene
Concen: 5.153 ng/ul
RT: 14.33 min Scan# 1929
Delta R.T. 0.00 min
Lab File: BN012187.D
Acq: 14 Oct 2020 08:05

Tgt Ion	Ratio	Lower	Upper
153	100		
152	45.3	35.9	53.9
154	83.2	70.2	105.2

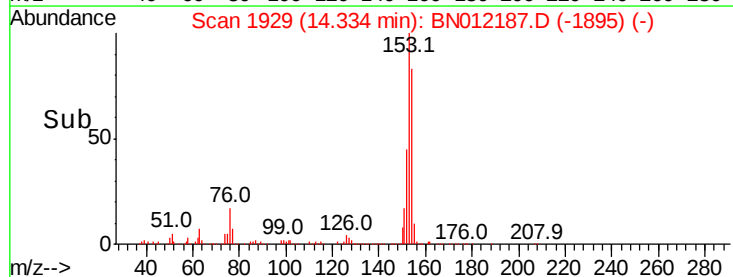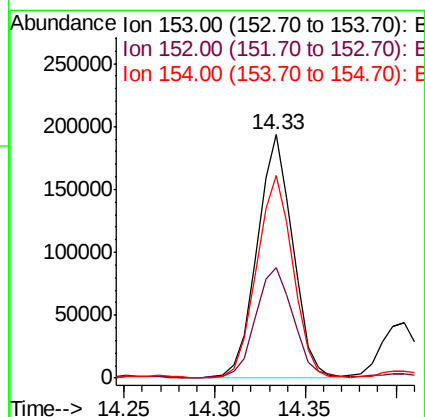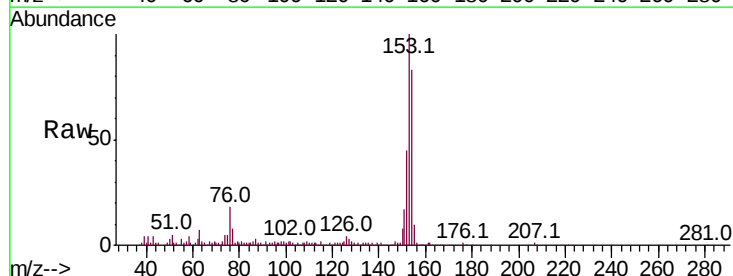

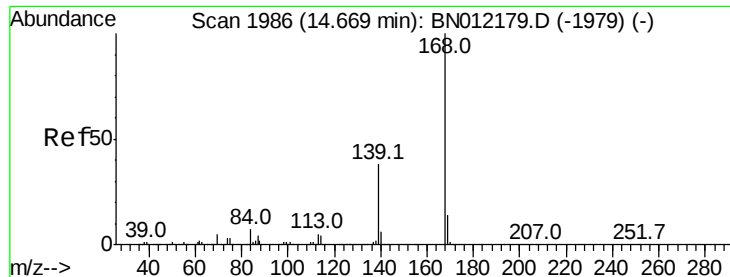

#54

Dibenzenofuran

Concen: 1.914 ng/ul

RT: 14.67 min Scan# 1986

Delta R.T. -0.01 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05

Instrument :

BNA_N

ClientSampleId :


CB7X0

Tot Ion:168 Resp: 135627

Ion Ratio Lower Upper

168 100

139 39.1 31.5 47.3

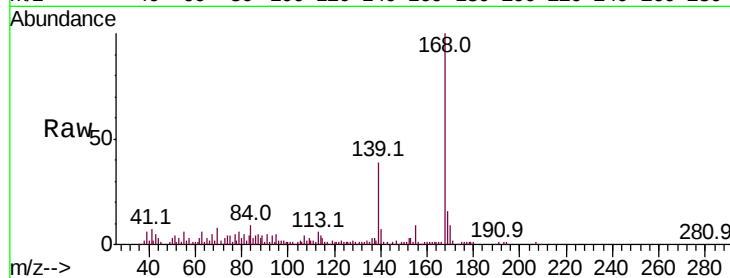

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.67

100000

80000



60000

40000

20000

0

Time--> 14.60 14.65 14.70

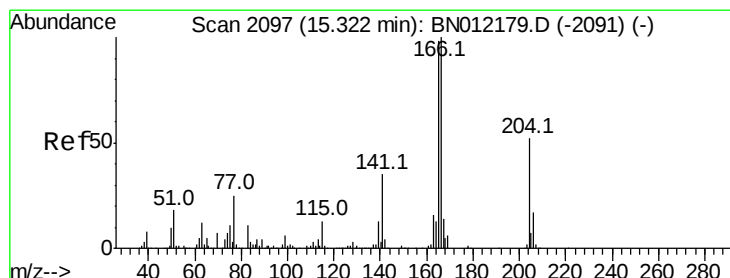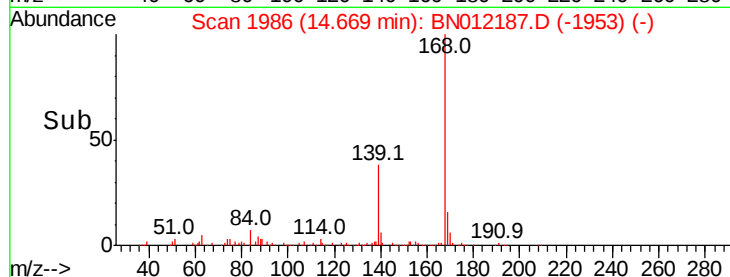

#59

Fluorene

Concen: 2.073 ng/ul

RT: 15.32 min Scan# 2097

Delta R.T. -0.01 min

Lab File: BN012187.D

Acq: 14 Oct 2020 08:05


Tgt Ion:166 Resp: 123541

Ion Ratio Lower Upper

166 100

165 98.8 79.0 118.6

167 14.2 10.5 15.7

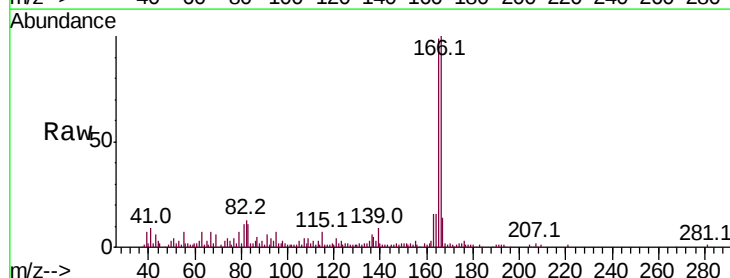

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.32

120000

100000

80000

60000

40000

20000

0

Time--> 15.30 15.35

