

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101320\
 Data File : BN012163.D
 Acq On : 13 Oct 2020 17:00
 Operator : CG/JU
 Sample : L4360-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7W0

Quant Time: Oct 13 17:30:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 13 11:24:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	249281	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	997167	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	629551	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1417863	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1462149	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1528953	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	33550	5.95	ng/uL	0.00
5) Phenol-d5	6.80	99	110223	5.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	299983	22.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	337350	19.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	220430	12.66	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	192378	23.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	207186	22.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	408847	24.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	504635	24.07	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1534484	29.77	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1725684	28.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	44642	4.64	ng/ul	0.00
58) Fluorene-d10	15.27	176	1308869	29.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	195565	20.82	ng/ul	0.00
71) Anthracene-d10	17.12	188	2159989	31.12	ng/ul	0.00
79) Pyrene-d10	19.42	212	2456133	32.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	2671004	30.95	ng/ul	0.00

Target Compounds


					Ovalue
2) 1,4-Dioxane	3.20	88	70575	11.058 ng/uL	95
45) Dimethylphthalate	13.73	163	281975	5.242 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101320\
Data File : BN012163.D
Acq On : 13 Oct 2020 17:00
Operator : CG/JU
Sample : L4360-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7W0

Quant Time: Oct 13 17:30:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100920.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 13 11:24:33 2020
Response via : Initial Calibration

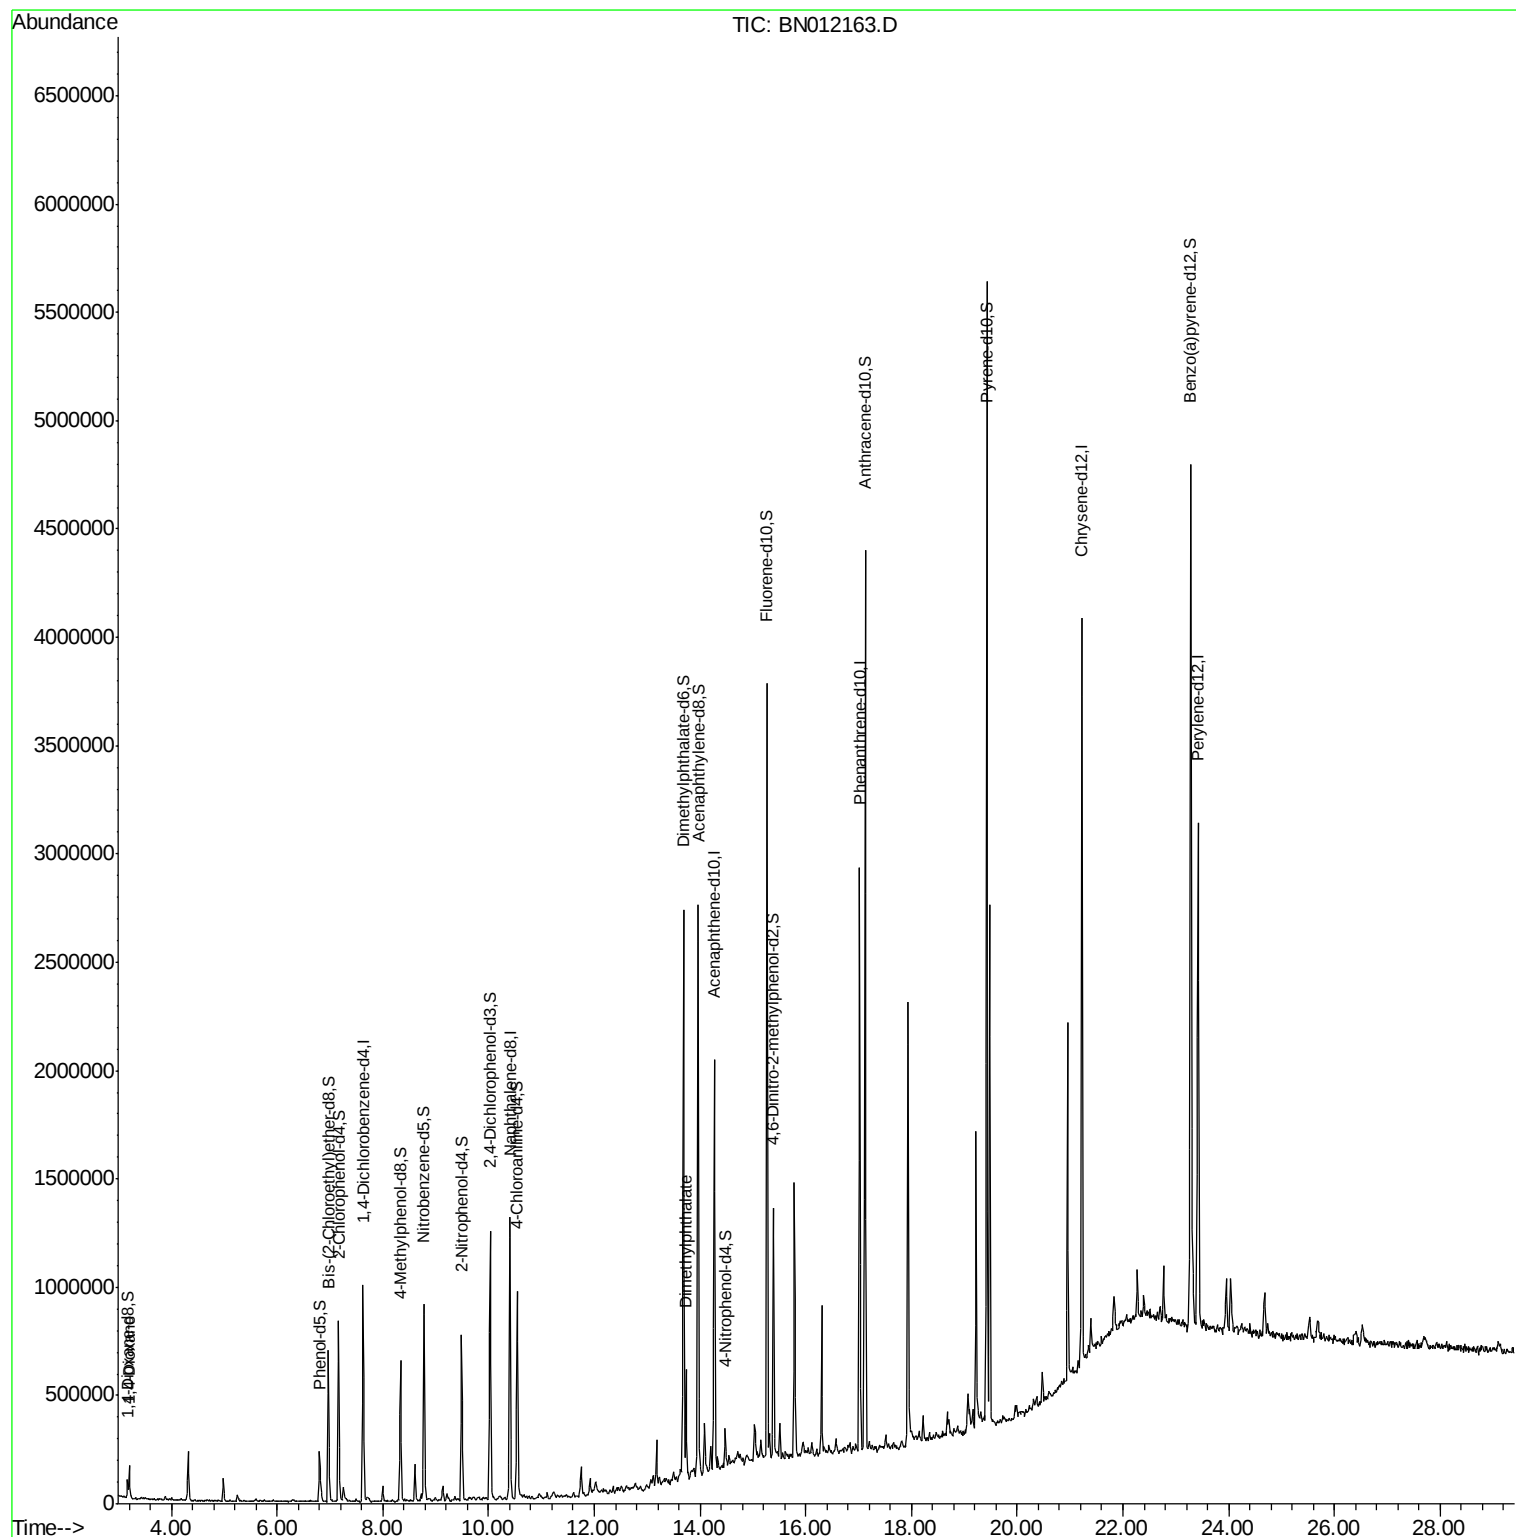

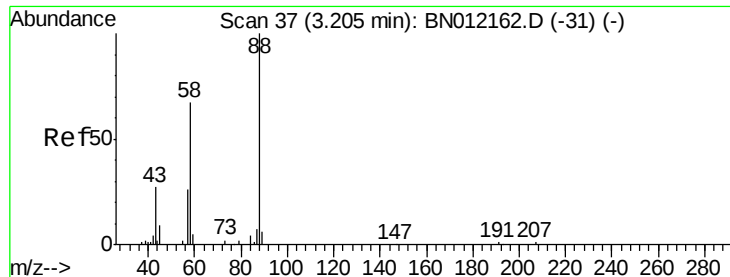

#2

1,4-Dioxane

Concen: 11.058 ng/uL

RT: 3.20 min Scan# 37

Delta R.T. 0.01 min

Lab File: BN012163.D

Acq: 13 Oct 2020 17:00

Instrument :

BNA_N

ClientSampleId :

CB7W0


Tot Ion: 88 Resp: 70575

Ion Ratio Lower Upper

88 100

43 32.3 25.3 37.9




58 73.2 54.3 81.5

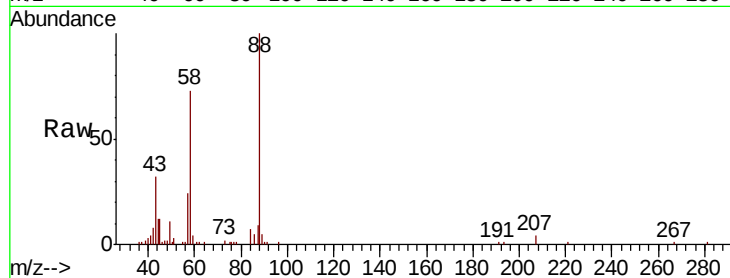

Abundance Ion 88.00 (87.70 to 88.70): BN012163.D (-2) (-)

Ion 43.00 (42.70 to 43.70): BN012163.D (-2) (-)

Ion 58.00 (57.70 to 58.70): BN012163.D (-2) (-)

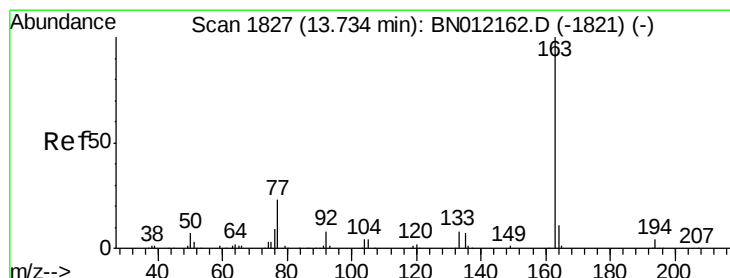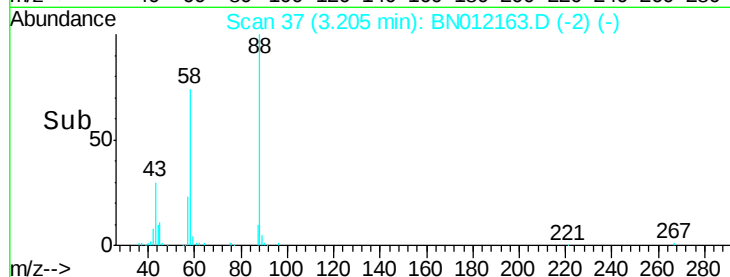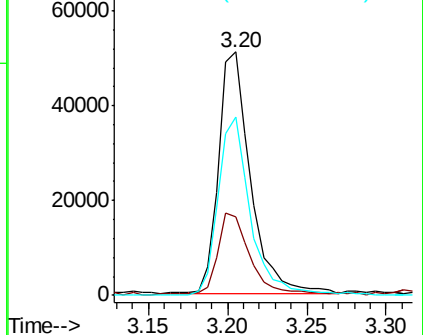

#45

Dimethylphthalate

Concen: 5.242 ng/uL

RT: 13.73 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BN012163.D

Acq: 13 Oct 2020 17:00


Tgt Ion: 163 Resp: 281975

Ion Ratio Lower Upper

163 100

194 4.7 3.7 5.5

164 10.8 8.6 12.8

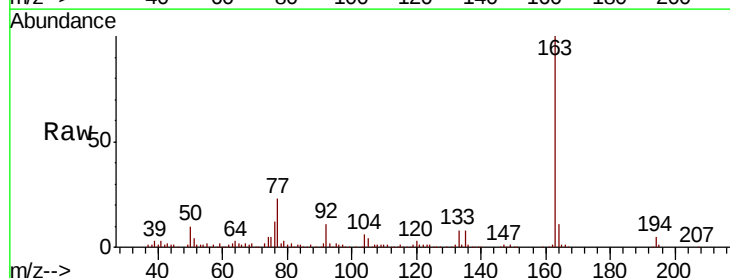

Abundance Ion 163.00 (162.70 to 163.70): BN012163.D (-1793) (-)

Ion 194.00 (193.70 to 194.70): BN012163.D (-1793) (-)

Ion 164.00 (163.70 to 164.70): BN012163.D (-1793) (-)

