
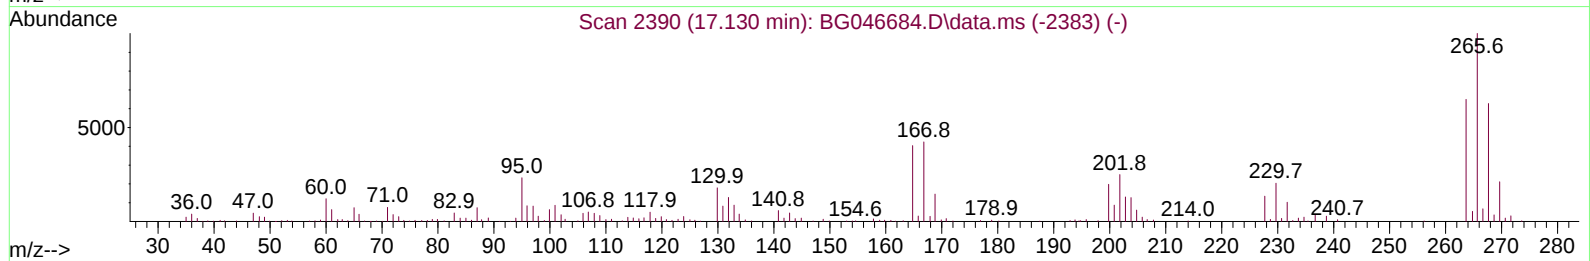
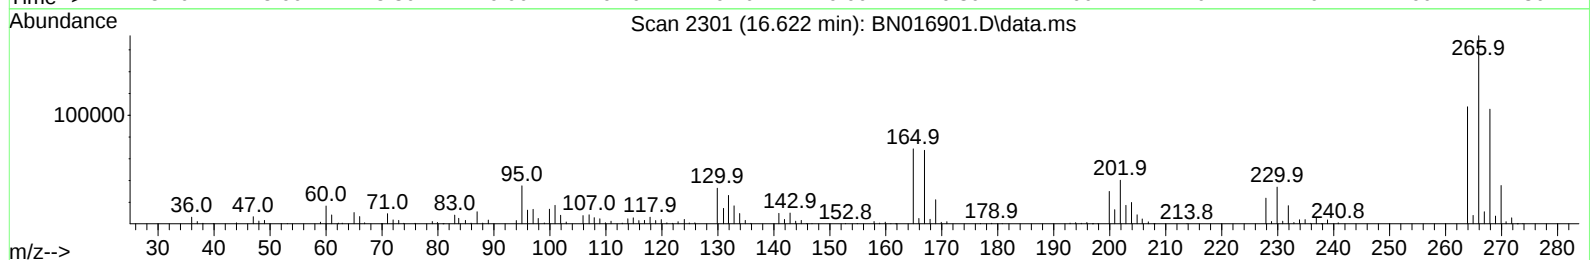


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016901.D
Acq On : 12 Oct 2021 16:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 05:53:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 05:53:33 2021
Response via : Initial Calibration

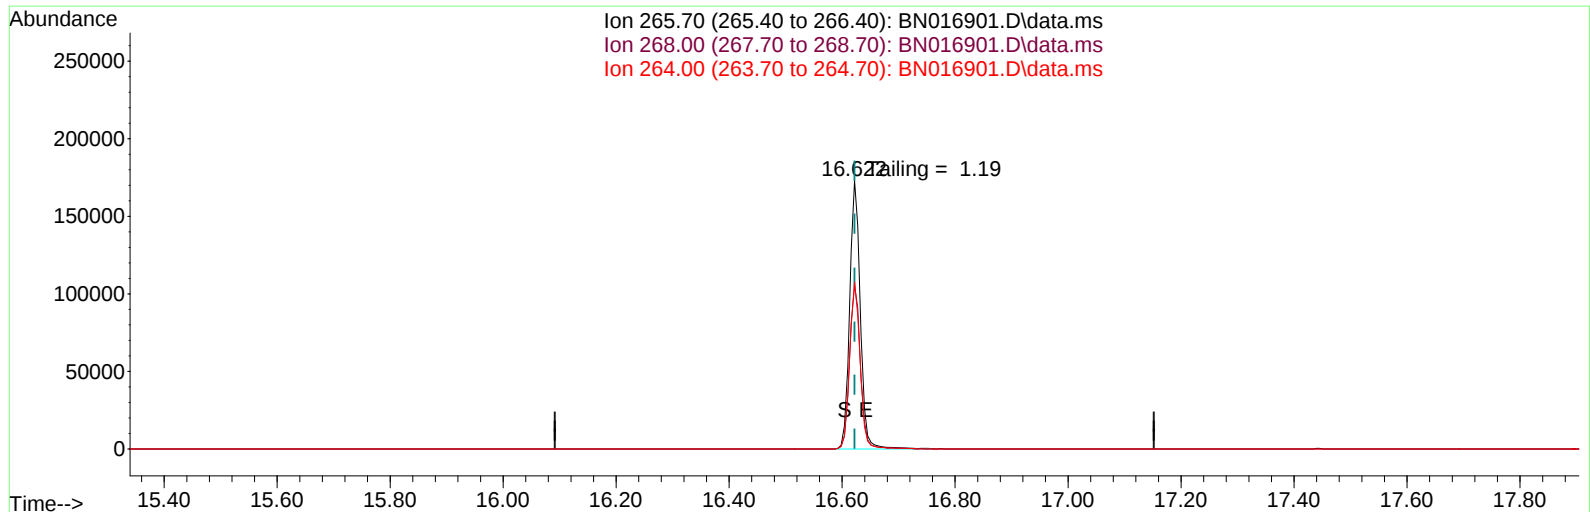

TIC: BN016901.D\data.ms

(70) Pentachlorophenol (C)




16.622min (0.000) 26834.75 ng

response 226808

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.02
264.00	61.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016901.D
Acq On : 12 Oct 2021 16:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 05:53:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 05:53:33 2021
Response via : Initial Calibration

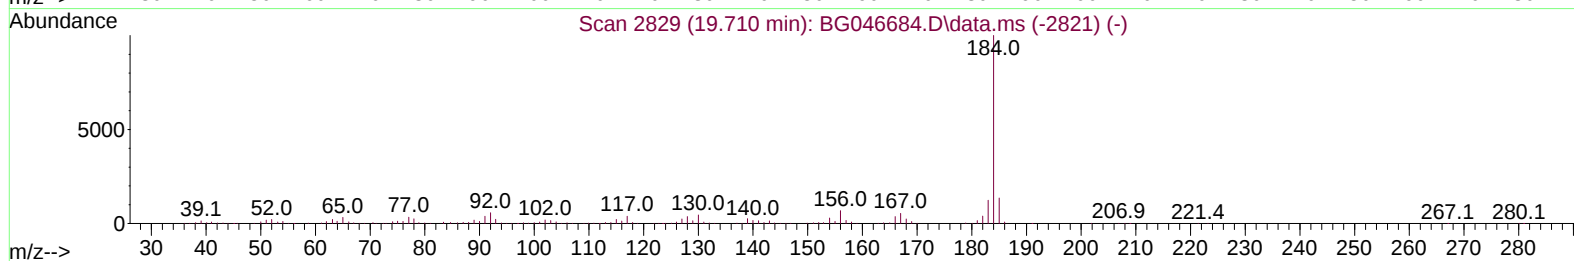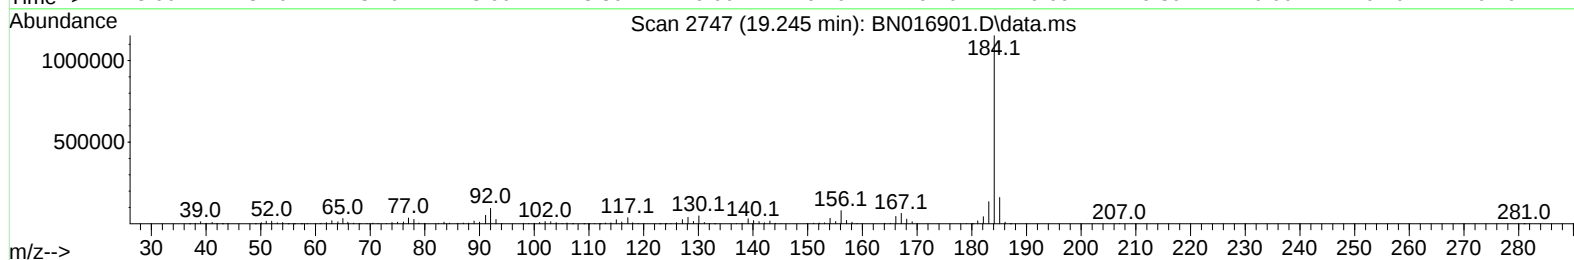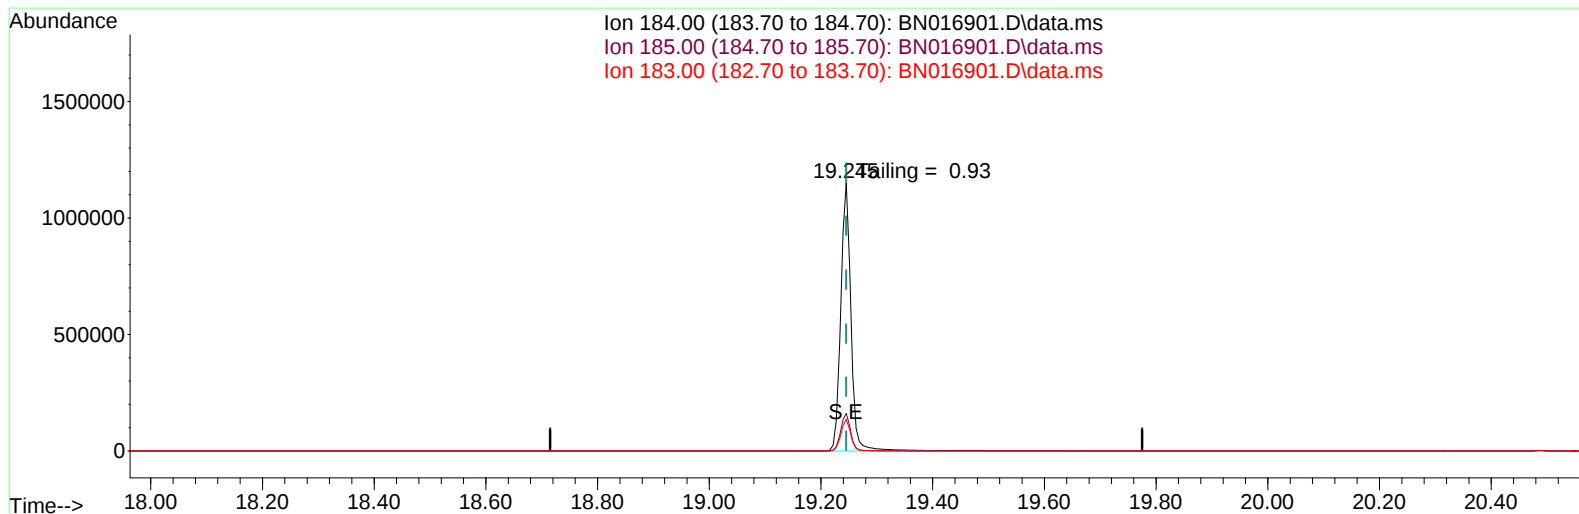

TIC: BN016901.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 1469274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	11.76
0.00	0.00	0.00