
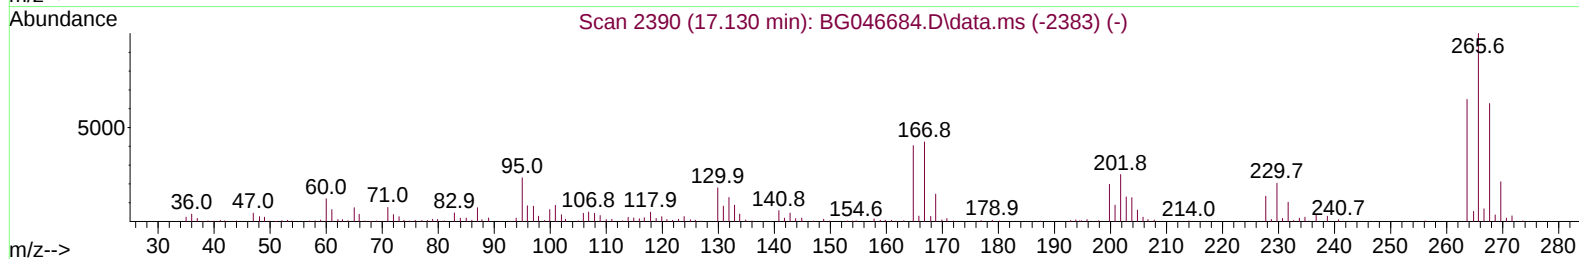
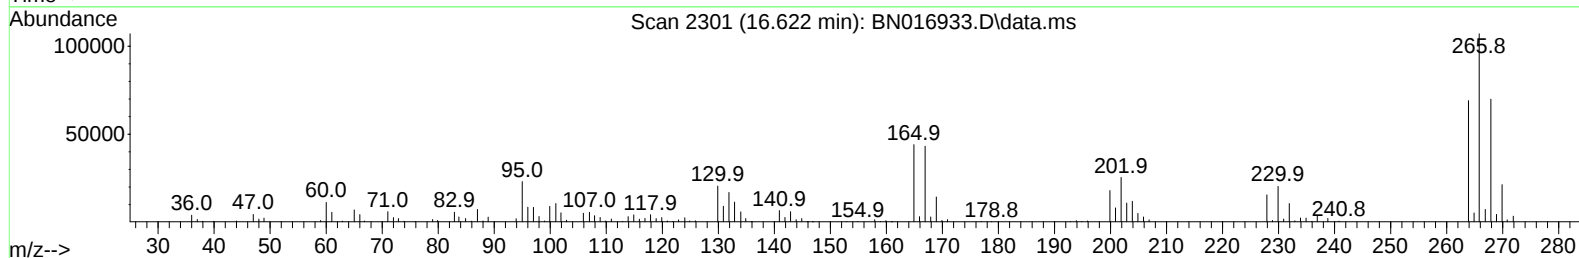


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016933.D
Acq On : 13 Oct 2021 17:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:07:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

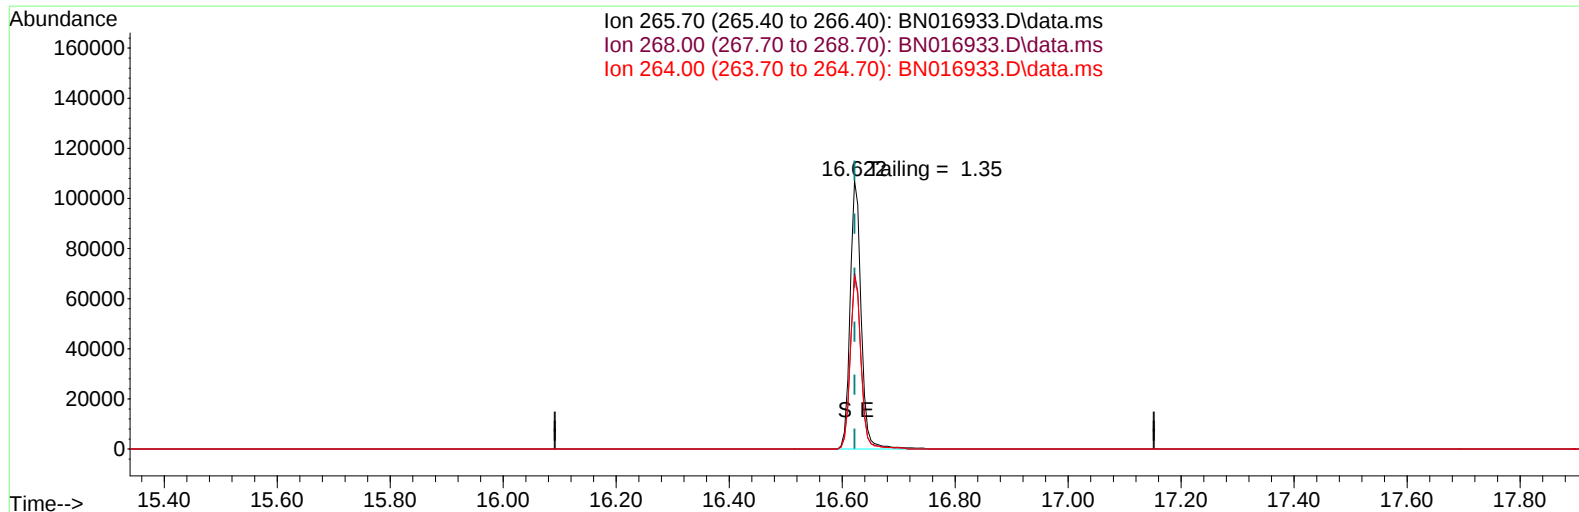

TIC: BN016933.D\data.ms

(70) Pentachlorophenol (C)




16.622min (+ 0.000) 33193.44 ng

response 146137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.33
264.00	61.60	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016933.D
Acq On : 13 Oct 2021 17:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:07:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

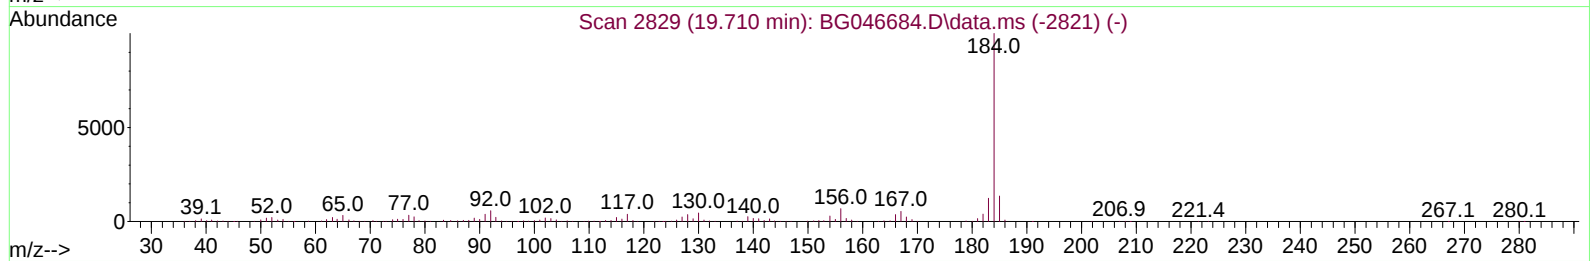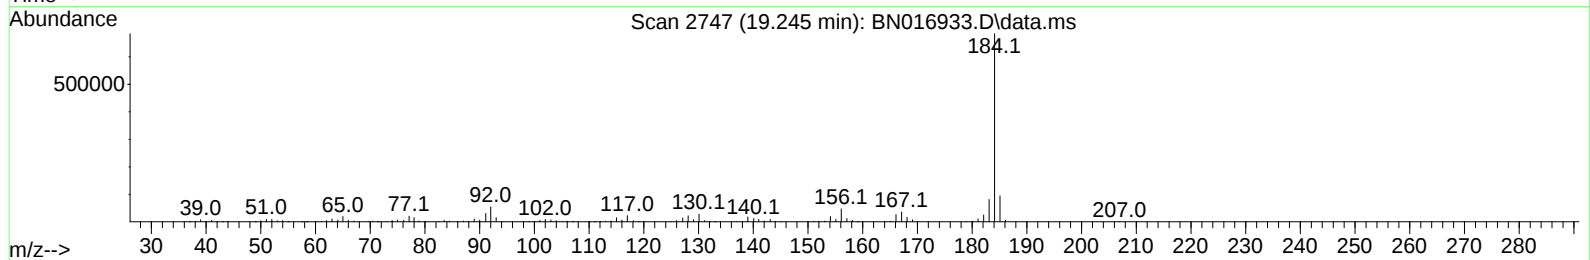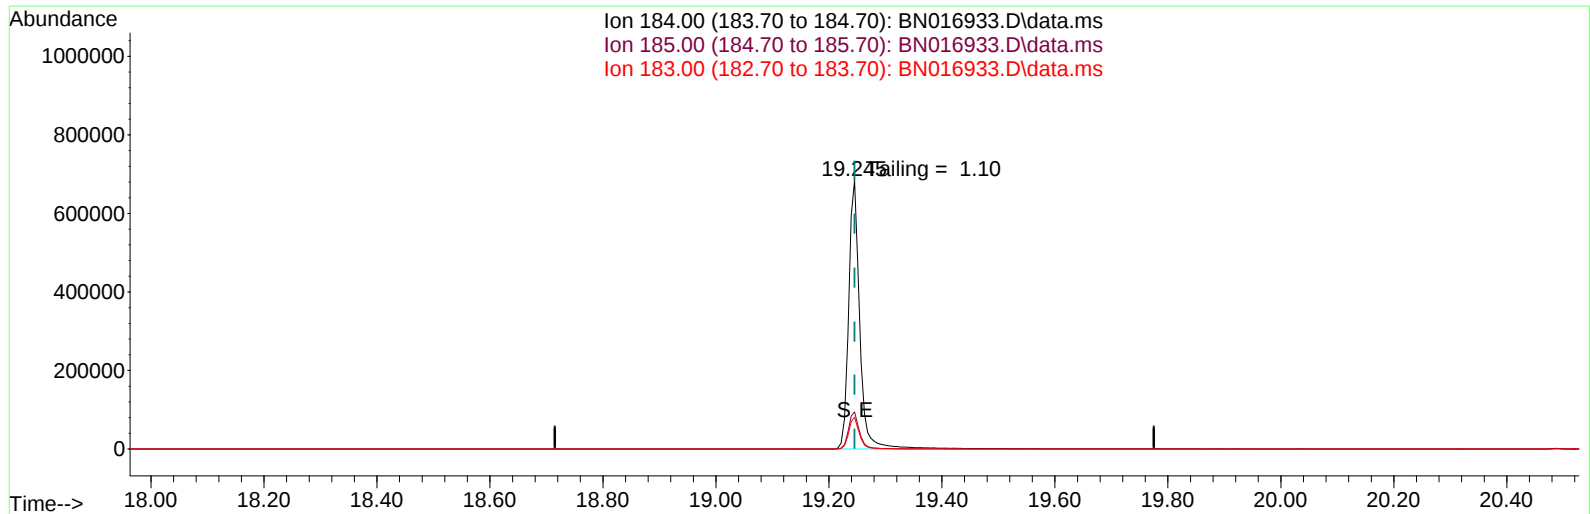

TIC: BN016933.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 936274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.90
0.00	0.00	0.00