

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
 Data File : BN016908.D
 Acq On : 12 Oct 2021 21:11
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Oct 13 01:54:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 01:50:22 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	21339	0.40	ng	0.00
7) Naphthalene-d8	10.444	136	89216	0.40	ng	#-0.01
13) Acenaphthene-d10	14.294	164	48142	0.40	ng	0.00
19) Phenanthrene-d10	17.042	188	89923	0.40	ng	0.00
29) Chrysene-d12	21.227	240	89992	0.40	ng	0.00
35) Perylene-d12	23.471	264	92200	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	157693	2.89	ng	0.00
5) Phenol-d6	6.868	99	181295	2.96	ng	0.00
8) Nitrobenzene-d5	8.822	82	205177	3.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.038	152	397830	3.08	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	82342	3.53	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	555299	3.01	ng	0.00
27) Fluoranthene-d10	19.073	212	753590	3.19	ng	0.00
31) Terphenyl-d14	19.678	244	628226	3.07	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.272	88	45418	2.84	ng	Qvalue 93
3) n-Nitrosodimethylamine	3.603	42	56086	3.22	ng	98
6) bis(2-Chloroethyl)ether	7.126	93	177203	2.96	ng	99
9) Naphthalene	10.495	128	714760	2.94	ng	100
10) Hexachlorobutadiene	10.787	225	139962	3.07	ng	# 100
12) 2-Methylnaphthalene	12.114	142	456466	3.00	ng	100
16) Acenaphthylene	14.015	152	678690	3.30	ng	100
17) Acenaphthene	14.357	154	418643	3.07	ng	98
18) Fluorene	15.347	166	516206	3.13	ng	99
20) 4,6-Dinitro-2-methylph...	15.436	198	60540	4.81	ng	# 81
21) 4-Bromophenyl-phenylether	16.238	248	175257	3.25	ng	99
22) Hexachlorobenzene	16.348	284	189303	3.08	ng	99
24) Pentachlorophenol	16.689	266	91866	3.73	ng	100
25) Phenanthrene	17.078	178	804429	3.11	ng	100
26) Anthracene	17.163	178	747218	3.29	ng	100
28) Fluoranthene	19.102	202	879704	3.09	ng	99
30) Pyrene	19.465	202	910042	3.08	ng	100
32) Benzo(a)anthracene	21.217	228	922239	3.20	ng	99
33) Chrysene	21.270	228	899226	3.04	ng	100
34) Bis(2-ethylhexyl)phtha...	21.163	149	525273	3.32	ng	99
36) Indeno(1,2,3-cd)pyrene	25.743	276	1111348	3.07	ng	99
37) Benzo(b)fluoranthene	22.796	252	970824	3.15	ng	100
38) Benzo(k)fluoranthene	22.841	252	911304	2.99	ng	97
39) Benzo(a)pyrene	23.371	252	881357	3.14	ng	99
40) Dibenzo(a,h)anthracene	25.764	278	909406	3.08	ng	99
41) Benzo(g,h,i)perylene	26.435	276	959460	3.09	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016908.D
Acq On : 12 Oct 2021 21:11
Operator : CG/JU
Sample : SSTDIC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Oct 13 01:54:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 01:50:22 2021
Response via : Initial Calibration

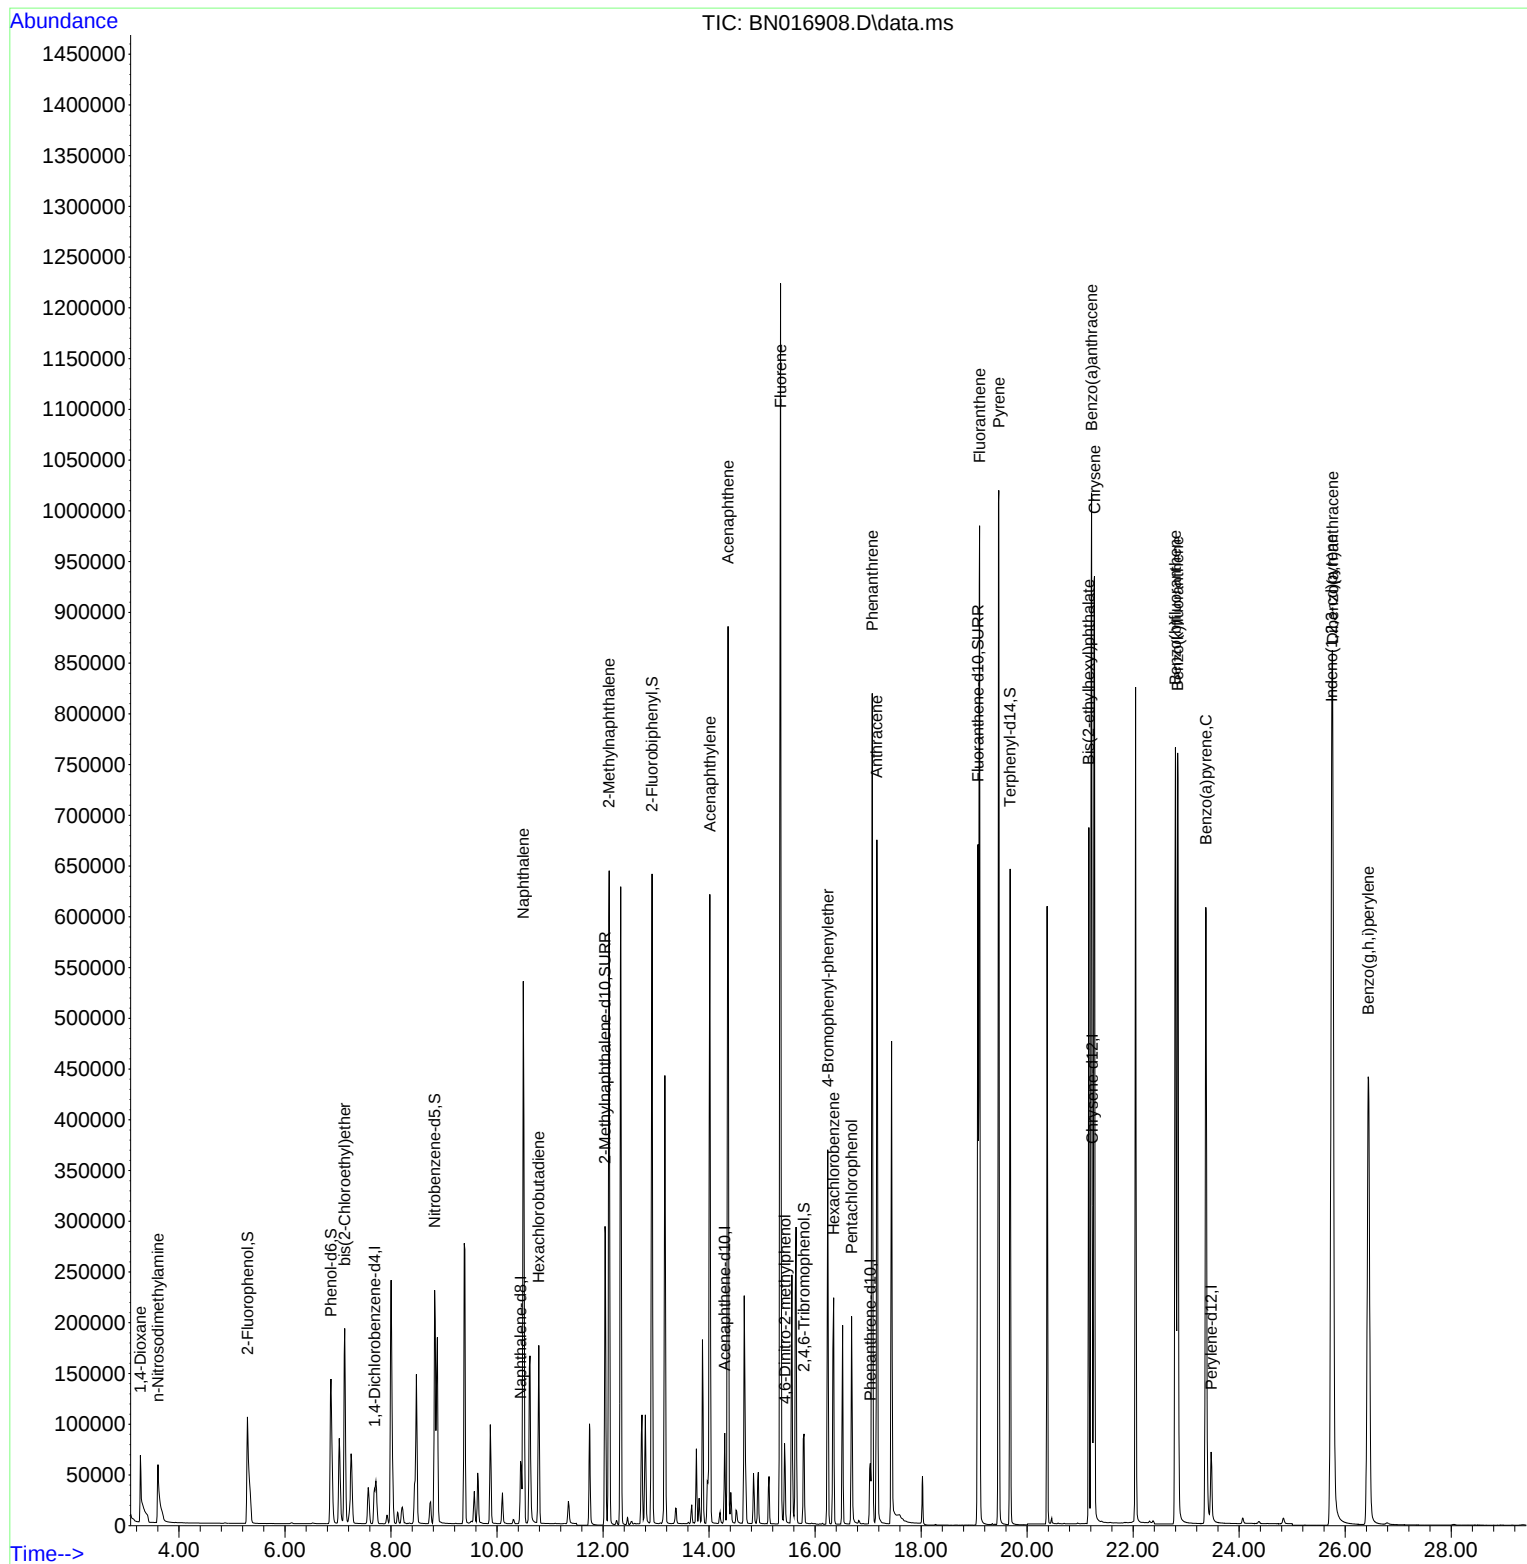







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.688 min Scan# 500
 Delta R.T. -0.001 min
 Lab File: BN016908.D
 Acq: 12 Oct 2021 21:11

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:152 Resp: 21339




Ion	Ratio	Lower	Upper
152	100		
150	156.7	122.6	183.8
115	57.8	46.1	69.1

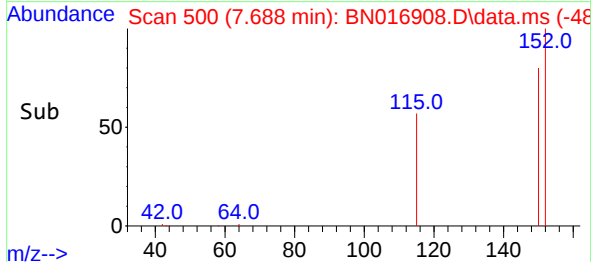


#2
 1,4-Dioxane
 Concen: 2.84 ng
 RT: 3.272 min Scan# 21
 Delta R.T. -0.010 min
 Lab File: BN016908.D
 Acq: 12 Oct 2021 21:11

Tgt Ion: 88 Resp: 45418

Ion	Ratio	Lower	Upper
88	100		
43	27.5	24.3	36.5
58	75.2	65.2	97.8


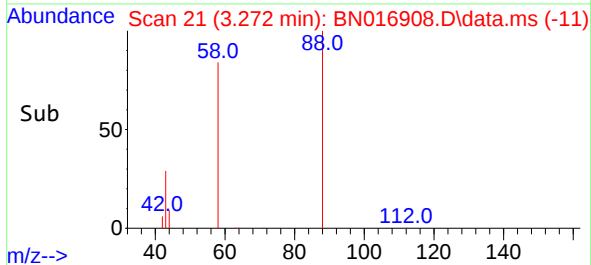

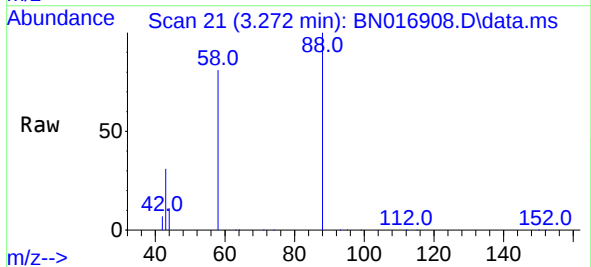


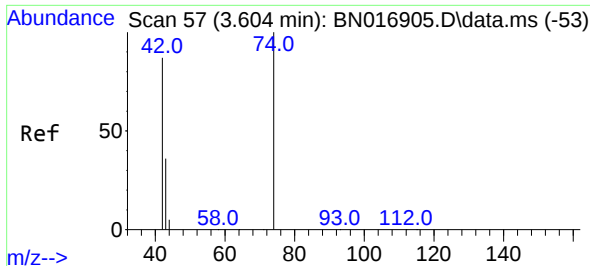

#3
n-Nitrosodimethylamine
Concen: 3.22 ng
RT: 3.603 min Scan# 57
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 56086
Ion Ratio Lower Upper
42 100
74 145.7 114.4 171.6
44 6.5 5.7 8.5

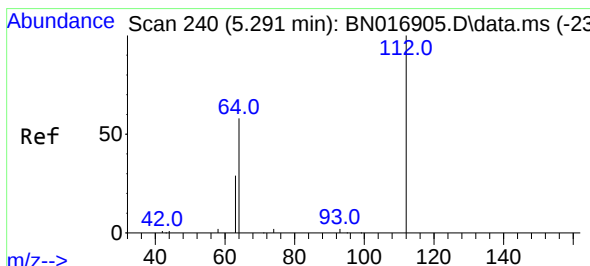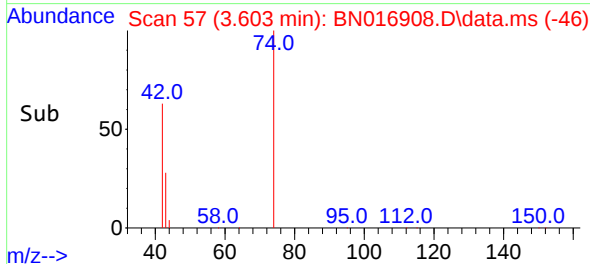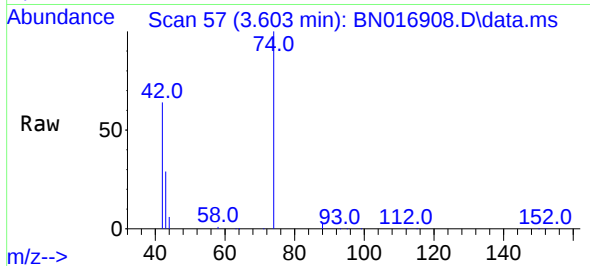

#4
2-Fluorophenol
Concen: 2.89 ng
RT: 5.291 min Scan# 240
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion: 112 Resp: 157693
Ion Ratio Lower Upper
112 100
64 56.0 45.0 67.4
63 28.2 22.6 33.8


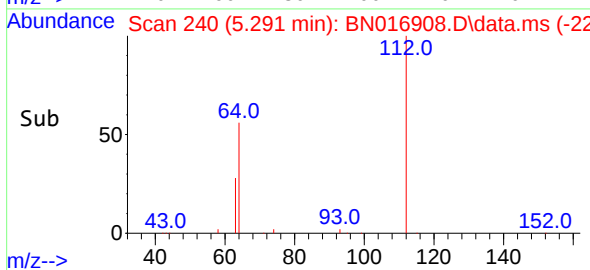

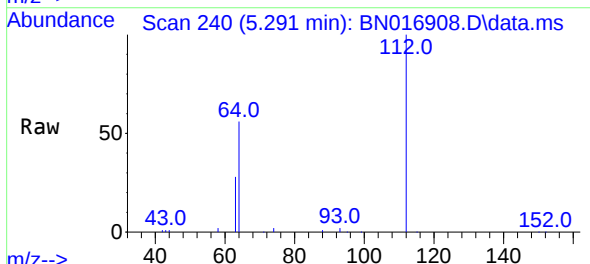




#5
Phenol-d6
Concen: 2.96 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 181295
Ion Ratio Lower Upper
99 100
42 17.5 14.2 21.4
71 30.7 24.5 36.7

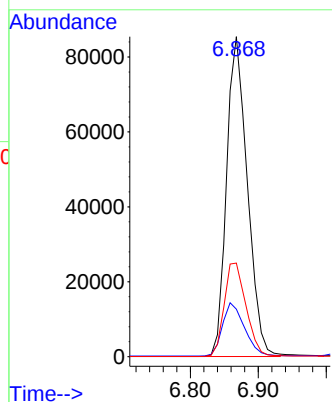

#6
bis(2-Chloroethyl)ether
Concen: 2.96 ng
RT: 7.126 min Scan# 439
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion: 93 Resp: 177203
Ion Ratio Lower Upper
93 100
63 74.1 60.3 90.5
95 32.5 26.2 39.4


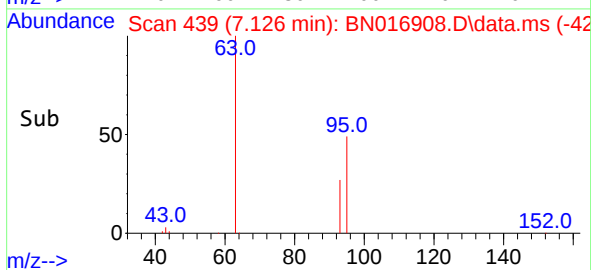
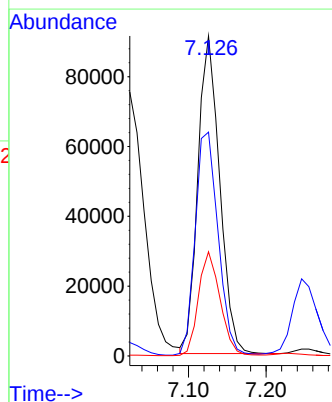





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.444 min Scan# 736
Delta R.T. -0.013 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	89216
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	9.1	3.7	5.5#
68	7.3	3.2	4.8#

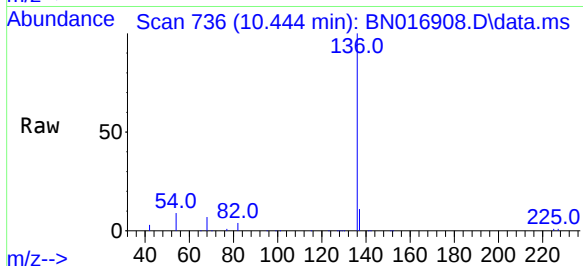

#8
Nitrobenzene-d5
Concen: 3.40 ng
RT: 8.822 min Scan# 608
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:	82	Resp:	205177
Ion	Ratio	Lower	Upper
82	100		
128	37.3	28.3	42.5
54	50.9	43.0	64.4


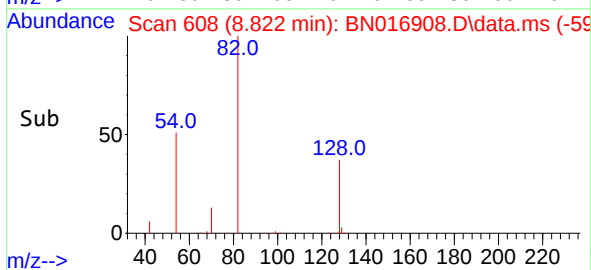

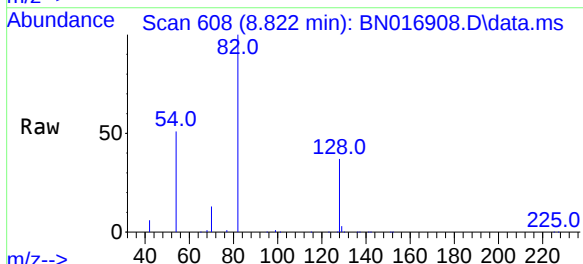




#9
Naphthalene
Concen: 2.94 ng
RT: 10.495 min Scan# 740
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampled :
SSTDICC3.2


Tgt Ion:128 Resp: 714760
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 13.1 10.6 16.0

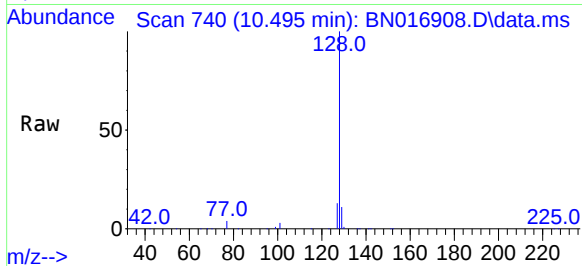

#10
Hexachlorobutadiene
Concen: 3.07 ng
RT: 10.787 min Scan# 763
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:225 Resp: 139962
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 51.1 76.7



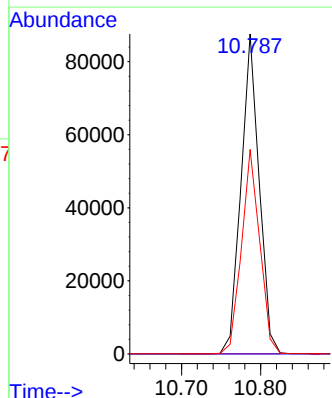
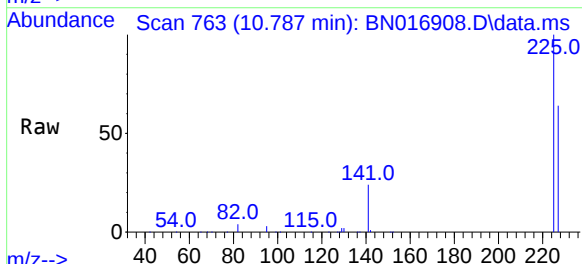


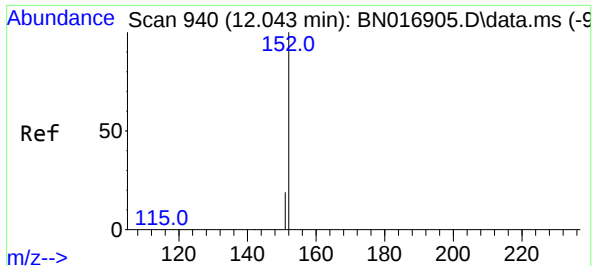

#11
2-Methylnaphthalene-d10
Concen: 3.08 ng
RT: 12.038 min Scan# 939
Delta R.T. -0.005 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 397830
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4

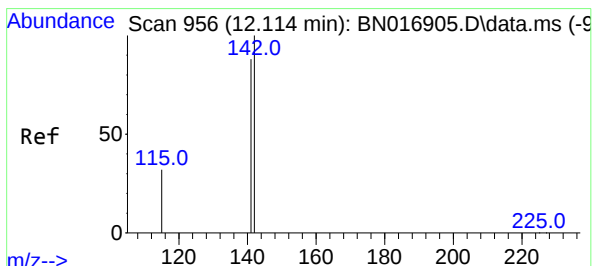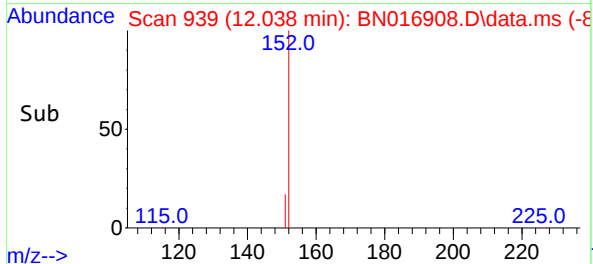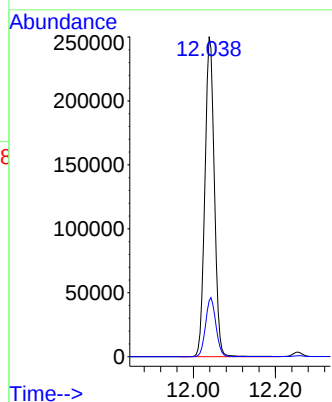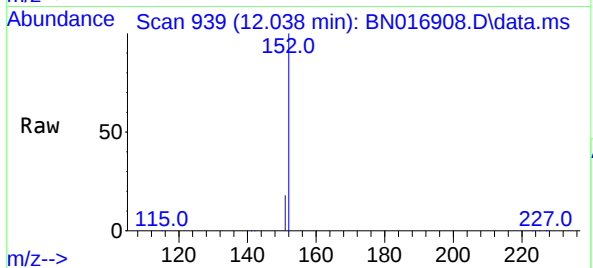

#12
2-Methylnaphthalene
Concen: 3.00 ng
RT: 12.114 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:142 Resp: 456466
Ion Ratio Lower Upper
142 100
141 88.1 70.5 105.7
115 32.7 26.0 39.0


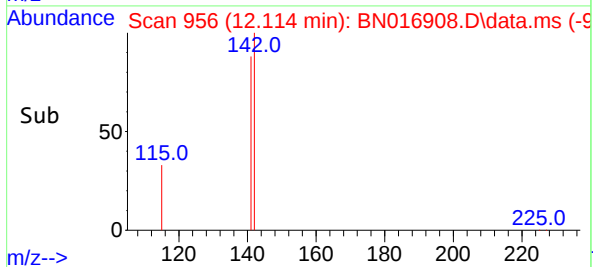
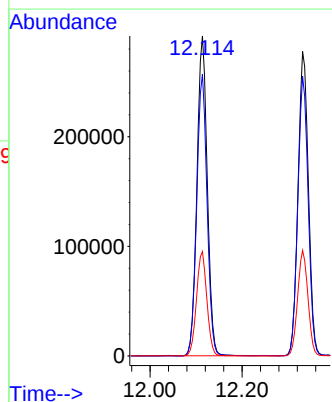
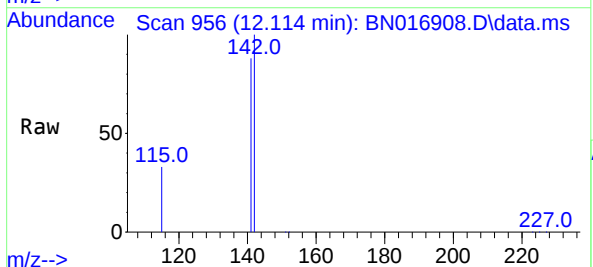




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.294 min Scan# 1185
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 48142
Ion Ratio Lower Upper
164 100
162 102.2 81.4 122.0
160 45.8 37.0 55.4

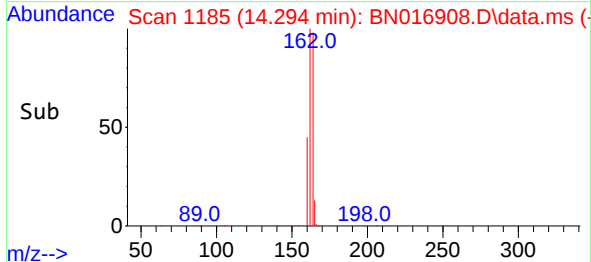

#14
2,4,6-Tribromophenol
Concen: 3.53 ng
RT: 15.791 min Scan# 1303
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:330 Resp: 82342
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.8 24.4 36.6


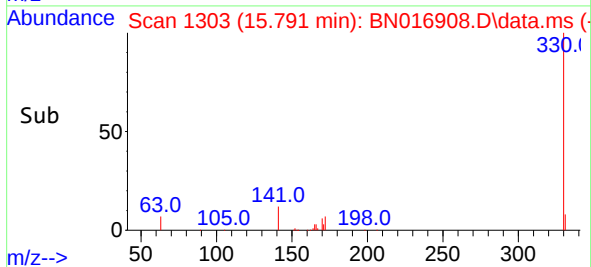

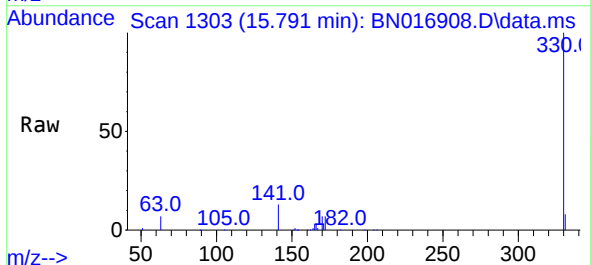


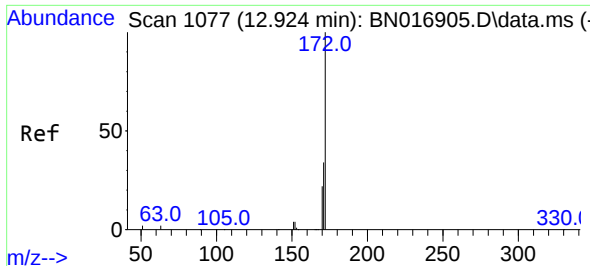

#15
2-Fluorobiphenyl
Concen: 3.01 ng
RT: 12.924 min Scan# 1077
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 555299
Ion Ratio Lower Upper
172 100
171 34.2 27.4 41.0
170 22.3 18.1 27.1

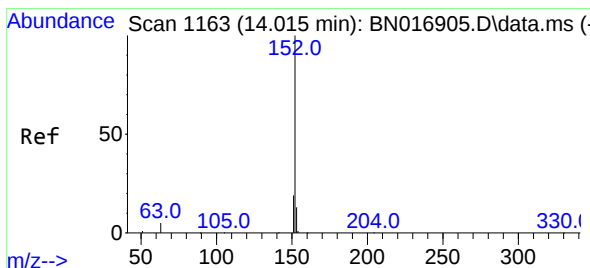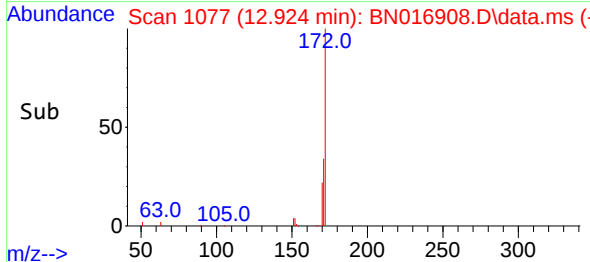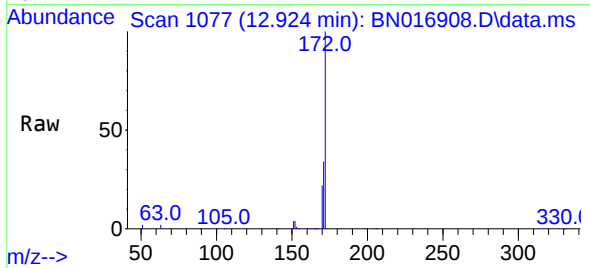

#16
Acenaphthylene
Concen: 3.30 ng
RT: 14.015 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:152 Resp: 678690
Ion Ratio Lower Upper
152 100
151 19.5 15.5 23.3
153 13.0 10.3 15.5


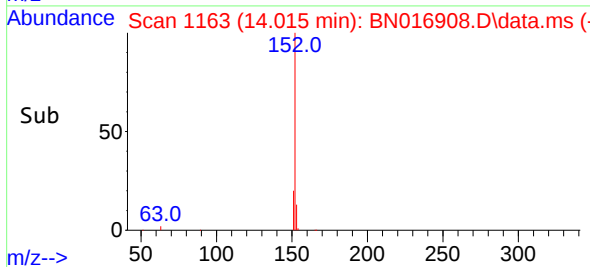

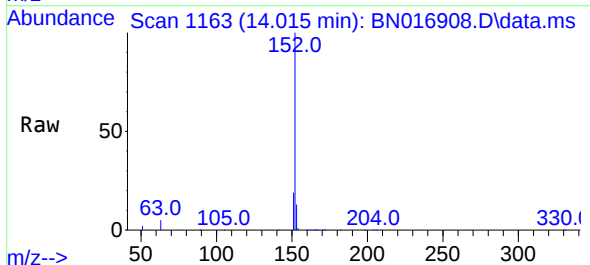




#17
Acenaphthene
Concen: 3.07 ng
RT: 14.357 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 418643
Ion Ratio Lower Upper
154 100
153 112.0 91.2 136.8
152 53.6 44.4 66.6



#18
Fluorene
Concen: 3.13 ng
RT: 15.347 min Scan# 1268
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:166 Resp: 516206
Ion Ratio Lower Upper
166 100
165 96.8 78.1 117.1
167 13.5 10.7 16.1


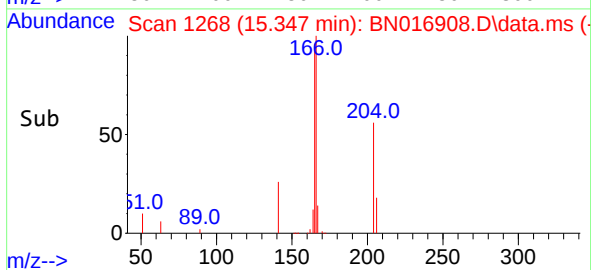






#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 89923
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.5 4.9 7.3

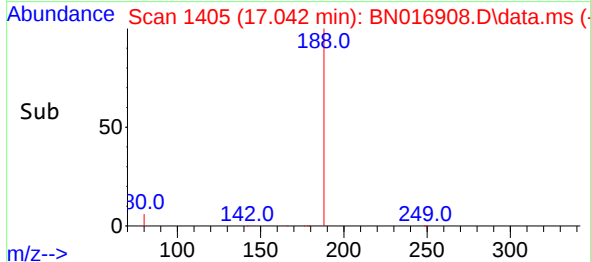

#20
4,6-Dinitro-2-methylphenol
Concen: 4.81 ng
RT: 15.436 min Scan# 1275
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:198 Resp: 60540
Ion Ratio Lower Upper
198 100
182 6.1 11.0 16.6#
77 0.0 0.0 0.0


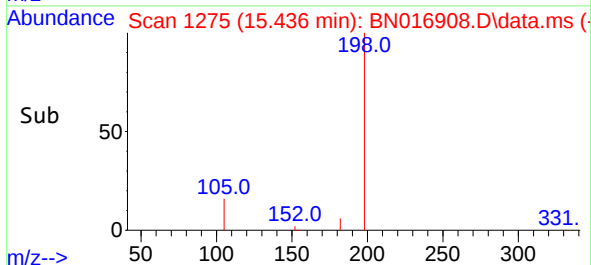
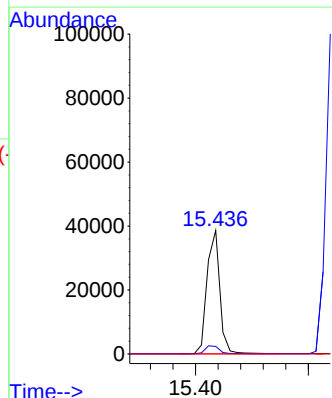
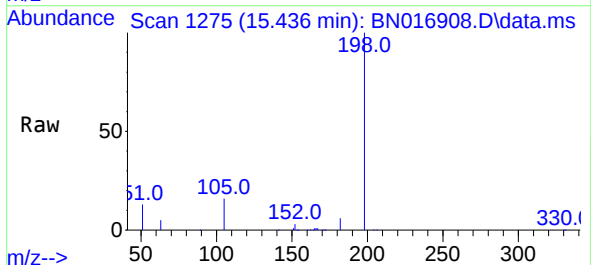




#21
4-Bromophenyl-phenylether
Concen: 3.25 ng
RT: 16.238 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 175257
Ion Ratio Lower Upper
248 100
250 97.1 78.2 117.2
141 51.9 43.1 64.7



#22
Hexachlorobenzene
Concen: 3.08 ng
RT: 16.348 min Scan# 1348
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:284 Resp: 189303
Ion Ratio Lower Upper
284 100
142 31.8 25.1 37.7
249 29.6 23.2 34.8


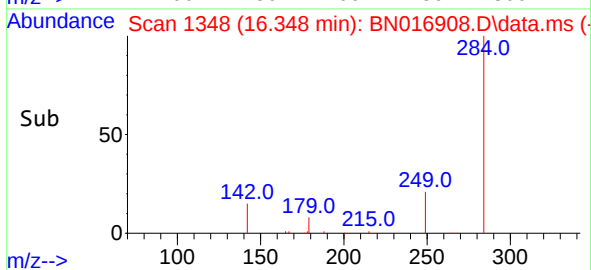






#24
Pentachlorophenol
Concen: 3.73 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:266 Resp: 91866
Ion Ratio Lower Upper
266 100
264 62.7 50.5 75.7
268 63.7 51.2 76.8

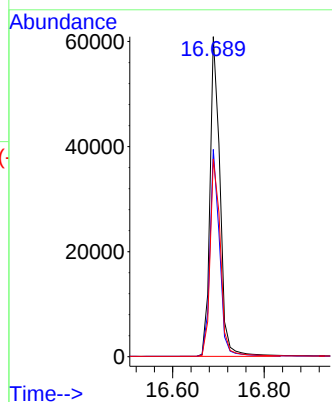

#25
Phenanthrene
Concen: 3.11 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:178 Resp: 804429
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.4
179 15.4 12.3 18.5









#26
 Anthracene
 Concen: 3.29 ng
 RT: 17.163 min Scan# 1415
 Delta R.T. -0.000 min
 Lab File: BN016908.D
 Acq: 12 Oct 2021 21:11

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:178 Resp: 747218




Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.6	21.8
179	15.5	12.2	18.4

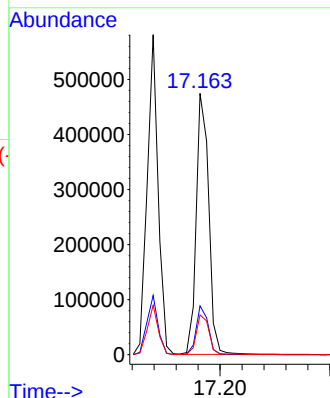


#27
 Fluoranthene-d10
 Concen: 3.19 ng
 RT: 19.073 min Scan# 1698
 Delta R.T. -0.000 min
 Lab File: BN016908.D
 Acq: 12 Oct 2021 21:11

Tgt Ion:212 Resp: 753590

Ion	Ratio	Lower	Upper
212	100		
106	13.6	10.7	16.1
104	7.4	5.8	8.8



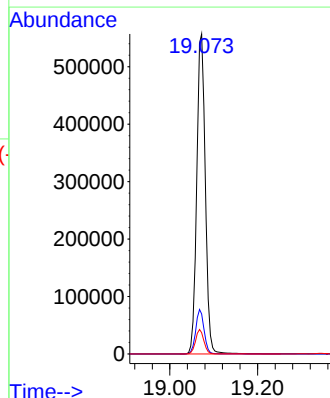





#28
Fluoranthene
Concen: 3.09 ng
RT: 19.102 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:202 Resp: 879704
Ion Ratio Lower Upper
202 100
101 11.5 9.0 13.4
203 17.5 13.8 20.8



#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:240 Resp: 89992
Ion Ratio Lower Upper
240 100
120 9.6 8.6 12.8
236 26.3 21.0 31.4



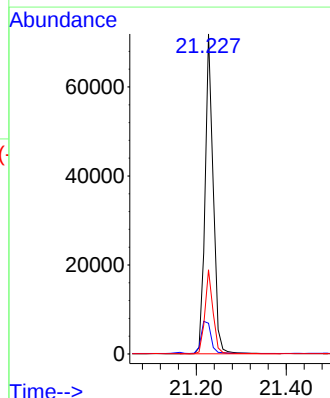





#30
Pyrene
Concen: 3.08 ng
RT: 19.465 min Scan# 1777
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:202 Resp: 910042
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 17.6 14.0 21.0



#31
Terphenyl-d14
Concen: 3.07 ng
RT: 19.678 min Scan# 1820
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:244 Resp: 628226
Ion Ratio Lower Upper
244 100
212 7.1 5.7 8.5
122 12.3 9.8 14.6


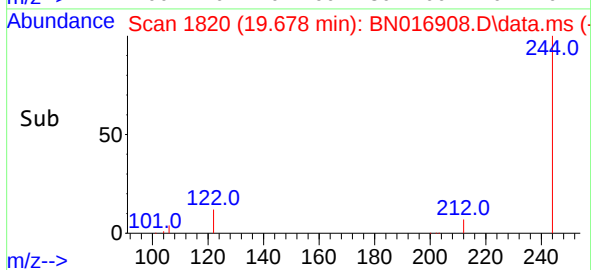






#32
Benzo(a)anthracene
Concen: 3.20 ng
RT: 21.217 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:228 Resp: 922239
Ion Ratio Lower Upper
228 100
226 26.0 20.6 31.0
229 20.2 15.8 23.8

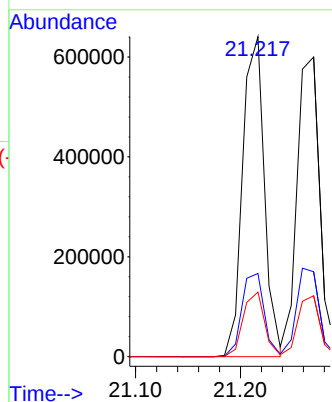

#33
Chrysene
Concen: 3.04 ng
RT: 21.270 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:228 Resp: 899226
Ion Ratio Lower Upper
228 100
226 28.3 22.6 34.0
229 20.3 16.0 24.0


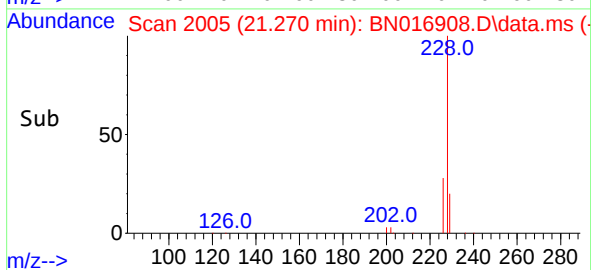




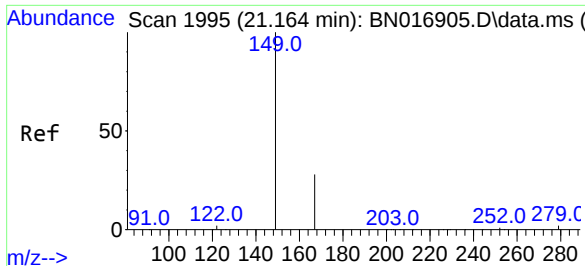

#34
Bis(2-ethylhexyl)phthalate
Concen: 3.32 ng
RT: 21.163 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:149 Resp: 525273
Ion Ratio Lower Upper
149 100
167 28.2 22.1 33.1
279 4.5 3.4 5.0

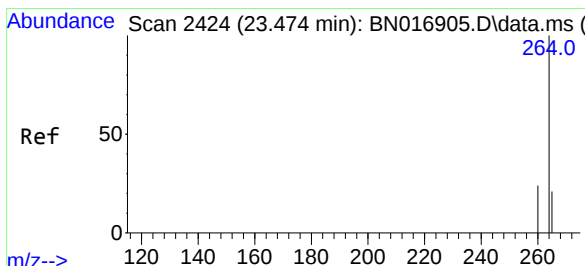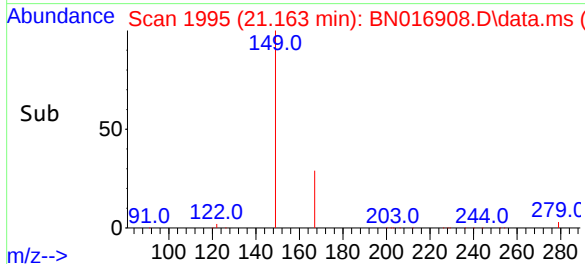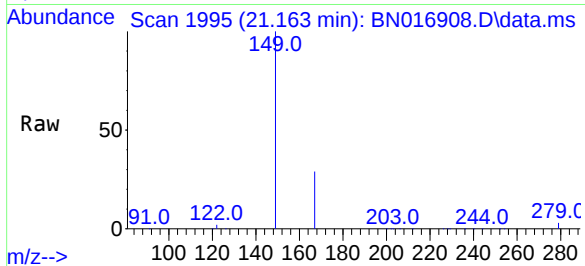

#35
Perylene-d12
Concen: 0.40 ng
RT: 23.471 min Scan# 2423
Delta R.T. -0.004 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11


Tgt Ion:264 Resp: 92200
Ion Ratio Lower Upper
264 100
260 24.4 19.4 29.2
265 22.9 18.6 27.8

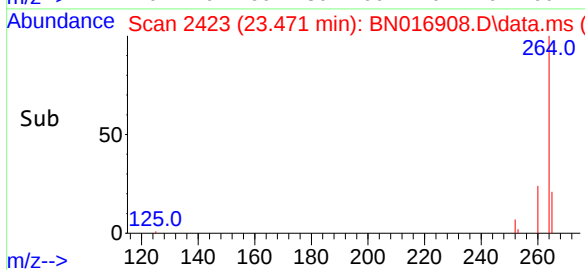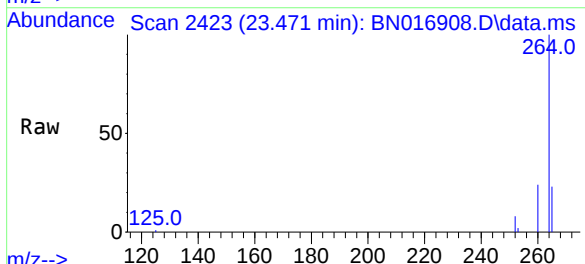






#36
Indeno(1,2,3-cd)pyrene
Concen: 3.07 ng
RT: 25.743 min Scan# 3087
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2





Tgt Ion:276 Resp: 1111348
Ion Ratio Lower Upper
276 100
138 24.3 20.2 30.4
277 25.2 20.2 30.4

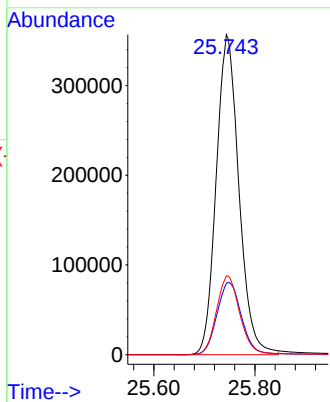


#37
Benzo(b)fluoranthene
Concen: 3.15 ng
RT: 22.796 min Scan# 2226
Delta R.T. -0.004 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

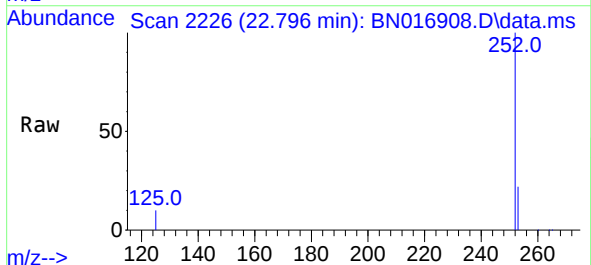

Tgt Ion:252 Resp: 970824
Ion Ratio Lower Upper
252 100
253 22.1 17.7 26.5
125 9.9 7.8 11.8




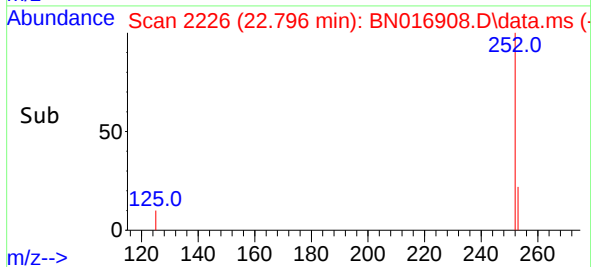




#38
Benzo(k)fluoranthene
Concen: 2.99 ng
RT: 22.841 min Scan# 2239
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 911304
Ion Ratio Lower Upper
252 100
253 21.8 18.1 27.1
125 9.9 9.8 14.8

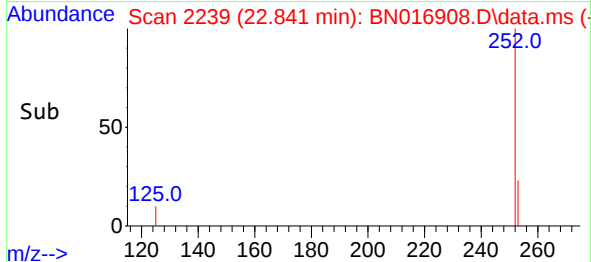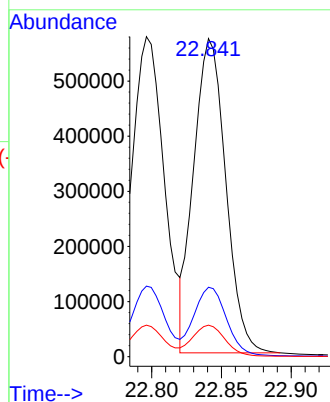

#39
Benzo(a)pyrene
Concen: 3.14 ng
RT: 23.371 min Scan# 2394
Delta R.T. -0.004 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:252 Resp: 881357
Ion Ratio Lower Upper
252 100
253 21.9 18.1 27.1
125 10.8 9.0 13.4


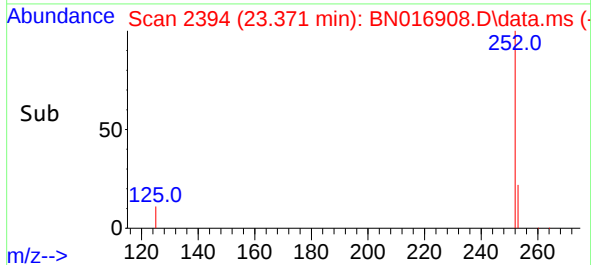

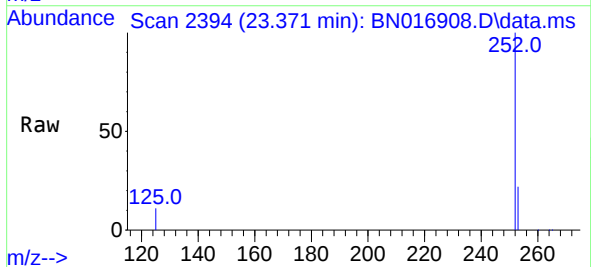




#40
Dibenzo(a,h)anthracene
Concen: 3.08 ng
RT: 25.764 min Scan# 3093
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:278 Resp: 909406
Ion Ratio Lower Upper
278 100
139 16.1 13.8 20.6
279 23.6 19.0 28.6

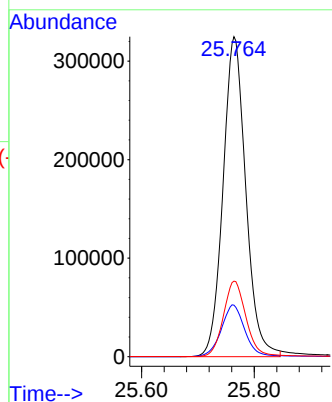

#41
Benzo(g,h,i)perylene
Concen: 3.09 ng
RT: 26.435 min Scan# 3289
Delta R.T. -0.000 min
Lab File: BN016908.D
Acq: 12 Oct 2021 21:11

Tgt Ion:276 Resp: 959460
Ion Ratio Lower Upper
276 100
277 23.7 19.1 28.7
138 20.8 16.6 24.8

