

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
 Data File : BN016916.D
 Acq On : 13 Oct 2021 02:37
 Operator : CG/JU
 Sample : M4170-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P287-DITCH

Manual Integrations
 APPROVED

mohammad
 10/14/2021 10:52:06 AM

Quant Time: Oct 13 06:19:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 02:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.689	152	20912	0.40	ng	0.00
7) Naphthalene-d8	10.445	136	94082	0.40	ng	#-0.01
13) Acenaphthene-d10	14.294	164	52413	0.40	ng	0.00
19) Phenanthrene-d10	17.030	188	99178	0.40	ng	#-0.01
29) Chrysene-d12	21.228	240	98638	0.40	ng	# 0.00
35) Perylene-d12	23.467	264	102952	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.310	112	7409	0.16	ng	0.02
5) Phenol-d6	6.877	99	4861	0.09	ng	0.00
8) Nitrobenzene-d5	8.823	82	18850	0.32	ng	0.00
11) 2-Methylnaphthalene-d10	12.038	152	44994	0.34	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	10407	0.44	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	61799	0.31	ng	0.00
27) Fluoranthene-d10	19.068	212	107256	0.43	ng	0.00
31) Terphenyl-d14	19.679	244	89413	0.41	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.290	88	526m	0.04	ng	
24) Pentachlorophenol	16.689	266	200	0.20	ng	99
34) Bis(2-ethylhexyl)phtha...	21.164	149	17391	0.28	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016916.D
Acq On : 13 Oct 2021 02:37
Operator : CG/JU
Sample : M4170-01
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
P287-DITCH

Manual Integrations
APPROVED


mohammad
10/14/2021 10:52:06 AM

Quant Time: Oct 13 06:19:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 02:19:57 2021
Response via : Initial Calibration



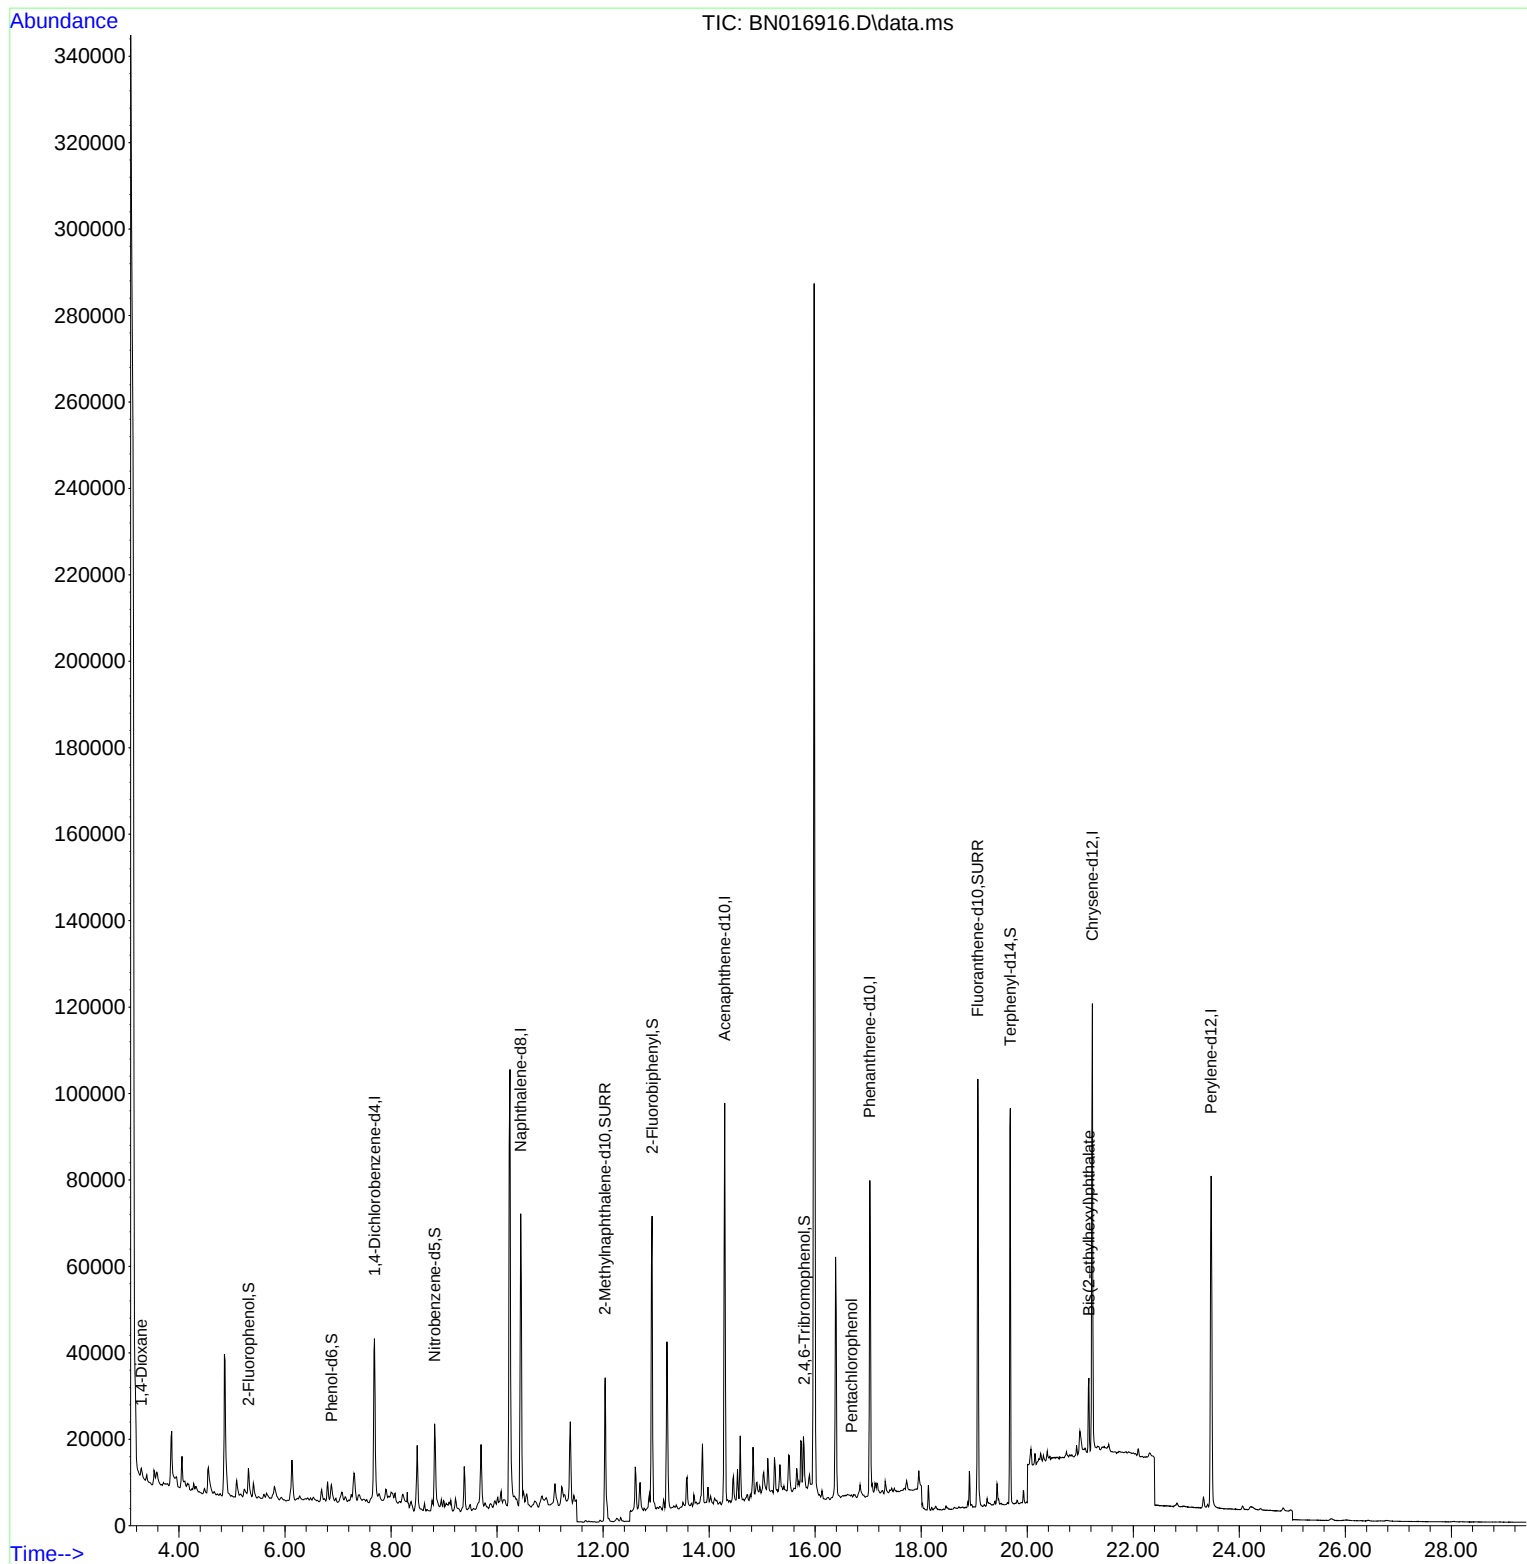





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.689 min Scan# 500
 Delta R.T. -0.000 min
 Lab File: BN016916.D
 Acq: 13 Oct 2021 02:37

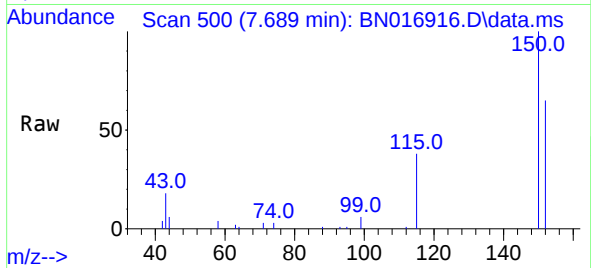



Tgt Ion: 152 Resp: 20912
 Ion Ratio Lower Upper
 152 100
 150 152.9 122.6 183.8
 115 58.2 46.1 69.1

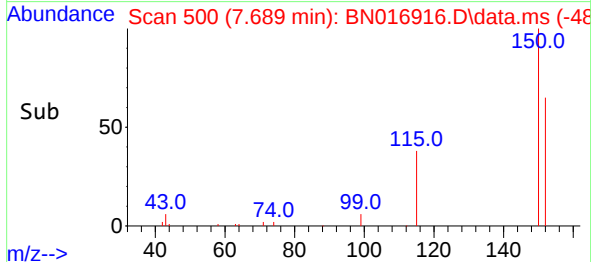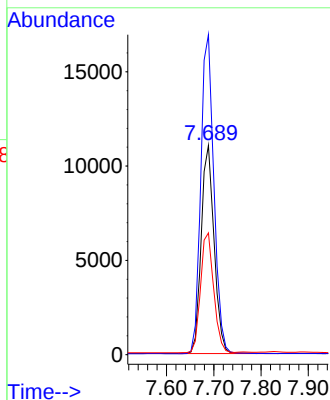

#2
 1,4-Dioxane
 Concen: 0.04 ng m
 RT: 3.290 min Scan# 23
 Delta R.T. 0.009 min
 Lab File: BN016916.D
 Acq: 13 Oct 2021 02:37

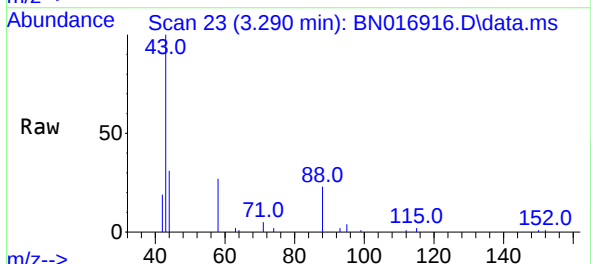


Tgt Ion: 88 Resp: 526
 Ion Ratio Lower Upper
 88 100
 43 218.8 24.3 36.5#
 58 39.5 65.2 97.8#

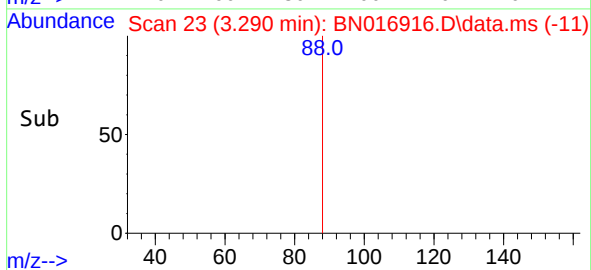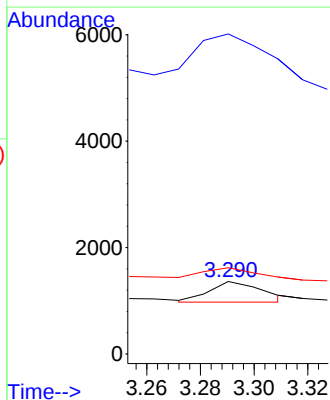

Instrument :
 BNA_N
 ClientSampleId :
 P287-DITCH

Manual Integrations
 APPROVED

mohammad
 10/14/2021 10:52:06 AM







#4
2-Fluorophenol
Concen: 0.16 ng
RT: 5.310 min Scan# 242
Delta R.T. 0.018 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

Tgt Ion: 112 Resp: 7409
Ion Ratio Lower Upper
112 100
64 53.3 45.0 67.4
63 27.4 22.6 33.8

Instrument :
BNA_N
ClientSampleId :
P287-DITCH




Manual Integrations
APPROVED


mohammad
10/14/2021 10:52:06 AM

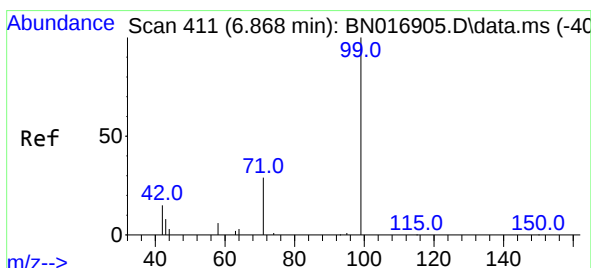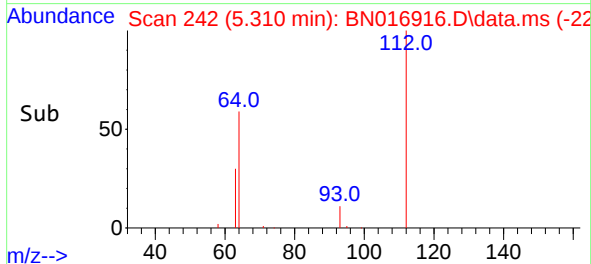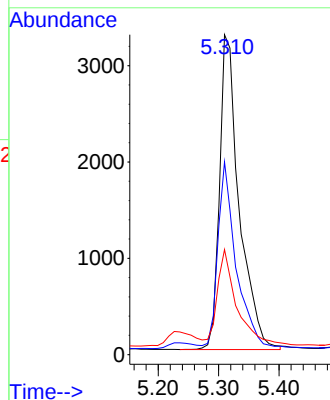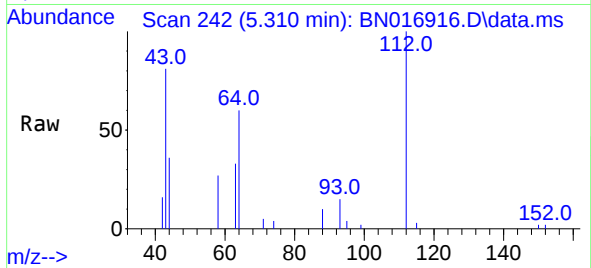

#5
Phenol-d6
Concen: 0.09 ng
RT: 6.877 min Scan# 412
Delta R.T. 0.009 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37


Tgt Ion: 99 Resp: 4861
Ion Ratio Lower Upper
99 100
42 19.0 14.2 21.4
71 33.5 24.5 36.7

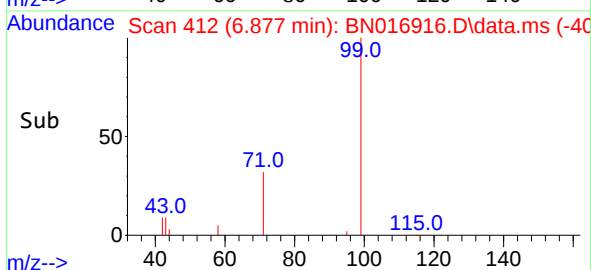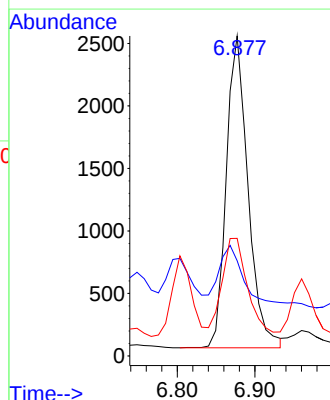

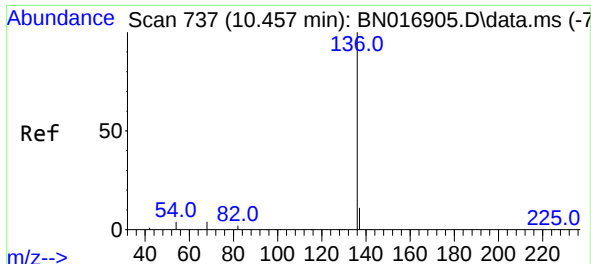

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.445 min Scan# 736
Delta R.T. -0.012 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37




Instrument :
BNA_N
ClientSampleId :
P287-DITCH



Tgt Ion:136 Resp: 94082
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 8.6 3.7 5.5#
68 7.3 3.2 4.8#




Manual Integrations
APPROVED


mohammad
10/14/2021 10:52:06 AM

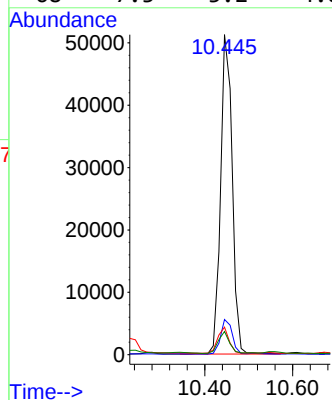

#8
Nitrobenzene-d5
Concen: 0.32 ng
RT: 8.823 min Scan# 608
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

Tgt Ion: 82 Resp: 18850
Ion Ratio Lower Upper
82 100
128 38.4 28.3 42.5
54 52.8 43.0 64.4

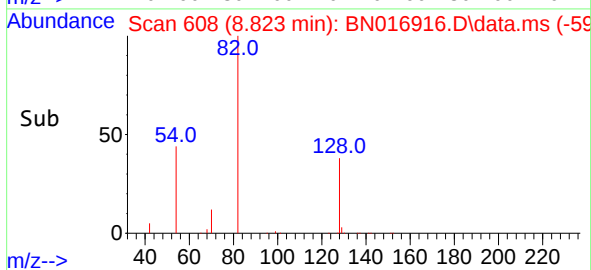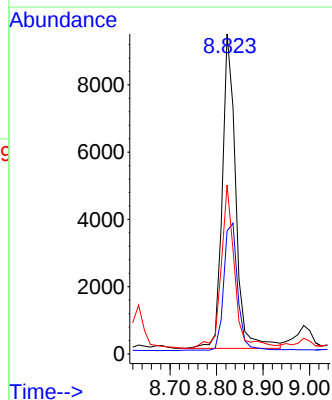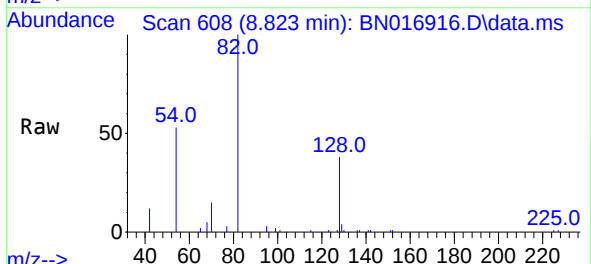

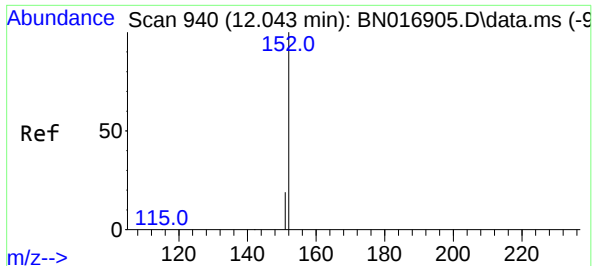





#11
2-Methylnaphthalene-d10
Concen: 0.34 ng
RT: 12.038 min Scan# 939
Delta R.T. -0.004 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

Tgt Ion:152 Resp: 44994
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
P287-DITCH




Manual Integrations
APPROVED


mohammad
10/14/2021 10:52:06 AM

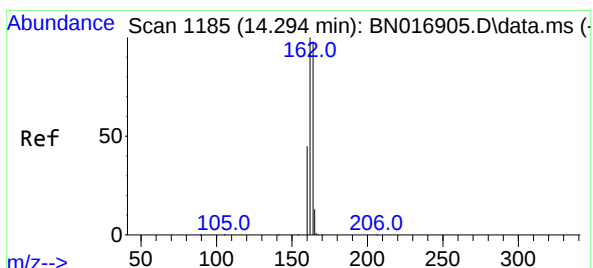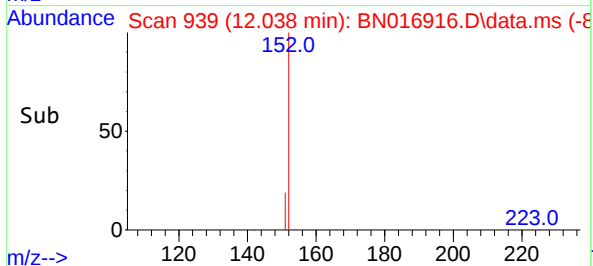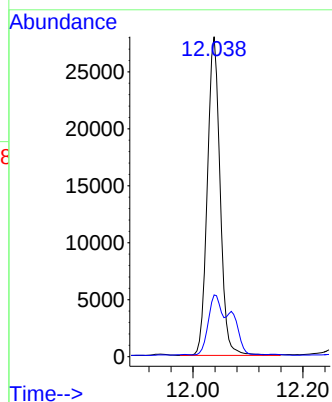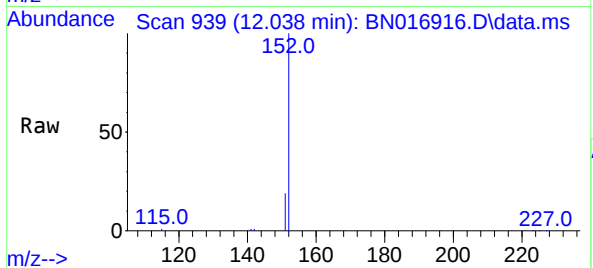

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.294 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37


Tgt Ion:164 Resp: 52413
Ion Ratio Lower Upper
164 100
162 103.0 81.4 122.0
160 45.0 37.0 55.4

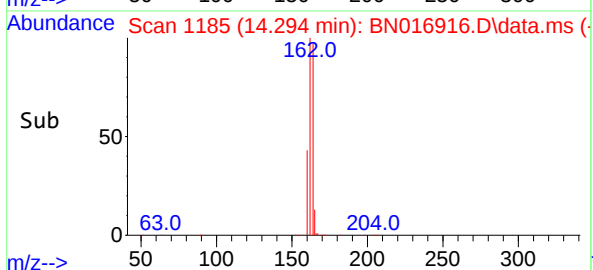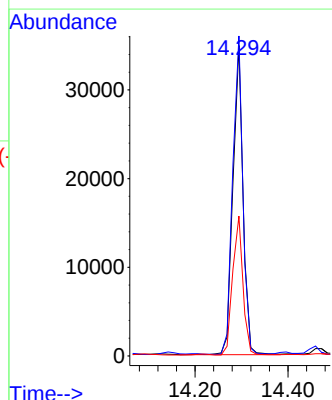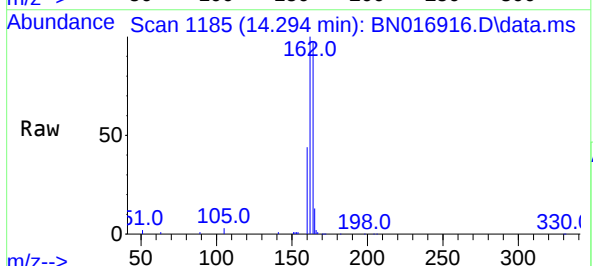



#14
2,4,6-Tribromophenol
Concen: 0.44 ng
RT: 15.791 min Scan# 1303
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37




Instrument :
BNA_N
ClientSampleId :
P287-DITCH

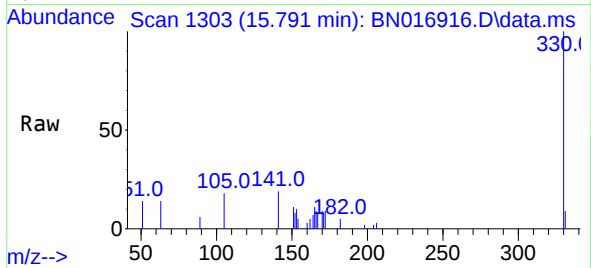


Tgt Ion: 330 Resp: 10407
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 32.0 24.4 36.6

Manual Integrations
APPROVED



mohammad
10/14/2021 10:52:06 AM

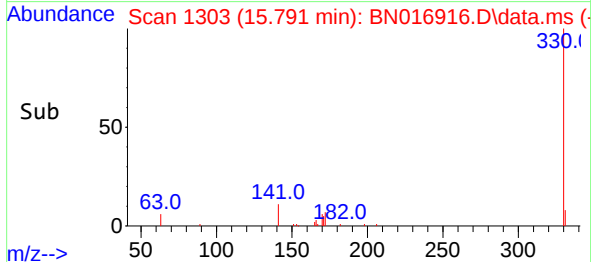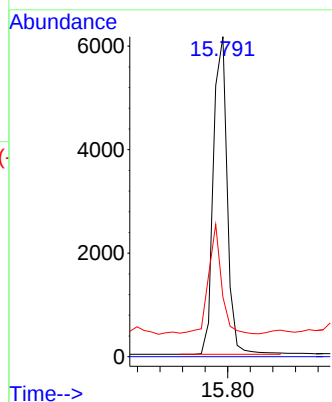


#15
2-Fluorobiphenyl
Concen: 0.31 ng
RT: 12.924 min Scan# 1077
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

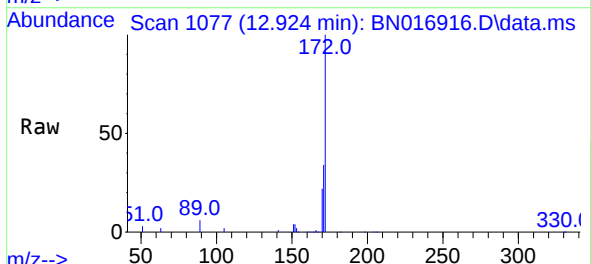

Tgt Ion: 172 Resp: 61799
Ion Ratio Lower Upper
172 100
171 34.0 27.4 41.0
170 22.0 18.1 27.1

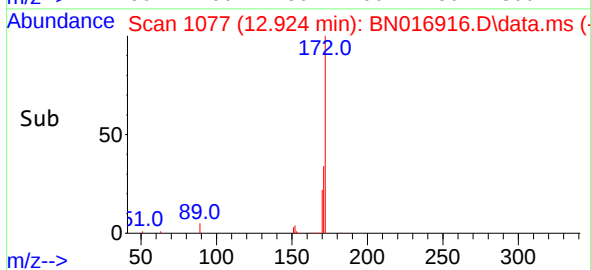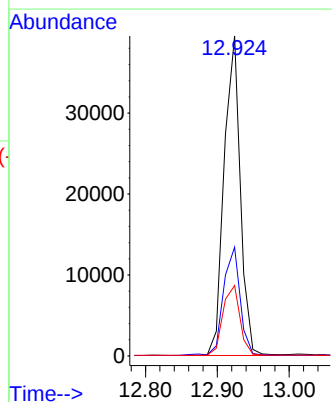







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.030 min Scan# 1404
Delta R.T. -0.012 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

Tgt Ion:188 Resp: 99178
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.5 4.9 7.3#

Instrument :
BNA_N
ClientSampleId :
P287-DITCH




Manual Integrations
APPROVED


mohammad
10/14/2021 10:52:06 AM

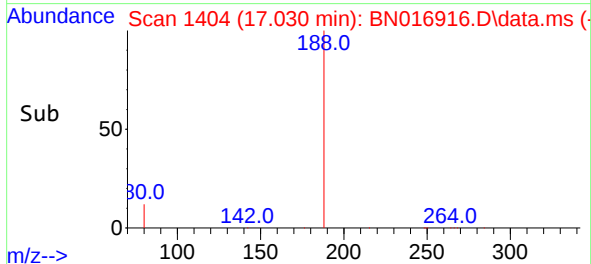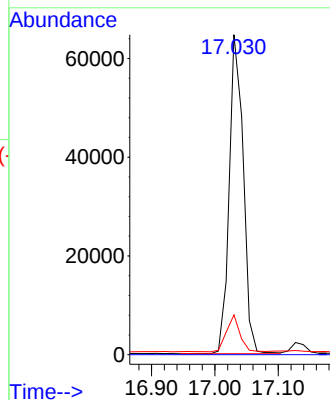


#24
Pentachlorophenol
Concen: 0.20 ng
RT: 16.689 min Scan# 1376
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

Tgt Ion:266 Resp: 200
Ion Ratio Lower Upper
266 100
264 63.0 50.5 75.7
268 66.0 51.2 76.8

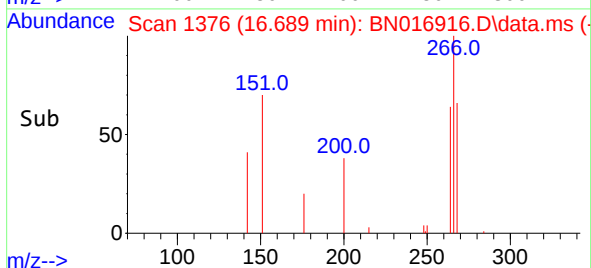
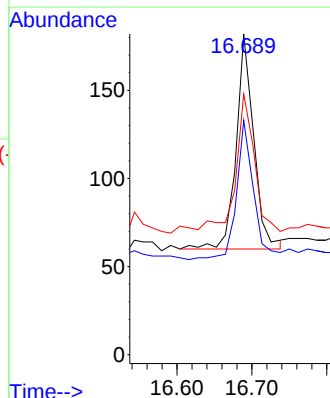
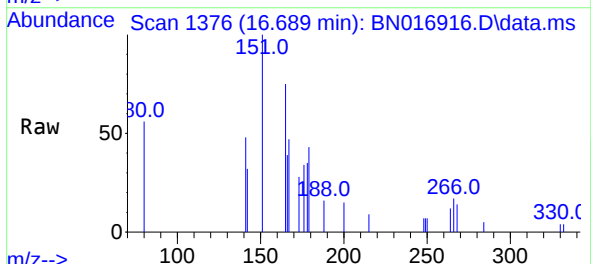


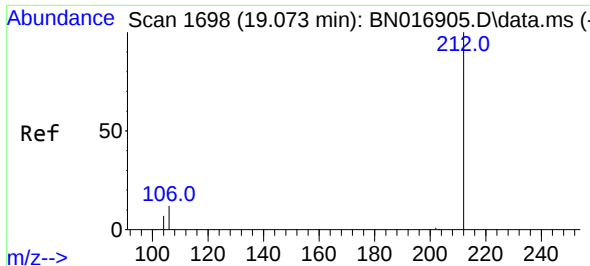


#27
Fluoranthene-d10
Concen: 0.43 ng
RT: 19.068 min Scan# 1697
Delta R.T. -0.005 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

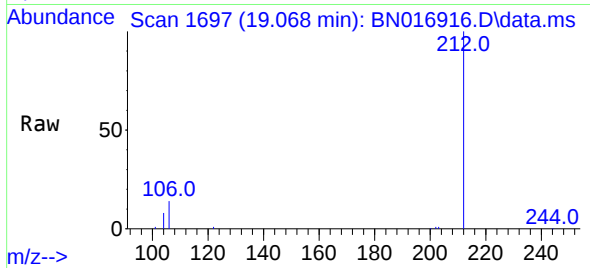



Tgt Ion:212 Resp: 107256
Ion Ratio Lower Upper
212 100
106 13.6 10.7 16.1
104 7.3 5.8 8.8

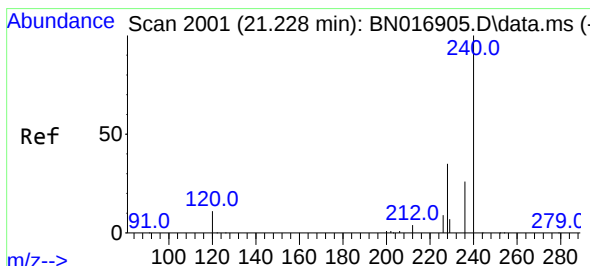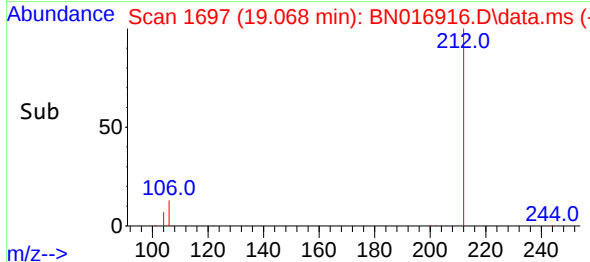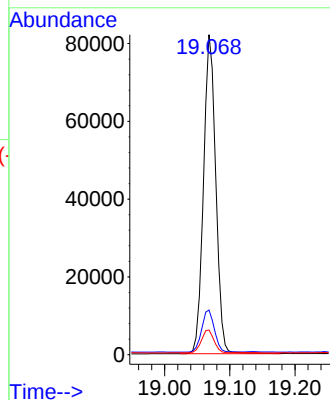

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.228 min Scan# 2001
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

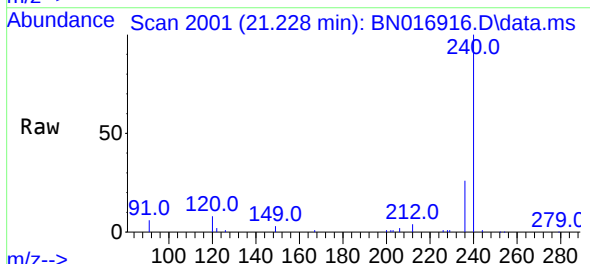


Tgt Ion:240 Resp: 98638
Ion Ratio Lower Upper
240 100
120 8.0 8.6 12.8#
236 25.7 21.0 31.4

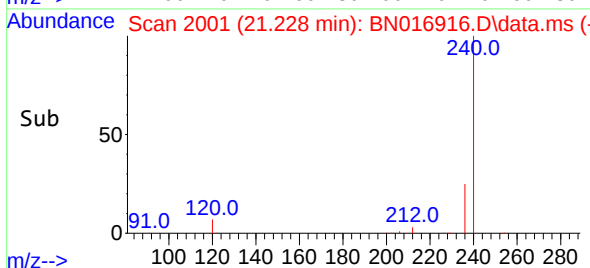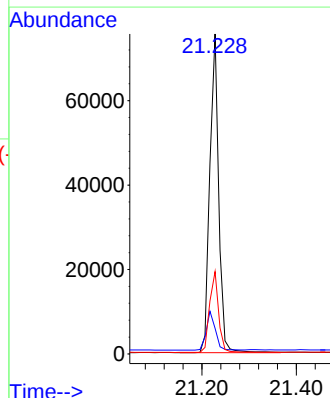


Instrument :
BNA_N
ClientSampleId :
P287-DITCH

Manual Integrations
APPROVED



mohammad
10/14/2021 10:52:06 AM

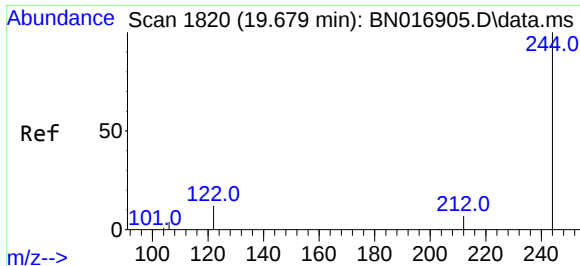

#31
Terphenyl-d14
Concen: 0.41 ng
RT: 19.679 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

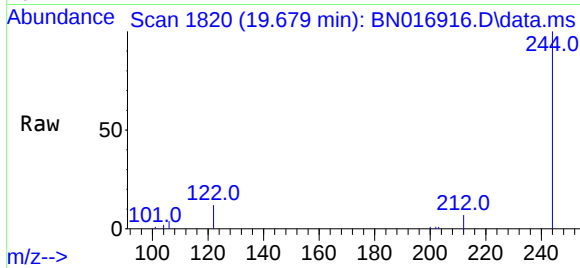


Tgt Ion:244 Resp: 89413
Ion Ratio Lower Upper
244 100
212 7.2 5.7 8.5
122 12.2 9.8 14.6

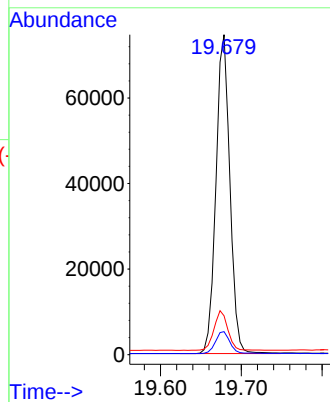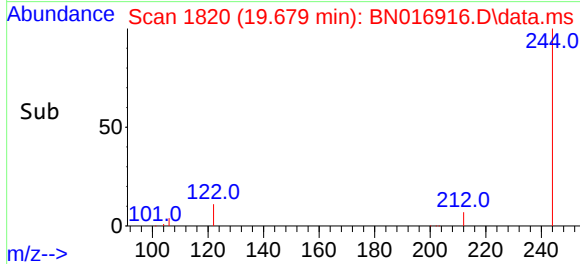


Instrument :
BNA_N
ClientSampleId :
P287-DITCH

Manual Integrations
APPROVED



mohammad
10/14/2021 10:52:06 AM

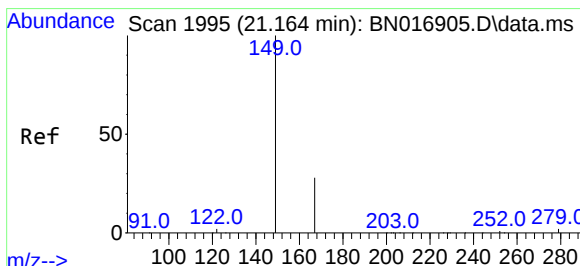


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.28 ng
RT: 21.164 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BN016916.D
Acq: 13 Oct 2021 02:37

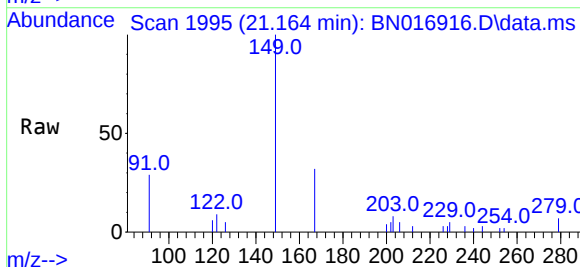


Tgt Ion:149 Resp: 17391
Ion Ratio Lower Upper
149 100
167 27.9 22.1 33.1
279 4.8 3.4 5.0

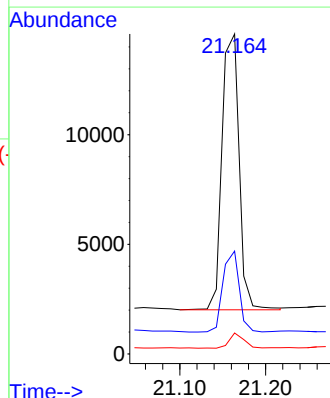
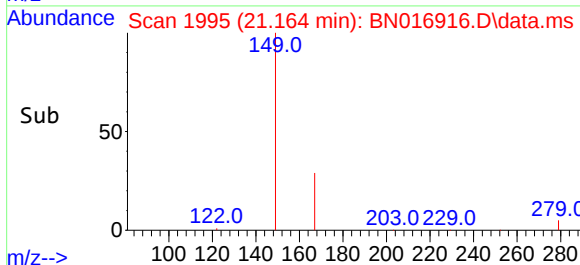


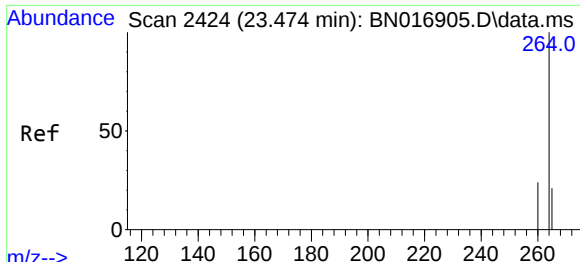

#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.467 min Scan# 2422
 Delta R.T. -0.007 min
 Lab File: BN016916.D
 Acq: 13 Oct 2021 02:37

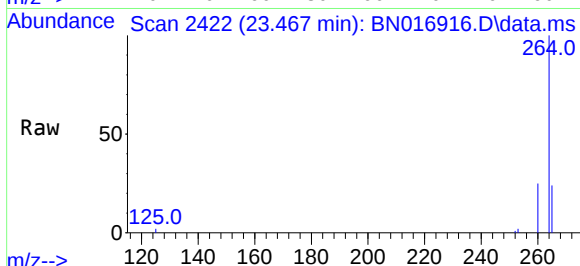

Tgt Ion:	264	Resp:	102952
Ion Ratio	Lower	Upper	
264	100		
260	24.8	19.4	29.2
265	23.8	18.6	27.8

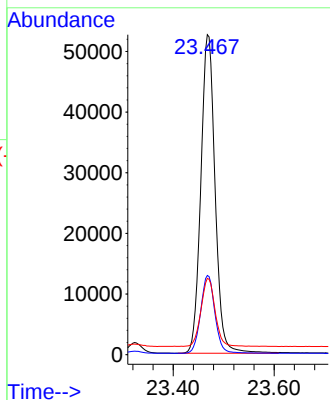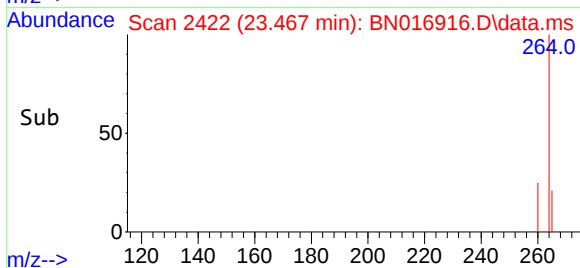

Instrument :
 BNA_N
 ClientSampleId :
 P287-DITCH

Manual Integrations
 APPROVED

mohammad
 10/14/2021 10:52:06 AM